


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091019\
 Data File : BN007571.D
 Acq On : 10 Sep 2019 10:17
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 11 14:14:20 2019

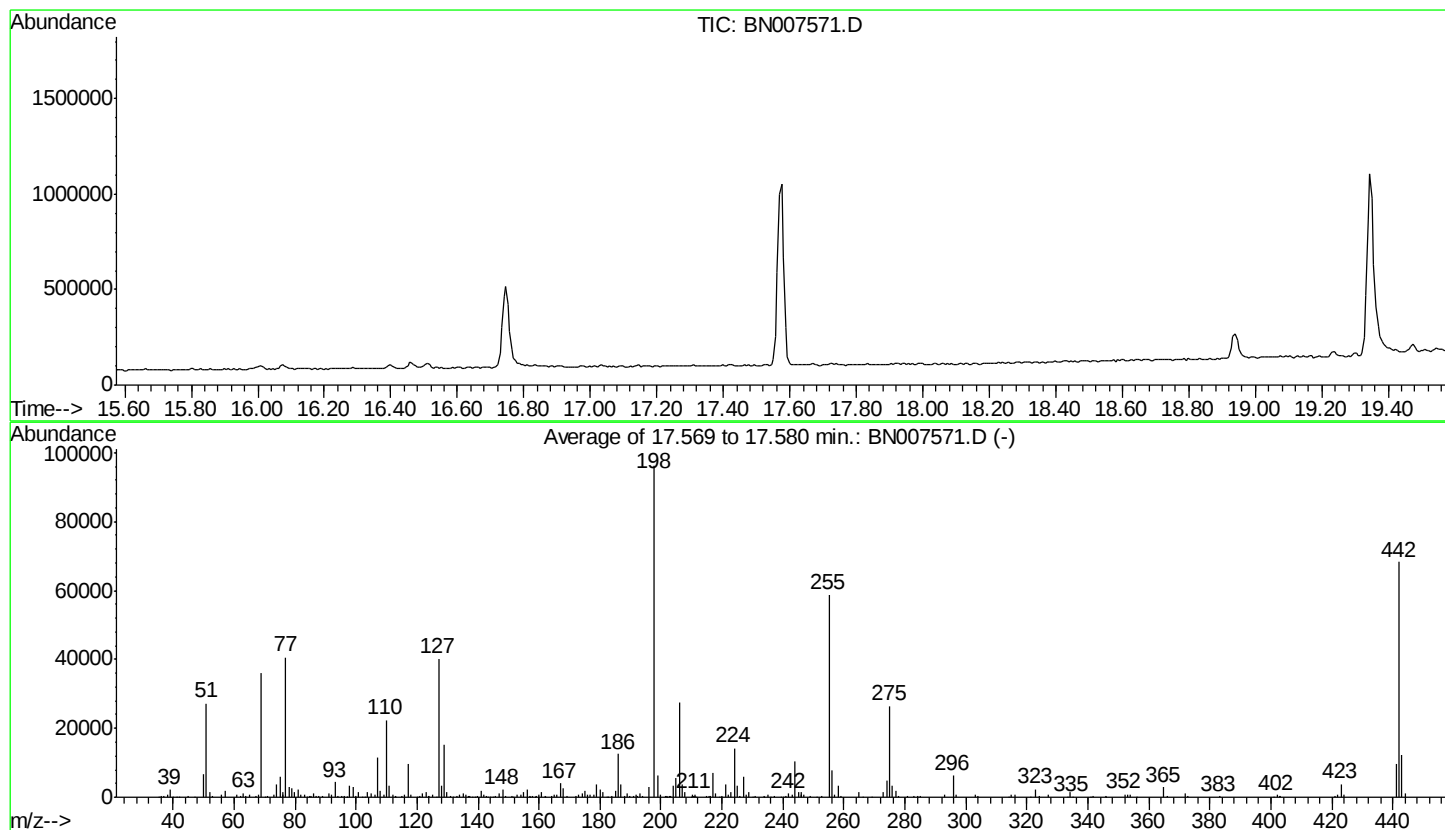

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	27295	PASS
68	69	0.00	2	1.9	684	PASS
69	198	0.00	100	37.3	35949	PASS
70	69	0.00	2	0.2	59	PASS
127	198	10	80	41.8	40194	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	96253	PASS
199	198	5	9	6.7	6416	PASS
275	198	10	60	27.5	26456	PASS
365	198	1	100	3.1	2965	PASS
441	198	0.01	100	10.2	9787	PASS
442	198	50	100	70.9	68250	PASS
443	442	15	24	17.7	12099	PASS