


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091119\
 Data File : BN007585.D
 Acq On : 11 Sep 2019 12:36
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 11 14:14:20 2019

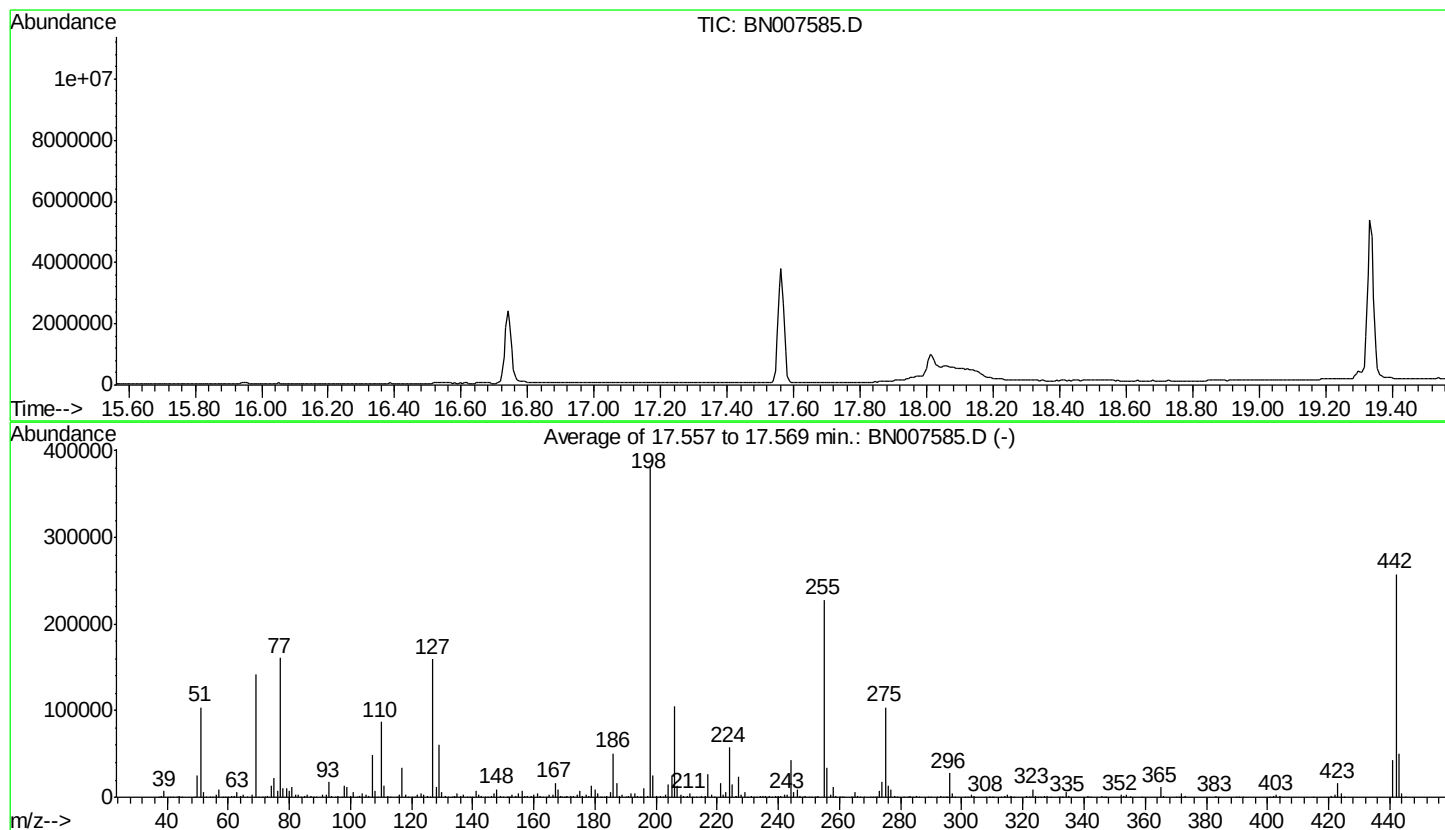

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	103753	PASS
68	69	0.00	2	1.7	2375	PASS
69	198	0.00	100	37.2	142436	PASS
70	69	0.00	2	0.4	523	PASS
127	198	10	80	41.6	159210	PASS
197	198	0.00	2	0.3	1003	PASS
198	198	100	100	100.0	382997	PASS
199	198	5	9	6.7	25776	PASS
275	198	10	60	27.2	104010	PASS
365	198	1	100	3.0	11472	PASS
441	198	0.01	100	11.0	42256	PASS
442	198	50	100	67.2	257344	PASS
443	442	15	24	19.6	50325	PASS