
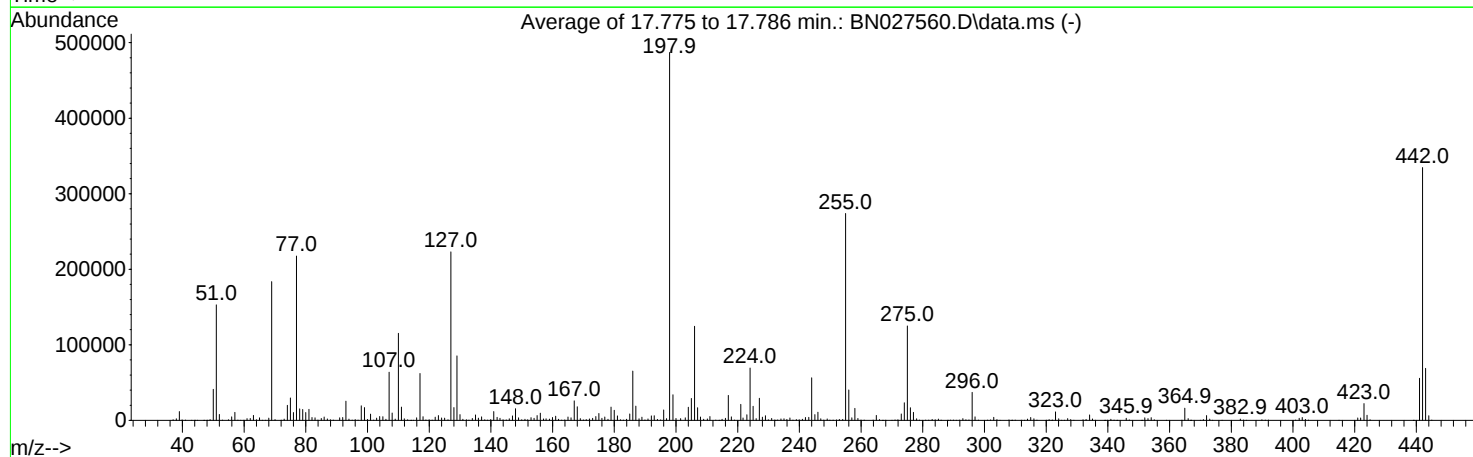


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091123\
Data File : BN027560.D
Acq On : 11 Sep 2023 04:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 12 02:45:58 2023

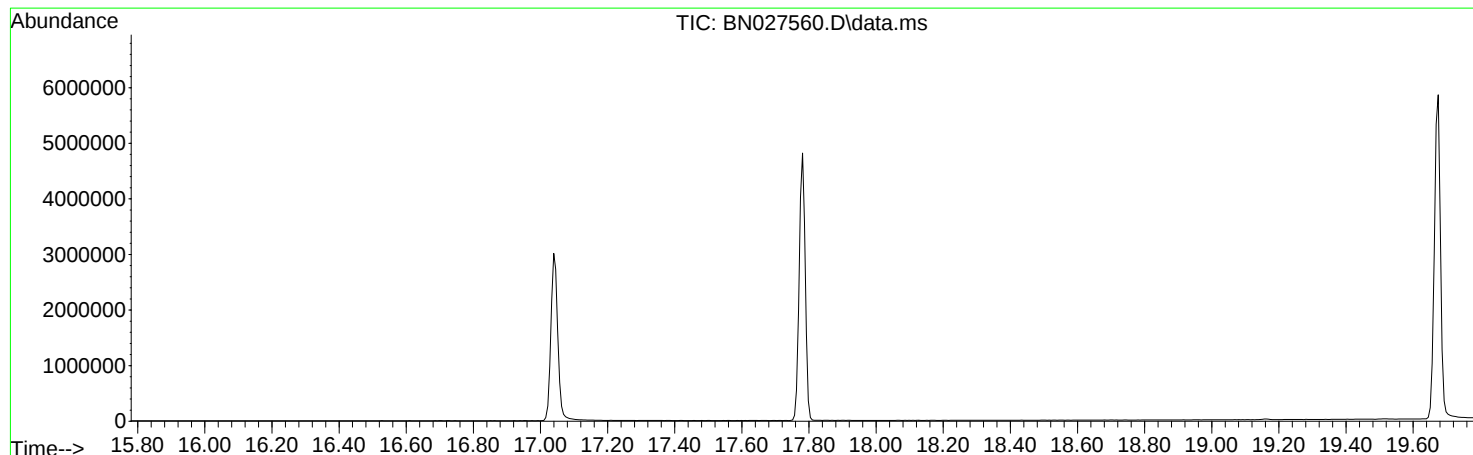




AutoFind: Scans 2531, 2532, 2533; Background Corrected with Scan 2524

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	152965	PASS
68	69	0.00	2	1.7	3076	PASS
69	198	0.00	100	37.7	183659	PASS
70	69	0.00	2	0.5	983	PASS
127	198	10	80	45.8	223147	PASS
197	198	0.00	2	0.5	2419	PASS
198	198	100	100	100.0	486976	PASS
199	198	5	9	7.0	33885	PASS
275	198	10	60	25.7	124984	PASS
365	198	1	100	3.3	16058	PASS
441	198	0.01	100	11.4	55699	PASS
442	442	50	100	100.0	334720	PASS
443	442	15	24	20.6	68872	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091023\
Data File : BN027560.D
Acq On : 11 Sep 2023 04:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 11 05:05:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 11 05:05:02 2023
Response via : Initial Calibration

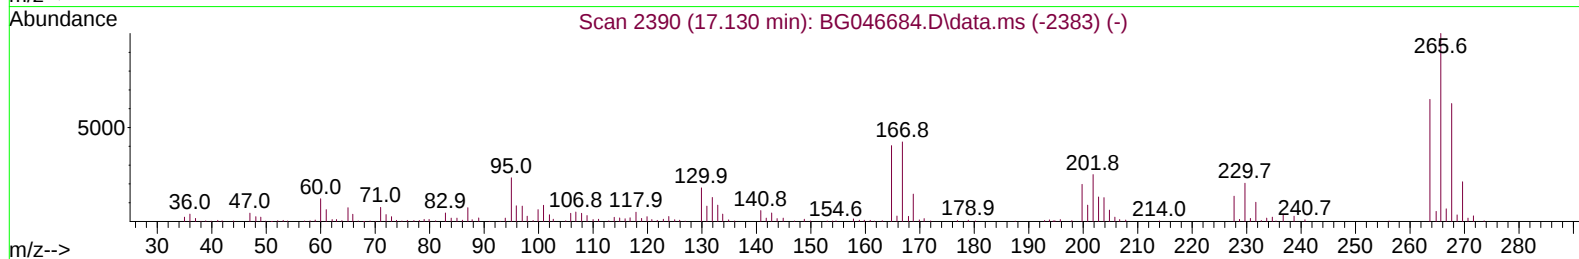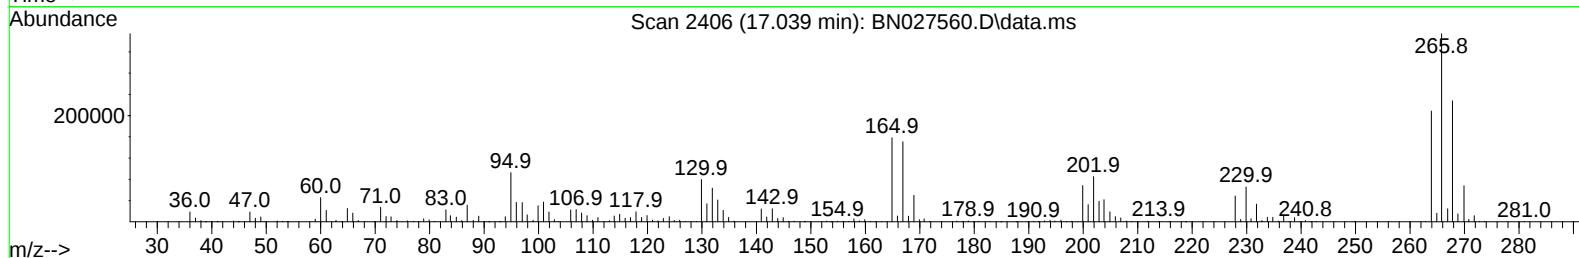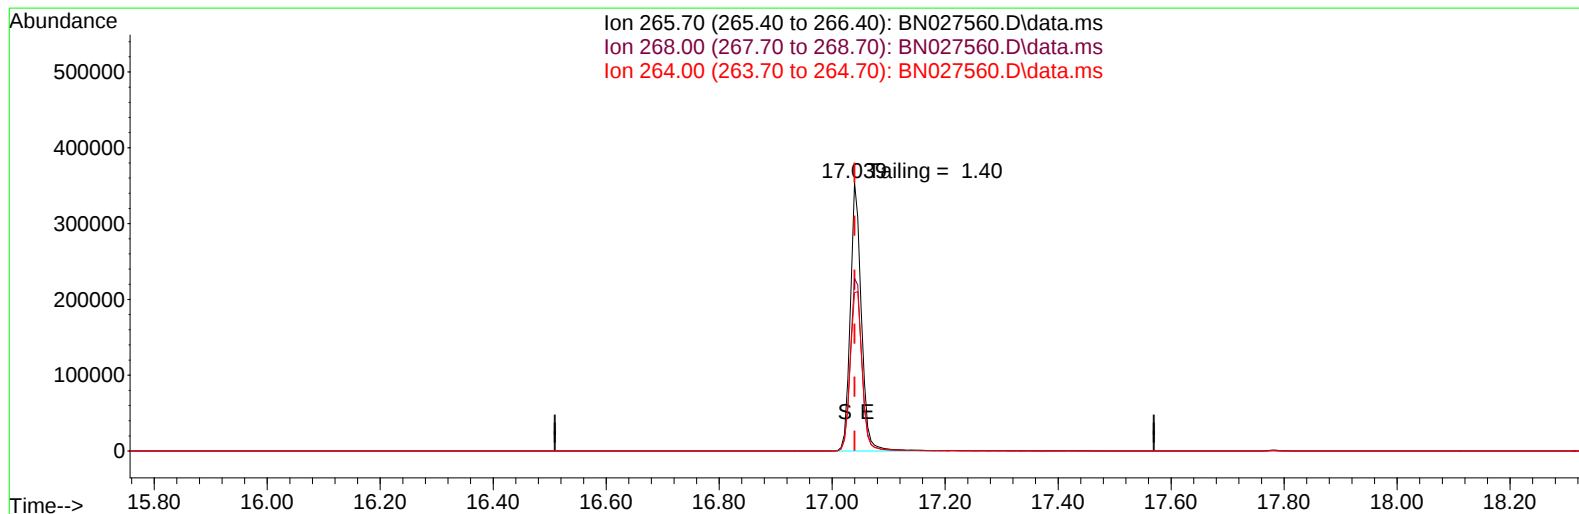

TIC: BN027560.D\data.ms

(70) Pentachlorophenol (C)

17.039min (0.000) 18876.54 ng




response 483968

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.35
264.00	61.60	58.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091023\
Data File : BN027560.D
Acq On : 11 Sep 2023 04:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 11 05:05:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 11 05:05:02 2023
Response via : Initial Calibration

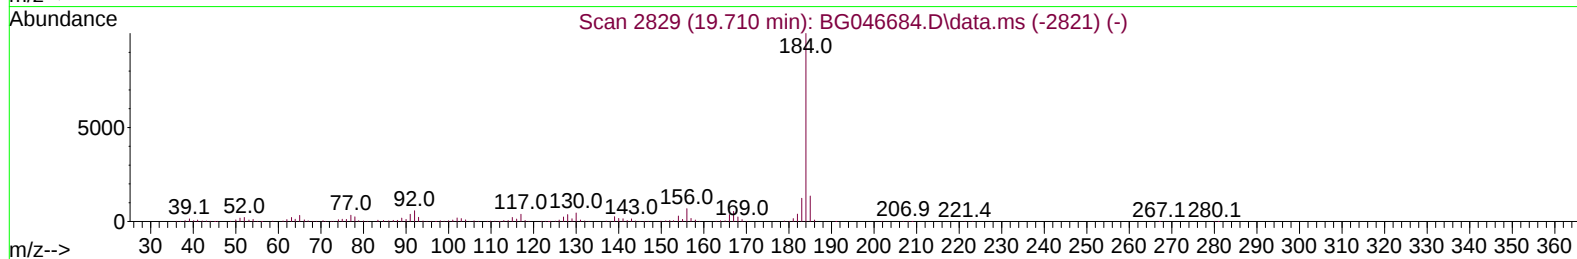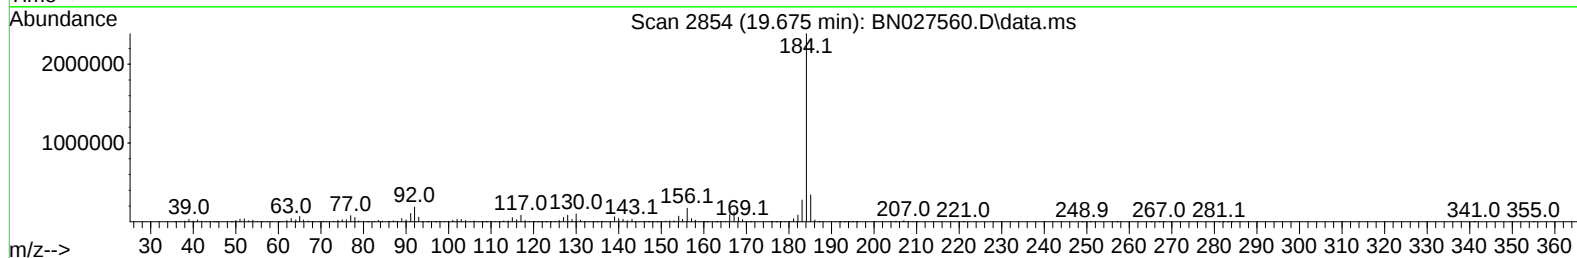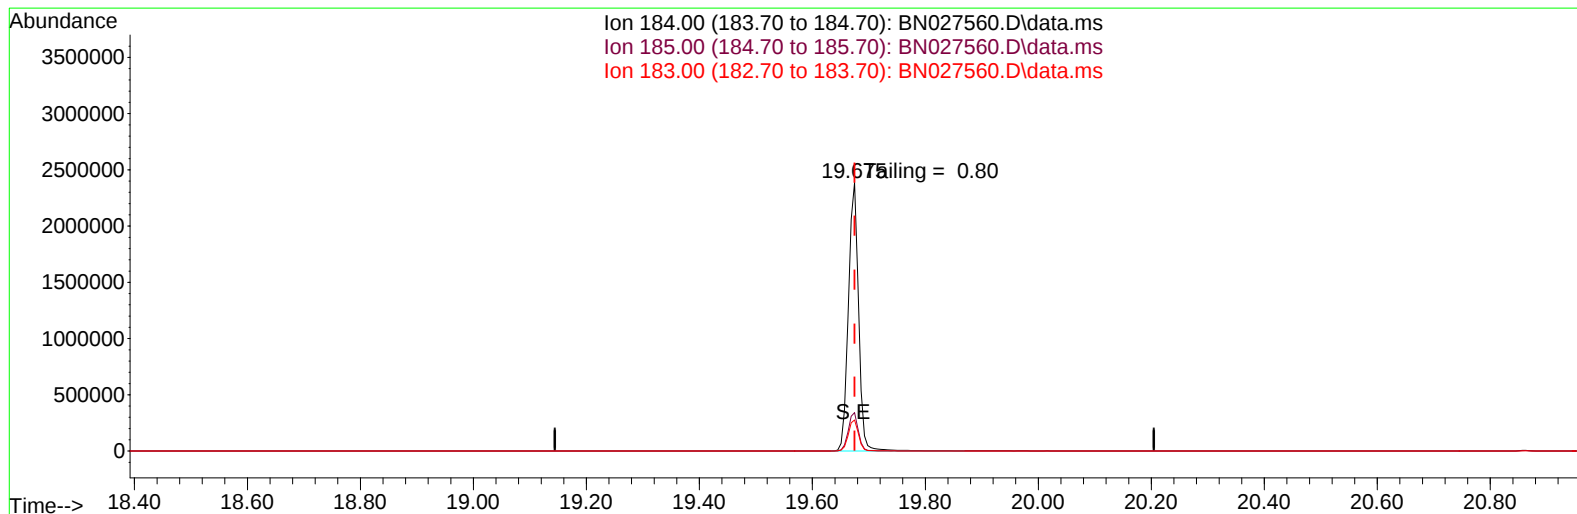

TIC: BN027560.D\data.ms

(77) Benzidine

19.675min (0.000) 0.00 ng

response 3000358

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.30
183.00	13.20	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/10/2023	BNA_N	<u>BN027560.D</u>
Compound Name	Response	Retention Time
DDT	1553187	20.863
DDD	44235	20.427
DDE	4111	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
48346	1601533	3.02

Instrument :
BNA_N
ClientSampleId :
DFTPP