

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091125\
 Data File : BN037702.D
 Acq On : 11 Sep 2025 16:34
 Operator : RC/JU
 Sample : Q2893-09
 Misc : MDL-WATER 0.1ng
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 11 17:03:14 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 11 14:20:01 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	4178	0.400	ng	0.00
7) Naphthalene-d8	10.648	136	11003	0.400	ng	0.00
13) Acenaphthene-d10	14.495	164	4984	0.400	ng	0.00
19) Phenanthrene-d10	17.235	188	9211	0.400	ng	0.00
29) Chrysene-d12	21.420	240	7580	0.400	ng	0.00
35) Perylene-d12	23.750	264	7919	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.399	112	2953	0.308	ng	0.00
5) Phenol-d6	6.988	99	3802	0.306	ng	0.00
8) Nitrobenzene-d5	8.993	82	2938	0.365	ng	0.00
11) 2-Methylnaphthalene-d10	12.243	152	5961	0.409	ng	0.00
14) 2,4,6-Tribromophenol	15.982	330	400	0.308	ng	0.00
15) 2-Fluorobiphenyl	13.115	172	7796	0.374	ng	0.00
27) Fluoranthene-d10	19.271	212	9855	0.426	ng	0.00
31) Terphenyl-d14	19.870	244	6148	0.400	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.304	88	538	0.124	ng	90
3) n-Nitrosodimethylamine	3.615	42	569	0.100	ng	# 91
6) bis(2-Chloroethyl)ether	7.255	93	1175	0.106	ng	97
9) Naphthalene	10.690	128	3058	0.102	ng	# 93
10) Hexachlorobutadiene	11.000	225	586	0.108	ng	# 98
12) 2-Methylnaphthalene	12.314	142	1704	0.092	ng	97
16) Acenaphthylene	14.206	152	2561	0.112	ng	100
17) Acenaphthene	14.559	154	1575	0.102	ng	97
18) Fluorene	15.535	166	1862	0.099	ng	99
20) 4,6-Dinitro-2-methylph...	15.609	198	76	0.089	ng	# 1
21) 4-Bromophenyl-phenylether	16.441	248	601	0.100	ng	96
22) Hexachlorobenzene	16.553	284	720	0.104	ng	96
23) Atrazine	16.702	200	372	0.097	ng	# 88
24) Pentachlorophenol	16.888	266	194	0.097	ng	# 81
25) Phenanthrene	17.285	178	3016	0.104	ng	99
26) Anthracene	17.372	178	2662	0.104	ng	98
28) Fluoranthene	19.299	202	3198	0.101	ng	99
30) Pyrene	19.661	202	3113	0.105	ng	100
32) Benzo(a)anthracene	21.402	228	2770	0.105	ng	96
33) Chrysene	21.456	228	2964	0.105	ng	97
34) Bis(2-ethylhexyl)phtha...	21.349	149	940	0.120	ng	# 98
36) Indeno(1,2,3-cd)pyrene	26.142	276	3330	0.100	ng	95
37) Benzo(b)fluoranthene	23.046	252	2945	0.094	ng	# 77
38) Benzo(k)fluoranthene	23.092	252	3213	0.101	ng	# 68
39) Benzo(a)pyrene	23.648	252	2504	0.100	ng	# 73
40) Dibenzo(a,h)anthracene	26.162	278	2596	0.098	ng	# 72
41) Benzo(g,h,i)perylene	26.867	276	2871	0.096	ng	# 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091125\
Data File : BN037702.D
Acq On : 11 Sep 2025 16:34
Operator : RC/JU
Sample : Q2893-09
Misc : MDL-WATER 0.1ng
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Sep 11 17:03:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 14:20:01 2025
Response via : Initial Calibration







#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.840 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN037702.D
 Acq: 11 Sep 2025 16:34

Instrument :
 BNA_N
 ClientSampleId :






Tgt Ion:152 Resp: 4178
 Ion Ratio Lower Upper
 152 100
 150 156.1 124.5 186.7
 115 60.7 49.2 73.8



#2
 1,4-Dioxane
 Concen: 0.124 ng
 RT: 3.304 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN037702.D
 Acq: 11 Sep 2025 16:34

Tgt Ion: 88 Resp: 538
 Ion Ratio Lower Upper
 88 100
 43 37.9 26.8 40.2
 58 67.7 61.9 92.9








#3
 n-Nitrosodimethylamine
 Concen: 0.100 ng
 RT: 3.615 min Scan# 74
 Delta R.T. 0.007 min
 Lab File: BN037702.D
 Acq: 11 Sep 2025 16:34




Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion: 42 Resp: 569
 Ion Ratio Lower Upper
 42 100
 74 116.3 86.0 129.0
 44 15.6 8.4 12.6#



#4
 2-Fluorophenol
 Concen: 0.308 ng
 RT: 5.399 min Scan# 321
 Delta R.T. -0.000 min
 Lab File: BN037702.D
 Acq: 11 Sep 2025 16:34

Tgt Ion: 112 Resp: 2953
 Ion Ratio Lower Upper
 112 100
 64 57.2 44.9 67.3
 63 31.6 24.7 37.1








#5
Phenol-d6
Concen: 0.306 ng
RT: 6.988 min Scan# 541
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34




Instrument :
BNA_N
ClientSampleId :

Tgt Ion: 99 Resp: 3802
Ion Ratio Lower Upper
99 100
42 20.8 16.6 24.8
71 33.6 26.7 40.1



#6
bis(2-Chloroethyl)ether
Concen: 0.106 ng
RT: 7.255 min Scan# 578
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34


Tgt Ion: 93 Resp: 1175
Ion Ratio Lower Upper
93 100
63 78.6 60.6 90.8
95 33.3 26.0 39.0







#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.648 min Scan# 943
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34

Instrument :
BNA_N
ClientSampleId :






Tgt Ion:	136	Resp:	11003
Ion	Ratio	Lower	Upper
136	100		
137	11.9	9.1	13.7
54	7.5	6.3	9.5
68	6.1	5.0	7.4



#8
Nitrobenzene-d5
Concen: 0.365 ng
RT: 8.993 min Scan# 788
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34

Tgt Ion:	82	Resp:	2938
Ion	Ratio	Lower	Upper
82	100		
128	49.0	38.3	57.5
54	52.7	41.4	62.2









#9
Naphthalene
Concen: 0.102 ng
RT: 10.690 min Scan# 947
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34




Instrument :
BNA_N
ClientSampleId :

Tgt Ion:128 Resp: 3058
Ion Ratio Lower Upper
128 100
129 14.3 9.1 13.7#
127 16.4 10.9 16.3#



#10
Hexachlorobutadiene
Concen: 0.108 ng
RT: 11.000 min Scan# 976
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34

Tgt Ion:225 Resp: 586
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.8 50.9 76.3








#11
2-Methylnaphthalene-d10
Concen: 0.409 ng
RT: 12.243 min Scan# 1168
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34




Instrument :
BNA_N
ClientSampleId :

Tgt Ion:152 Resp: 5961
Ion Ratio Lower Upper
152 100
151 20.3 17.0 25.6



#12
2-Methylnaphthalene
Concen: 0.092 ng
RT: 12.314 min Scan# 1182
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34


Tgt Ion:142 Resp: 1704
Ion Ratio Lower Upper
142 100
141 90.4 71.6 107.4
115 40.5 28.6 43.0








#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.495 min Scan# 1458
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34

Instrument :
BNA_N
ClientSampleId :







Tgt Ion:164 Resp: 4984
Ion Ratio Lower Upper
164 100
162 104.5 83.1 124.7
160 57.3 44.3 66.5



#14
2,4,6-Tribromophenol
Concen: 0.308 ng
RT: 15.982 min Scan# 1591
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34

Tgt Ion:330 Resp: 400
Ion Ratio Lower Upper
330 100
332 100.0 75.3 112.9
141 44.5 35.0 52.4







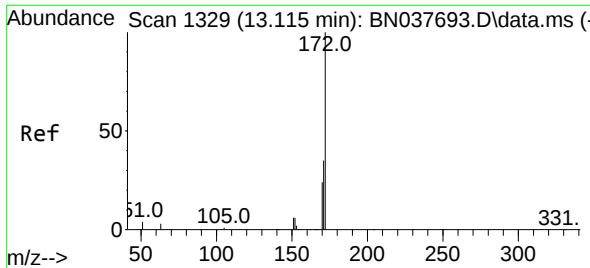

#15
2-Fluorobiphenyl
Concen: 0.374 ng
RT: 13.115 min Scan# 1329
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:172	Resp:	7796
Ion	Ratio	Lower Upper
172	100	
171	36.4	28.6 43.0
170	26.1	19.8 29.8



#16
Acenaphthylene
Concen: 0.112 ng
RT: 14.206 min Scan# 1431
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34

Tgt Ion:152	Resp:	2561
Ion	Ratio	Lower Upper
152	100	
151	20.1	16.2 24.2
153	13.0	10.4 15.6





#17

Acenaphthene

Concen: 0.102 ng

RT: 14.559 min Scan# 1464

Delta R.T. -0.000 min

Lab File: BN037702.D

Acq: 11 Sep 2025 16:34

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:154 Resp: 1575

Ion Ratio Lower Upper

154 100

153 115.4 89.8 134.8

152 65.7 50.2 75.2



#18

Fluorene

Concen: 0.099 ng

RT: 15.535 min Scan# 1555

Delta R.T. -0.000 min

Lab File: BN037702.D

Acq: 11 Sep 2025 16:34




Tgt Ion:166 Resp: 1862


Ion Ratio Lower Upper

166 100

165 98.8 79.6 119.4

167 14.7 10.6 16.0





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.235 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037702.D





Acq: 11 Sep 2025 16:34

Instrument :

BNA_N

ClientSampleId :

Tgt Ion:188	Resp:	9211
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0
80	13.5	10.6



#20

4,6-Dinitro-2-methylphenol

Concen: 0.089 ng




RT: 15.609 min Scan# 1561


Delta R.T. 0.000 min

Lab File: BN037702.D

Acq: 11 Sep 2025 16:34

Tgt Ion:198	Resp:	76
Ion Ratio	Lower	Upper
198	100	
51	291.6	95.1
105	130.1	53.8









#21
4-Bromophenyl-phenylether
Concen: 0.100 ng
RT: 16.441 min Scan# 1628
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34




Instrument :
BNA_N
ClientSampleId :


Tgt Ion	Ratio	Lower	Upper
248	100		
250	101.2	81.5	122.3
141	45.3	30.8	46.2



#22
Hexachlorobenzene
Concen: 0.104 ng
RT: 16.553 min Scan# 1637
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34

Tgt Ion	Ratio	Lower	Upper
284	100		
142	41.1	30.9	46.3
249	29.4	24.8	37.2





#23

Atrazine

Concen: 0.097 ng

RT: 16.702 min Scan# 1649

Delta R.T. -0.000 min

Lab File: BN037702.D





Acq: 11 Sep 2025 16:34

Instrument :

BNA_N

ClientSampleId :

Tgt Ion:	200	Resp:	372
Ion Ratio	Lower	Upper	
200	100		
173	36.0	21.4	32.2#
215	54.8	39.2	58.8



#24

Pentachlorophenol

Concen: 0.097 ng




RT: 16.888 min Scan# 1664


Delta R.T. -0.000 min

Lab File: BN037702.D

Acq: 11 Sep 2025 16:34


Tgt Ion:	266	Resp:	194
Ion Ratio	Lower	Upper	
266	100		
264	55.2	51.6	77.4
268	46.4	53.2	79.8#







#25
 Phenanthrene
 Concen: 0.104 ng
 RT: 17.285 min Scan# 1696
 Delta R.T. -0.000 min
 Lab File: BN037702.D
 Acq: 11 Sep 2025 16:34

Instrument :
 BNA_N
 ClientSampleId :



Tgt Ion:178 Resp: 3016




Ion	Ratio	Lower	Upper
178	100		
176	18.9	15.3	22.9
179	16.2	12.2	18.2




#26
 Anthracene
 Concen: 0.104 ng
 RT: 17.372 min Scan# 1703
 Delta R.T. -0.000 min
 Lab File: BN037702.D
 Acq: 11 Sep 2025 16:34

Tgt Ion:178 Resp: 2662

Ion	Ratio	Lower	Upper
178	100		
176	19.3	14.6	22.0
179	15.6	12.2	18.4





#27

Fluoranthene-d10

Concen: 0.426 ng

RT: 19.271 min Scan# 1958

Delta R.T. -0.000 min

Lab File: BN037702.D





Acq: 11 Sep 2025 16:34

Instrument :

BNA_N

ClientSampleId :

Tgt Ion:212	Resp:	9855
Ion Ratio	Lower	Upper
212	100	
106	15.2	12.2 18.2
104	8.6	6.9 10.3



#28

Fluoranthene

Concen: 0.101 ng




RT: 19.299 min Scan# 1964


Delta R.T. -0.000 min

Lab File: BN037702.D

Acq: 11 Sep 2025 16:34

Tgt Ion:202	Resp:	3198
Ion Ratio	Lower	Upper
202	100	
101	11.5	9.3 13.9
203	17.5	13.7 20.5





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.420 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN037702.D

Acq: 11 Sep 2025 16:34

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:240 Resp: 7580

Ion Ratio Lower Upper

240 100

120 10.9 9.2 13.8

236 27.7 22.6 33.8



#30

Pyrene

Concen: 0.105 ng

RT: 19.661 min Scan# 2042

Delta R.T. -0.000 min

Lab File: BN037702.D

Acq: 11 Sep 2025 16:34




Tgt Ion:202 Resp: 3113


Ion Ratio Lower Upper

202 100

200 21.3 16.8 25.2

203 17.9 14.3 21.5





#31

Terphenyl-d14

Concen: 0.400 ng

RT: 19.870 min Scan# 2087

Delta R.T. -0.000 min


Lab File: BN037702.D

Acq: 11 Sep 2025 16:34



Instrument :

BNA_N

ClientSampleId :



Tgt Ion:	244	Resp:	6148
Ion Ratio	Lower	Upper	
244	100		
212	9.7	7.5	11.3
122	16.7	13.2	19.8



#32

Benzo(a)anthracene

Concen: 0.105 ng




RT: 21.402 min Scan# 2272

Delta R.T. -0.000 min

Lab File: BN037702.D

Acq: 11 Sep 2025 16:34


Tgt Ion:	228	Resp:	2770
Ion Ratio	Lower	Upper	
228	100		
226	28.8	22.2	33.2
229	22.8	15.8	23.6








#33
Chrysene
Concen: 0.105 ng
RT: 21.456 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34


Instrument :
BNA_N
ClientSampleId :





Tgt Ion:228 Resp: 2964
Ion Ratio Lower Upper
228 100
226 30.5 23.5 35.3
229 21.5 15.9 23.9

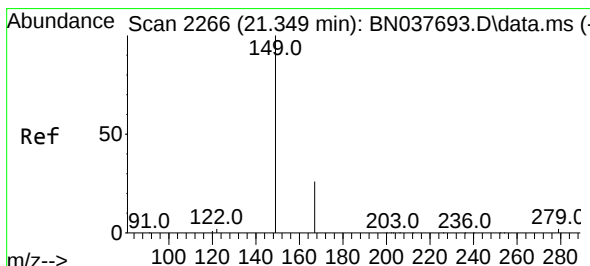

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.120 ng
RT: 21.349 min Scan# 2266
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34




Tgt Ion:149 Resp: 940
Ion Ratio Lower Upper
149 100
167 25.2 20.8 31.2
279 6.5 3.3 4.9#







#35
Perylene-d12
Concen: 0.400 ng
RT: 23.750 min Scan# 21
Delta R.T. -0.003 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34

Instrument :
BNA_N
ClientSampleId :







Tgt Ion:264 Resp: 7919
Ion Ratio Lower Upper
264 100
260 26.4 21.8 32.8
265 51.7 39.4 59.2



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.100 ng
RT: 26.142 min Scan# 3662
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34


Tgt Ion:276 Resp: 3330
Ion Ratio Lower Upper
276 100
138 31.0 21.9 32.9
277 24.1 20.1 30.1







#37
Benzo(b)fluoranthene
Concen: 0.094 ng
RT: 23.046 min Scan# 2603
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34

Instrument :
BNA_N
ClientSampleId :







Tgt Ion:252 Resp: 2945
Ion Ratio Lower Upper
252 100
253 34.0 19.4 29.2#
125 26.0 11.2 16.8#



#38
Benzo(k)fluoranthene
Concen: 0.101 ng
RT: 23.092 min Scan# 2619
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34


Tgt Ion:252 Resp: 3213
Ion Ratio Lower Upper
252 100
253 34.0 19.4 29.0#
125 35.7 11.6 17.4#








#39
Benzo(a)pyrene
Concen: 0.100 ng
RT: 23.648 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34

Instrument :
BNA_N
ClientSampleId :







Tgt Ion:252 Resp: 2504
Ion Ratio Lower Upper
252 100
253 37.3 20.8 31.2#
125 32.9 13.9 20.9#



#40
Dibenzo(a,h)anthracene
Concen: 0.098 ng
RT: 26.162 min Scan# 3669
Delta R.T. -0.000 min
Lab File: BN037702.D
Acq: 11 Sep 2025 16:34

Tgt Ion:278 Resp: 2596
Ion Ratio Lower Upper
278 100
139 38.8 17.8 26.6#
279 39.7 22.0 33.0#





#41

Benzo(g,h,i)perylene

Concen: 0.096 ng

RT: 26.867 min Scan# 3910

Delta R.T. -0.000 min


Lab File: BN037702.D

Acq: 11 Sep 2025 16:34

Instrument :

BNA_N

ClientSampleId :



Tgt Ion:276 Resp: 2871

Ion Ratio Lower Upper

276 100

277 30.5 20.6 31.0

138 31.5 20.2 30.2#

