

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091125\
 Data File : BN037703.D
 Acq On : 11 Sep 2025 17:10
 Operator : RC/JU
 Sample : Q2893-09
 Misc : MDL-WATER 0.2ng
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Quant Time: Sep 11 18:14:33 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 11 14:20:01 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	4069	0.400	ng	0.00
7) Naphthalene-d8	10.648	136	10666	0.400	ng	0.00
13) Acenaphthene-d10	14.494	164	4928	0.400	ng	0.00
19) Phenanthrene-d10	17.235	188	8855	0.400	ng	0.00
29) Chrysene-d12	21.420	240	7304	0.400	ng	0.00
35) Perylene-d12	23.750	264	7594	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.399	112	2991	0.320	ng	0.00
5) Phenol-d6	6.988	99	3944	0.326	ng	0.00
8) Nitrobenzene-d5	8.993	82	2986	0.383	ng	0.00
11) 2-Methylnaphthalene-d10	12.243	152	5808	0.411	ng	0.00
14) 2,4,6-Tribromophenol	15.982	330	406	0.316	ng	0.00
15) 2-Fluorobiphenyl	13.115	172	7990	0.388	ng	0.00
27) Fluoranthene-d10	19.271	212	9254	0.416	ng	0.00
31) Terphenyl-d14	19.870	244	5998	0.405	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.304	88	931	0.220	ng	96
3) n-Nitrosodimethylamine	3.608	42	1081	0.195	ng	93
6) bis(2-Chloroethyl)ether	7.255	93	2233	0.206	ng	99
9) Naphthalene	10.690	128	5791	0.199	ng	97
10) Hexachlorobutadiene	11.000	225	1142	0.217	ng	# 99
12) 2-Methylnaphthalene	12.314	142	3220	0.179	ng	99
16) Acenaphthylene	14.206	152	4700	0.208	ng	99
17) Acenaphthene	14.559	154	2964	0.194	ng	98
18) Fluorene	15.535	166	3624	0.196	ng	98
20) 4,6-Dinitro-2-methylph...	15.609	198	145	0.177	ng	# 48
21) 4-Bromophenyl-phenylether	16.441	248	1121	0.194	ng	96
22) Hexachlorobenzene	16.553	284	1335	0.201	ng	98
23) Atrazine	16.702	200	701	0.191	ng	97
24) Pentachlorophenol	16.888	266	375	0.194	ng	96
25) Phenanthrene	17.285	178	5655	0.203	ng	99
26) Anthracene	17.372	178	4942	0.200	ng	99
28) Fluoranthene	19.299	202	5795	0.190	ng	100
30) Pyrene	19.661	202	5716	0.200	ng	100
32) Benzo(a)anthracene	21.402	228	5127	0.201	ng	99
33) Chrysene	21.456	228	5411	0.198	ng	98
34) Bis(2-ethylhexyl)phtha...	21.348	149	1645	0.218	ng	97
36) Indeno(1,2,3-cd)pyrene	26.142	276	6208	0.195	ng	97
37) Benzo(b)fluoranthene	23.046	252	5460	0.183	ng	# 91
38) Benzo(k)fluoranthene	23.092	252	5992	0.197	ng	# 86
39) Benzo(a)pyrene	23.648	252	4765	0.199	ng	# 87
40) Dibenzo(a,h)anthracene	26.159	278	4911	0.193	ng	# 89
41) Benzo(g,h,i)perylene	26.864	276	5244	0.183	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091125\
Data File : BN037703.D
Acq On : 11 Sep 2025 17:10
Operator : RC/JU
Sample : Q2893-09
Misc : MDL-WATER 0.2ng
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Quant Time: Sep 11 18:14:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 14:20:01 2025
Response via : Initial Calibration

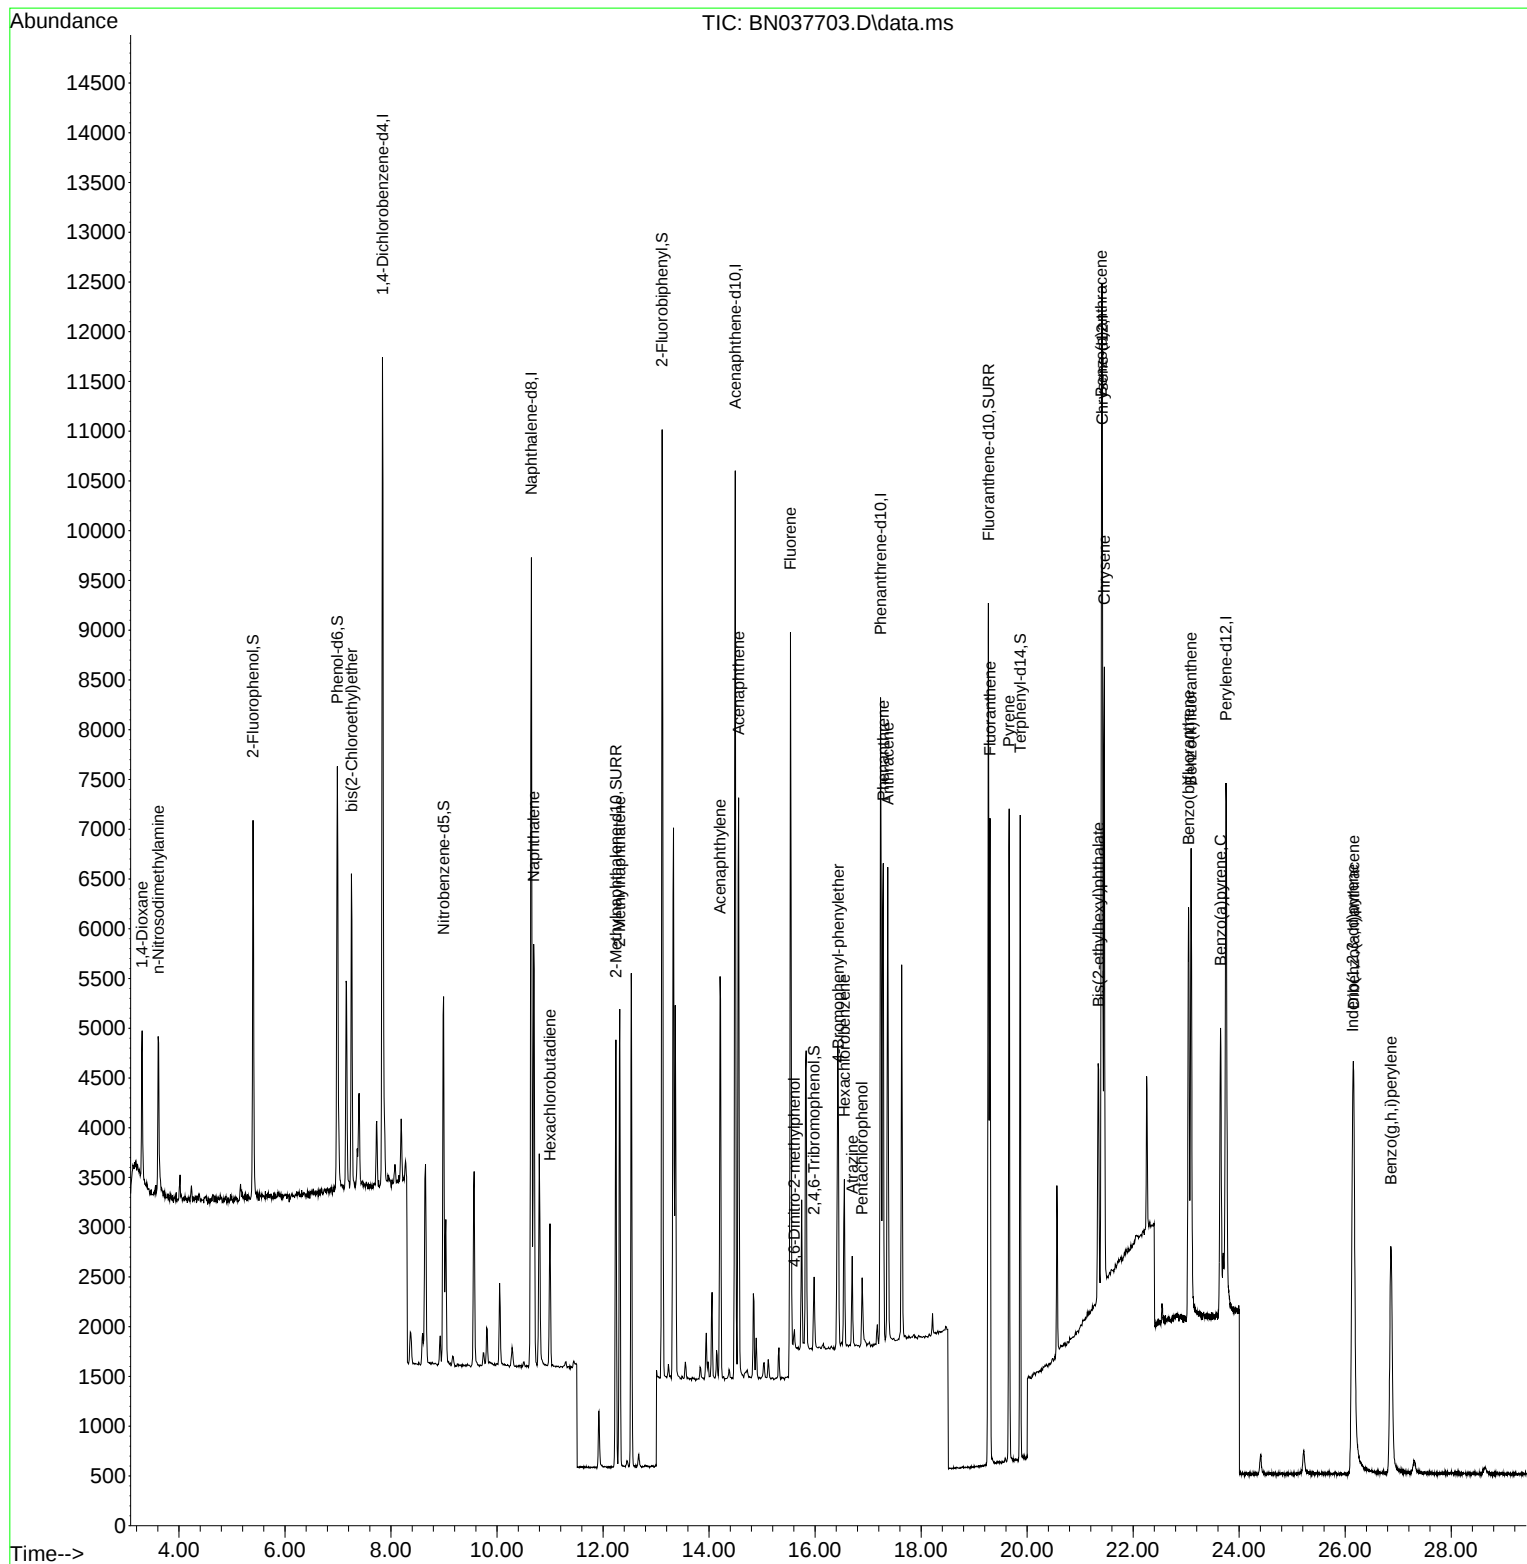






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.840 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN037703.D
 Acq: 11 Sep 2025 17:10

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-03-QT3-2025



Tgt Ion:152 Resp: 4069




Ion	Ratio	Lower	Upper
152	100		
150	155.4	124.5	186.7
115	60.9	49.2	73.8

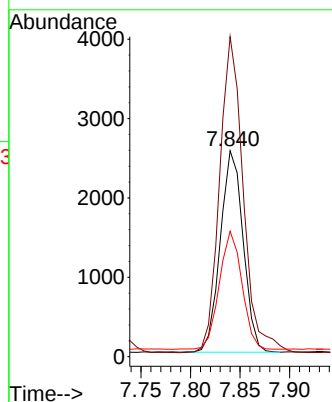


#2
 1,4-Dioxane
 Concen: 0.220 ng
 RT: 3.304 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN037703.D
 Acq: 11 Sep 2025 17:10

Tgt Ion: 88 Resp: 931

Ion	Ratio	Lower	Upper
88	100		
43	35.1	26.8	40.2
58	73.6	61.9	92.9


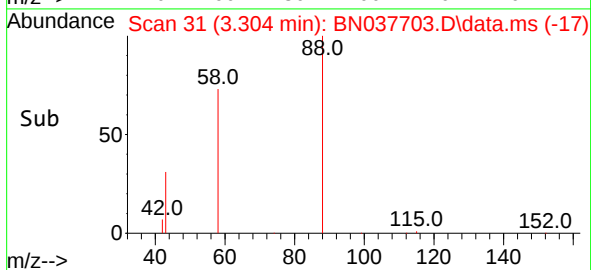




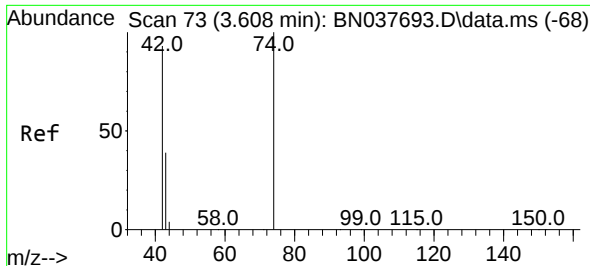

#3
n-Nitrosodimethylamine
Concen: 0.195 ng
RT: 3.608 min Scan# 73
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion: 42 Resp: 1081
Ion Ratio Lower Upper
42 100
74 115.7 86.0 129.0
44 10.2 8.4 12.6

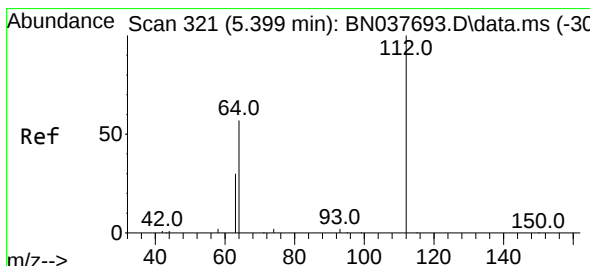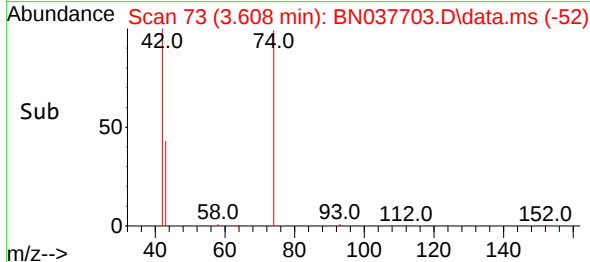

#4
2-Fluorophenol
Concen: 0.320 ng
RT: 5.399 min Scan# 321
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion: 112 Resp: 2991
Ion Ratio Lower Upper
112 100
64 56.9 44.9 67.3
63 31.5 24.7 37.1


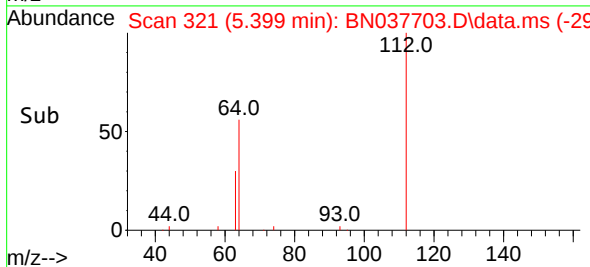

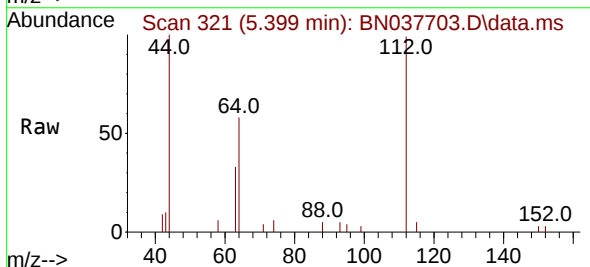




#5
Phenol-d6
Concen: 0.326 ng
RT: 6.988 min Scan# 541
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion: 99 Resp: 3944
Ion Ratio Lower Upper
99 100
42 20.9 16.6 24.8
71 33.1 26.7 40.1

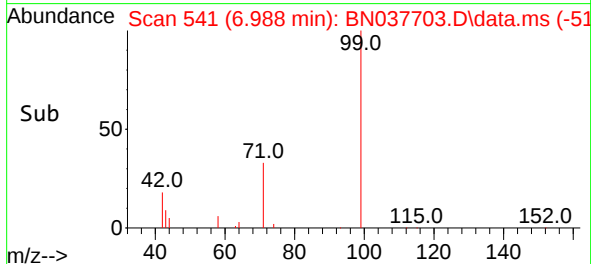

#6
bis(2-Chloroethyl)ether
Concen: 0.206 ng
RT: 7.255 min Scan# 578
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion: 93 Resp: 2233
Ion Ratio Lower Upper
93 100
63 76.3 60.6 90.8
95 31.8 26.0 39.0


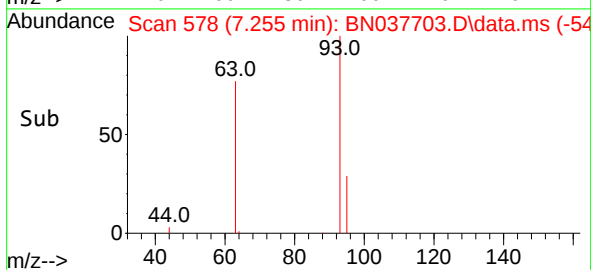

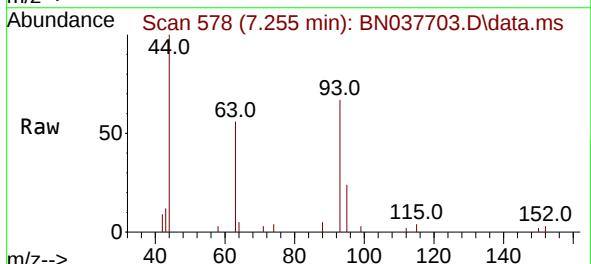




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.648 min Scan# 943
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion:	136	Resp:	10666
Ion	Ratio	Lower	Upper
136	100		
137	11.6	9.1	13.7
54	7.6	6.3	9.5
68	6.1	5.0	7.4

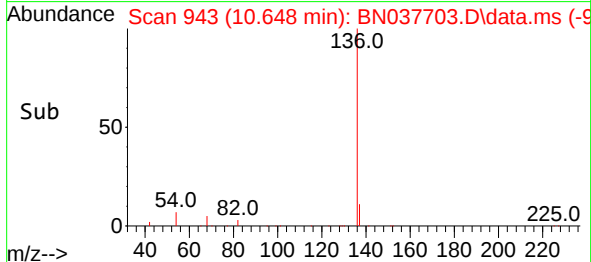

#8
Nitrobenzene-d5
Concen: 0.383 ng
RT: 8.993 min Scan# 788
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion:	82	Resp:	2986
Ion	Ratio	Lower	Upper
82	100		
128	49.6	38.3	57.5
54	52.9	41.4	62.2




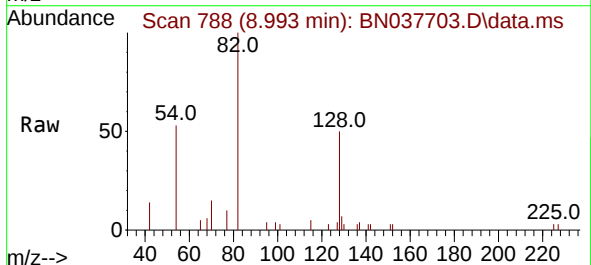




#9
Naphthalene
Concen: 0.199 ng
RT: 10.690 min Scan# 947
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion:128	Resp:	5791
Ion	Ratio	Lower Upper
128	100	
129	13.1	9.1 13.7
127	14.2	10.9 16.3

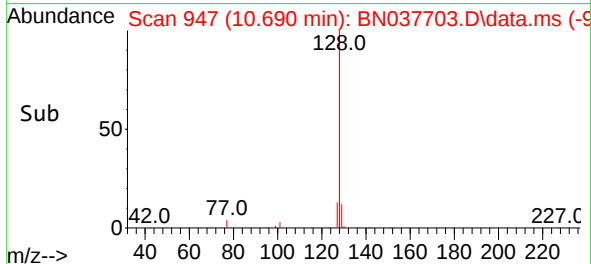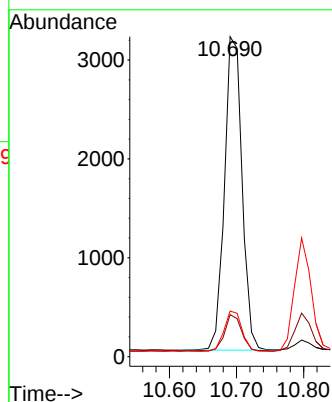

#10
Hexachlorobutadiene
Concen: 0.217 ng
RT: 11.000 min Scan# 976
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion:225	Resp:	1142
Ion	Ratio	Lower Upper
225	100	
223	0.0	0.0 0.0
227	62.9	50.9 76.3









#11
2-Methylnaphthalene-d10
Concen: 0.411 ng
RT: 12.243 min Scan# 1168
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion:152 Resp: 5808
Ion Ratio Lower Upper
152 100
151 20.3 17.0 25.6

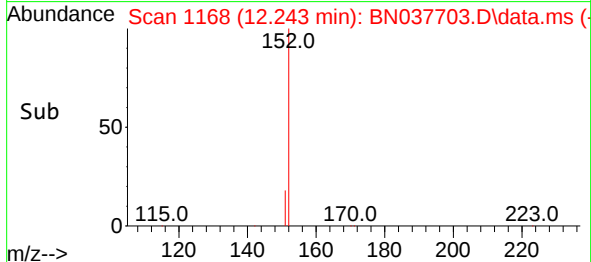

#12
2-Methylnaphthalene
Concen: 0.179 ng
RT: 12.314 min Scan# 1182
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion:142 Resp: 3220
Ion Ratio Lower Upper
142 100
141 88.9 71.6 107.4
115 37.9 28.6 43.0


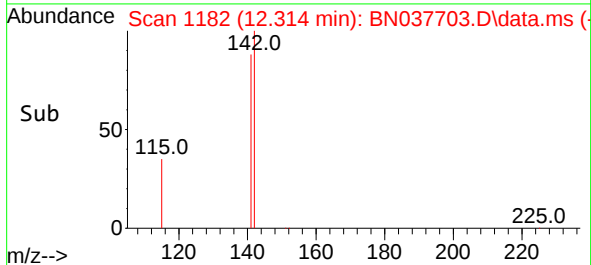




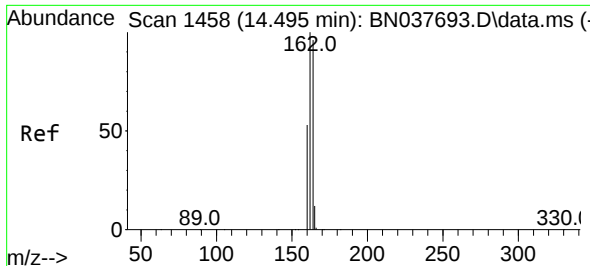

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.494 min Scan# 1458
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion:164 Resp: 4928
Ion Ratio Lower Upper
164 100
162 103.9 83.1 124.7
160 54.2 44.3 66.5

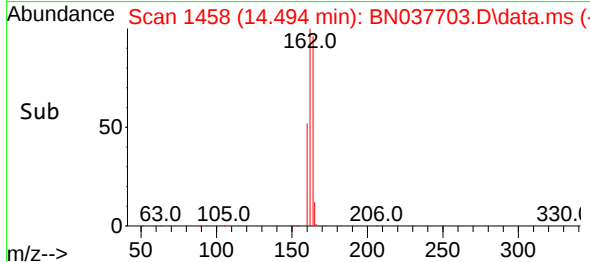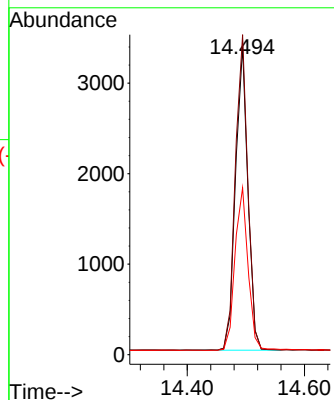

#14
2,4,6-Tribromophenol
Concen: 0.316 ng
RT: 15.982 min Scan# 1591
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion:330 Resp: 406
Ion Ratio Lower Upper
330 100
332 96.8 75.3 112.9
141 43.6 35.0 52.4


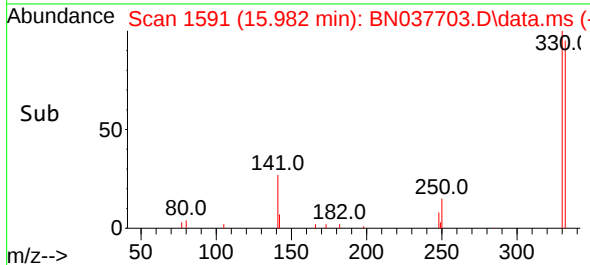
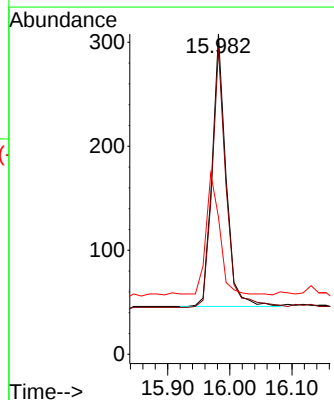
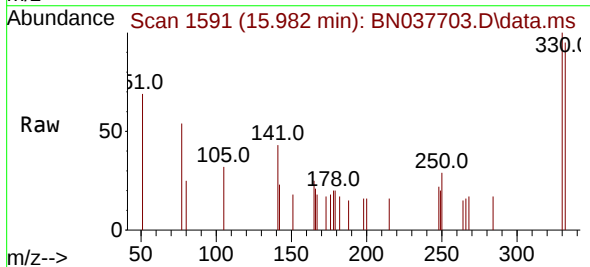


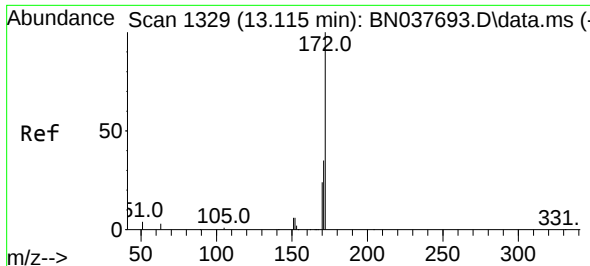

#15
2-Fluorobiphenyl
Concen: 0.388 ng
RT: 13.115 min Scan# 1329
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion:	172	Resp:	7990
Ion Ratio	Lower	Upper	
172	100		
171	36.6	28.6	43.0
170	25.6	19.8	29.8

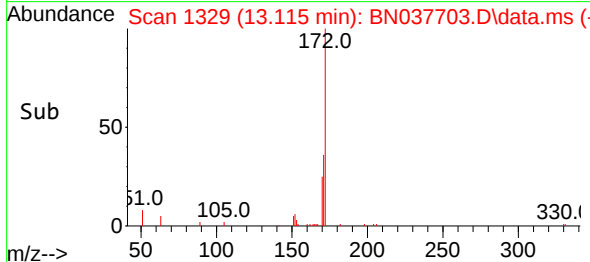

#16
Acenaphthylene
Concen: 0.208 ng
RT: 14.206 min Scan# 1431
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion:	152	Resp:	4700
Ion Ratio	Lower	Upper	
152	100		
151	20.1	16.2	24.2
153	13.8	10.4	15.6


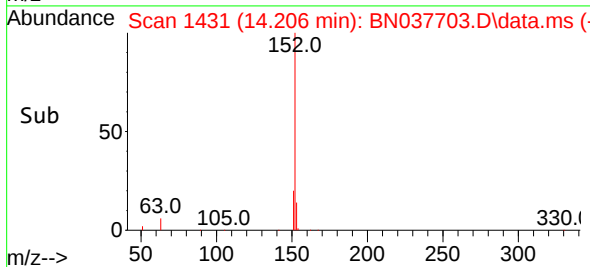

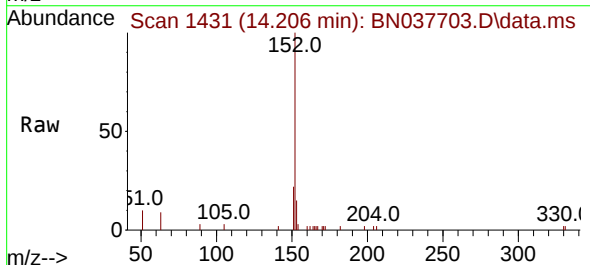


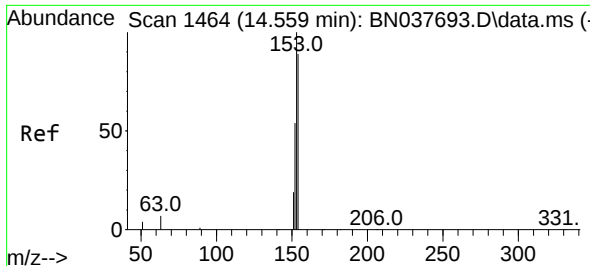

#17
Acenaphthene
Concen: 0.194 ng
RT: 14.559 min Scan# 1464
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion:154 Resp: 2964
Ion Ratio Lower Upper
154 100
153 114.8 89.8 134.8
152 63.9 50.2 75.2

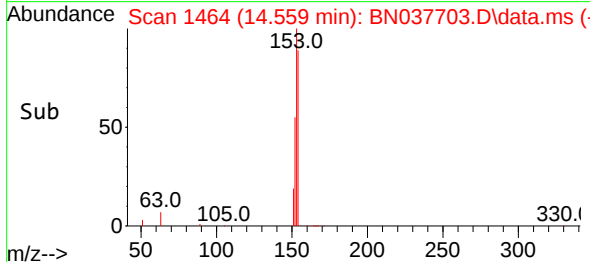

#18
Fluorene
Concen: 0.196 ng
RT: 15.535 min Scan# 1555
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion:166 Resp: 3624
Ion Ratio Lower Upper
166 100
165 97.7 79.6 119.4
167 13.2 10.6 16.0

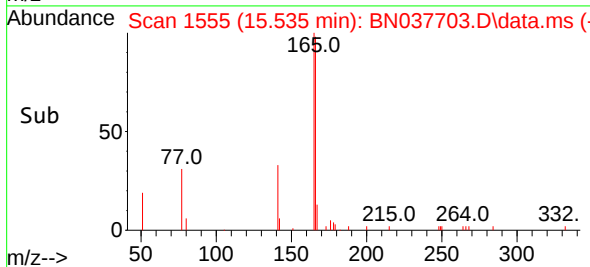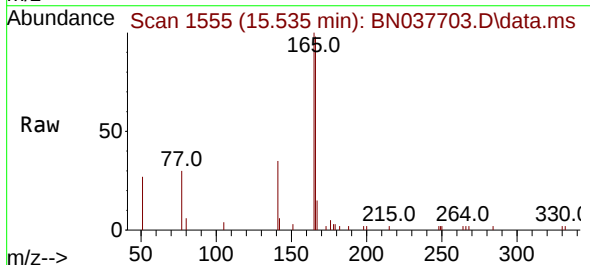



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.235 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037703.D

Acq: 11 Sep 2025 17:10

Instrument :

BNA_N

ClientSampleId :

MDL-WATER-03-QT3-2025





Tgt Ion:188 Resp: 8855

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 13.6 10.6 15.8

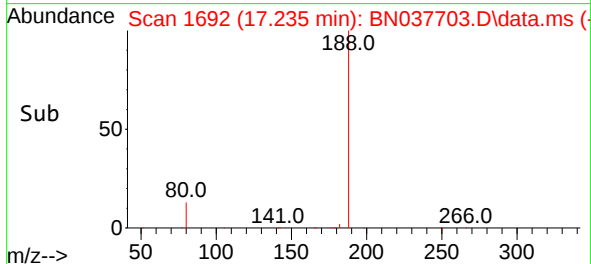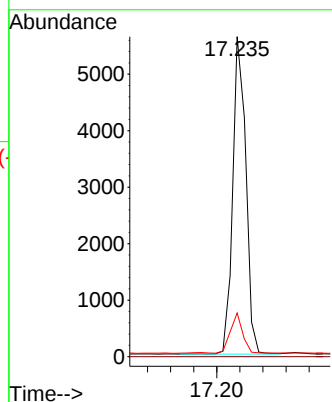

#20

4,6-Dinitro-2-methylphenol

Concen: 0.177 ng

RT: 15.609 min Scan# 1561

Delta R.T. 0.000 min

Lab File: BN037703.D

Acq: 11 Sep 2025 17:10




Tgt Ion:198 Resp: 145


Ion Ratio Lower Upper

198 100

51 185.6 95.1 142.7#

105 96.2 53.8 80.6#


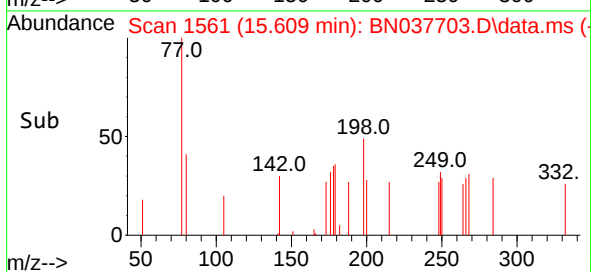
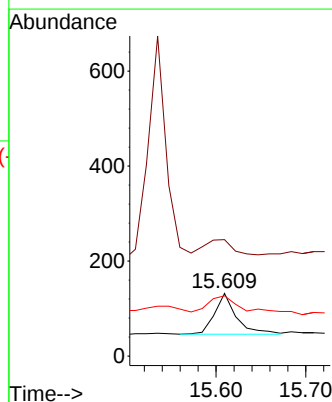





#21
4-Bromophenyl-phenylether
Concen: 0.194 ng
RT: 16.441 min Scan# 1628
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion:	248	Resp:	1121
Ion	Ratio	Lower	Upper
248	100		
250	104.2	81.5	122.3
141	43.6	30.8	46.2

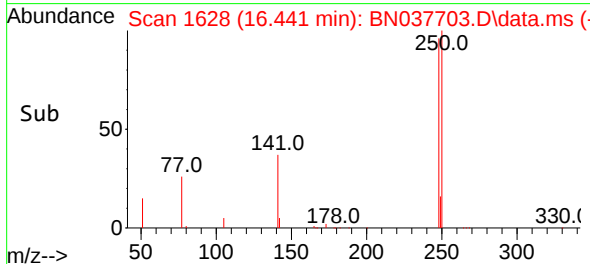

#22
Hexachlorobenzene
Concen: 0.201 ng
RT: 16.553 min Scan# 1637
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion:	284	Resp:	1335
Ion	Ratio	Lower	Upper
284	100		
142	40.2	30.9	46.3
249	31.8	24.8	37.2


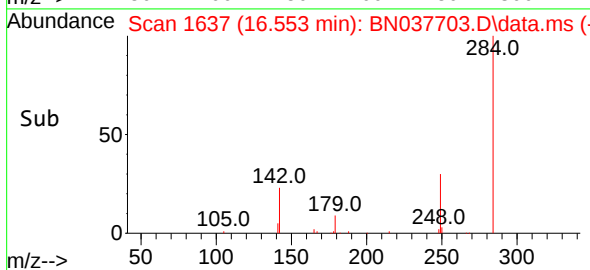

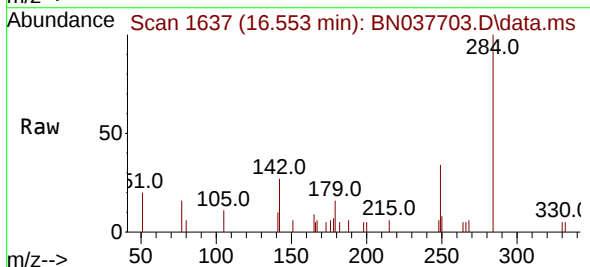




#23
Atrazine
Concen: 0.191 ng
RT: 16.702 min Scan# 1649
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion:200 Resp: 701
Ion Ratio Lower Upper
200 100
173 29.9 21.4 32.2
215 48.4 39.2 58.8

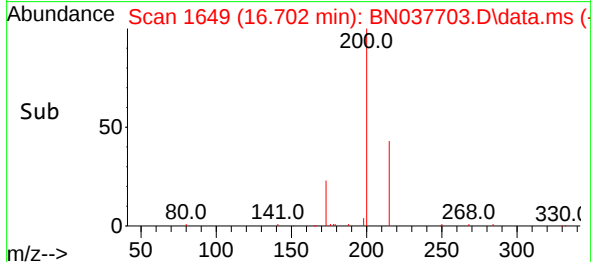

#24
Pentachlorophenol
Concen: 0.194 ng
RT: 16.888 min Scan# 1664
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion:266 Resp: 375
Ion Ratio Lower Upper
266 100
264 63.5 51.6 77.4
268 61.6 53.2 79.8




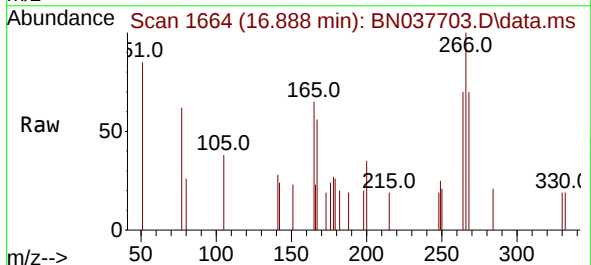




#25
Phenanthrene
Concen: 0.203 ng
RT: 17.285 min Scan# 1696
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion:178 Resp: 5655
Ion Ratio Lower Upper
178 100
176 19.2 15.3 22.9
179 15.6 12.2 18.2

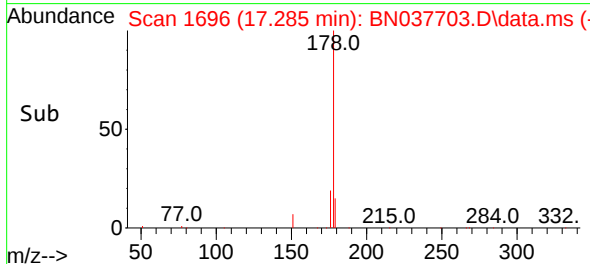

#26
Anthracene
Concen: 0.200 ng
RT: 17.372 min Scan# 1703
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion:178 Resp: 4942
Ion Ratio Lower Upper
178 100
176 19.0 14.6 22.0
179 15.2 12.2 18.4


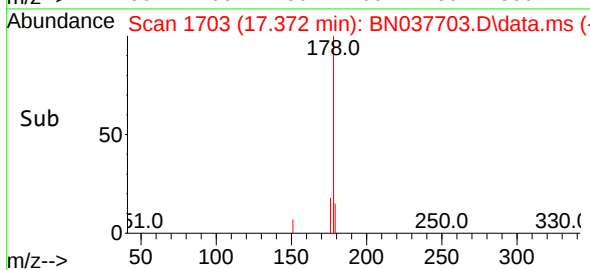

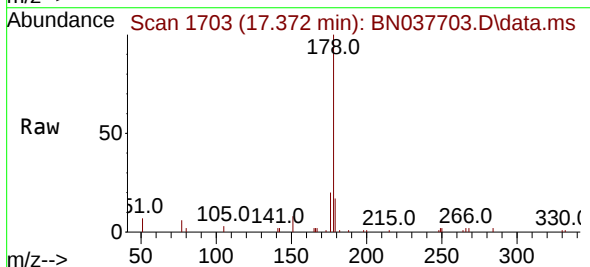




#27
Fluoranthene-d10
Concen: 0.416 ng
RT: 19.271 min Scan# 1958
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion:212 Resp: 9254
Ion Ratio Lower Upper
212 100
106 15.4 12.2 18.2
104 9.0 6.9 10.3

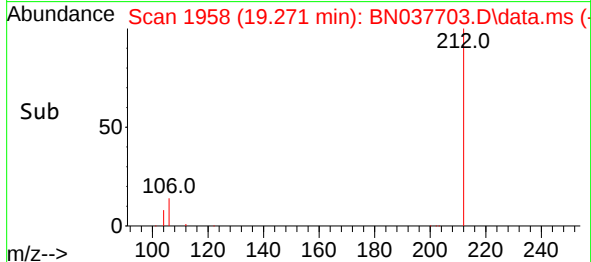

#28
Fluoranthene
Concen: 0.190 ng
RT: 19.299 min Scan# 1964
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion:202 Resp: 5795
Ion Ratio Lower Upper
202 100
101 11.5 9.3 13.9
203 17.2 13.7 20.5


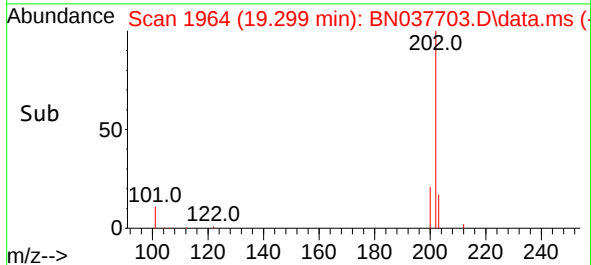






#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.420 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion:240 Resp: 7304
Ion Ratio Lower Upper
240 100
120 11.5 9.2 13.8
236 28.1 22.6 33.8

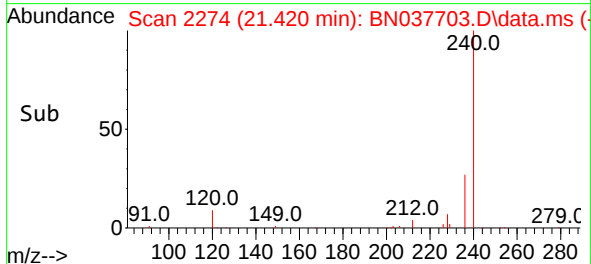

#30
Pyrene
Concen: 0.200 ng
RT: 19.661 min Scan# 2042
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion:202 Resp: 5716
Ion Ratio Lower Upper
202 100
200 20.8 16.8 25.2
203 18.1 14.3 21.5


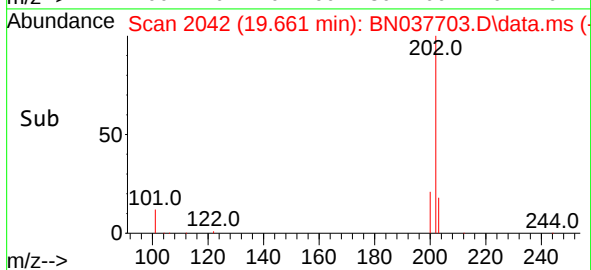

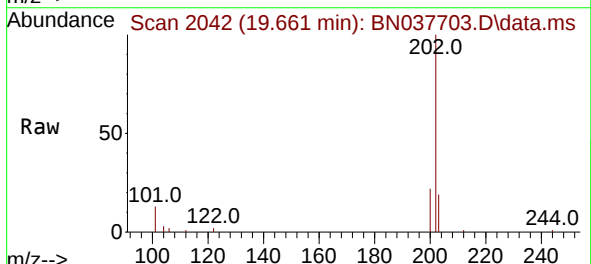




#31
 Terphenyl-d14
 Concen: 0.405 ng
 RT: 19.870 min Scan# 2087
 Delta R.T. -0.000 min
 Lab File: BN037703.D
 Acq: 11 Sep 2025 17:10




Instrument : BNA_N
 ClientSampleId : MDL-WATER-03-QT3-2025


Tgt Ion:	244	Resp:	5998
Ion Ratio	Lower	Upper	
244	100		
212	9.5	7.5	11.3
122	16.2	13.2	19.8

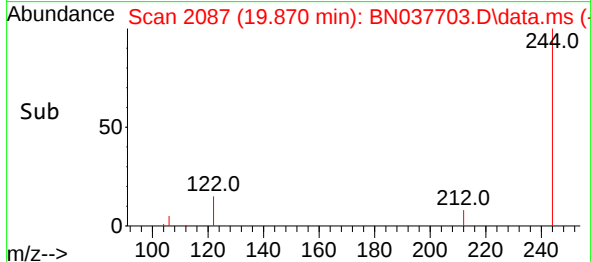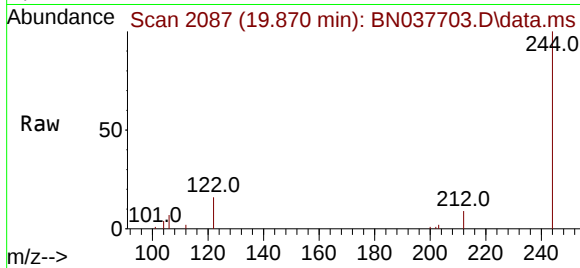

#32
 Benzo(a)anthracene
 Concen: 0.201 ng
 RT: 21.402 min Scan# 2272
 Delta R.T. -0.000 min
 Lab File: BN037703.D
 Acq: 11 Sep 2025 17:10

Tgt Ion:	228	Resp:	5127
Ion Ratio	Lower	Upper	
228	100		
226	27.7	22.2	33.2
229	21.0	15.8	23.6




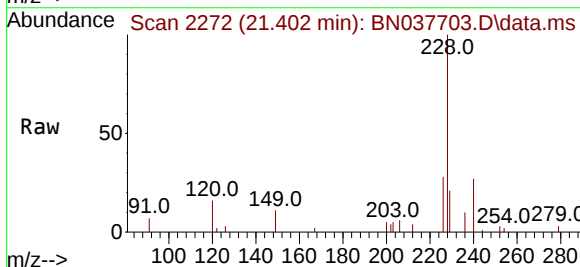


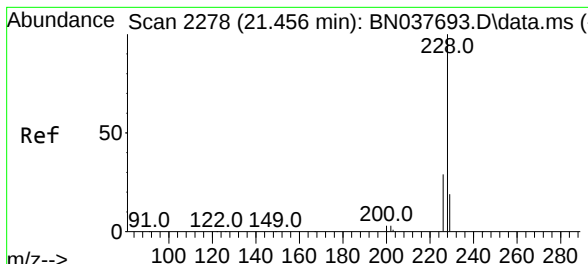

#33
 Chrysene
 Concen: 0.198 ng
 RT: 21.456 min Scan# 21456
 Delta R.T. -0.000 min
 Lab File: BN037703.D
 Acq: 11 Sep 2025 17:10




Instrument : BNA_N
 ClientSampleId : MDL-WATER-03-QT3-2025


Tgt Ion:	228	Resp:	5411
Ion Ratio	Lower	Upper	
228	100		
226	30.9	23.5	35.3
229	20.6	15.9	23.9

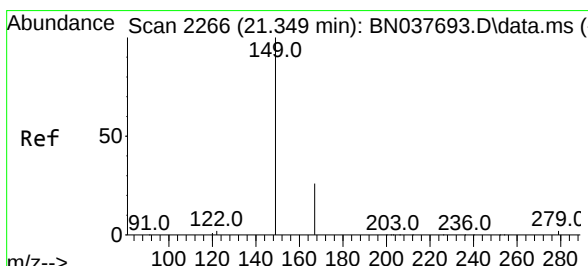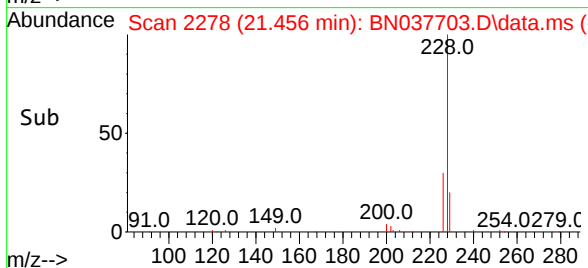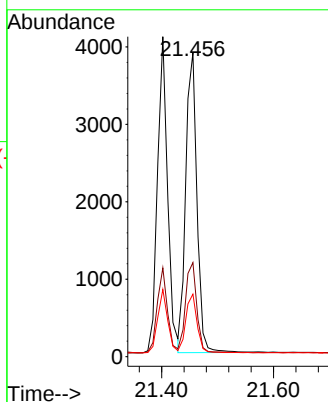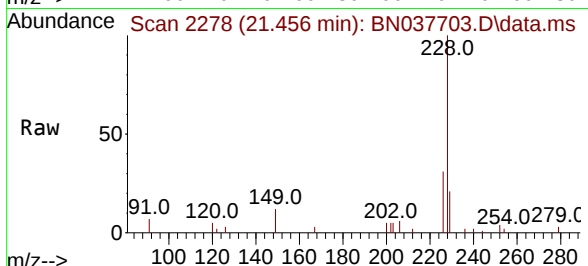

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.218 ng
 RT: 21.348 min Scan# 2266
 Delta R.T. -0.000 min
 Lab File: BN037703.D
 Acq: 11 Sep 2025 17:10

Tgt Ion:	149	Resp:	1645
Ion Ratio	Lower	Upper	
149	100		
167	27.8	20.8	31.2
279	4.6	3.3	4.9


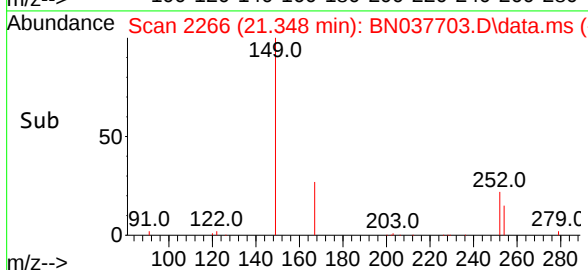
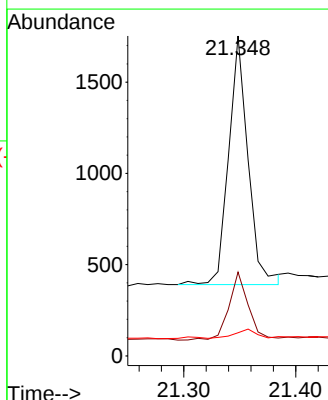
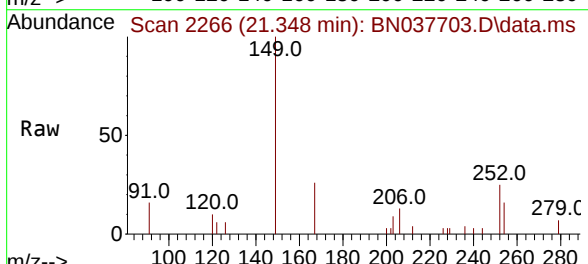




#35
Perylene-d12
Concen: 0.400 ng
RT: 23.750 min Scan# 21
Delta R.T. -0.003 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion:264 Resp: 7594
Ion Ratio Lower Upper
264 100
260 27.0 21.8 32.8
265 54.6 39.4 59.2

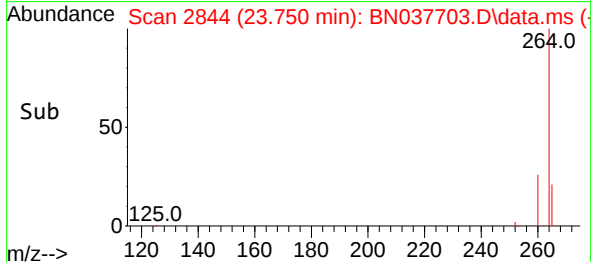

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.195 ng
RT: 26.142 min Scan# 3662
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion:276 Resp: 6208
Ion Ratio Lower Upper
276 100
138 29.7 21.9 32.9
277 25.5 20.1 30.1

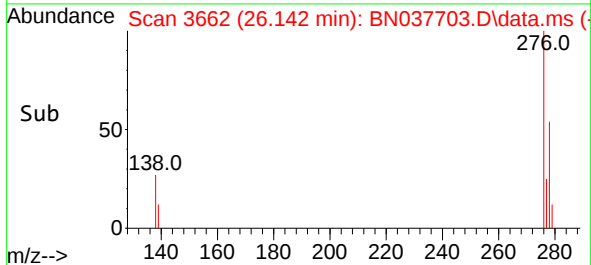



#37

Benzo(b)fluoranthene

Concen: 0.183 ng

RT: 23.046 min Scan# 2603

Delta R.T. -0.000 min

Lab File: BN037703.D

Acq: 11 Sep 2025 17:10





Instrument :

BNA_N

ClientSampleId :

MDL-WATER-03-QT3-2025

Tgt Ion:	252	Resp:	5460
Ion Ratio	Lower	Upper	
252	100		
253	27.4	19.4	29.2
125	19.6	11.2	16.8

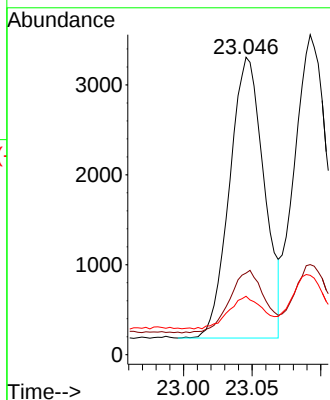

#38

Benzo(k)fluoranthene

Concen: 0.197 ng




RT: 23.092 min Scan# 2619


Delta R.T. -0.000 min

Lab File: BN037703.D

Acq: 11 Sep 2025 17:10

Tgt Ion:	252	Resp:	5992
Ion Ratio	Lower	Upper	
252	100		
253	28.2	19.4	29.0
125	24.8	11.6	17.4


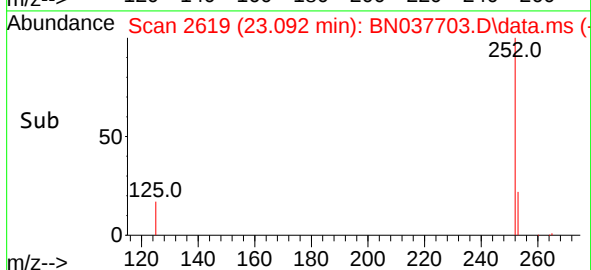
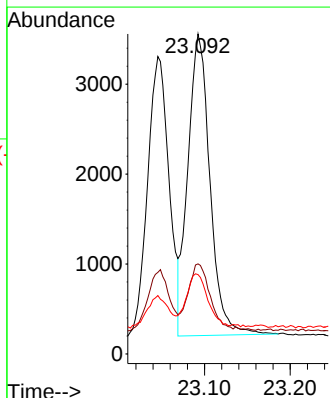





#39
Benzo(a)pyrene
Concen: 0.199 ng
RT: 23.648 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03-QT3-2025


Tgt Ion:252 Resp: 4765
Ion Ratio Lower Upper
252 100
253 31.7 20.8 31.2#
125 24.3 13.9 20.9#

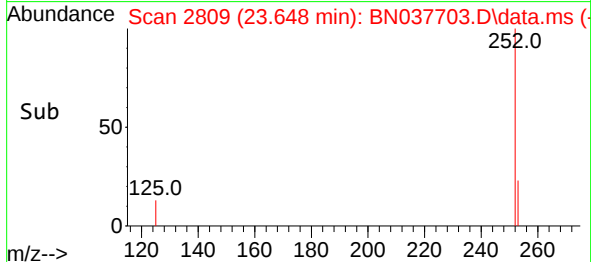

#40
Dibenzo(a,h)anthracene
Concen: 0.193 ng
RT: 26.159 min Scan# 3668
Delta R.T. -0.003 min
Lab File: BN037703.D
Acq: 11 Sep 2025 17:10

Tgt Ion:278 Resp: 4911
Ion Ratio Lower Upper
278 100
139 30.3 17.8 26.6#
279 31.2 22.0 33.0

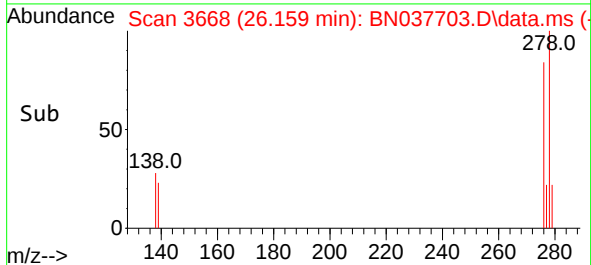

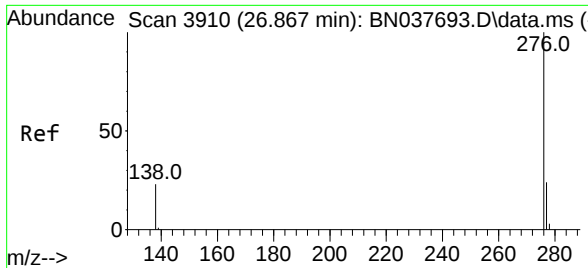

#41

Benzo(g,h,i)perylene

Concen: 0.183 ng

RT: 26.864 min Scan# 3910

Delta R.T. -0.003 min

Lab File: BN037703.D


Acq: 11 Sep 2025 17:10

Instrument :

BNA_N

ClientSampleId :

MDL-WATER-03-QT3-2025

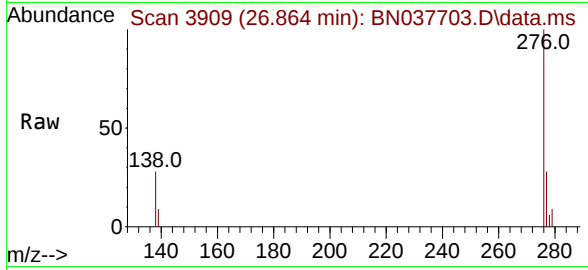

Tgt Ion:276 Resp: 5244

Ion	Ratio	Lower	Upper
-----	-------	-------	-------

276	100		
-----	-----	--	--

277	28.3	20.6	31.0
-----	------	------	------

138	27.8	20.2	30.2
-----	------	------	------

