
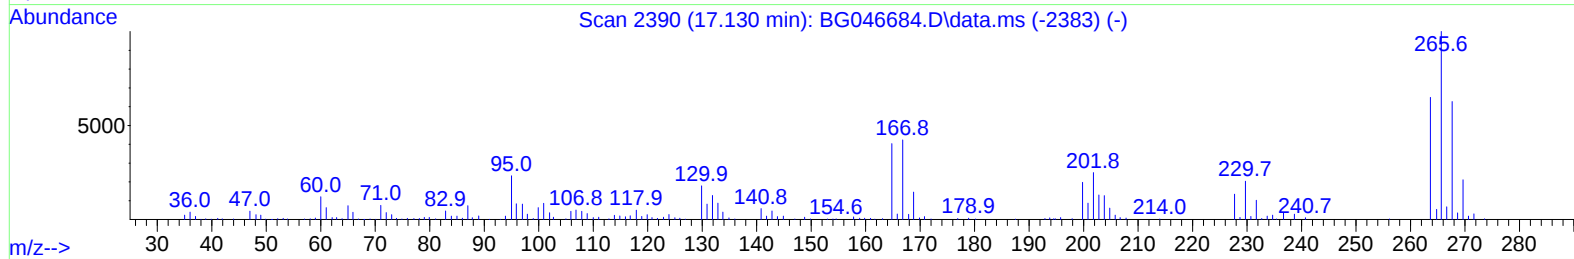
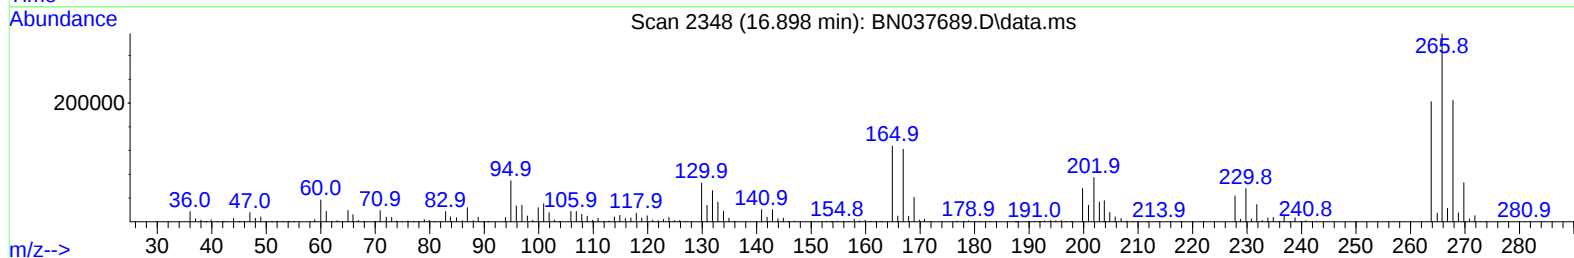


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN091125\  
Data File : BN037689.D  
Acq On : 11 Sep 2025 07:54  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 13:15:02 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Sep 11 13:14:53 2025  
Response via : Initial Calibration

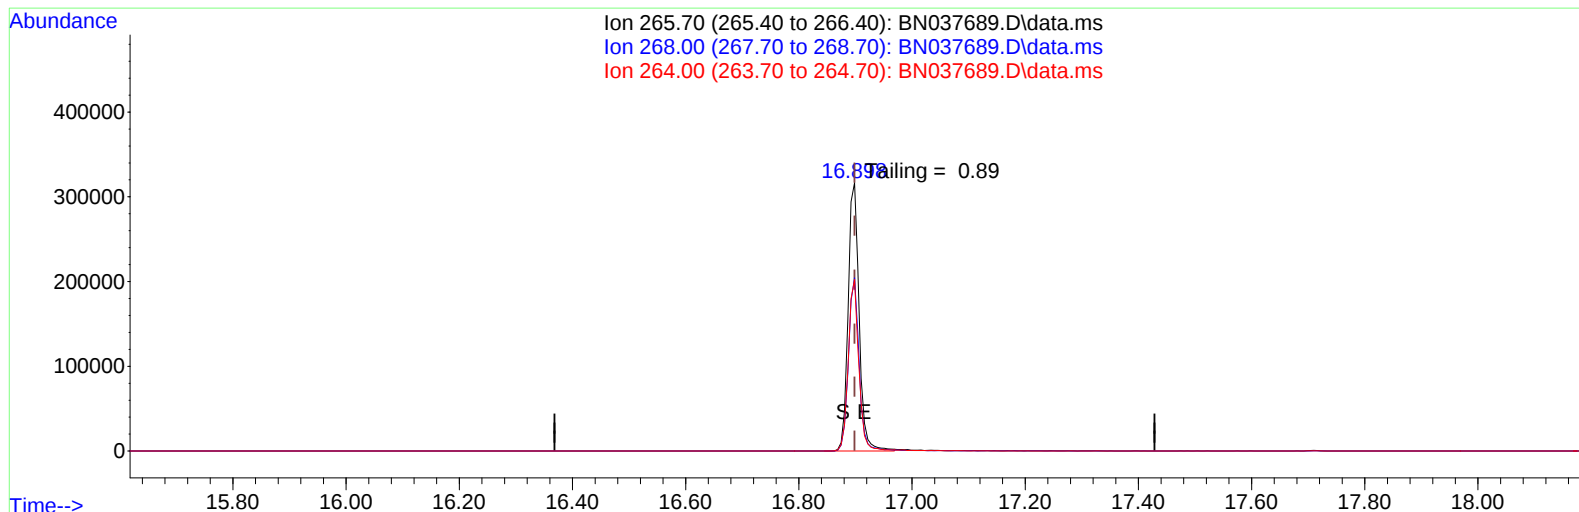

TIC: BN037689.D\data.ms

**(70) Pentachlorophenol (C)**




16.898min ( 0.000) 277.63 ng

response 430126

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.50  | 64.54  |
| 264.00 | 63.90  | 63.87  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN091125\  
Data File : BN037689.D  
Acq On : 11 Sep 2025 07:54  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 13:15:02 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Sep 11 13:14:53 2025  
Response via : Initial Calibration

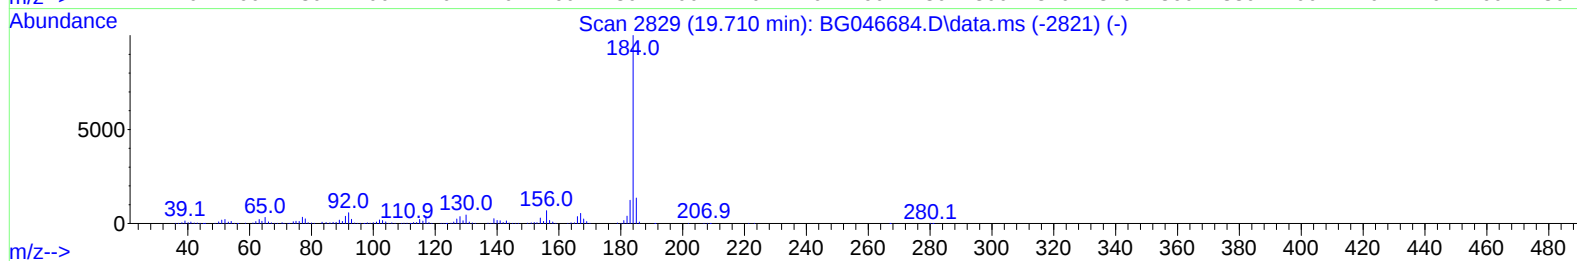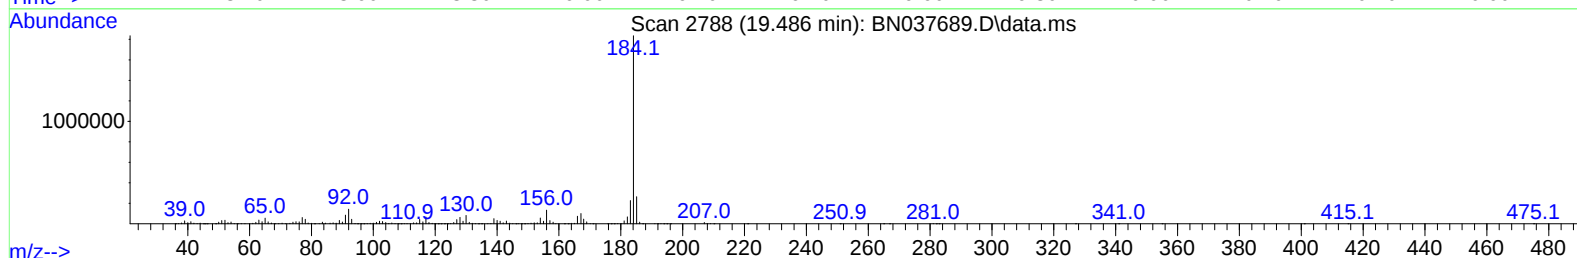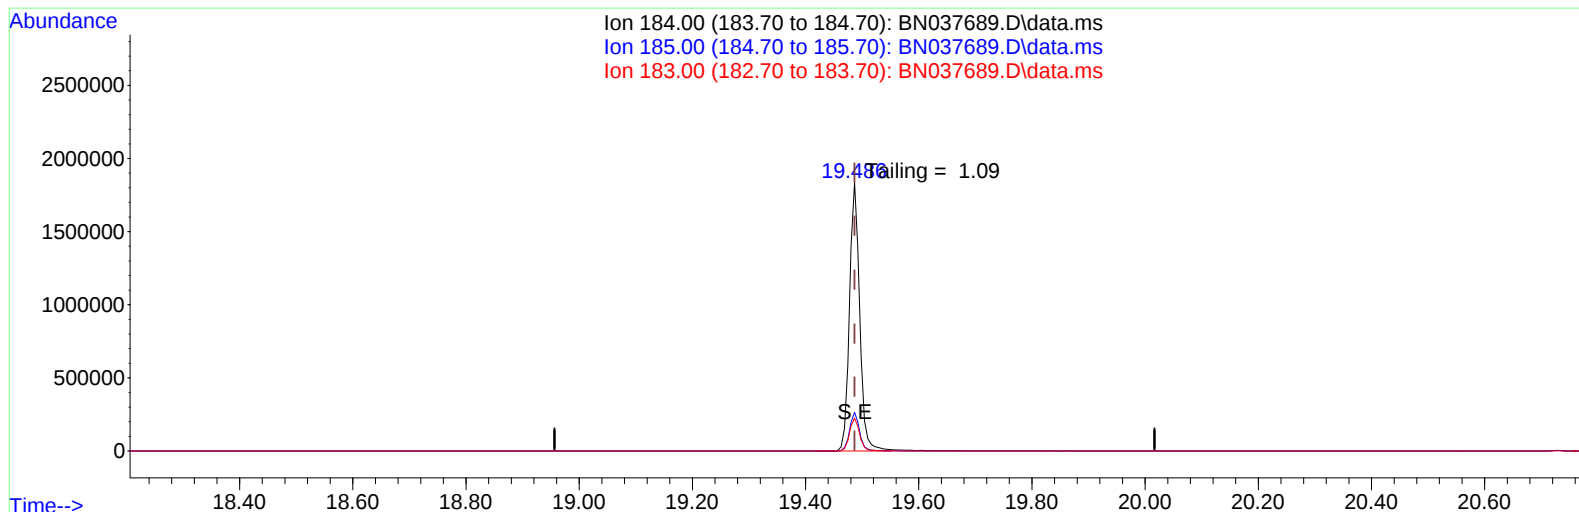

TIC: BN037689.D\data.ms

**(77) Benzidine****19.486min ( 0.000) 64237.37 ng****response 2281946**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.43  |
| 183.00 | 12.30  | 12.32  |
| 0.00   | 0.00   | 0.00   |