

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091218\
 Data File : BN002655.D
 Acq On : 12 Sep 2018 15:21
 Operator : JU/SJ
 Sample : J4792-21
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z36

Quant Time: Sep 13 05:03:38 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 13 05:01:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	179705	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	828055	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.29	164	494775	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	1132615	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1132470	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	1007518	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	14174	3.72	ng/uL	0.00
5) Phenol-d5	6.85	99	313090	19.00	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	215213	20.79	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	269279	21.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	227672	17.28	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	143700	21.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	169255	24.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	286994	22.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	387851	28.17	ng/ul	0.00
43) Dimethylphthalate-d6	13.70	166	1029101	25.09	ng/ul	0.00
46) Acenaphthylene-d8	13.98	160	1294649	25.73	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	154843	19.97	ng/ul	0.00
57) Fluorene-d10	15.29	176	922127	25.93	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	153232	21.25	ng/ul	0.00
70) Anthracene-d10	17.14	188	1448183	26.76	ng/ul	0.00
78) Pyrene-d10	19.45	212	1570236	28.98	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	1416852	26.89	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.75	163	517000	12.852	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091218\
Data File : BN002655.D
Acq On : 12 Sep 2018 15:21
Operator : JU/SJ
Sample : J4792-21
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z36

Quant Time: Sep 13 05:03:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 13 05:01:35 2018
Response via : Initial Calibration

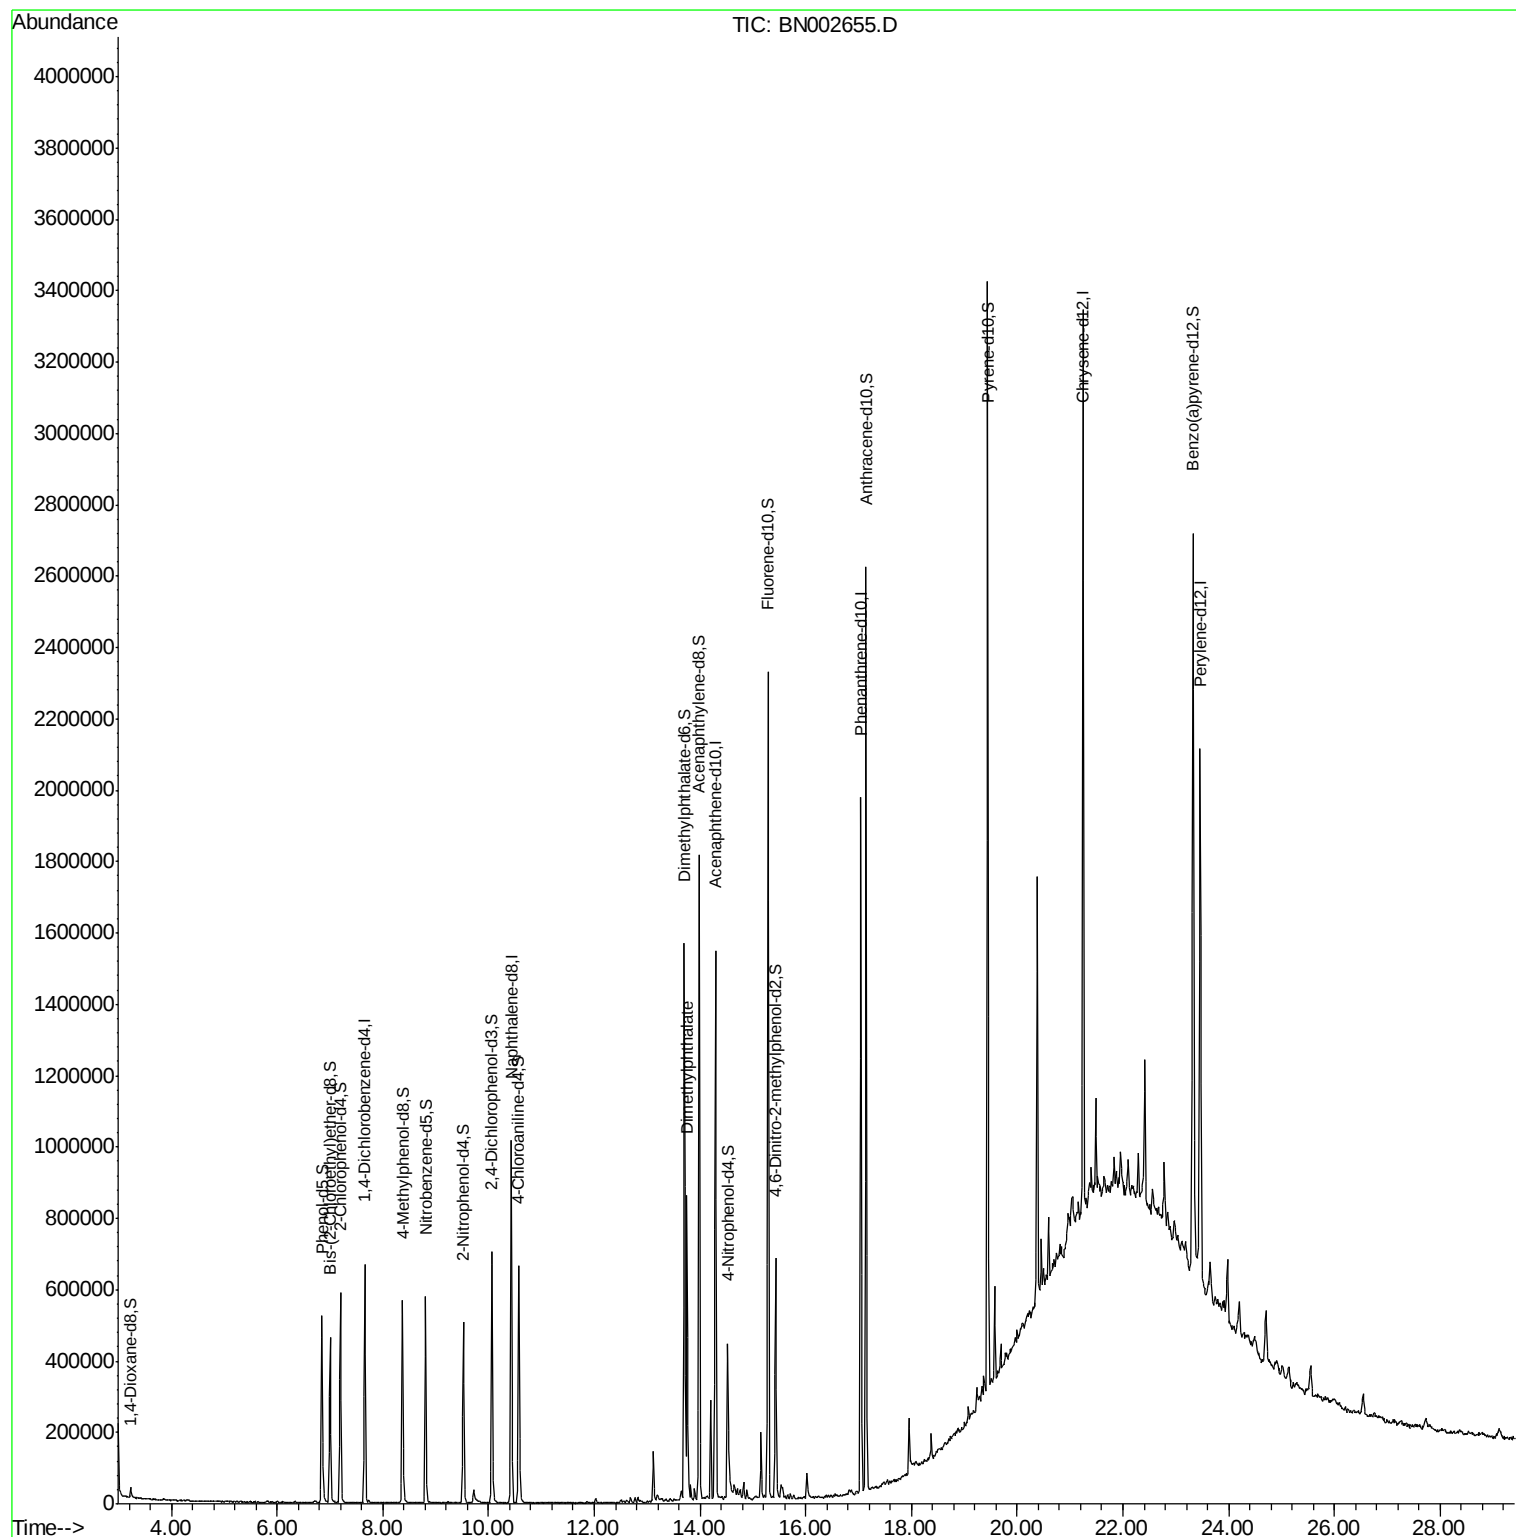

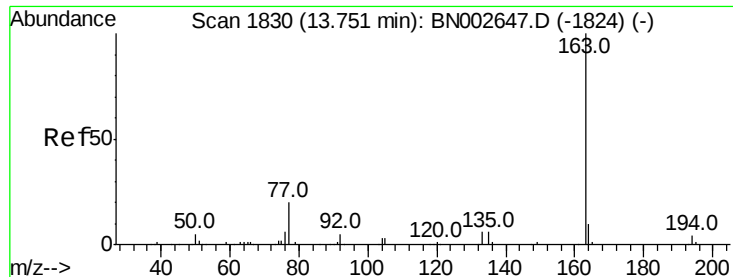

#44

Dimethylphthalate

Concen: 12.852 ng/ul

RT: 13.75 min Scan# 1830

Delta R.T. 0.00 min

Lab File: BN002655.D

Acq: 12 Sep 2018 15:21

Instrument :

BNA_N

ClientSampleId :

A3Z36


Tot Ion:163 Resp: 517000

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 10.0 7.8 11.8

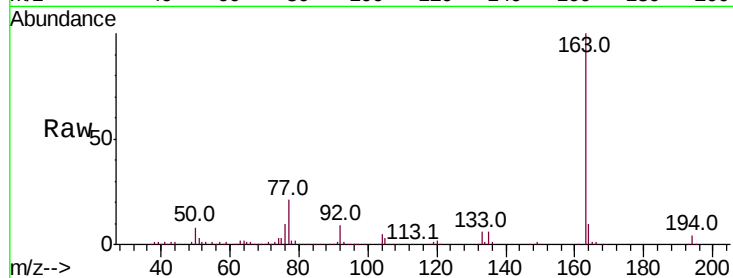

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

