


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091219\
Data File : BN007599.D
Acq On : 12 Sep 2019 09:14
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091219.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 12 14:27:51 2019

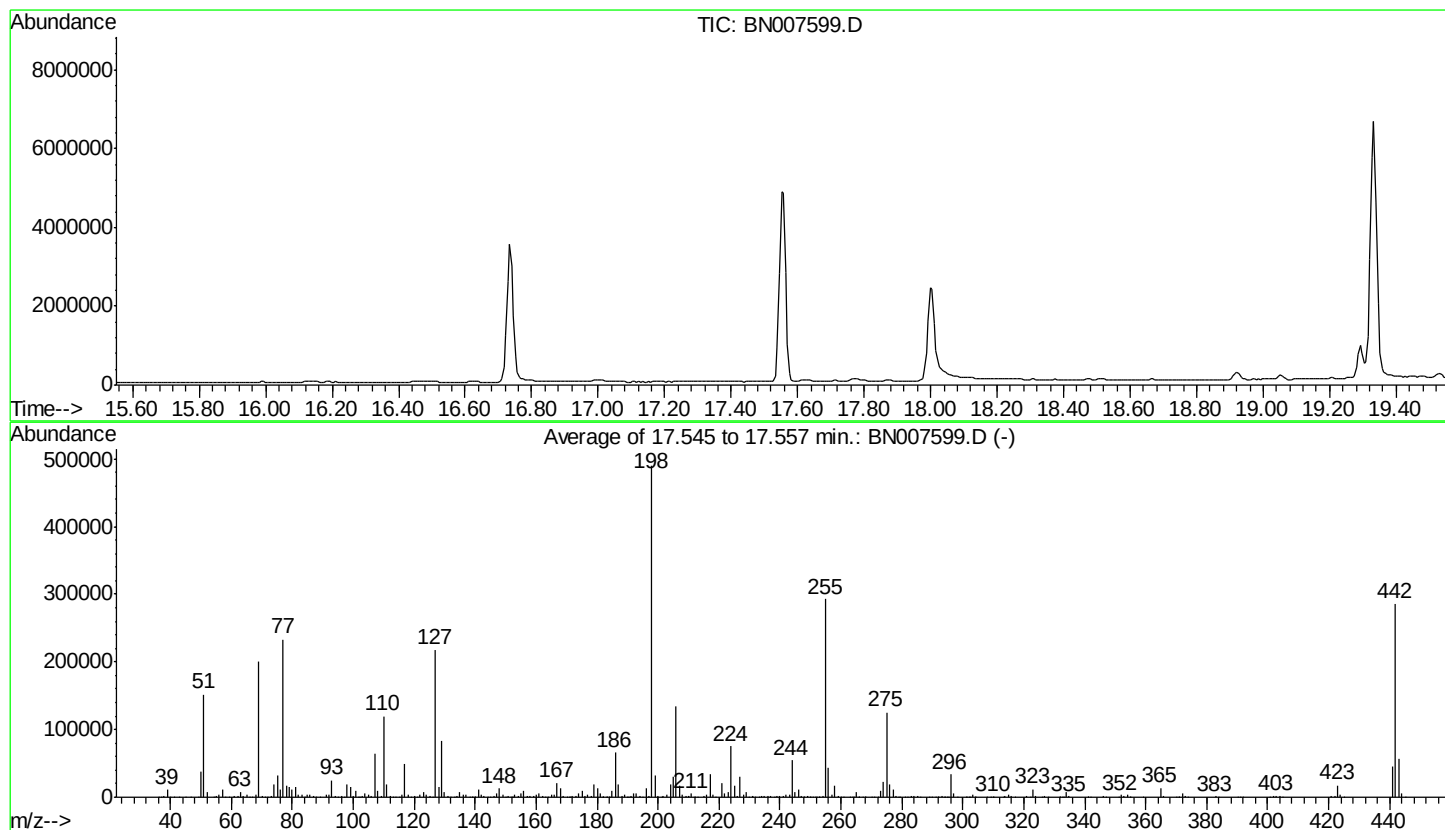

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	151972	PASS
68	69	0.00	2	1.8	3528	PASS
69	198	0.00	100	41.0	201175	PASS
70	69	0.00	2	0.6	1214	PASS
127	198	10	80	44.5	217962	PASS
197	198	0.00	2	0.4	2071	PASS
198	198	100	100	100.0	490090	PASS
199	198	5	9	6.7	32800	PASS
275	198	10	60	25.6	125453	PASS
365	198	1	100	2.8	13617	PASS
441	198	0.01	100	9.1	44562	PASS
442	198	50	100	58.4	286341	PASS
443	442	15	24	19.9	57114	PASS