

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091223\
 Data File : BN027582.D
 Acq On : 11 Sep 2023 19:06
 Operator : MA/JU
 Sample : PB155129BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK129

Quant Time: Sep 12 02:13:39 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 02:09:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	6296	0.400	ng/ul	0.00
4) Naphthalene-d8	10.856	136	18021	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.666	164	8718	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	16903	0.400	ng/ul	0.00
17) Chrysene-d12	21.592	240	12272	0.400	ng/ul	0.00
23) Perylene-d12	24.094	264	12796	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.439	96	49008	5.852	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	8199	0.300	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	13332	0.317	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.803	202	2299	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.930	252	4672	0.099	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091223\
Data File : BN027582.D
Acq On : 11 Sep 2023 19:06
Operator : MA/JU
Sample : PB155129BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK129

Quant Time: Sep 12 02:13:39 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:09:21 2023
Response via : Initial Calibration




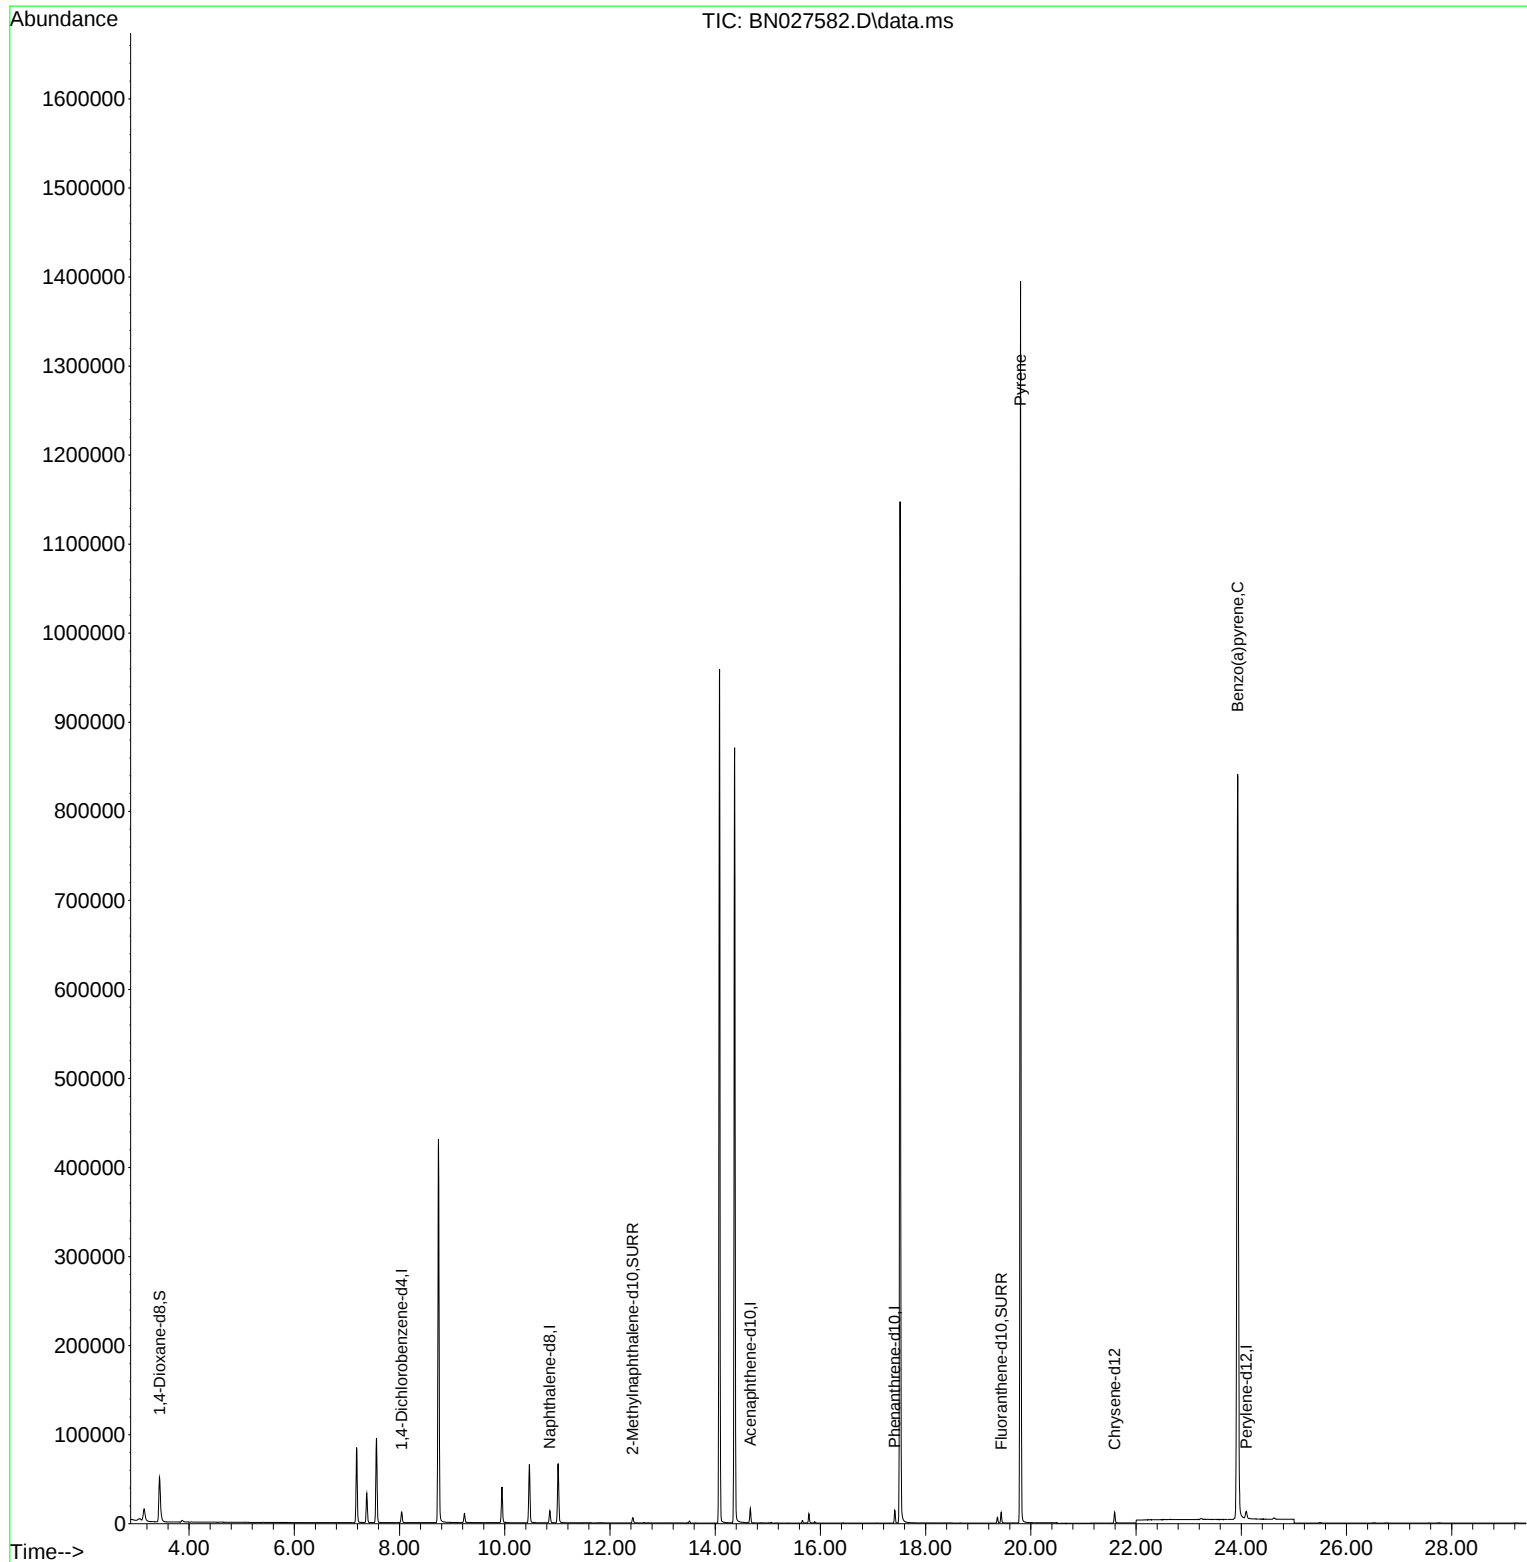


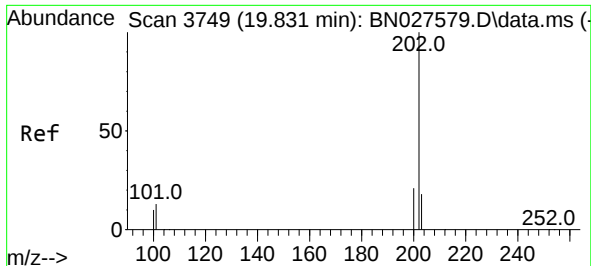

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.803 min Scan# 31
Delta R.T. -0.028 min
Lab File: BN027582.D
Acq: 11 Sep 2023 19:06

Instrument :
BNA_N
ClientSampleId :
SBLK129

Tgt Ion:202 Resp: 2299
Ion Ratio Lower Upper
202 100
101 159.0 11.4 17.2#
100 1173.4 9.4 14.2#

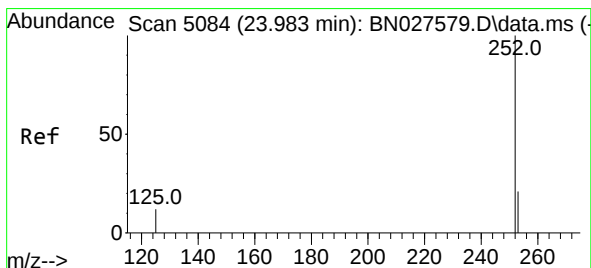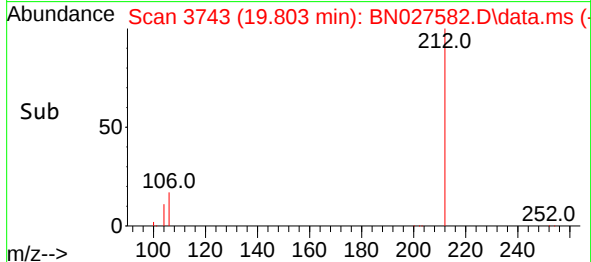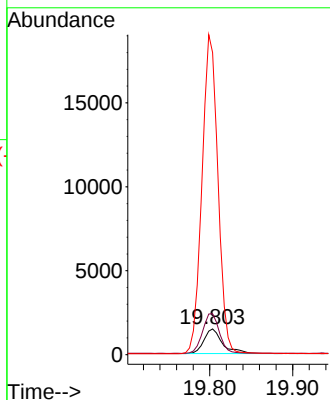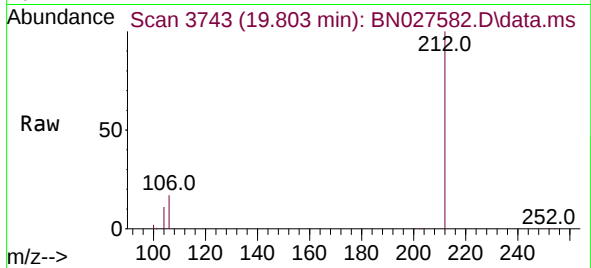

#26
Benzo(a)pyrene
Concen: 0.099 ng/ul
RT: 23.930 min Scan# 5066
Delta R.T. -0.053 min
Lab File: BN027582.D
Acq: 11 Sep 2023 19:06

Tgt Ion:252 Resp: 4672
Ion Ratio Lower Upper
252 100
253 49.9 22.4 33.6#
125 45.2 17.4 26.2#

