

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091223\
 Data File : BN027585.D
 Acq On : 11 Sep 2023 20:58
 Operator : MA/JU
 Sample : PB155161BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK161

Quant Time: Sep 12 02:14:16 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 02:09:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.038	152	5707	0.400	ng/ul	0.00
4) Naphthalene-d8	10.856	136	15740	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.666	164	7364	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	14186	0.400	ng/ul	0.00
17) Chrysene-d12	21.592	240	9906	0.400	ng/ul	0.00
23) Perylene-d12	24.094	264	10618	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.439	96	47156	6.212	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	8235	0.345	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	13295	0.392	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.803	202	2241	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.927	252	4420	0.113	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091223\
Data File : BN027585.D
Acq On : 11 Sep 2023 20:58
Operator : MA/JU
Sample : PB155161BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK161

Quant Time: Sep 12 02:14:16 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:09:21 2023
Response via : Initial Calibration




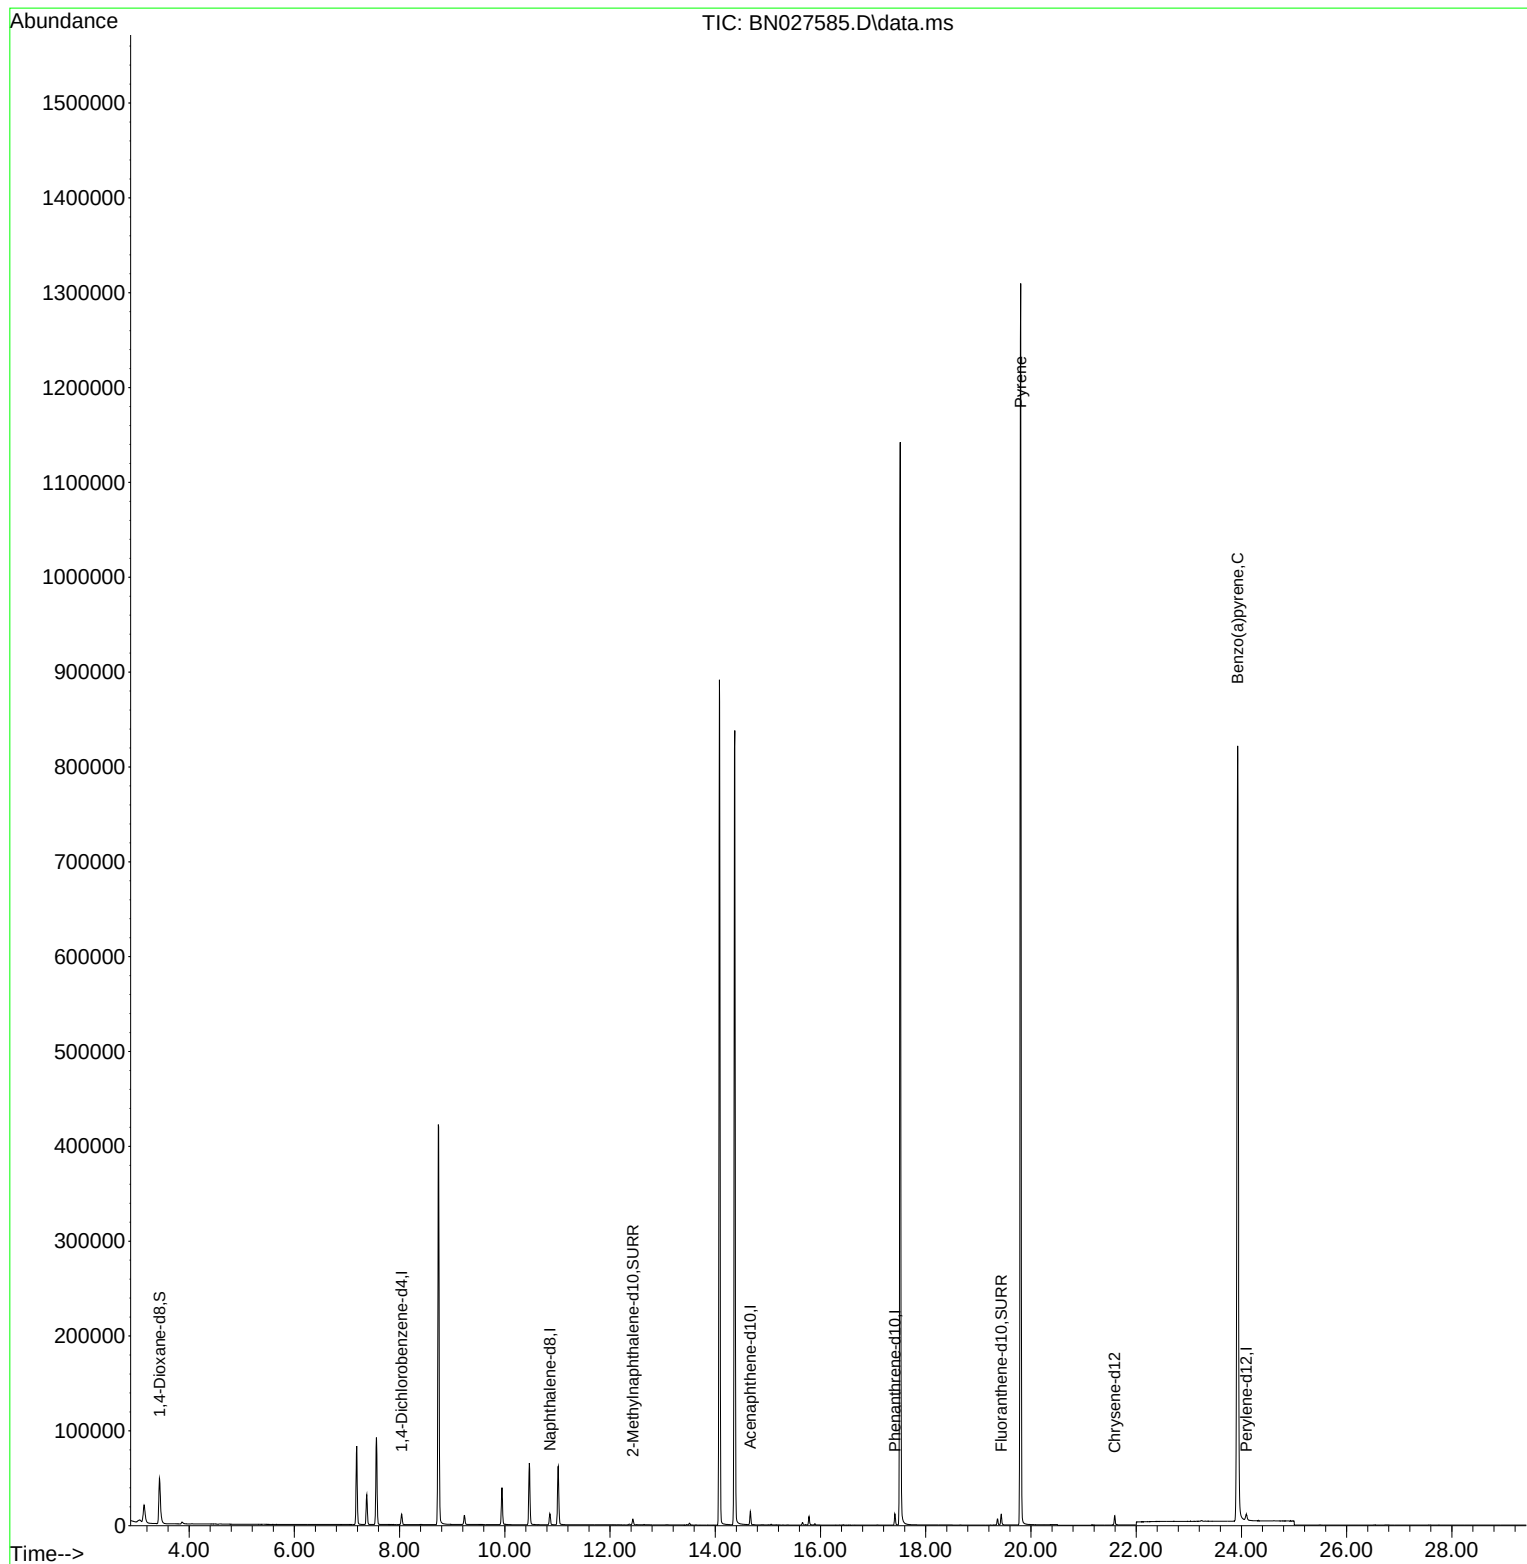


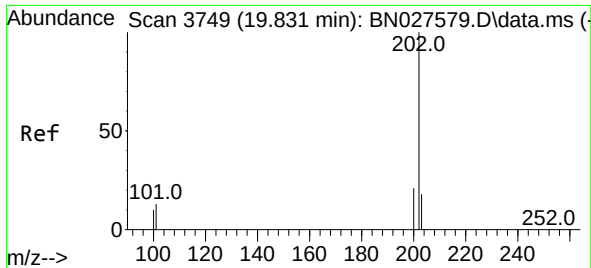

#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.803 min Scan# 31
Delta R.T. -0.028 min
Lab File: BN027585.D
Acq: 11 Sep 2023 20:58

Instrument :
BNA_N
ClientSampleId :
SBLK161

Tgt Ion:202 Resp: 2241
Ion Ratio Lower Upper
202 100
101 159.6 11.4 17.2#
100 1159.1 9.4 14.2#

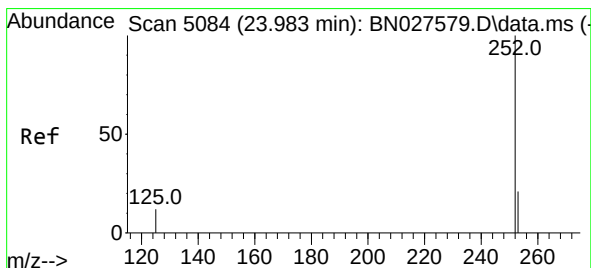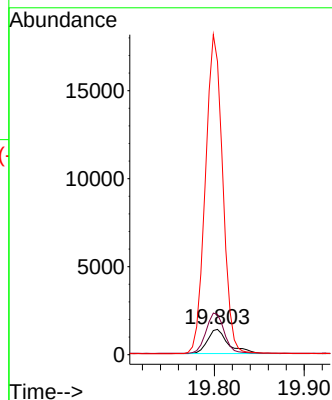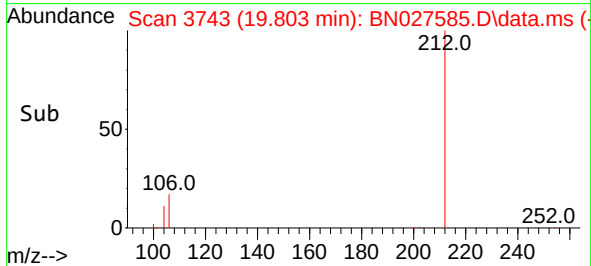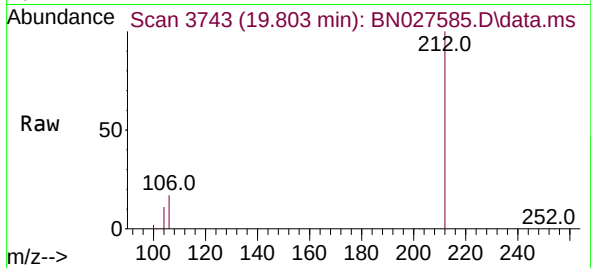

#26
Benzo(a)pyrene
Concen: 0.113 ng/ul
RT: 23.927 min Scan# 5065
Delta R.T. -0.055 min
Lab File: BN027585.D
Acq: 11 Sep 2023 20:58

Tgt Ion:252 Resp: 4420
Ion Ratio Lower Upper
252 100
253 50.9 22.4 33.6#
125 45.3 17.4 26.2#

