

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091319\
 Data File : BN007648.D
 Acq On : 14 Sep 2019 04:58
 Operator : HP/JU
 Sample : K4858-16
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE131D1-20190910

Quant Time: Sep 16 01:37:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 12 14:27:51 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	9333	0.40	ng	0.00
7) Naphthalene-d8	10.48	136	35494	0.40	ng	-0.01
13) Acenaphthene-d10	14.33	164	19662	0.40	ng	0.00
19) Phenanthrene-d10	17.08	188	40842	0.40	ng	0.00
27) Chrysene-d12	21.26	240	41006	0.40	ng	-0.02
34) Perylene-d12	23.49	264	42055	0.40	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.33	112	5201	0.17	ng	0.00
5) Phenol-d6	6.89	99	4820	0.14	ng	0.00
8) Nitrobenzene-d5	8.85	82	10569	0.37	ng	-0.01
11) 2-Methylnaphthalene-d10	12.07	152	24442	0.41	ng	0.00
14) 2,4,6-Tribromophenol	15.83	330	2352	0.32	ng	0.00
15) 2-Fluorobiphenyl	12.96	172	37853	0.44	ng	0.00
25) Fluoranthene-d10	19.11	212	57076	0.44	ng	0.00
29) Terphenyl-d14	19.72	244	56001	0.52	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.31	88	82411	7.369	ng	Qvalue 89
3) n-Nitrosodimethylamine	3.03	42	172711	34.034	ng	# 1
32) Bis(2-ethylhexyl)phthalate	21.20	149	6456	0.131	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091319\
Data File : BN007648.D
Acq On : 14 Sep 2019 04:58
Operator : HP/JU
Sample : K4858-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE131D1-20190910

Quant Time: Sep 16 01:37:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 12 14:27:51 2019
Response via : Initial Calibration

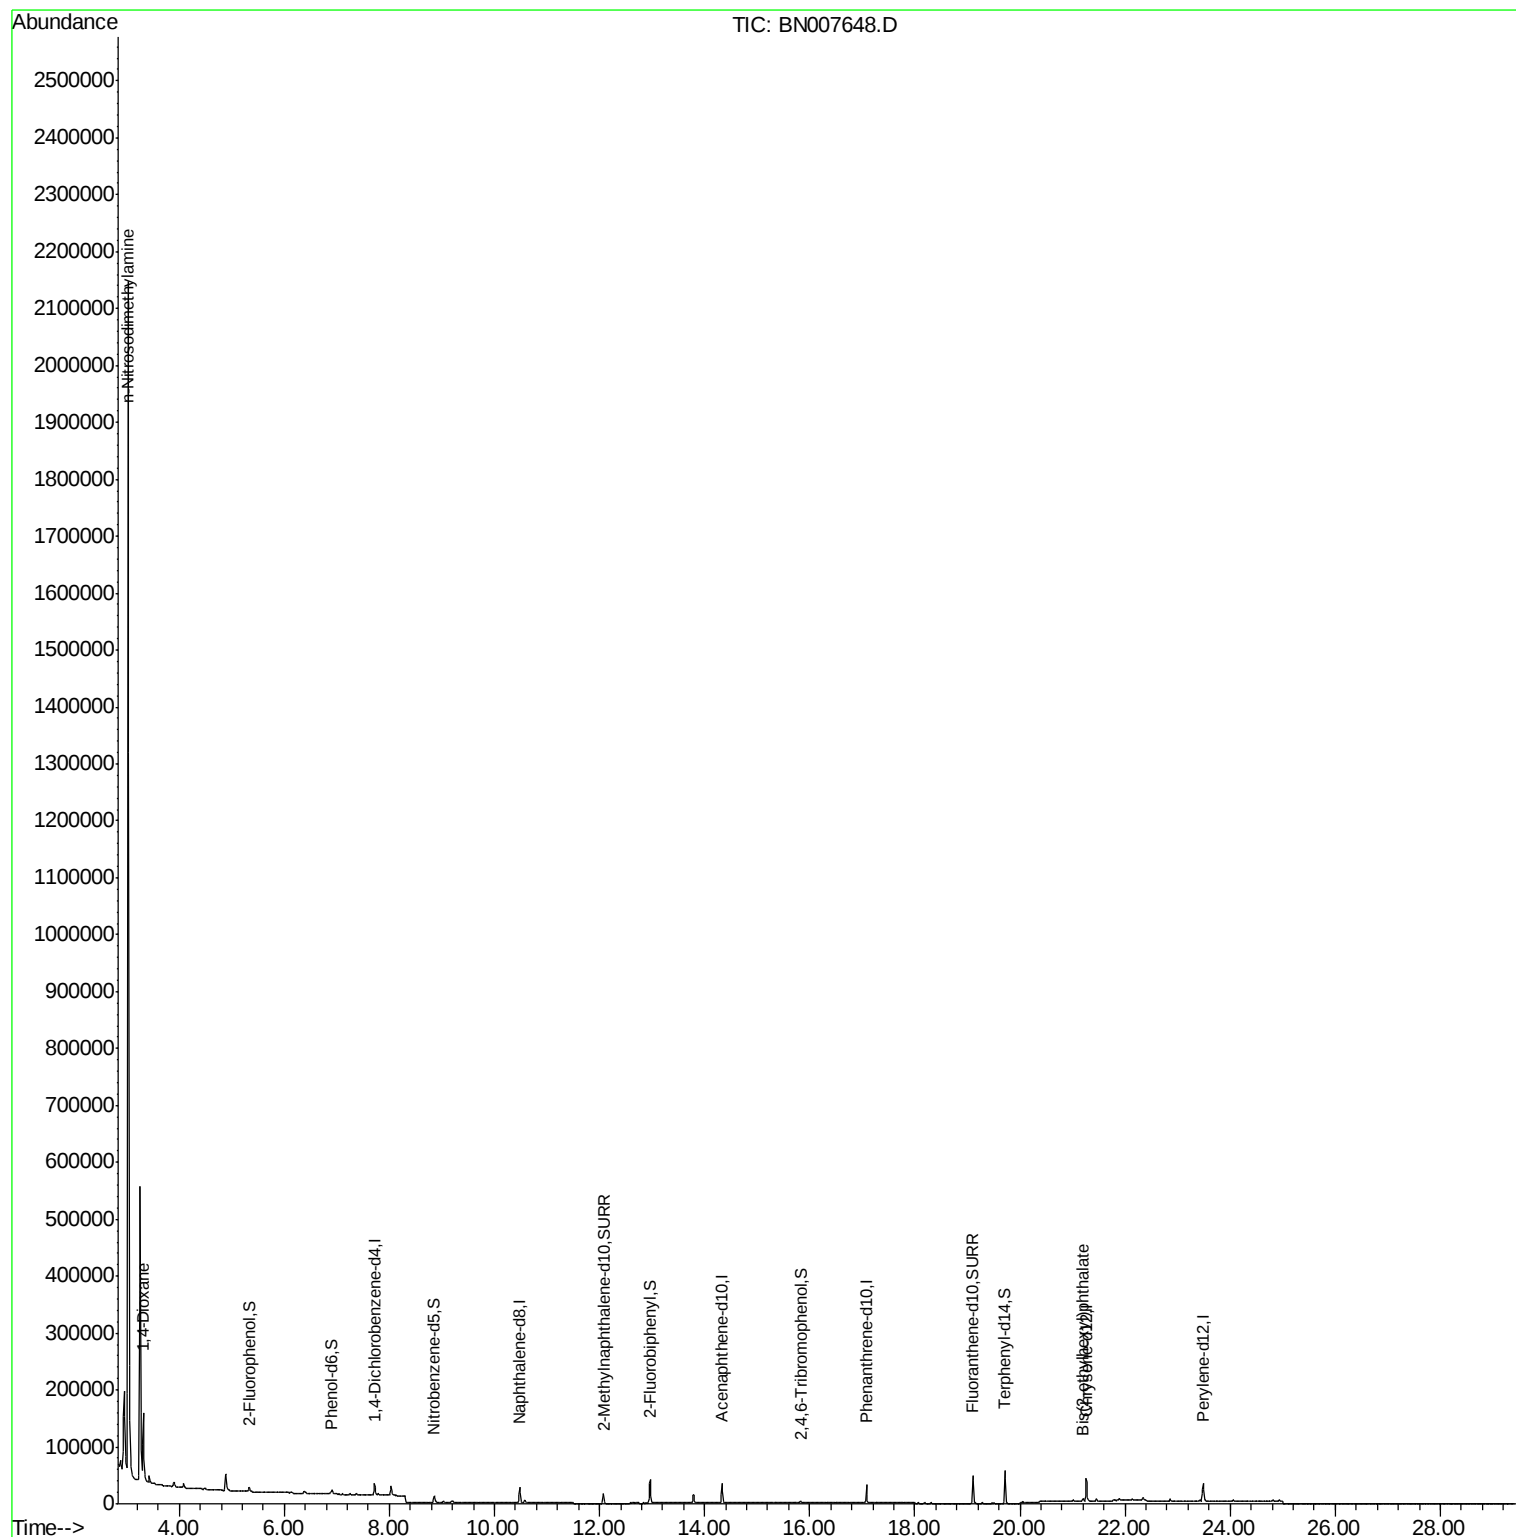




#1



1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.72 min Scan# 607
Delta R.T. -0.01 min
Lab File: BN007648.D
Acq: 14 Sep 2019 04:58

Instrument :
BNA_N
ClientSampleId :
RE131D1-20190910

Tot Ion:152 Resp: 9333
Ion Ratio Lower Upper
152 100
150 154.3 122.4 183.6
115 63.0 50.4 75.6

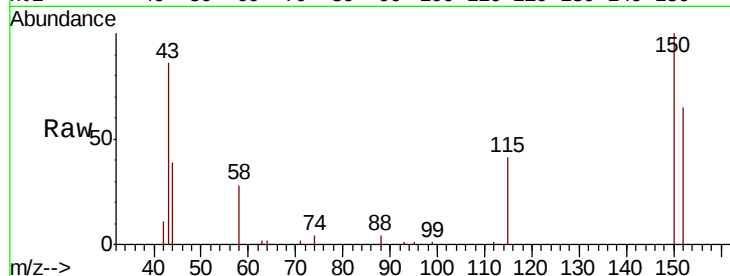


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

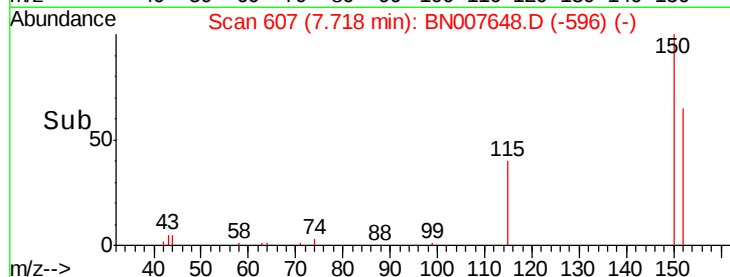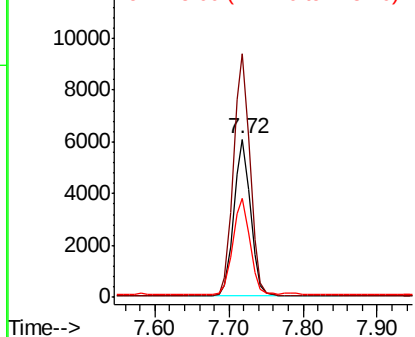



#2

1,4-Dioxane
Concen: 7.369 ng
RT: 3.31 min Scan# 60
Delta R.T. -0.02 min
Lab File: BN007648.D
Acq: 14 Sep 2019 04:58

Tgt Ion: 88 Resp: 82411
Ion Ratio Lower Upper
88 100
58 59.7 57.0 85.4
43 23.0 20.0 30.0

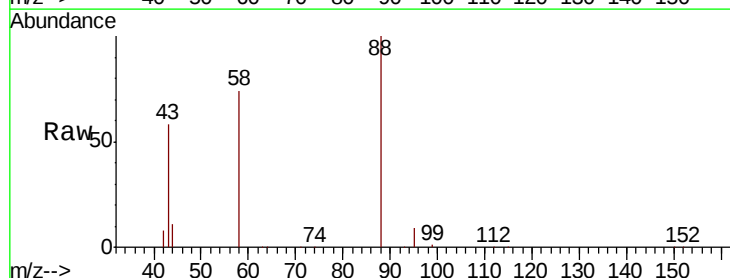

Abundance Ion 88.00 (87.70 to 88.70): BNC
Ion 58.00 (57.70 to 58.70): BNC
Ion 43.00 (42.70 to 43.70): BNC

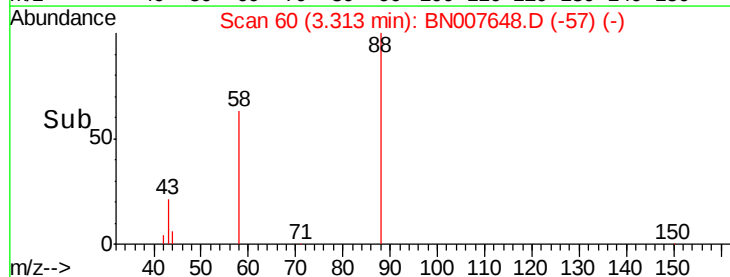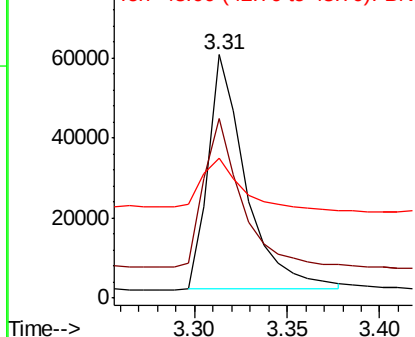







#3

n-Nitrosodimethylamine
 Concen: 34.034 ng
 RT: 3.03 min Scan# 25
 Delta R.T. -0.01 min
 Lab File: BN007648.D
 Acq: 14 Sep 2019 04:58

Instrument :
 BNA_N
 ClientSampleId :
 RE131D1-20190910




Tot Ion: 42 Resp: 172711
 Ion Ratio Lower Upper
 42 100
 74 145.7 9.8 14.8#
 44 26.6 0.0 0.0#

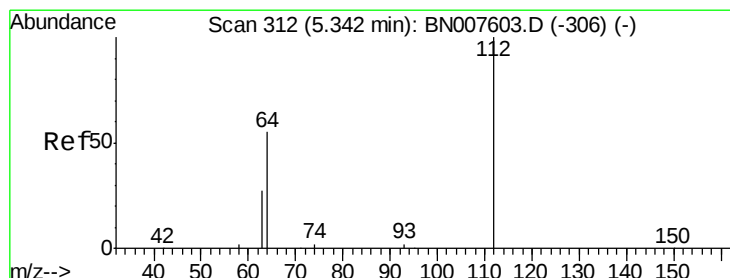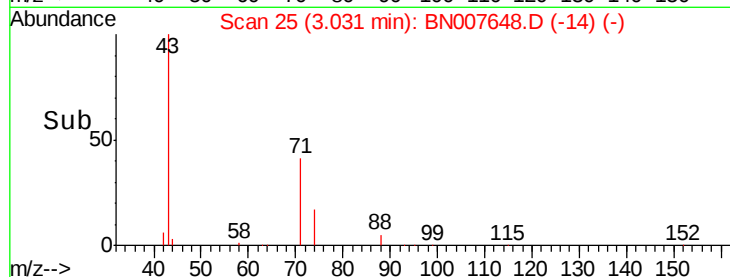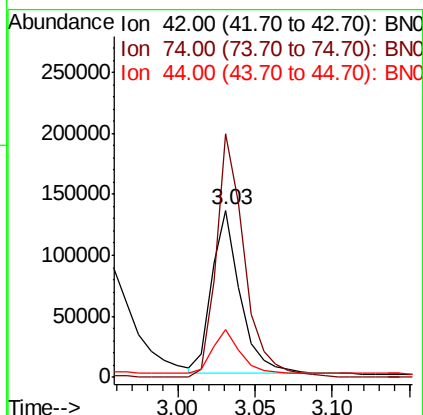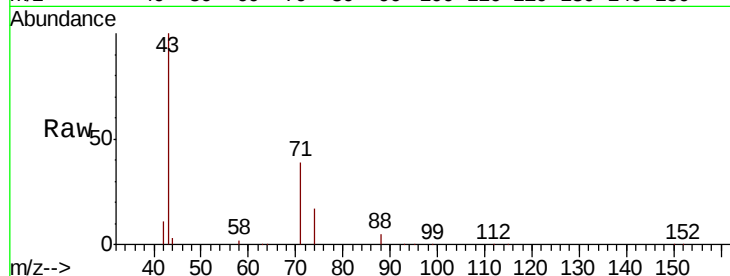


#4

2-Fluorophenol
 Concen: 0.174 ng
 RT: 5.33 min Scan# 311
 Delta R.T. -0.01 min
 Lab File: BN007648.D
 Acq: 14 Sep 2019 04:58

Tgt Ion: 112 Resp: 5201
 Ion Ratio Lower Upper
 112 100
 64 59.8 48.5 72.7
 63 29.7 24.4 36.6

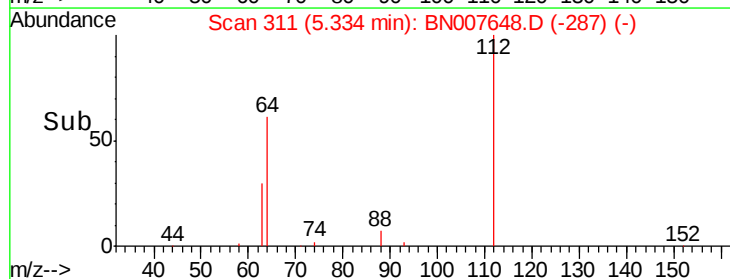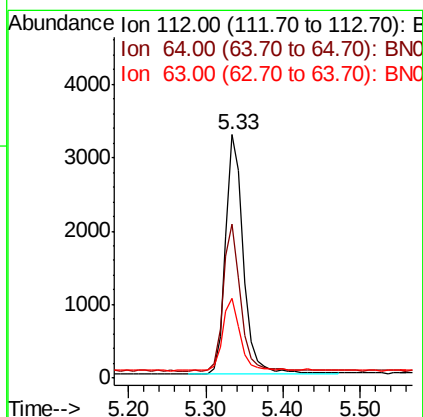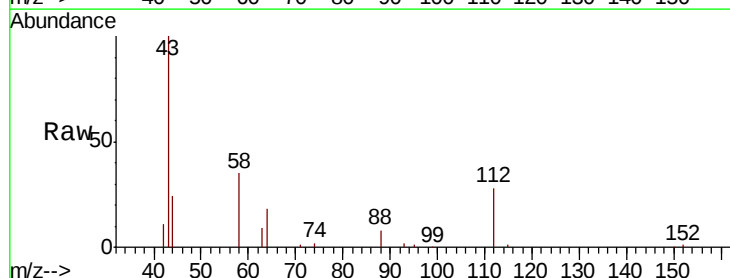

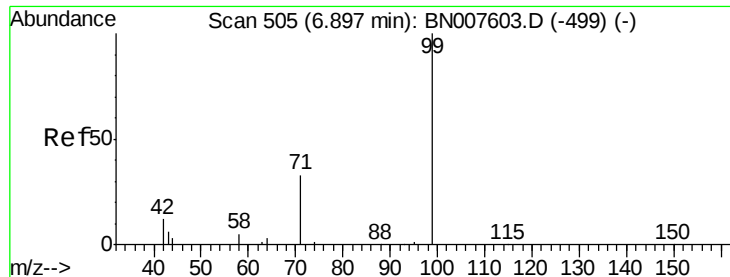

#5

Phenol-d6

Concen: 0.138 ng

RT: 6.89 min Scan# 504

Delta R.T. -0.01 min

Lab File: BN007648.D

Acq: 14 Sep 2019 04:58

Instrument :

BNA_N

ClientSampleId :

RE131D1-20190910


Tot Ion: 99 Resp: 4820

Ion Ratio Lower Upper

99 100

42 22.8 11.8 17.6#

71 37.5 28.0 42.0



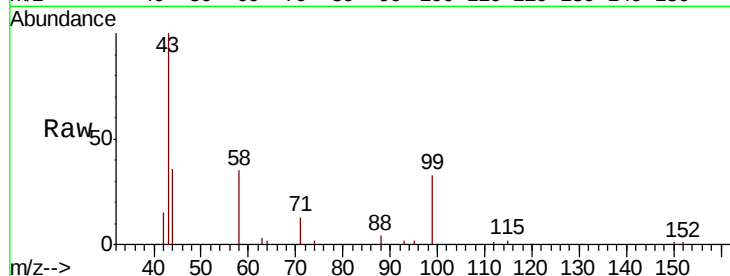


Abundance

Ion 99.00 (98.70 to 99.70): BN007603.D (-499) (-)

Ion 42.00 (41.70 to 42.70): BN007603.D (-499) (-)

Ion 71.00 (70.70 to 71.70): BN007603.D (-499) (-)

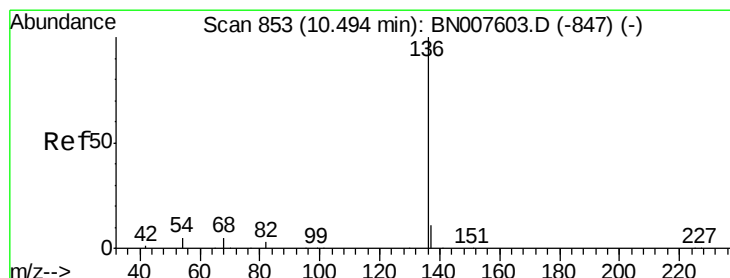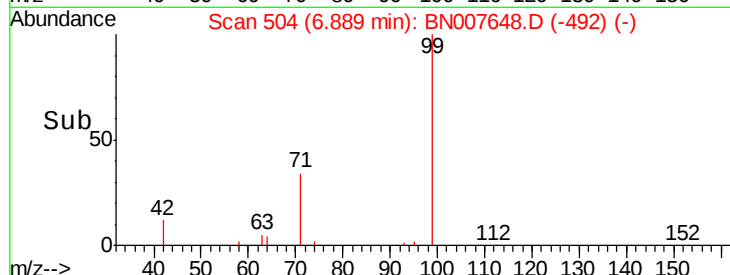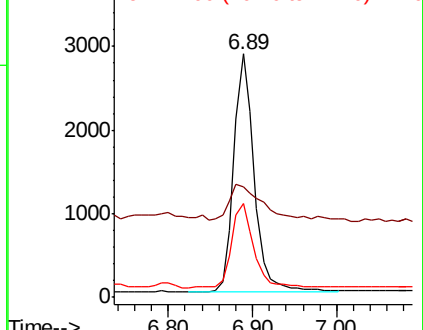

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.48 min Scan# 852

Delta R.T. -0.01 min

Lab File: BN007648.D

Acq: 14 Sep 2019 04:58

Tgt Ion: 136 Resp: 35494


Ion Ratio Lower Upper

136 100

137 11.3 8.8 13.2

54 7.3 4.2 6.4#

68 7.6 4.6 7.0#

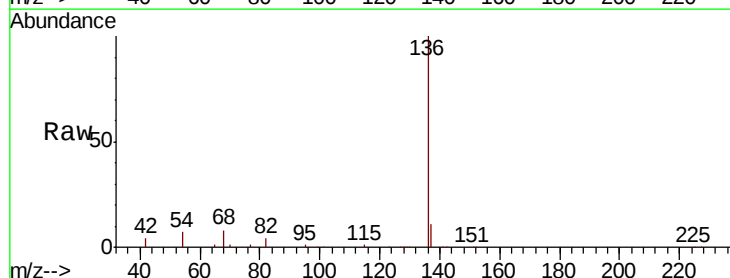



Abundance


Ion 136.00 (135.70 to 136.70): BN007603.D (-847) (-)

Ion 137.00 (136.70 to 137.70): BN007603.D (-847) (-)

Ion 54.00 (53.70 to 54.70): BN007603.D (-847) (-)

Ion 68.00 (67.70 to 68.70): BN007603.D (-847) (-)

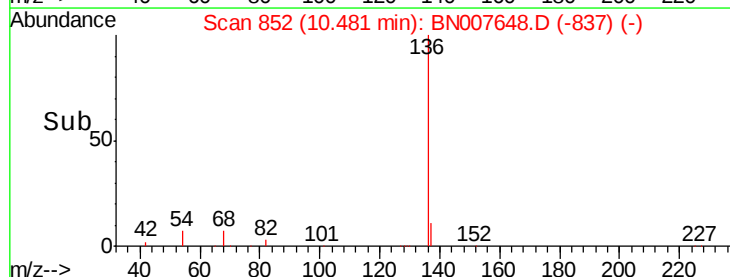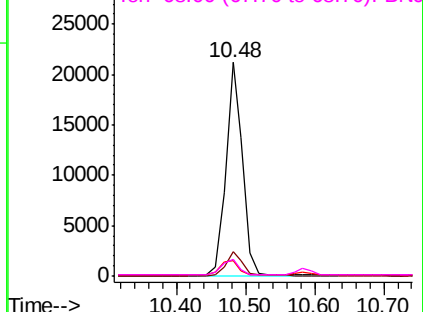

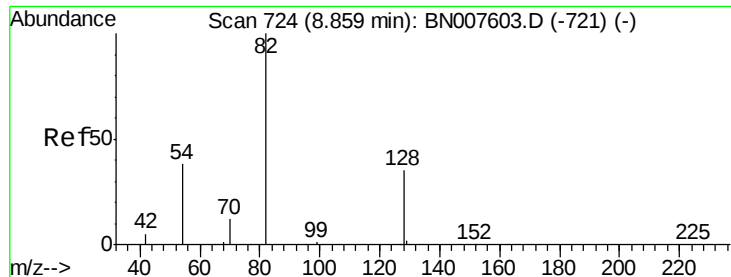

#8

Nitrobenzene-d5

Concen: 0.373 ng

RT: 8.85 min Scan# 723

Delta R.T. -0.01 min

Lab File: BN007648.D

Acq: 14 Sep 2019 04:58

Instrument :

BNA_N

ClientSampleId :

RE131D1-20190910


Tot Ion: 82 Resp: 10569

Ion Ratio Lower Upper

82 100

128 29.3 27.9 41.9




54 44.6 30.9 46.3

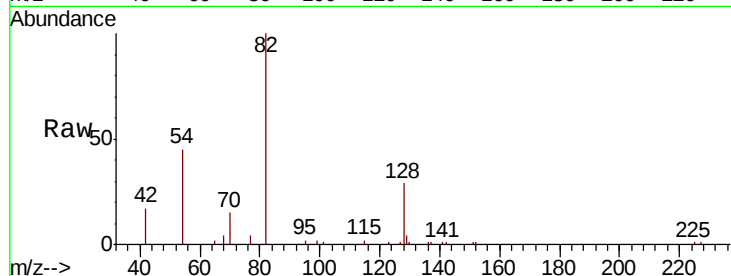

Abundance Ion 82.00 (81.70 to 82.70): BN007603.D (-721) (-)

Ion 128.00 (127.70 to 128.70): BN007603.D (-721) (-)

Ion 54.00 (53.70 to 54.70): BN007603.D (-721) (-)

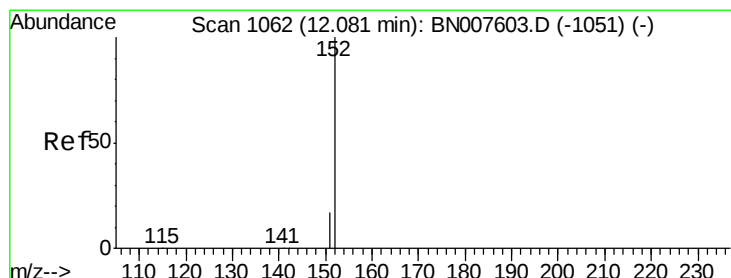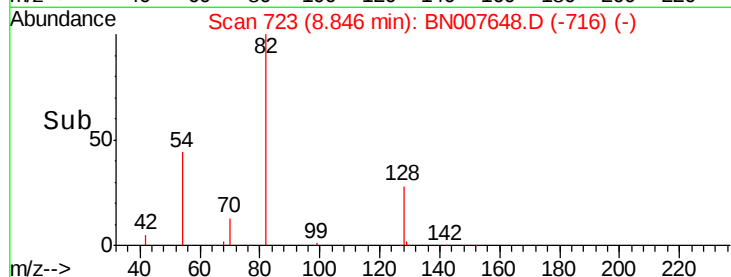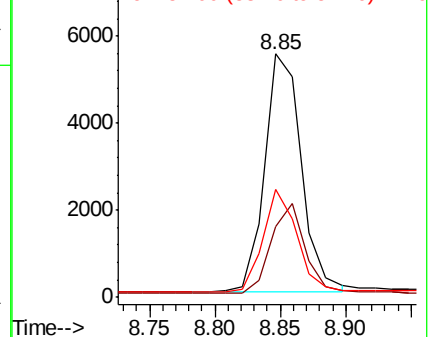

#11

2-Methylnaphthalene-d10

Concen: 0.407 ng

RT: 12.07 min Scan# 1060

Delta R.T. -0.01 min

Lab File: BN007648.D


Acq: 14 Sep 2019 04:58

Tgt Ion: 152 Resp: 24442

Ion Ratio Lower Upper



152 100


151 19.0 15.3 22.9

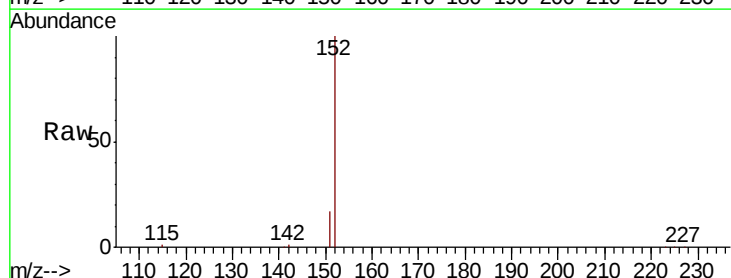

Abundance Ion 152.00 (151.70 to 152.70): BN007603.D (-1051) (-)

Ion 151.00 (150.70 to 151.70): BN007603.D (-1051) (-)

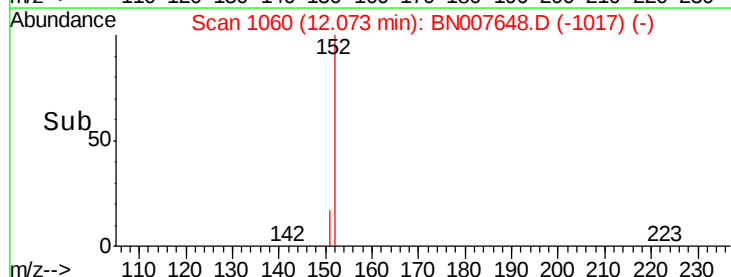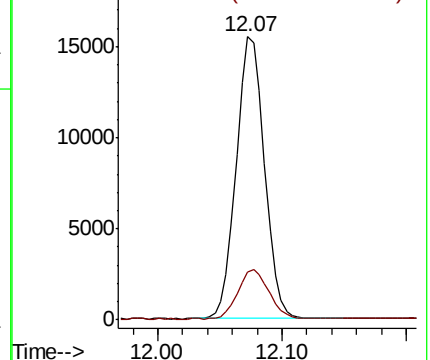

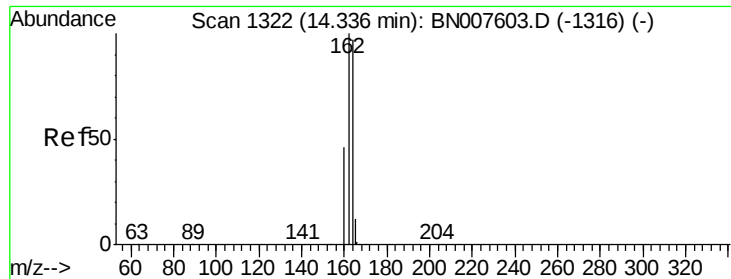

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.33 min Scan# 1321

Delta R.T. -0.00 min

Lab File: BN007648.D

Acq: 14 Sep 2019 04:58

Instrument :

BNA_N

ClientSampleId :

RE131D1-20190910


Tot Ion:164 Resp: 19662

Ion Ratio Lower Upper

164 100

162 102.0 82.8 124.2




160 46.8 38.0 57.0

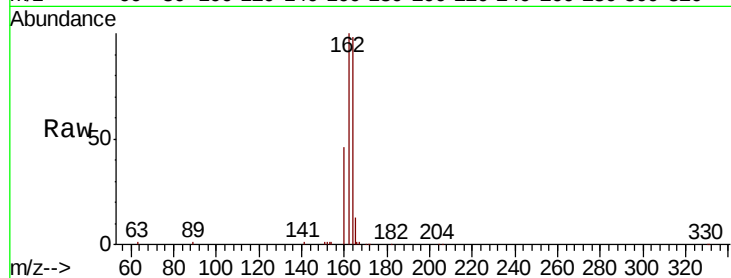

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

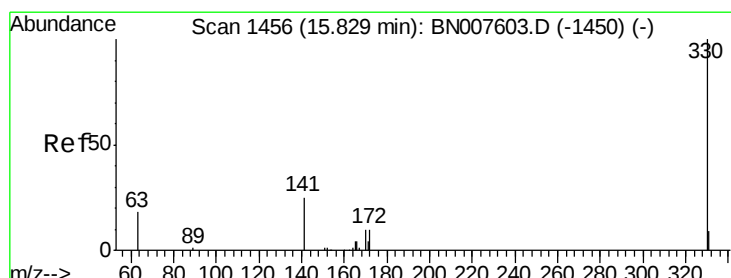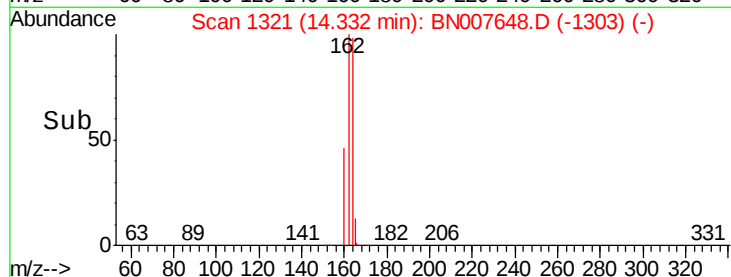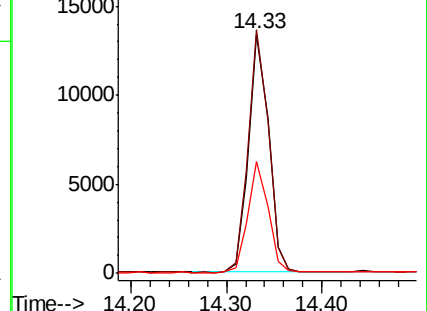

#14

2,4,6-Tribromophenol

Concen: 0.316 ng

RT: 15.83 min Scan# 1455

Delta R.T. -0.00 min

Lab File: BN007648.D

Acq: 14 Sep 2019 04:58


Tgt Ion:330 Resp: 2352

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0



141 41.5 30.1 45.1

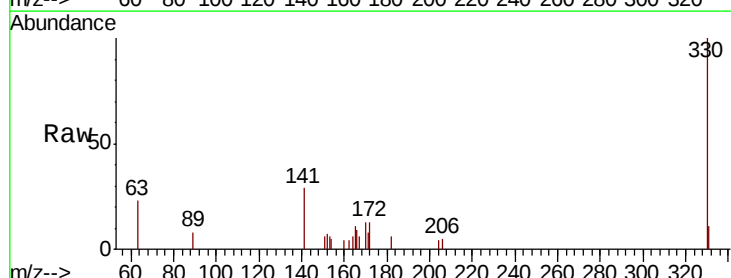


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



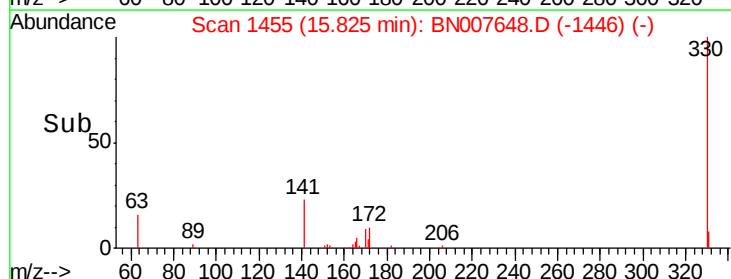
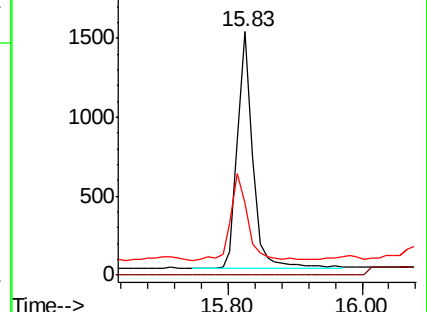


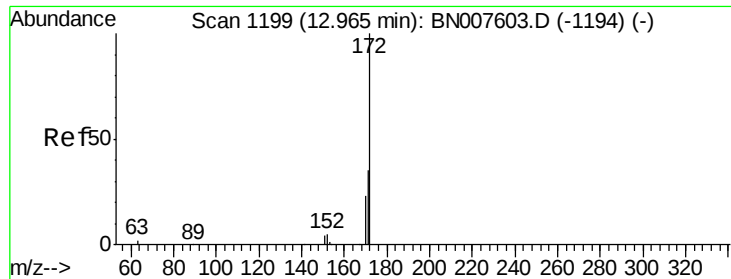

#15
2-Fluorobiphenyl
Concen: 0.441 ng
RT: 12.96 min Scan# 1198
Delta R.T. -0.00 min
Lab File: BN007648.D
Acq: 14 Sep 2019 04:58




Instrument :
BNA_N
ClientSampleId :
RE131D1-20190910


Tot Ion:172 Resp: 37853
Ion Ratio Lower Upper
172 100
171 33.9 27.9 41.9
170 22.0 18.5 27.7

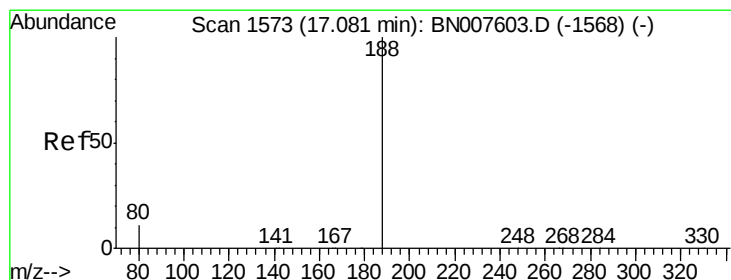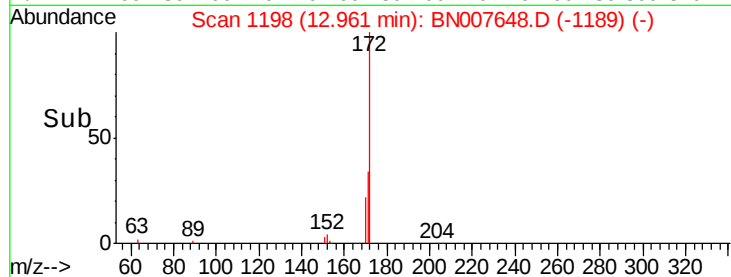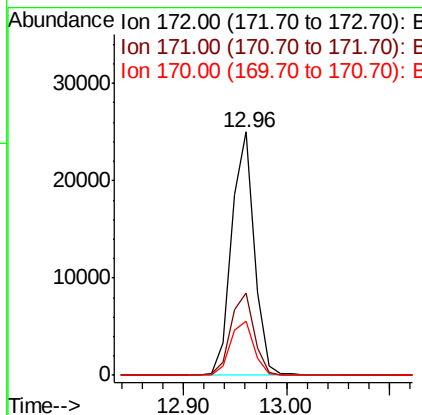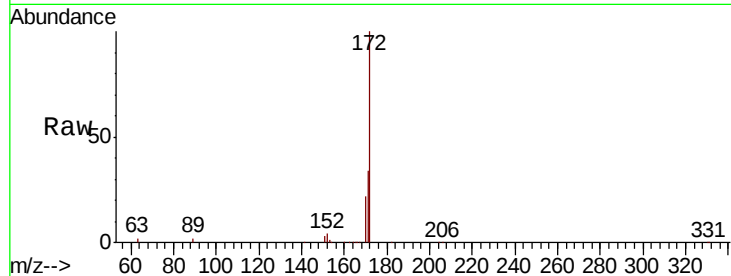

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.08 min Scan# 1572
Delta R.T. -0.00 min
Lab File: BN007648.D
Acq: 14 Sep 2019 04:58

Tgt Ion:188 Resp: 40842
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.3 8.8 13.2

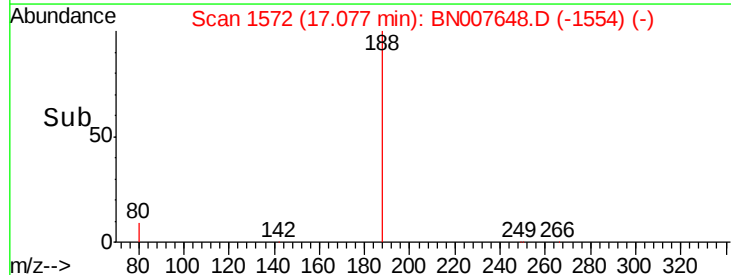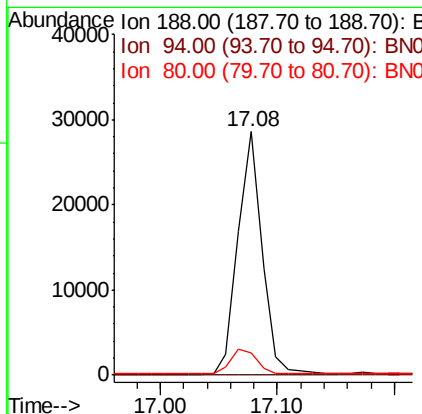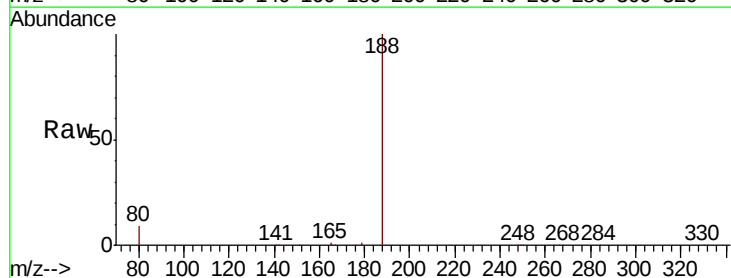

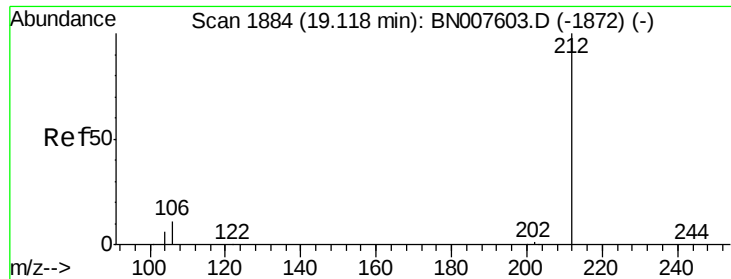

#25

Fluoranthene-d10

Concen: 0.443 ng

RT: 19.11 min Scan# 1881

Delta R.T. -0.01 min

Lab File: BN007648.D

Acq: 14 Sep 2019 04:58

Instrument :

BNA_N

ClientSampleId :

RE131D1-20190910


Tot Ion:212 Resp: 57076

Ion Ratio Lower Upper

212 100

106 12.4 9.6 14.4




104 7.0 5.4 8.0

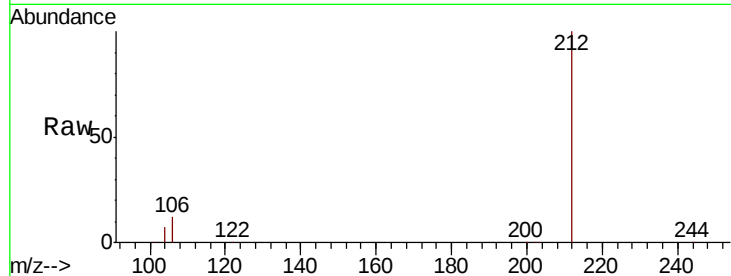

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

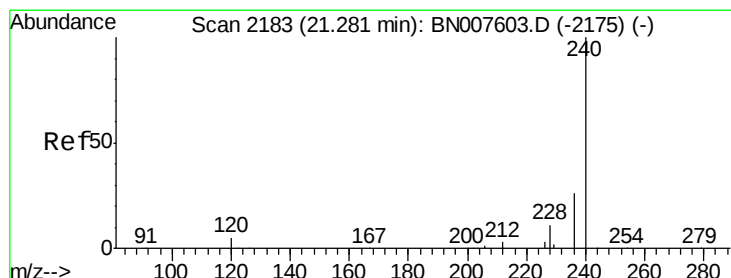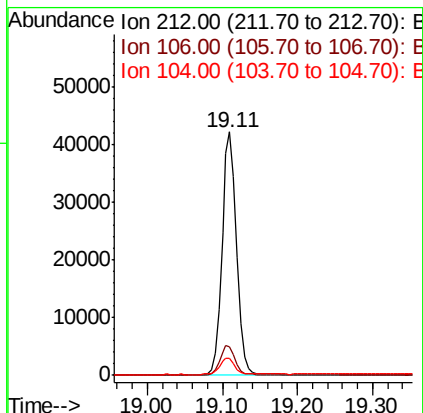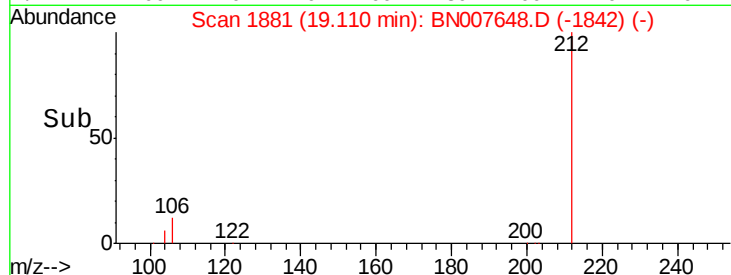

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.26 min Scan# 2180

Delta R.T. -0.02 min

Lab File: BN007648.D

Acq: 14 Sep 2019 04:58


Tgt Ion:240 Resp: 41006

Ion Ratio Lower Upper

240 100

120 13.9 4.3 6.5#



236 26.8 20.8 31.2

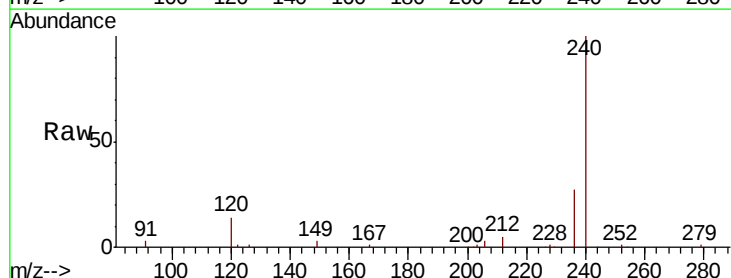


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

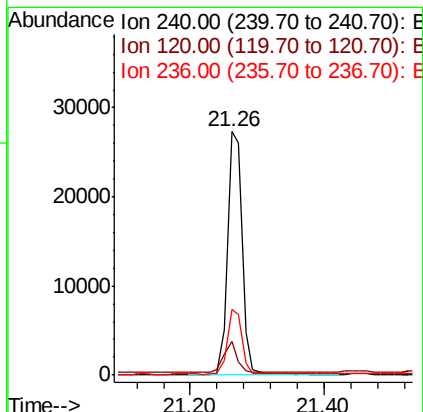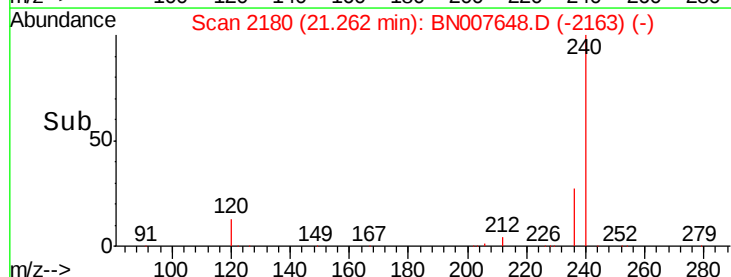

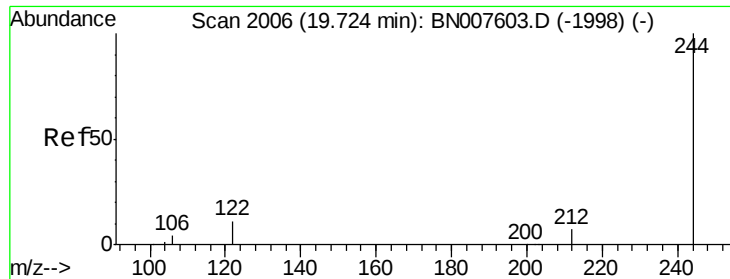

#29

Terphenyl-d14

Concen: 0.518 ng

RT: 19.72 min Scan# 2003

Delta R.T. -0.01 min

Lab File: BN007648.D

Acq: 14 Sep 2019 04:58

Instrument :

BNA_N

ClientSampleId :

RE131D1-20190910


Tot Ion:244 Resp: 56001

Ion Ratio Lower Upper

244 100

212 7.4 5.9 8.9




122 10.0 8.6 12.8

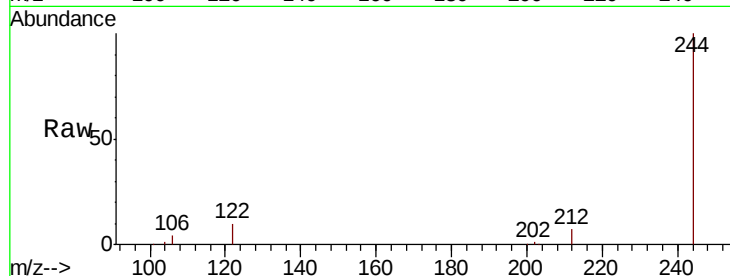

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

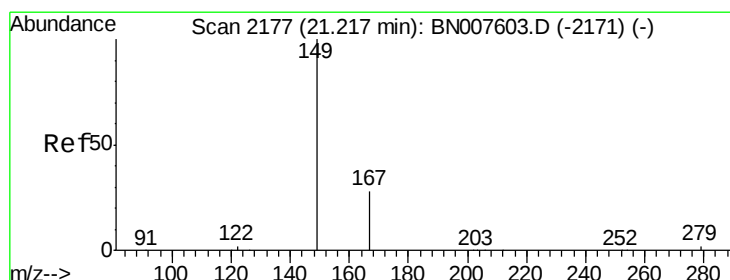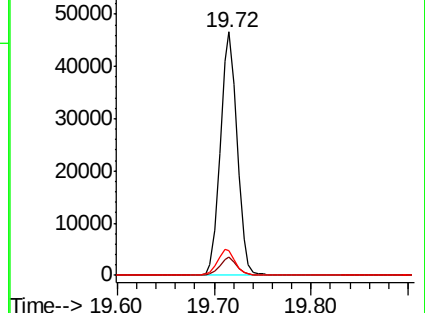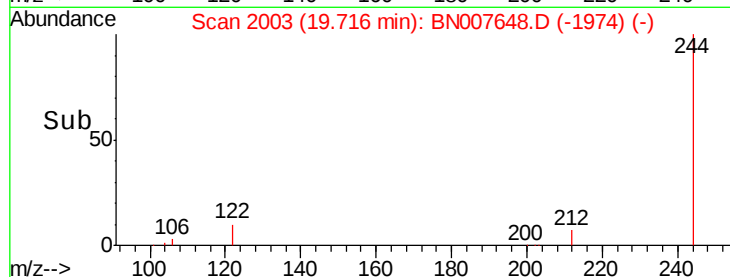

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.131 ng

RT: 21.20 min Scan# 2174

Delta R.T. -0.02 min

Lab File: BN007648.D

Acq: 14 Sep 2019 04:58


Tgt Ion:149 Resp: 6456

Ion Ratio Lower Upper

149 100

167 29.3 22.6 34.0



279 4.7 3.8 5.6



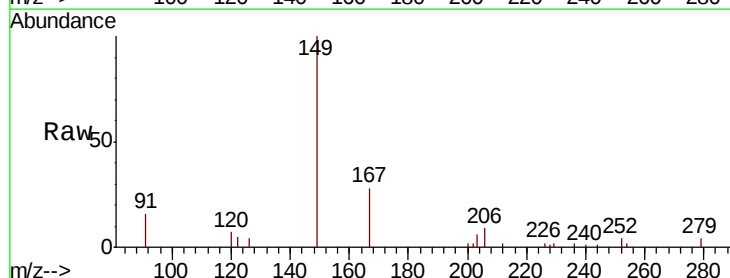


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

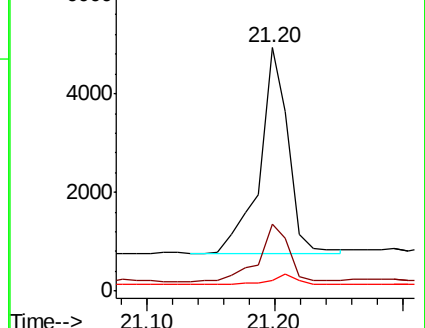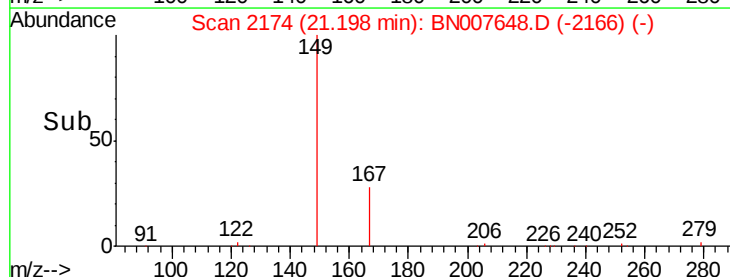

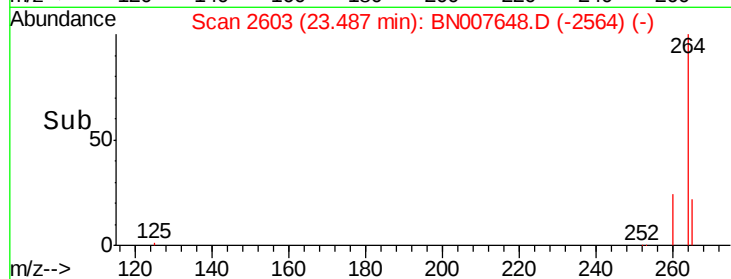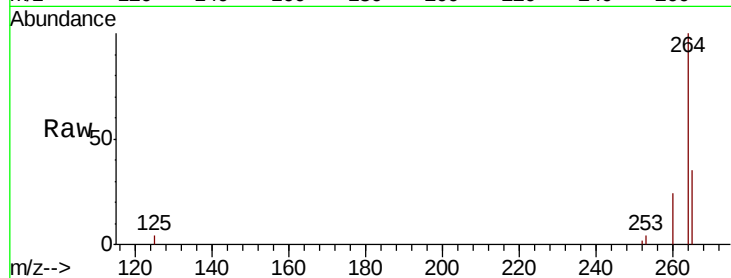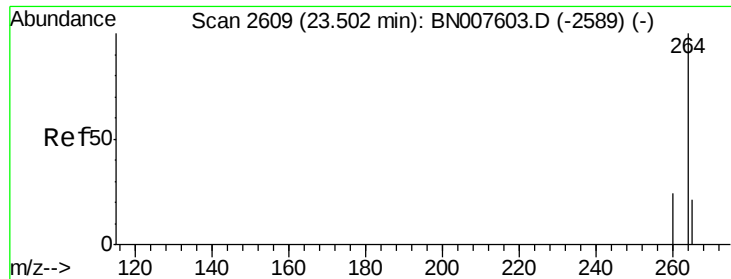

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.49 min Scan# 2603

Delta R.T. -0.02 min

Lab File: BN007648.D

Acq: 14 Sep 2019 04:58

Instrument :

BNA_N

ClientSampleId :

RE131D1-20190910

Tot Ion:264 Resp: 42055

Ion Ratio Lower Upper

264 100

260 23.9 19.1 28.7

265 35.1 24.6 37.0

