

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091319\
 Data File : BN007621.D
 Acq On : 13 Sep 2019 11:39
 Operator : HP/JU
 Sample : K4858-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE103D1-20190909

Quant Time: Sep 14 02:59:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 12 14:27:51 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	9170	0.40	ng	0.00
7) Naphthalene-d8	10.48	136	36607	0.40	ng	-0.01
13) Acenaphthene-d10	14.34	164	19555	0.40	ng	0.00
19) Phenanthrene-d10	17.08	188	43667	0.40	ng	0.00
27) Chrysene-d12	21.28	240	42910	0.40	ng	0.00
34) Perylene-d12	23.50	264	45393	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.34	112	3512	0.12	ng	0.00
5) Phenol-d6	6.89	99	2820	0.09	ng	0.00
8) Nitrobenzene-d5	8.86	82	8781	0.30	ng	0.00
11) 2-Methylnaphthalene-d10	12.08	152	20002	0.32	ng	0.00
14) 2,4,6-Tribromophenol	15.83	330	1957	0.26	ng	0.00
15) 2-Fluorobiphenyl	12.97	172	31657	0.37	ng	0.00
25) Fluoranthene-d10	19.11	212	46017	0.33	ng	0.00
29) Terphenyl-d14	19.72	244	40092	0.35	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.31	88	66568	6.058	ng	Qvalue 89
3) n-Nitrosodimethylamine	3.03	42	172987	34.695	ng	# 1
6) bis(2-Chloroethyl)ether	7.16	93	631	0.023	ng	# 58
32) Bis(2-ethylhexyl)phthalate	21.22	149	6522	0.126	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091319\
Data File : BN007621.D
Acq On : 13 Sep 2019 11:39
Operator : HP/JU
Sample : K4858-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE103D1-20190909

Quant Time: Sep 14 02:59:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 12 14:27:51 2019
Response via : Initial Calibration

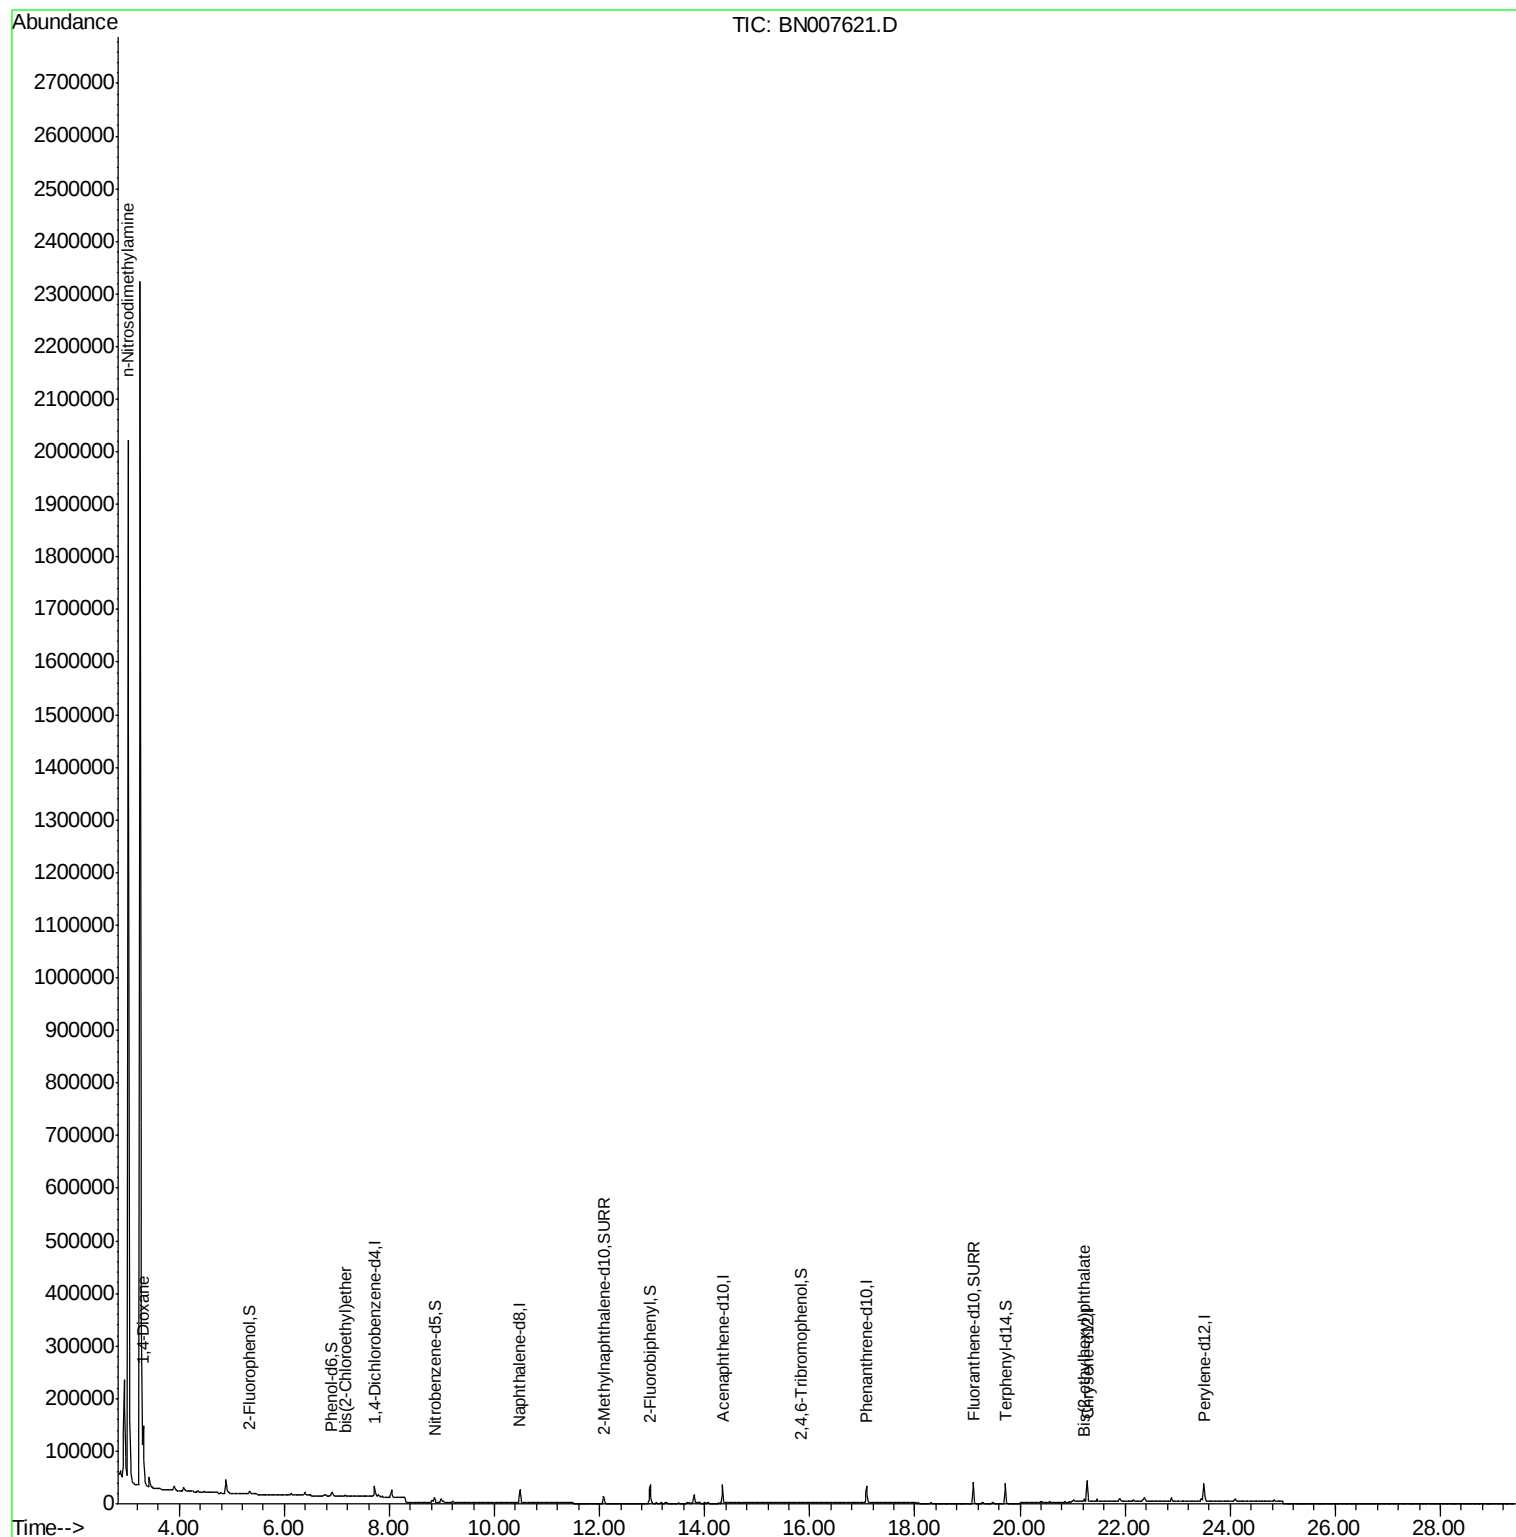

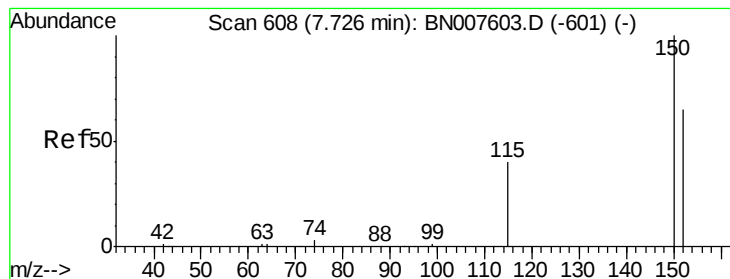


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.72 min Scan# 607
Delta R.T. -0.01 min
Lab File: BN007621.D
Acq: 13 Sep 2019 11:39

Instrument :
BNA_N
ClientSampleId :
RE103D1-20190909

Tot Ion:152 Resp: 9170
Ion Ratio Lower Upper
152 100
150 157.0 122.4 183.6
115 65.5 50.4 75.6




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

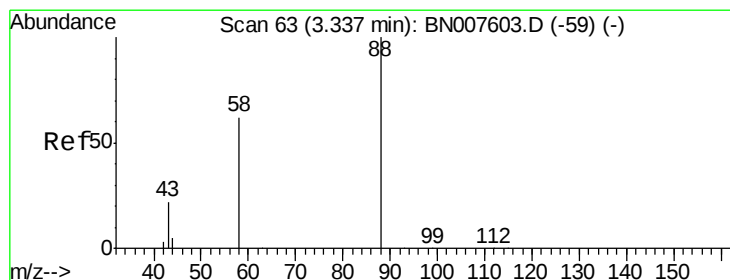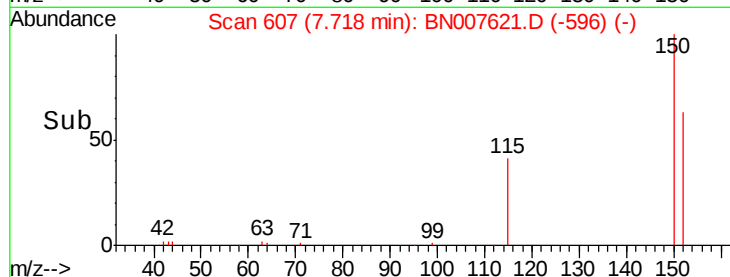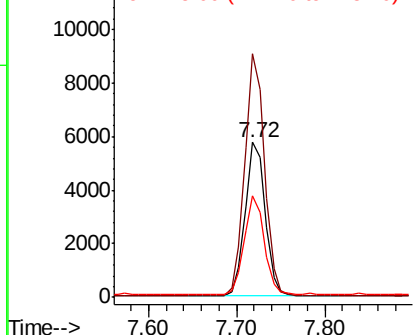



#2

1,4-Dioxane
Concen: 6.058 ng
RT: 3.31 min Scan# 60
Delta R.T. -0.02 min
Lab File: BN007621.D
Acq: 13 Sep 2019 11:39

Tgt Ion: 88 Resp: 66568
Ion Ratio Lower Upper
88 100
58 60.6 57.0 85.4
43 21.4 20.0 30.0



Abundance Ion 88.00 (87.70 to 88.70): BNC
Ion 58.00 (57.70 to 58.70): BNC
Ion 43.00 (42.70 to 43.70): BNC

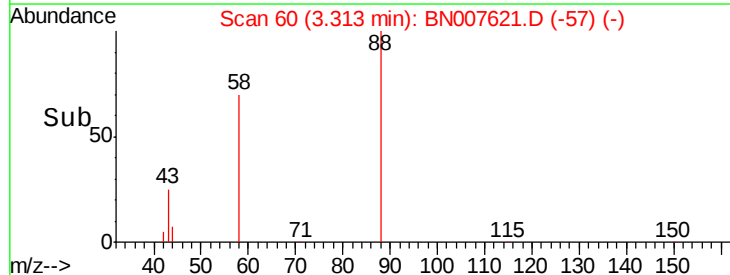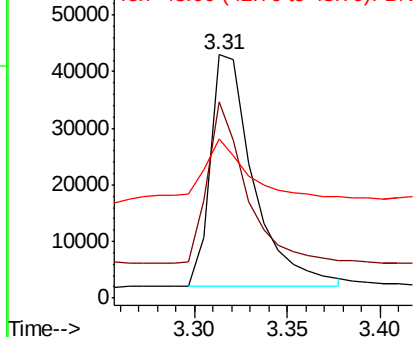



#3

n-Nitrosodimethylamine

Concen: 34.695 ng

RT: 3.03 min Scan# 25

Delta R.T. -0.01 min

Lab File: BN007621.D

Acq: 13 Sep 2019 11:39

Instrument :

BNA_N

ClientSampleId :

RE103D1-20190909


Tot Ion: 42 Resp: 172987

Ion Ratio Lower Upper

42 100

74 144.2 9.8 14.8#

44 26.5 0.0 0.0#



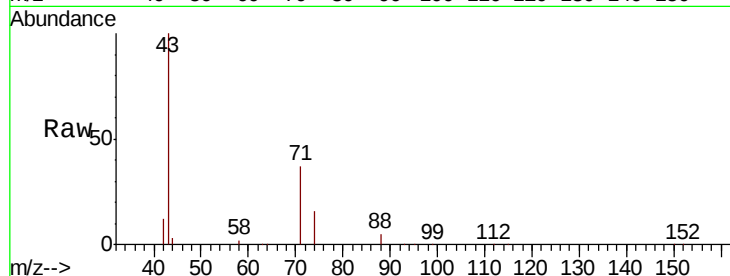


Abundance Ion 42.00 (41.70 to 42.70): BN007603.D (-24) (-)

Ion 74.00 (73.70 to 74.70): BN007603.D (-24) (-)

Ion 44.00 (43.70 to 44.70): BN007603.D (-24) (-)

Time-->

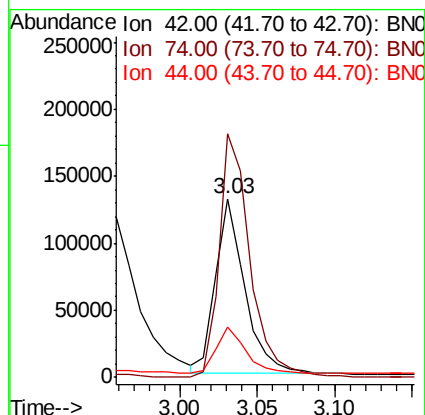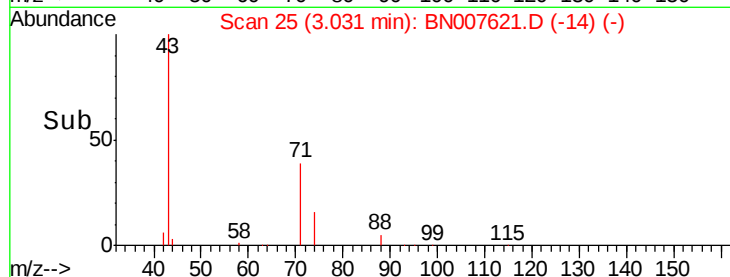

#4

2-Fluorophenol

Concen: 0.120 ng

RT: 5.34 min Scan# 312

Delta R.T. -0.00 min

Lab File: BN007621.D

Acq: 13 Sep 2019 11:39


Tgt Ion: 112 Resp: 3512

Ion Ratio Lower Upper

112 100

64 59.6 48.5 72.7

63 30.4 24.4 36.6






Abundance Ion 112.00 (111.70 to 112.70): BN007603.D (-306) (-)

Ion 64.00 (63.70 to 64.70): BN007603.D (-306) (-)

Ion 63.00 (62.70 to 63.70): BN007603.D (-306) (-)

Time-->

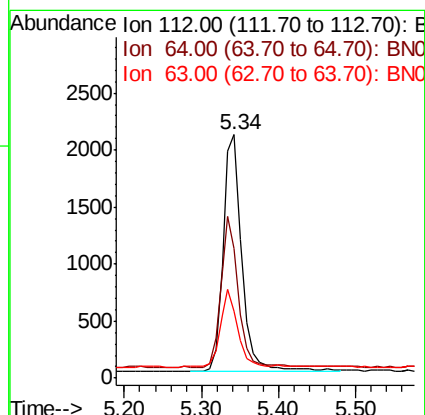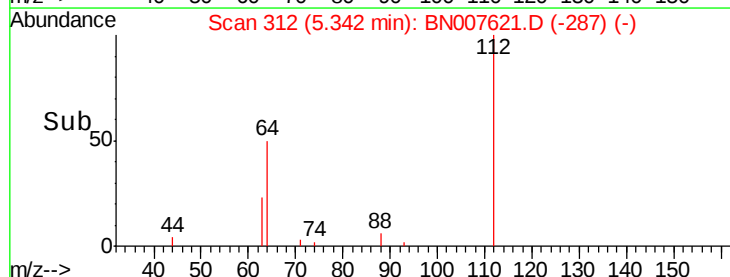

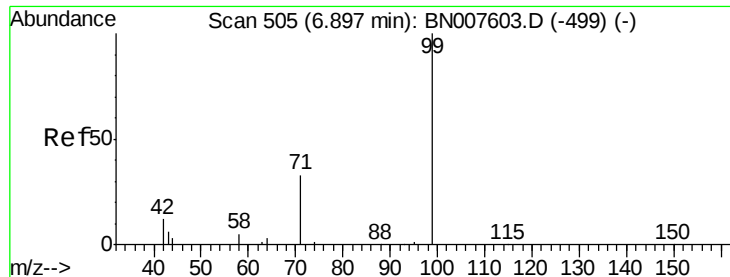

#5

Phenol-d6

Concen: 0.085 ng

RT: 6.89 min Scan# 504

Delta R.T. -0.01 min

Lab File: BN007621.D

Acq: 13 Sep 2019 11:39

Instrument :

BNA_N

ClientSampleId :

RE103D1-20190909


Tot Ion: 99 Resp: 2820

Ion Ratio Lower Upper

99 100

42 0.0 11.8 17.6#




71 41.5 28.0 42.0



Abundance Ion 99.00 (98.70 to 99.70): BNC

Ion 42.00 (41.70 to 42.70): BNC

Ion 71.00 (70.70 to 71.70): BNC

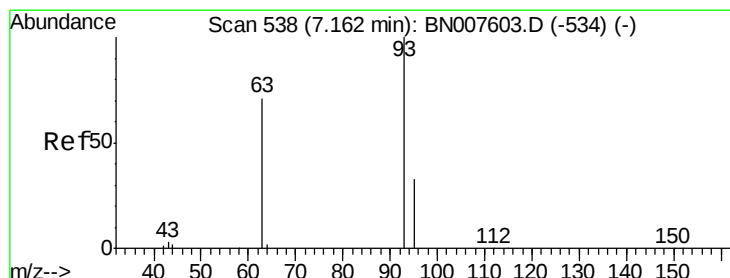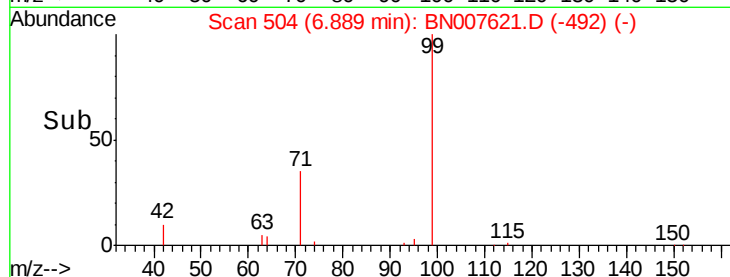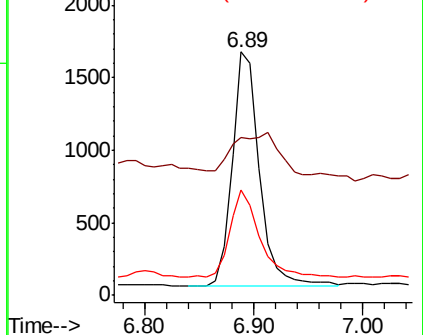

#6

bis(2-Chloroethyl)ether

Concen: 0.023 ng

RT: 7.16 min Scan# 538

Delta R.T. -0.00 min

Lab File: BN007621.D

Acq: 13 Sep 2019 11:39


Tgt Ion: 93 Resp: 631

Ion Ratio Lower Upper

93 100

63 119.2 61.2 91.8#



95 48.3 27.2 40.8#




Abundance Ion 93.00 (92.70 to 93.70): BNC

Ion 63.00 (62.70 to 63.70): BNC

Ion 95.00 (94.70 to 95.70): BNC

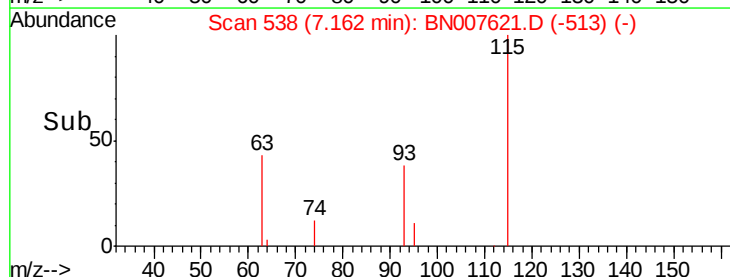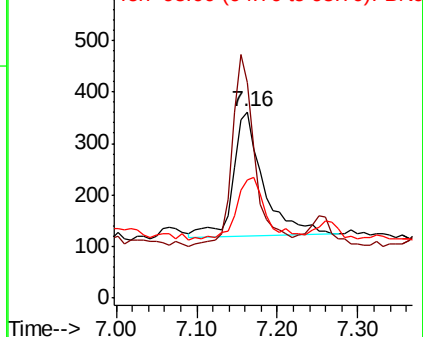

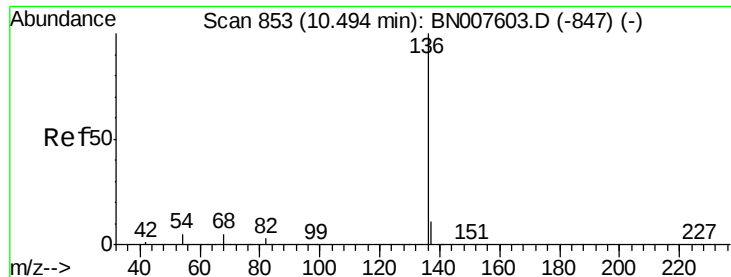

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.48 min Scan# 852

Delta R.T. -0.01 min

Lab File: BN007621.D

Acq: 13 Sep 2019 11:39

Instrument :

BNA_N

ClientSampleId :

RE103D1-20190909

Tot Ion:136 Resp: 36607


Ion Ratio Lower Upper

136 100

137 11.3 8.8 13.2

54 8.9 4.2 6.4#

68 9.3 4.6 7.0#



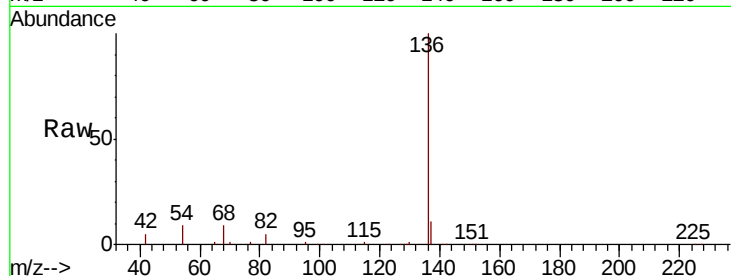


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

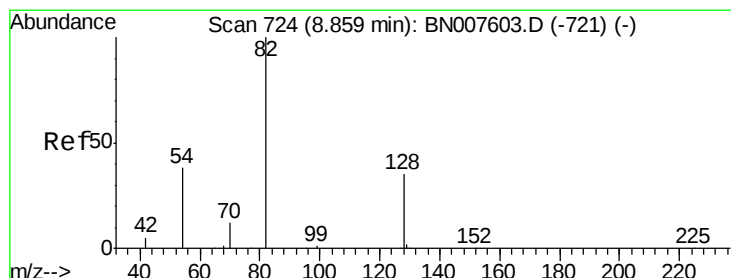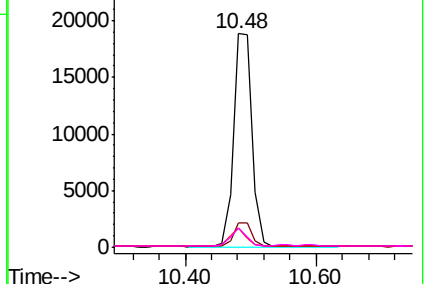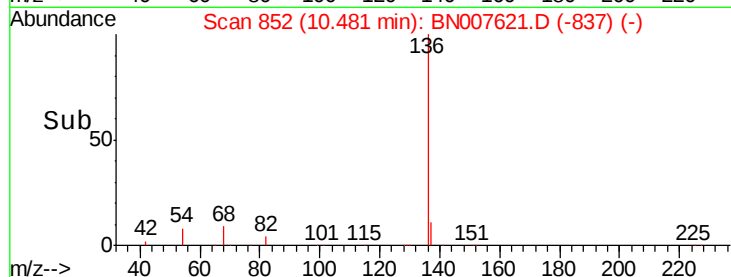

#8

Nitrobenzene-d5

Concen: 0.301 ng

RT: 8.86 min Scan# 724

Delta R.T. -0.00 min

Lab File: BN007621.D

Acq: 13 Sep 2019 11:39


Tgt Ion: 82 Resp: 8781

Ion Ratio Lower Upper

82 100

128 38.6 27.9 41.9



54 37.6 30.9 46.3

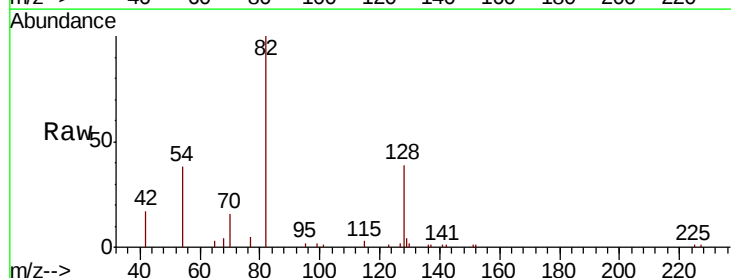


Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC



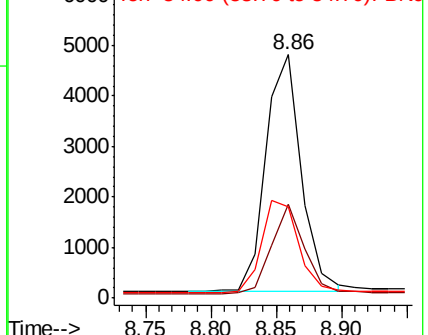
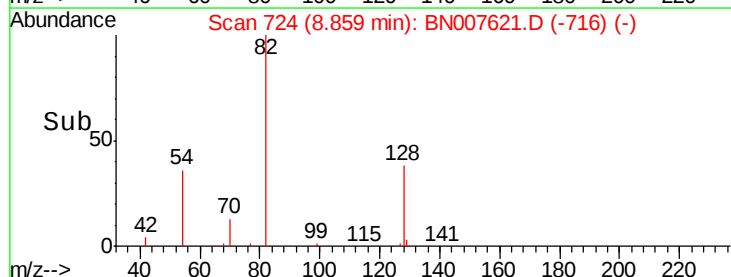


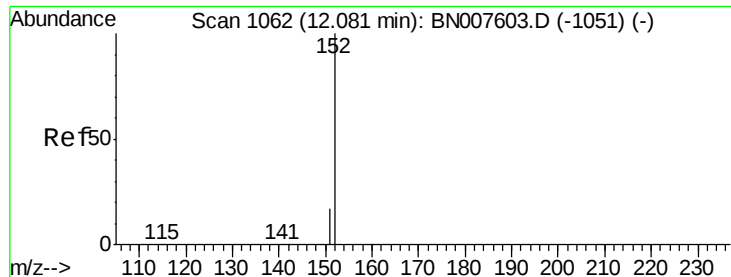

#11
2-Methylnaphthalene-d10
Concen: 0.323 ng
RT: 12.08 min Scan# 1062
Delta R.T. -0.00 min
Lab File: BN007621.D
Acq: 13 Sep 2019 11:39




Instrument :
BNA_N
ClientSampleId :
RE103D1-20190909


Tot Ion:152 Resp: 20002
Ion Ratio Lower Upper
152 100
151 19.3 15.3 22.9

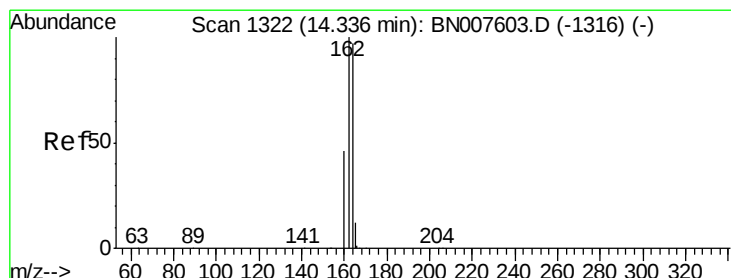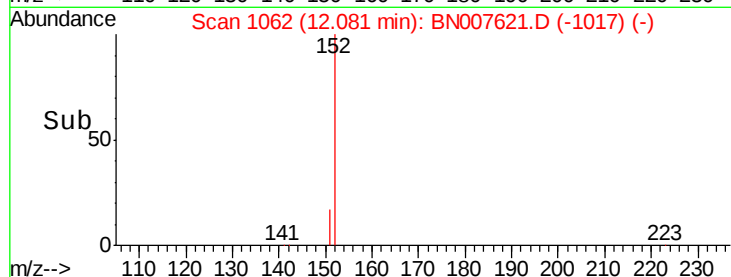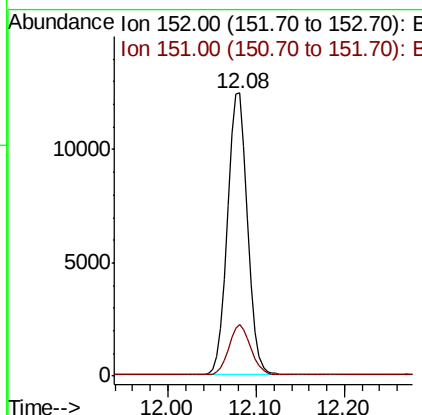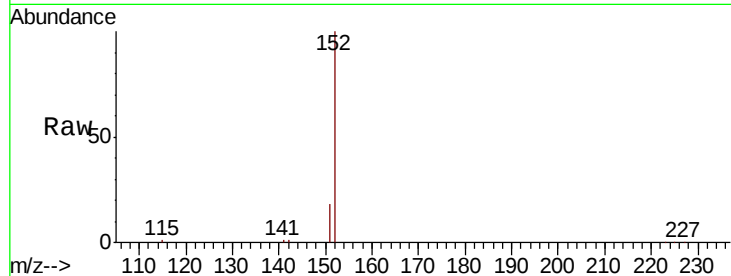

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.34 min Scan# 1322
Delta R.T. -0.00 min
Lab File: BN007621.D
Acq: 13 Sep 2019 11:39

Tgt Ion:164 Resp: 19555
Ion Ratio Lower Upper
164 100
162 102.0 82.8 124.2
160 47.4 38.0 57.0


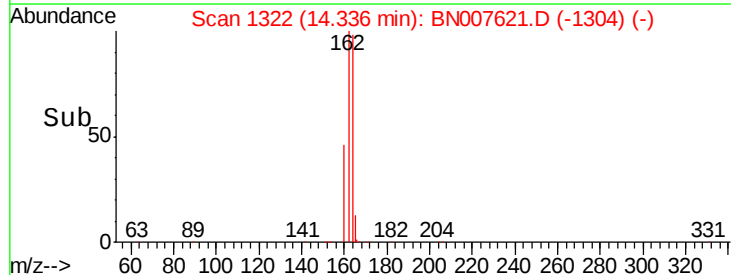
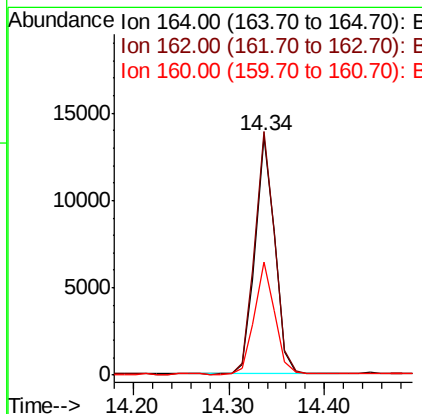
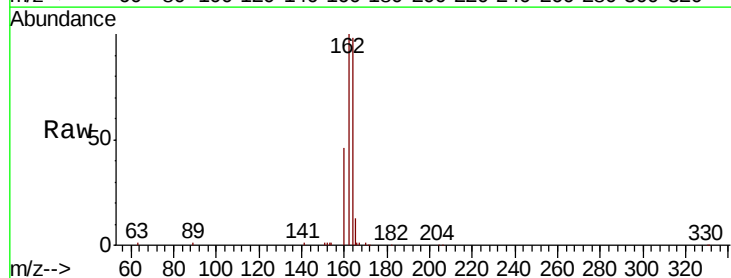


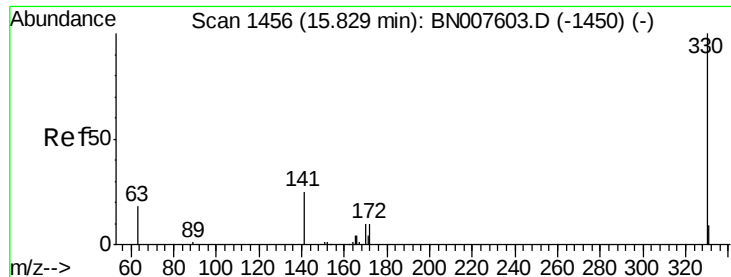

#14
 2,4,6-Tribromophenol
 Concen: 0.265 ng
 RT: 15.83 min Scan# 1456
 Delta R.T. -0.00 min
 Lab File: BN007621.D
 Acq: 13 Sep 2019 11:39




Instrument :
 BNA_N
 ClientSampleId :
 RE103D1-20190909


Tot Ion:330 Resp: 1957
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 37.6 30.1 45.1

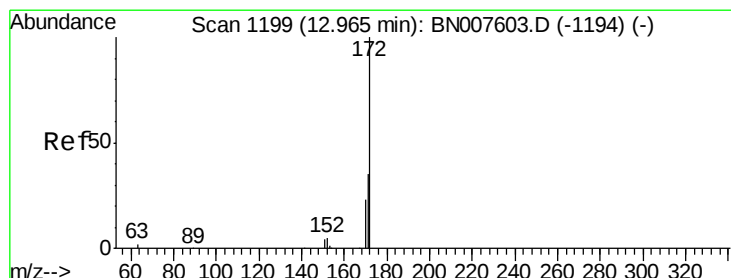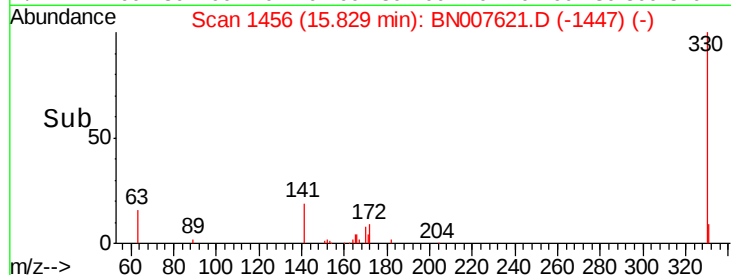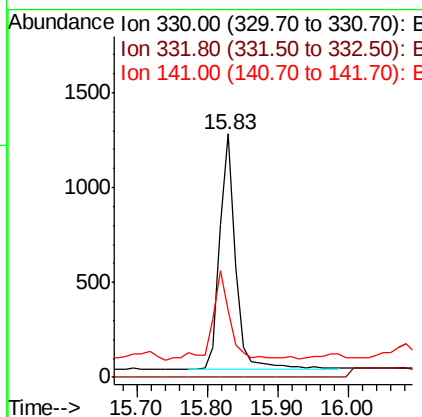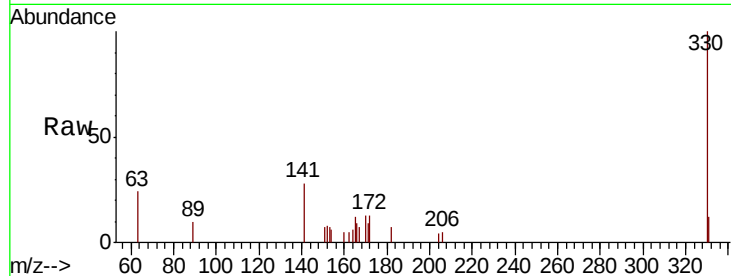

#15
 2-Fluorobiphenyl
 Concen: 0.371 ng
 RT: 12.97 min Scan# 1199
 Delta R.T. -0.00 min
 Lab File: BN007621.D
 Acq: 13 Sep 2019 11:39

Tgt Ion:172 Resp: 31657
 Ion Ratio Lower Upper
 172 100
 171 34.4 27.9 41.9
 170 22.0 18.5 27.7

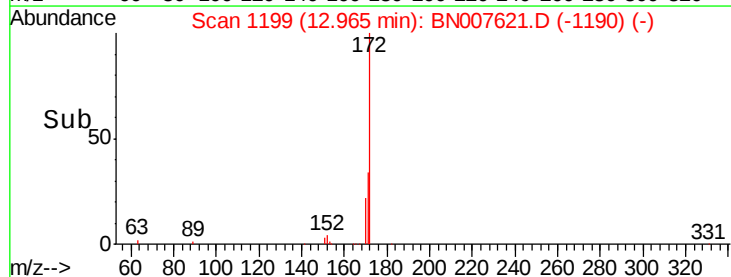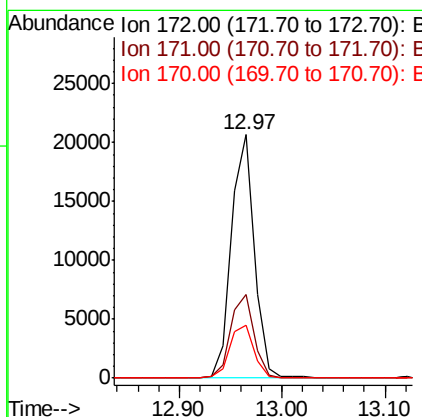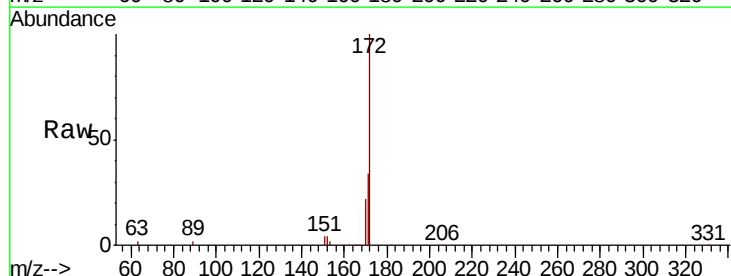

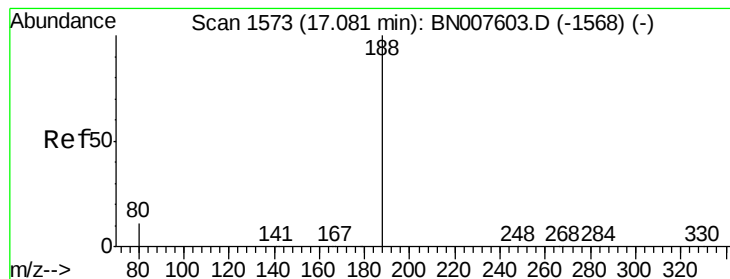

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.08 min Scan# 1573

Delta R.T. -0.00 min

Lab File: BN007621.D

Acq: 13 Sep 2019 11:39

Instrument :

BNA_N

ClientSampleId :

RE103D1-20190909


Tot Ion:188 Resp: 43667

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 9.8 8.8 13.2



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

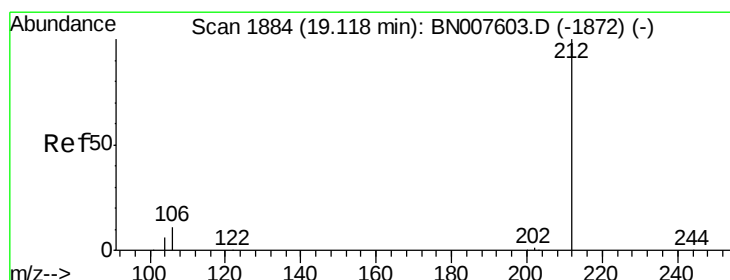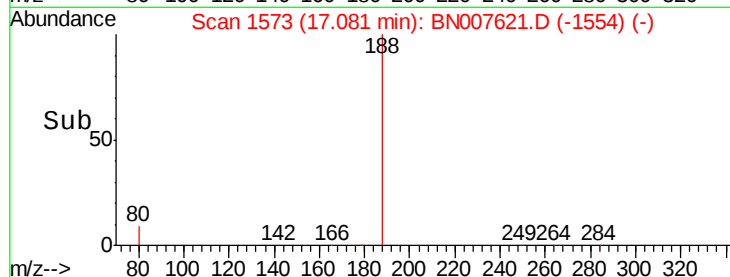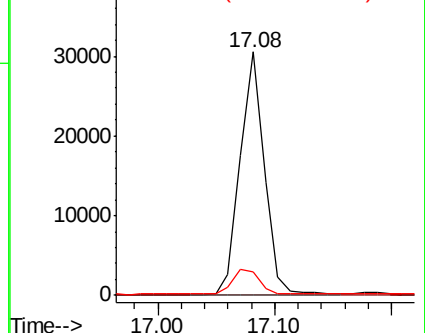

#25

Fluoranthene-d10

Concen: 0.334 ng

RT: 19.11 min Scan# 1883

Delta R.T. -0.00 min

Lab File: BN007621.D

Acq: 13 Sep 2019 11:39


Tgt Ion:212 Resp: 46017

Ion Ratio Lower Upper

212 100

106 12.2 9.6 14.4



104 6.8 5.4 8.0




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

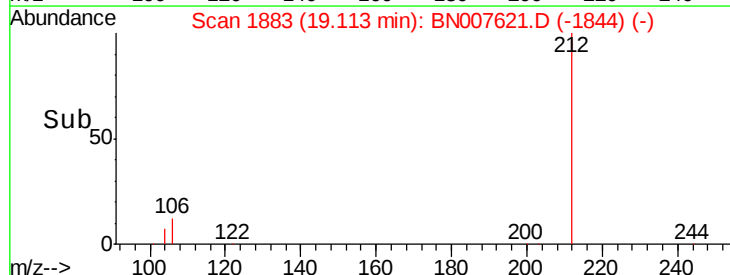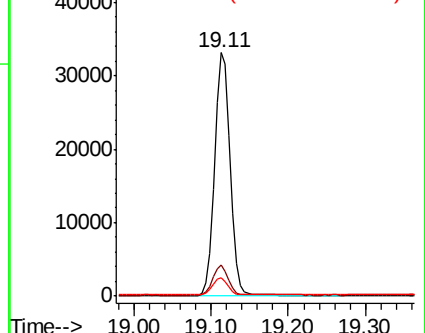

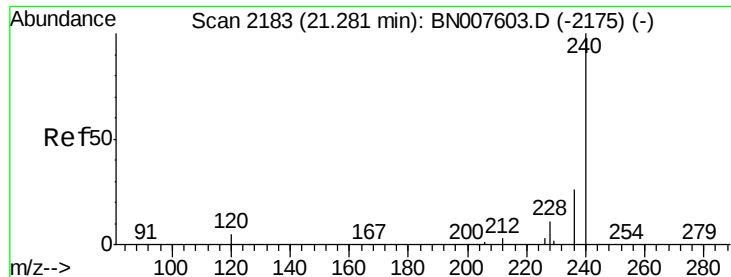

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.28 min Scan# 2183

Delta R.T. -0.00 min

Lab File: BN007621.D

Acq: 13 Sep 2019 11:39

Instrument :

BNA_N

ClientSampleId :

RE103D1-20190909


Tot Ion:240 Resp: 42910

Ion Ratio Lower Upper

240 100

120 5.3 4.3 6.5

236 25.8 20.8 31.2



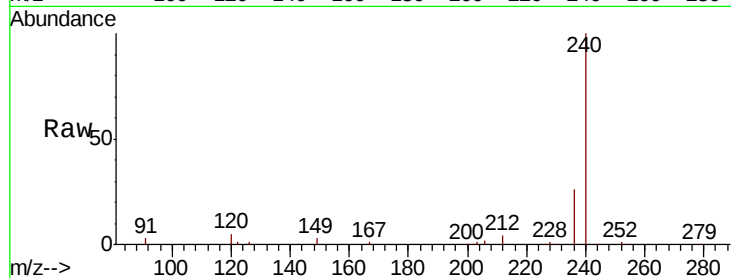


Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

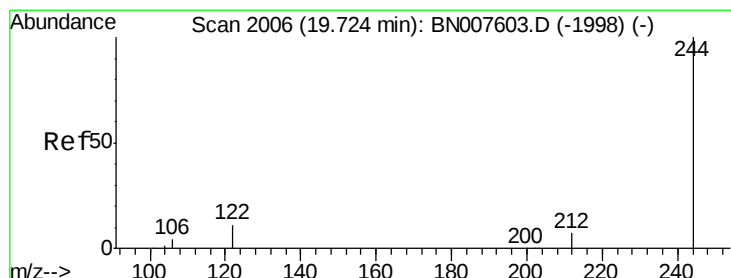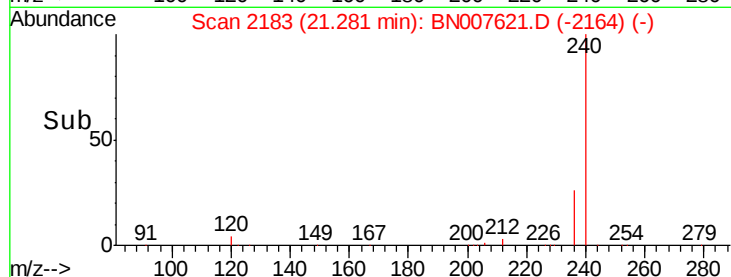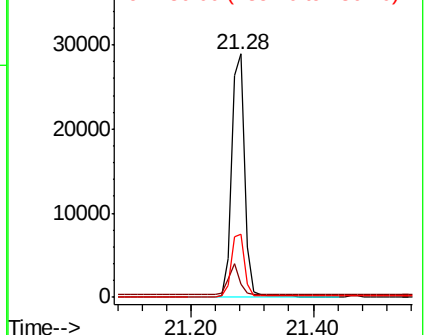

#29

Terphenyl-d14

Concen: 0.354 ng

RT: 19.72 min Scan# 2006

Delta R.T. -0.00 min

Lab File: BN007621.D

Acq: 13 Sep 2019 11:39


Tgt Ion:244 Resp: 40092

Ion Ratio Lower Upper

244 100

212 7.3 5.9 8.9

122 9.4 8.6 12.8


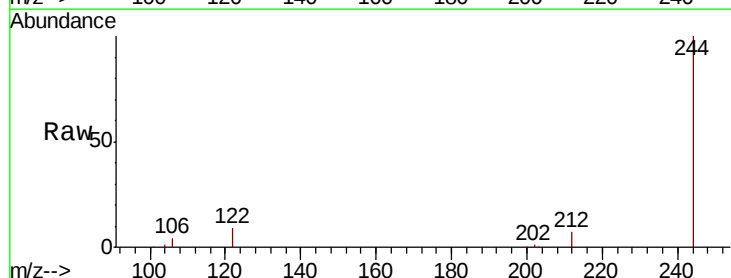



Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E



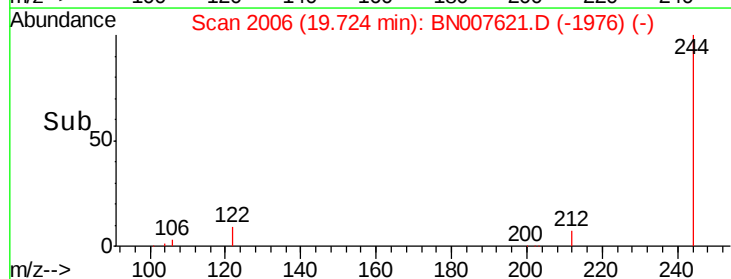
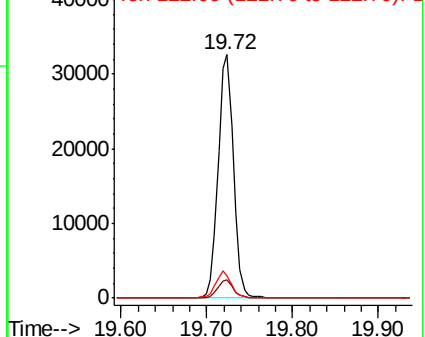


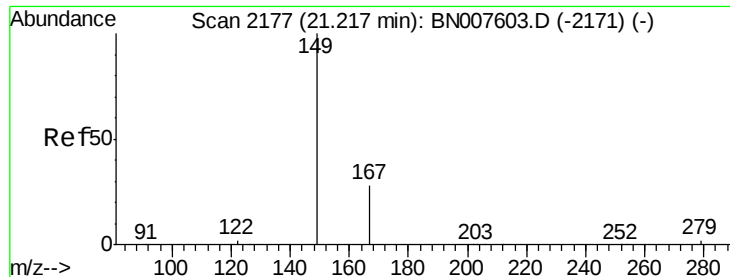

#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.126 ng
 RT: 21.22 min Scan# 2177
 Delta R.T. -0.00 min
 Lab File: BN007621.D
 Acq: 13 Sep 2019 11:39

Instrument :
 BNA_N
 ClientSampleId :
 RE103D1-20190909

Tot Ion:149 Resp: 6522
 Ion Ratio Lower Upper
 149 100
 167 29.3 22.6 34.0
 279 4.9 3.8 5.6

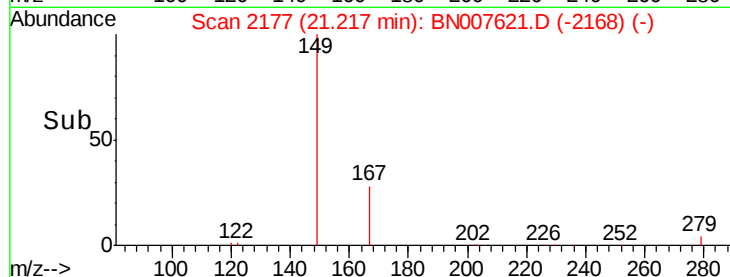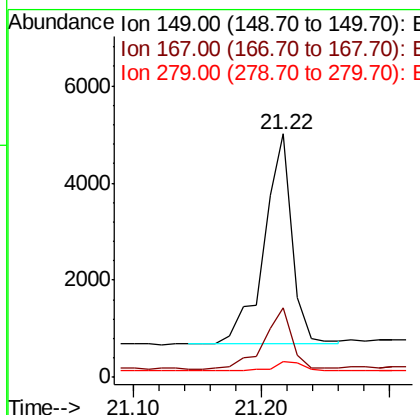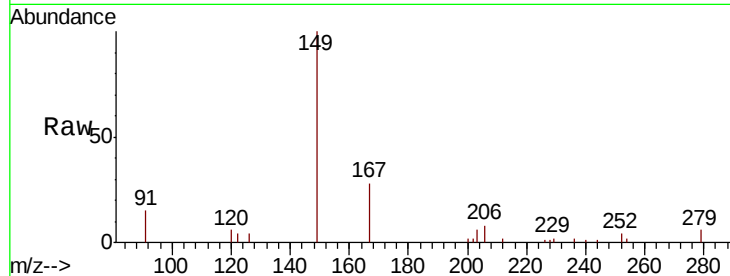

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.50 min Scan# 2608
 Delta R.T. -0.00 min
 Lab File: BN007621.D
 Acq: 13 Sep 2019 11:39

Tgt Ion:264 Resp: 45393
 Ion Ratio Lower Upper
 264 100
 260 24.2 19.1 28.7
 265 32.1 24.6 37.0

