


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091319\
 Data File : BN007614.D
 Acq On : 13 Sep 2019 07:29
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 12 14:27:51 2019

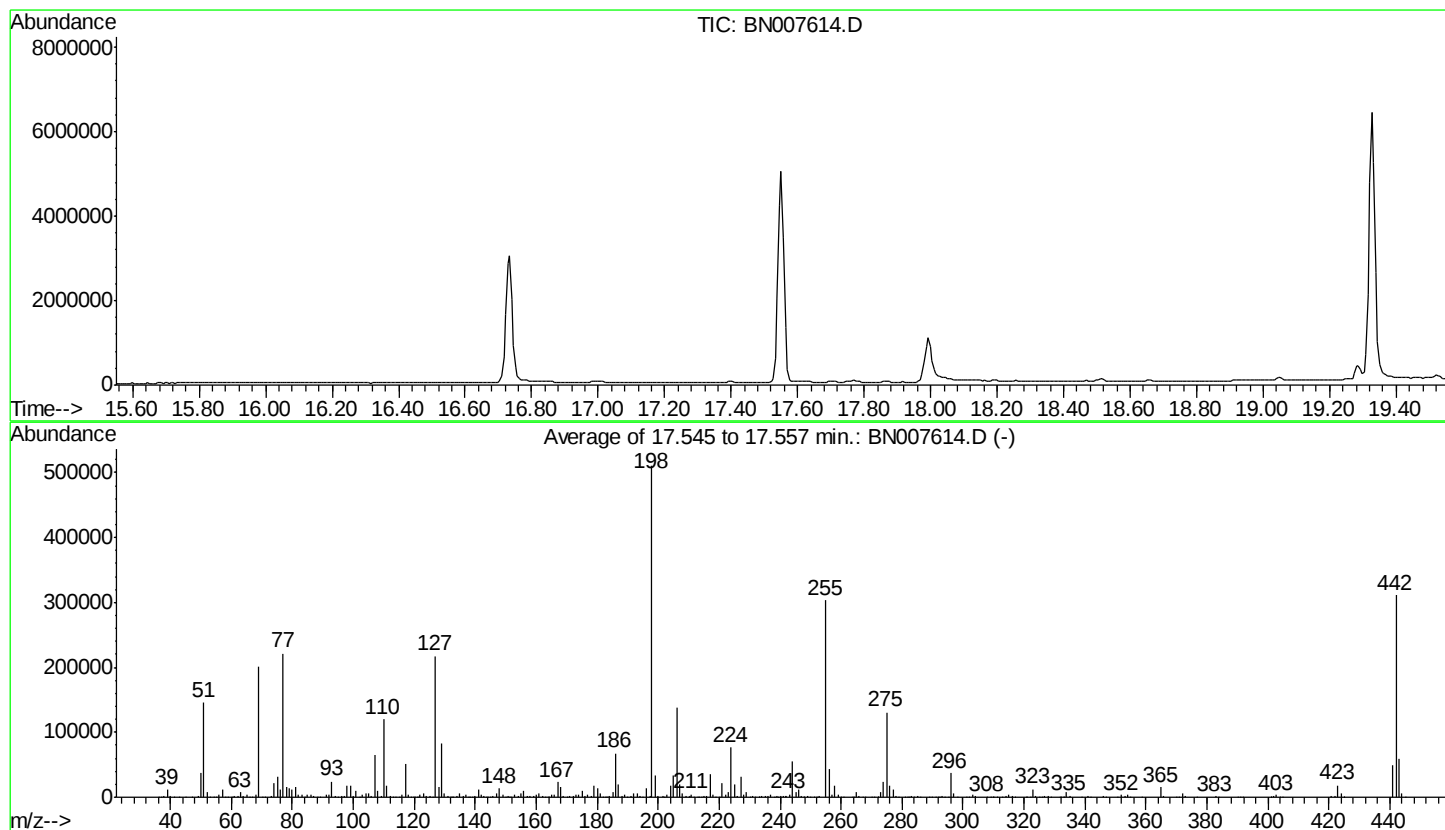

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.6	145912	PASS
68	69	0.00	2	1.6	3253	PASS
69	198	0.00	100	39.5	201673	PASS
70	69	0.00	2	0.5	977	PASS
127	198	10	80	42.6	217728	PASS
197	198	0.00	2	0.4	2087	PASS
198	198	100	100	100.0	510826	PASS
199	198	5	9	6.7	34056	PASS
275	198	10	60	25.6	130906	PASS
365	198	1	100	3.0	15123	PASS
441	198	0.01	100	9.7	49394	PASS
442	198	50	100	60.8	310784	PASS
443	442	15	24	19.1	59432	PASS