


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091319\
 Data File : BN007626.D
 Acq On : 13 Sep 2019 14:39
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 12 14:27:51 2019

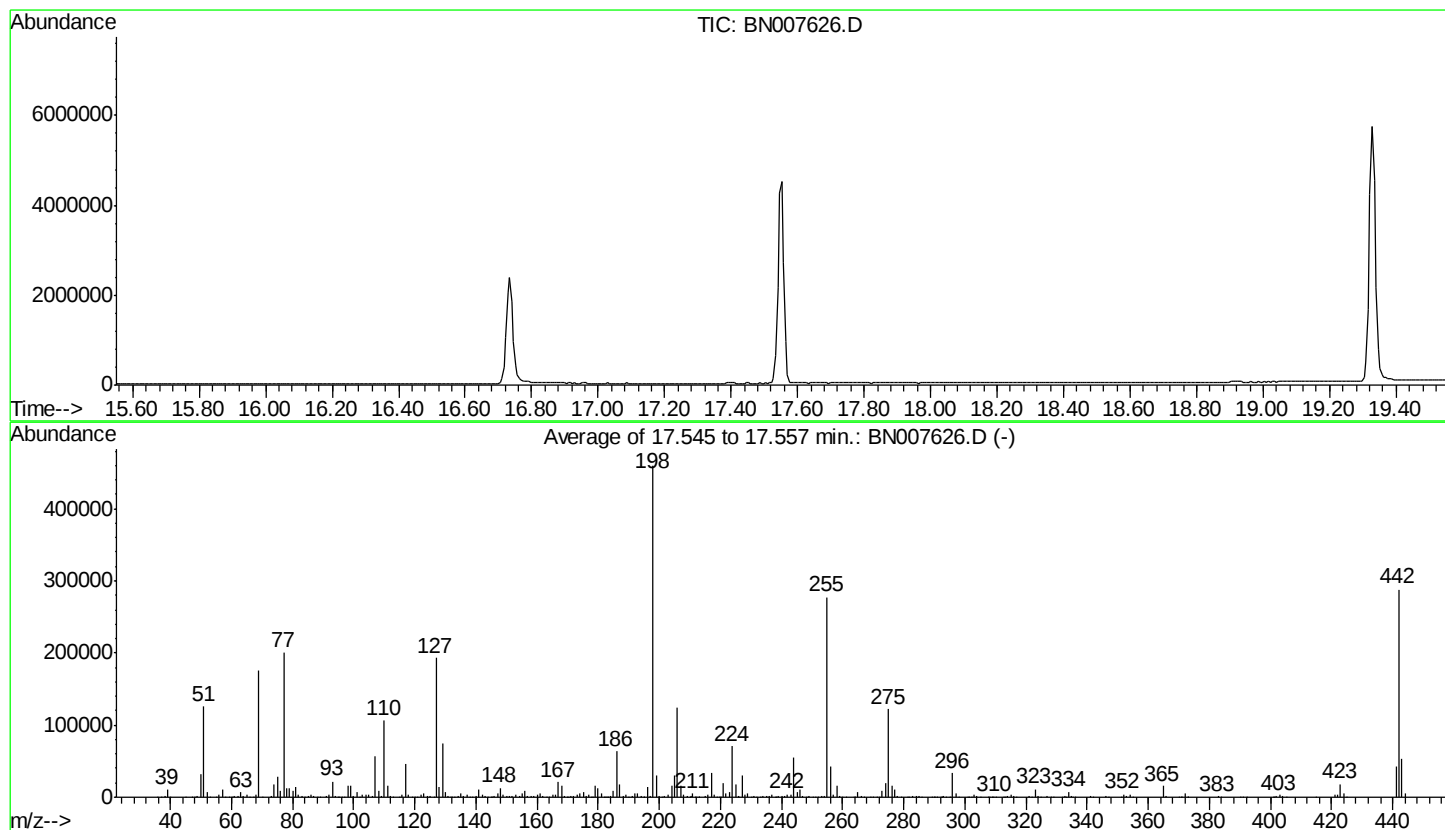

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	125973	PASS
68	69	0.00	2	1.9	3290	PASS
69	198	0.00	100	38.3	176333	PASS
70	69	0.00	2	0.5	929	PASS
127	198	10	80	42.0	193194	PASS
197	198	0.00	2	0.2	994	PASS
198	198	100	100	100.0	459840	PASS
199	198	5	9	6.6	30304	PASS
275	198	10	60	26.6	122298	PASS
365	198	1	100	3.4	15590	PASS
441	198	0.01	100	9.5	43530	PASS
442	198	50	100	62.7	288256	PASS
443	442	15	24	18.8	54141	PASS