


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091319\
 Data File : BN007644.D
 Acq On : 14 Sep 2019 02:35
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 12 14:27:51 2019

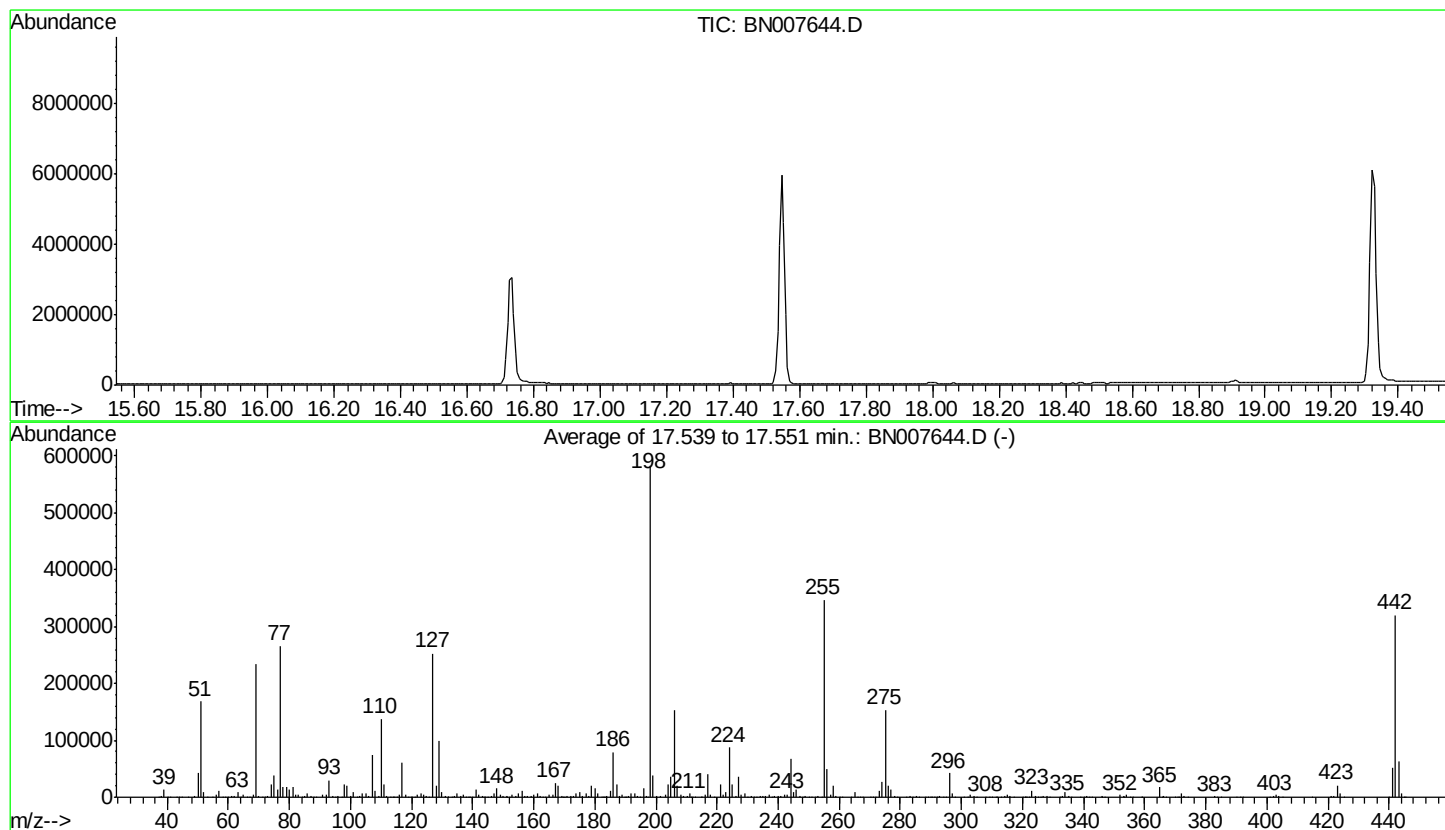

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	168196	PASS
68	69	0.00	2	1.8	4331	PASS
69	198	0.00	100	40.2	234424	PASS
70	69	0.00	2	0.6	1411	PASS
127	198	10	80	43.2	252138	PASS
197	198	0.00	2	0.2	1292	PASS
198	198	100	100	100.0	583082	PASS
199	198	5	9	6.7	38797	PASS
275	198	10	60	26.3	153544	PASS
365	198	1	100	3.0	17772	PASS
441	198	0.01	100	9.0	52346	PASS
442	198	50	100	55.0	320661	PASS
443	442	15	24	19.5	62378	PASS