

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
 Data File : BN027626.D
 Acq On : 13 Sep 2023 02:17
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 129 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Sep 13 06:04:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 02:45:58 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.037	152	7756	0.400	ng	0.00
7) Naphthalene-d8	10.853	136	20704	0.400	ng	# 0.00
13) Acenaphthene-d10	14.662	164	9263	0.400	ng	0.00
19) Phenanthrene-d10	17.406	188	18033	0.400	ng	0.00
29) Chrysene-d12	21.587	240	13167	0.400	ng	# 0.00
35) Perylene-d12	24.089	264	12129	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.567	112	8904	0.440	ng	0.00
5) Phenol-d6	7.178	99	10138	0.412	ng	0.00
8) Nitrobenzene-d5	9.219	82	6954	0.461	ng	-0.01
11) 2-Methylnaphthalene-d10	12.426	152	11452	0.377	ng	0.00
14) 2,4,6-Tribromophenol	16.152	330	1221	0.356	ng	0.00
15) 2-Fluorobiphenyl	13.283	172	16700	0.474	ng	-0.01
27) Fluoranthene-d10	19.430	212	17465	0.390	ng	0.00
31) Terphenyl-d14	20.015	244	11893	0.450	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.473	88	4068	0.430	ng	# 93
3) n-Nitrosodimethylamine	3.819	42	4334	0.432	ng	93
6) bis(2-Chloroethyl)ether	7.467	93	9854	0.415	ng	99
9) Naphthalene	10.896	128	24000	0.425	ng	99
10) Hexachlorobutadiene	11.130	225	4539	0.431	ng	# 100
12) 2-Methylnaphthalene	12.498	142	14995	0.373	ng	99
16) Acenaphthylene	14.384	152	16827	0.399	ng	99
17) Acenaphthene	14.715	154	12197	0.434	ng	98
18) Fluorene	15.705	166	14981	0.399	ng	100
20) 4,6-Dinitro-2-methylph...	16.859	198	109	0.424	ng	# 66
21) 4-Bromophenyl-phenylether	16.586	248	4362	0.459	ng	# 77
22) Hexachlorobenzene	16.673	284	4842	0.429	ng	99
23) Atrazine	16.859	200	2821	0.396	ng	98
24) Pentachlorophenol	17.046	266	1662	0.383	ng	99
25) Phenanthrene	17.443	178	22582	0.426	ng	100
26) Anthracene	17.542	178	18345	0.407	ng	100
28) Fluoranthene	19.463	202	23681	0.380	ng	100
30) Pyrene	19.825	202	23660	0.452	ng	100
32) Benzo(a)anthracene	21.569	228	19499	0.432	ng	99
33) Chrysene	21.623	228	21580	0.435	ng	100
34) Bis(2-ethylhexyl)phtha...	21.444	149	8063	0.370	ng	99
36) Indeno(1,2,3-cd)pyrene	26.726	276	21851	0.444	ng	100
37) Benzo(b)fluoranthene	23.309	252	19952	0.425	ng	99
38) Benzo(k)fluoranthene	23.361	252	19839	0.411	ng	98
39) Benzo(a)pyrene	23.972	252	17413	0.397	ng	98
40) Dibenzo(a,h)anthracene	26.747	278	17951	0.465	ng	98
41) Benzo(g,h,i)perylene	27.545	276	19875	0.444	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027626.D
Acq On : 13 Sep 2023 02:17
Operator : MA/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 129 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Sep 13 06:04:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:45:58 2023
Response via : Initial Calibration




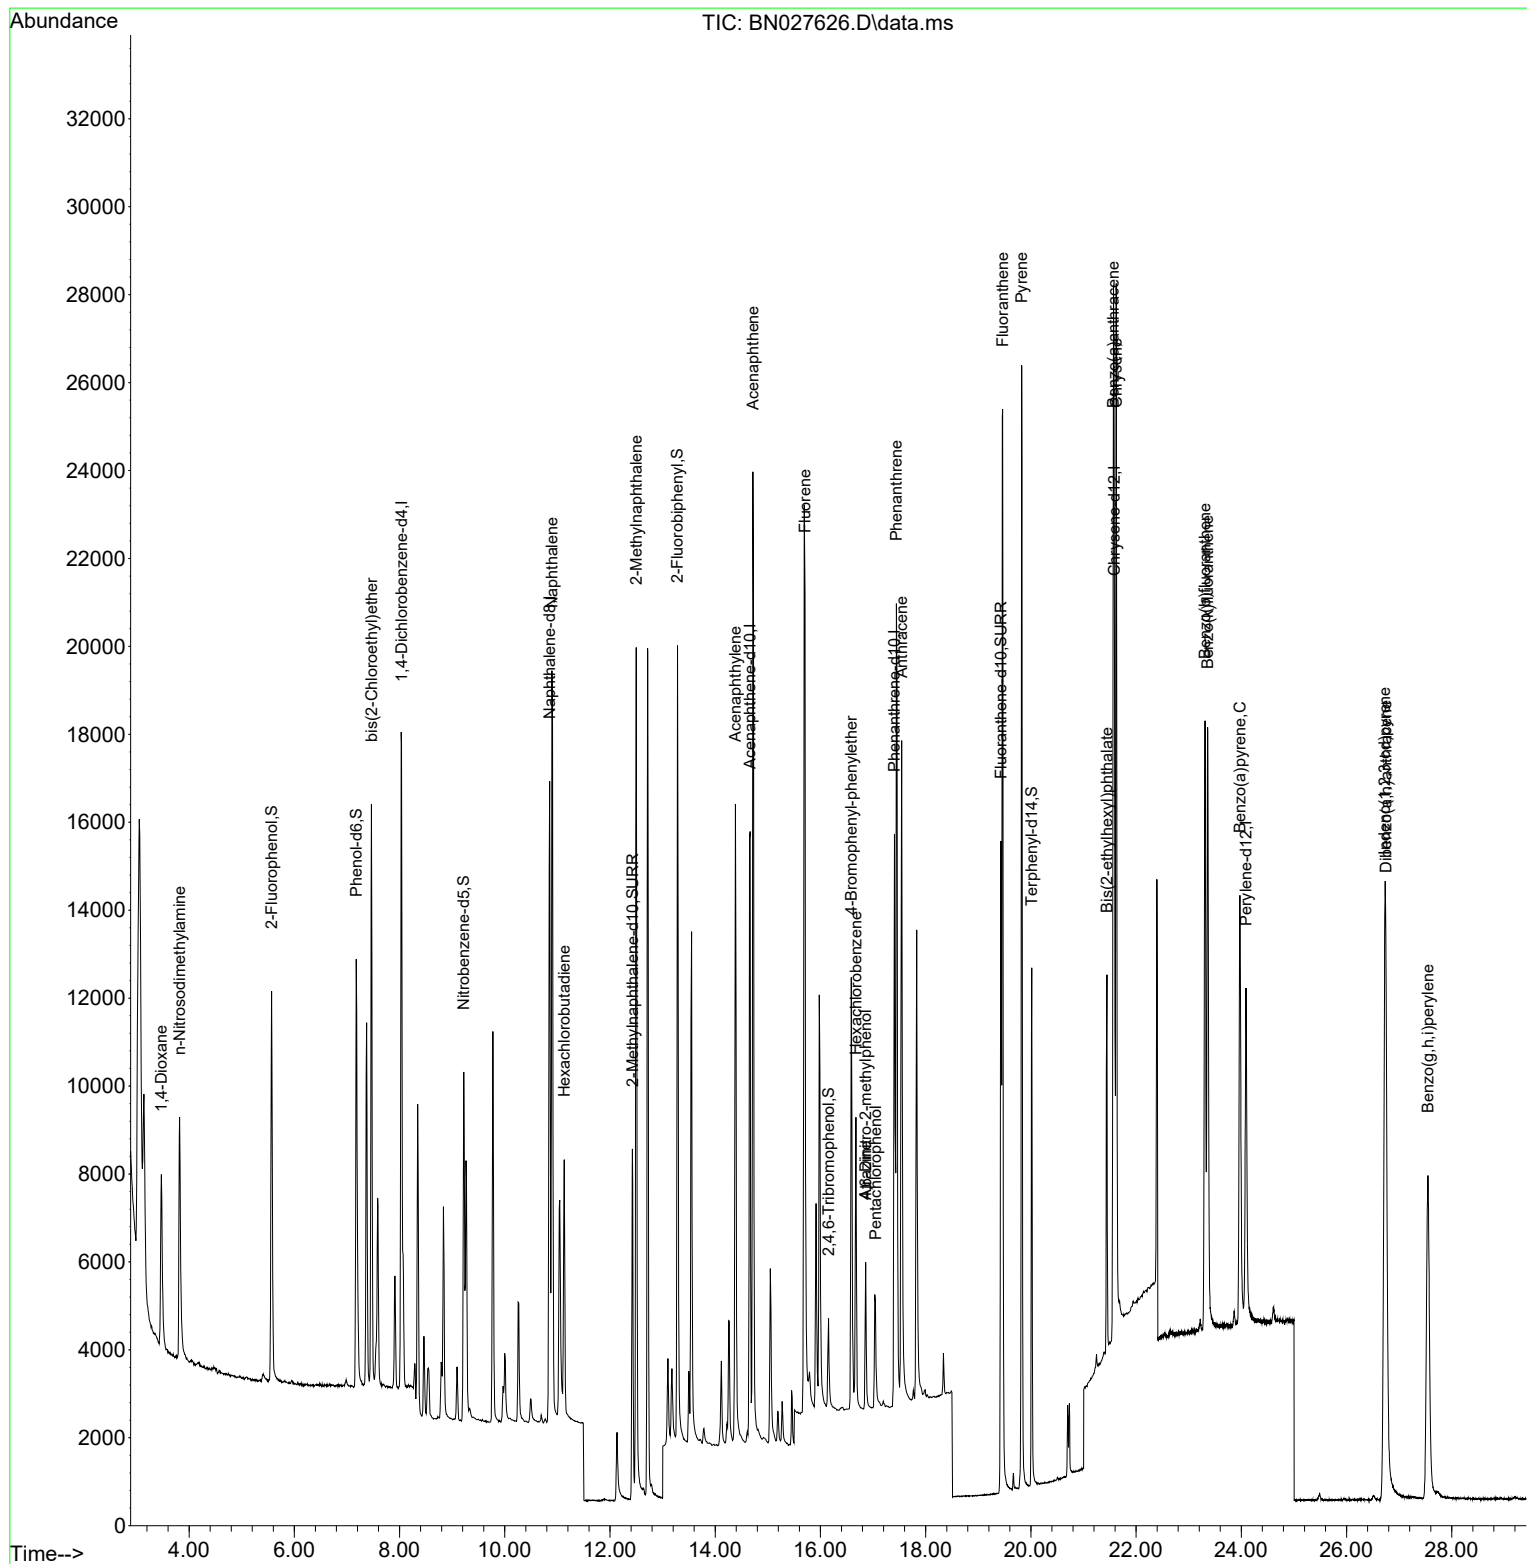




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.037 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BN027626.D
 Acq: 13 Sep 2023 02:17




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:152 Resp: 7756
 Ion Ratio Lower Upper
 152 100
 150 153.1 122.7 184.1
 115 60.9 48.6 73.0

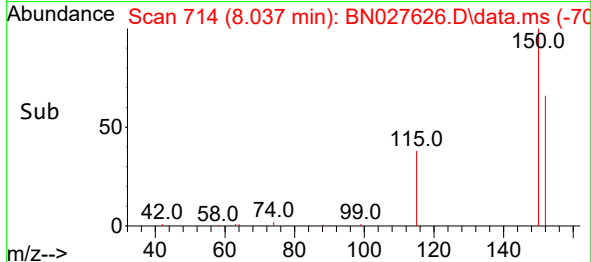

#2
 1,4-Dioxane
 Concen: 0.430 ng
 RT: 3.473 min Scan# 82
 Delta R.T. 0.000 min
 Lab File: BN027626.D
 Acq: 13 Sep 2023 02:17

Tgt Ion: 88 Resp: 4068
 Ion Ratio Lower Upper
 88 100
 43 28.7 19.1 28.7#
 58 70.5 52.2 78.2









#3
n-Nitrosodimethylamine
Concen: 0.432 ng
RT: 3.819 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 42 Resp: 4334
Ion Ratio Lower Upper
42 100
74 133.0 113.8 170.8
44 8.2 7.3 10.9

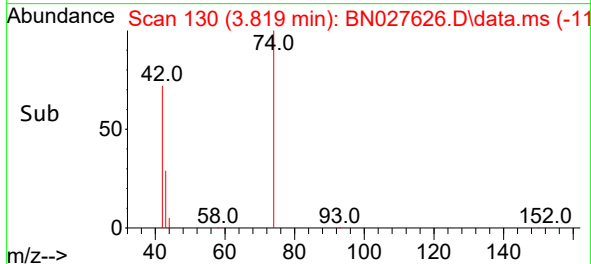

#4
2-Fluorophenol
Concen: 0.440 ng
RT: 5.567 min Scan# 372
Delta R.T. -0.007 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17

Tgt Ion: 112 Resp: 8904
Ion Ratio Lower Upper
112 100
64 55.9 44.4 66.6
63 29.9 23.1 34.7









#5
Phenol-d6
Concen: 0.412 ng
RT: 7.178 min Scan# 599
Delta R.T. -0.007 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	99	Resp:	10138
Ion	Ratio	Lower	Upper
99	100		
42	19.5	14.5	21.7
71	34.0	25.8	38.6

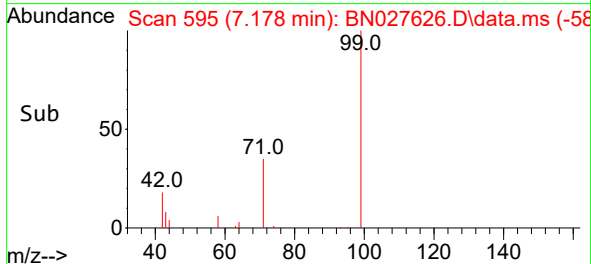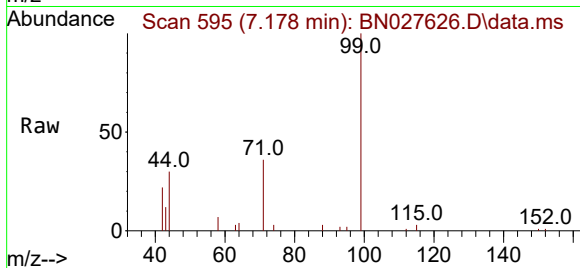

#6
bis(2-Chloroethyl)ether
Concen: 0.415 ng
RT: 7.467 min Scan# 635
Delta R.T. 0.000 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17

Tgt Ion:	93	Resp:	9854
Ion	Ratio	Lower	Upper
93	100		
63	74.0	58.5	87.7
95	32.7	26.1	39.1

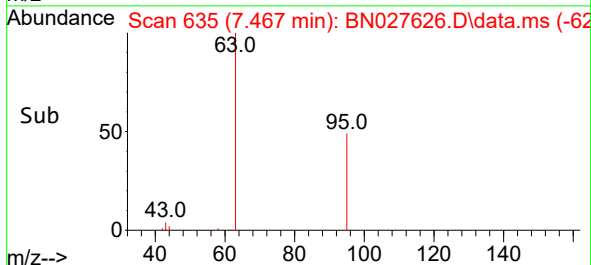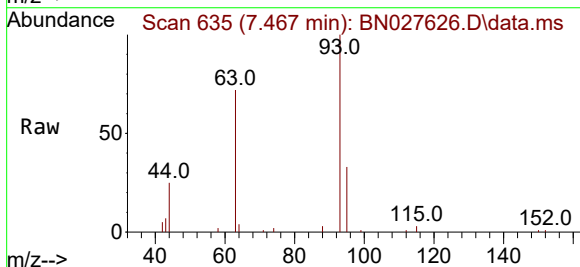



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.853 min Scan# 994

Delta R.T. 0.000 min

Lab File: BN027626.D

Acq: 13 Sep 2023 02:17

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4

Tgt Ion:136 Resp: 20704





Ion Ratio Lower Upper

136 100

137 11.1 9.3 13.9

54 6.4 6.7 10.1#

68 5.7 6.1 9.1#

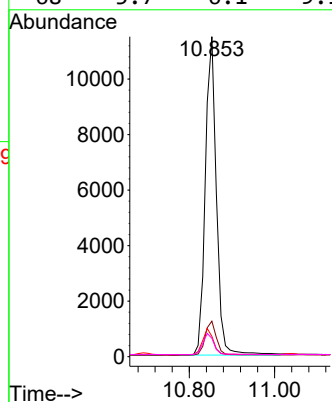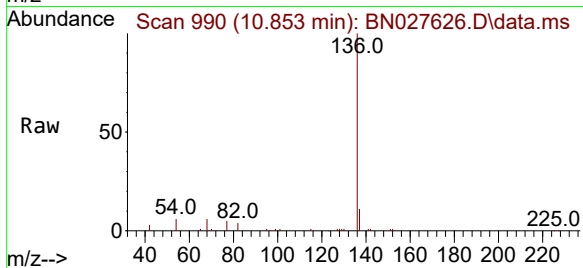

#8

Nitrobenzene-d5

Concen: 0.461 ng

RT: 9.219 min Scan# 837

Delta R.T. -0.011 min

Lab File: BN027626.D

Acq: 13 Sep 2023 02:17




Tgt Ion: 82 Resp: 6954


Ion Ratio Lower Upper

82 100

128 36.5 33.4 50.0

54 50.0 37.7 56.5

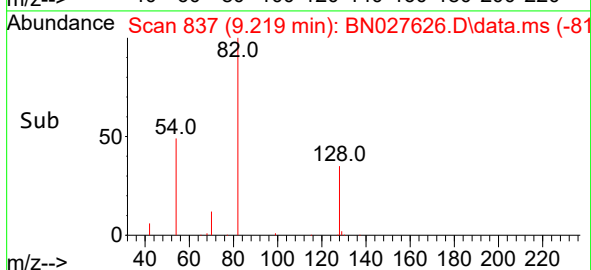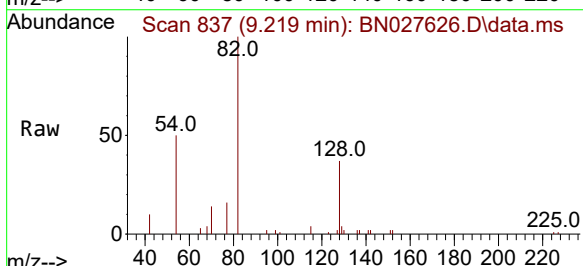



#9

Naphthalene

Concen: 0.425 ng

RT: 10.896 min Scan# 99

Delta R.T. -0.011 min

Lab File: BN027626.D

Acq: 13 Sep 2023 02:17

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:128 Resp: 24000

Ion Ratio Lower Upper

128 100

129 11.2 9.4 14.0

127 13.4 10.6 15.8

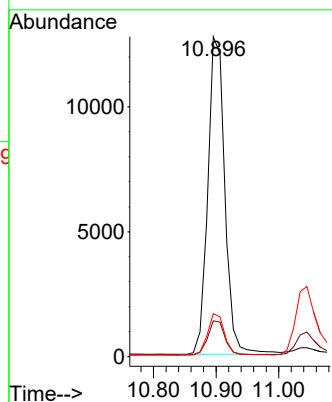

#10

Hexachlorobutadiene

Concen: 0.431 ng

RT: 11.130 min Scan# 1016

Delta R.T. 0.000 min

Lab File: BN027626.D

Acq: 13 Sep 2023 02:17




Tgt Ion:225 Resp: 4539


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 62.9 50.6 75.8


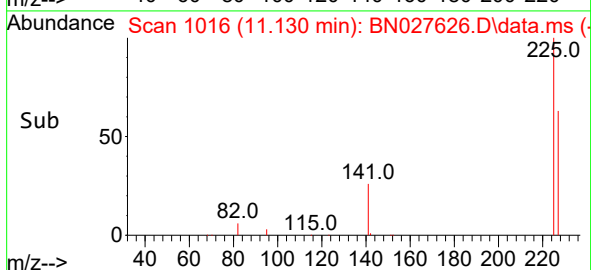






#11
2-Methylnaphthalene-d10
Concen: 0.377 ng
RT: 12.426 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 11452
Ion Ratio Lower Upper
152 100
151 20.6 16.6 25.0

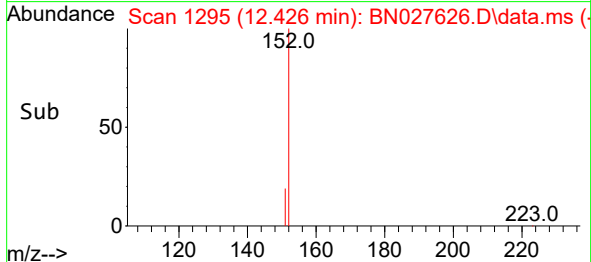

#12
2-Methylnaphthalene
Concen: 0.373 ng
RT: 12.498 min Scan# 1314
Delta R.T. -0.004 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17

Tgt Ion:142 Resp: 14995
Ion Ratio Lower Upper
142 100
141 88.5 71.1 106.7
115 37.6 29.6 44.4


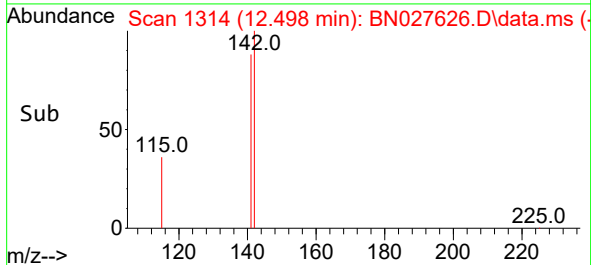






#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.662 min Scan# 1603
Delta R.T. 0.000 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 9263
Ion Ratio Lower Upper
164 100
162 100.8 85.8 128.8
160 49.2 44.2 66.2

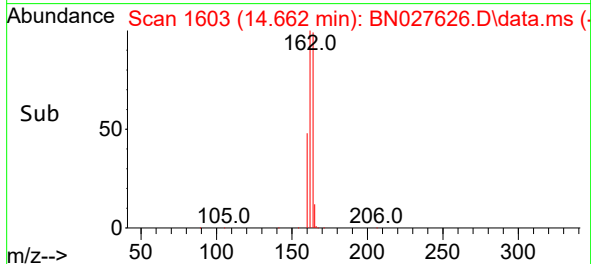

#14
2,4,6-Tribromophenol
Concen: 0.356 ng
RT: 16.152 min Scan# 1734
Delta R.T. 0.000 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17

Tgt Ion:330 Resp: 1221
Ion Ratio Lower Upper
330 100
332 96.2 75.2 112.8
141 47.2 36.2 54.4

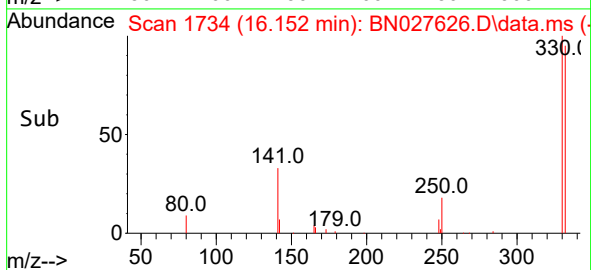



#15

2-Fluorobiphenyl

Concen: 0.474 ng

RT: 13.283 min Scan# 1478

Delta R.T. -0.011 min

Lab File: BN027626.D

Acq: 13 Sep 2023 02:17

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:172 Resp: 16700

Ion Ratio Lower Upper

172 100

171 35.1 27.8 41.8

170 24.1 19.3 28.9

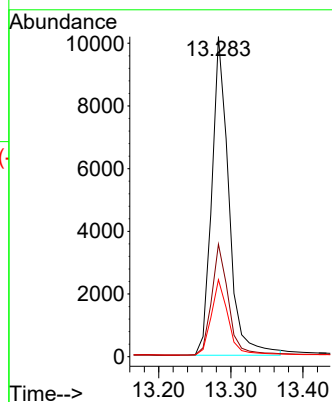

#16

Acenaphthylene

Concen: 0.399 ng

RT: 14.384 min Scan# 1577

Delta R.T. -0.011 min

Lab File: BN027626.D

Acq: 13 Sep 2023 02:17




Tgt Ion:152 Resp: 16827


Ion Ratio Lower Upper

152 100

151 19.8 15.5 23.3

153 13.0 10.3 15.5


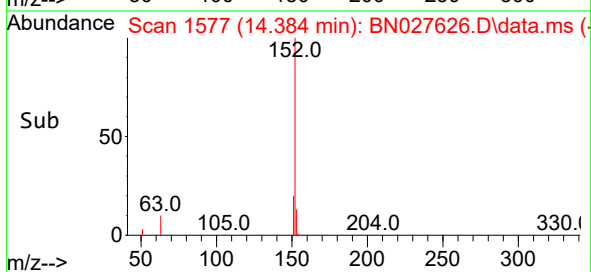
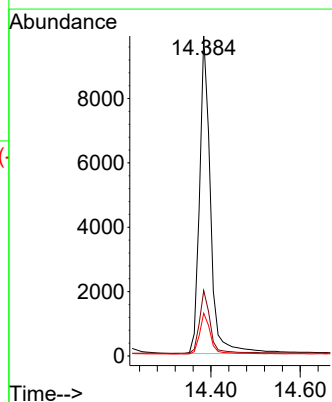





#17
Acenaphthene
Concen: 0.434 ng
RT: 14.715 min Scan# 1608
Delta R.T. -0.011 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 12197
Ion Ratio Lower Upper
154 100
153 113.8 93.1 139.7
152 58.8 48.6 73.0

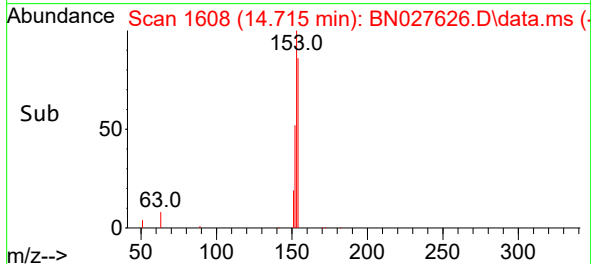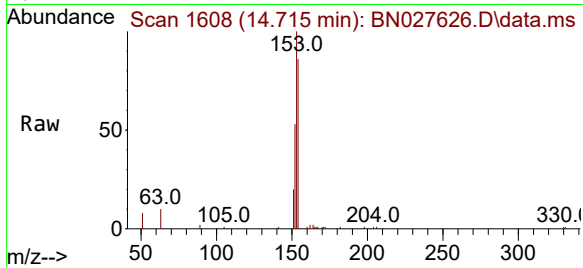

#18
Fluorene
Concen: 0.399 ng
RT: 15.705 min Scan# 1698
Delta R.T. 0.000 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17

Tgt Ion:166 Resp: 14981
Ion Ratio Lower Upper
166 100
165 98.5 79.0 118.4
167 13.3 10.8 16.2

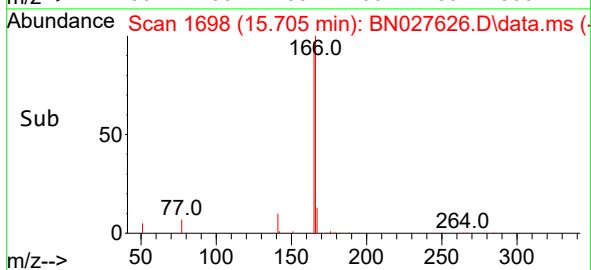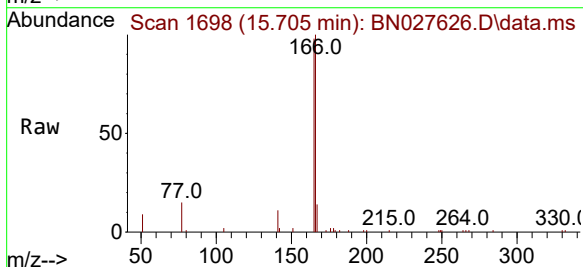



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.406 min Scan# 1835

Delta R.T. 0.000 min

Lab File: BN027626.D

Acq: 13 Sep 2023 02:17

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:188 Resp: 18033

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 11.1 11.0 16.6

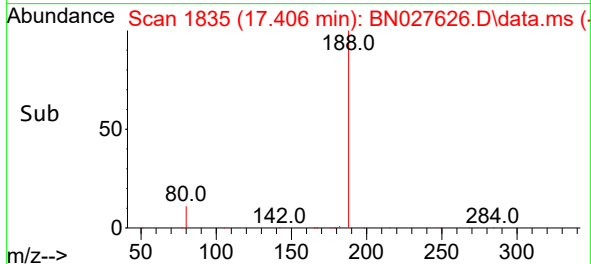

#20

4,6-Dinitro-2-methylphenol

Concen: 0.424 ng

RT: 16.859 min Scan# 1791

Delta R.T. 0.000 min

Lab File: BN027626.D

Acq: 13 Sep 2023 02:17




Tgt Ion:198 Resp: 109


Ion Ratio Lower Upper

198 100

51 241.1 282.2 423.2#

105 201.8 168.7 253.1


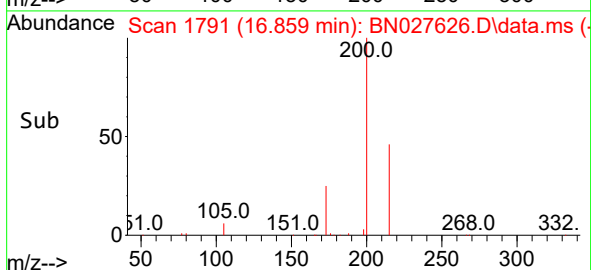






#21
4-Bromophenyl-phenylether
Concen: 0.459 ng
RT: 16.586 min Scan# 1769
Delta R.T. -0.012 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 4362
Ion Ratio Lower Upper
248 100
250 93.5 79.7 119.5
141 88.8 39.8 59.8#

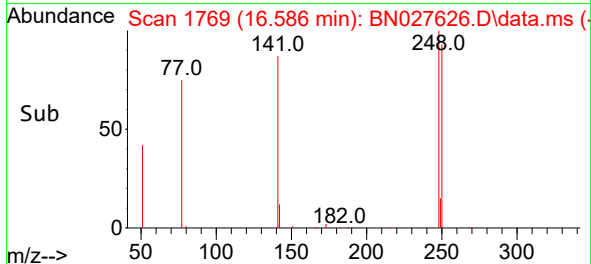

#22
Hexachlorobenzene
Concen: 0.429 ng
RT: 16.673 min Scan# 1776
Delta R.T. -0.012 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17

Tgt Ion:284 Resp: 4842
Ion Ratio Lower Upper
284 100
142 41.4 32.9 49.3
249 31.6 24.3 36.5


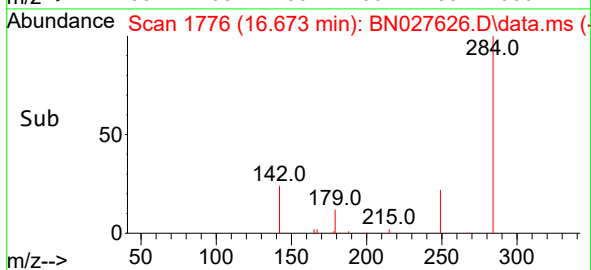






#23
 Atrazine
 Concen: 0.396 ng
 RT: 16.859 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN027626.D
 Acq: 13 Sep 2023 02:17




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:200 Resp: 2821
 Ion Ratio Lower Upper
 200 100
 173 27.0 22.5 33.7
 215 47.3 39.0 58.6

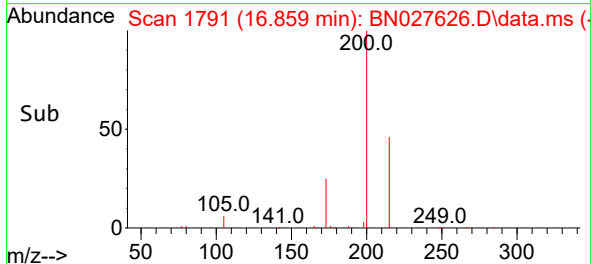

#24
 Pentachlorophenol
 Concen: 0.383 ng
 RT: 17.046 min Scan# 1806
 Delta R.T. 0.000 min
 Lab File: BN027626.D
 Acq: 13 Sep 2023 02:17

Tgt Ion:266 Resp: 1662
 Ion Ratio Lower Upper
 266 100
 264 61.6 50.3 75.5
 268 64.0 52.0 78.0

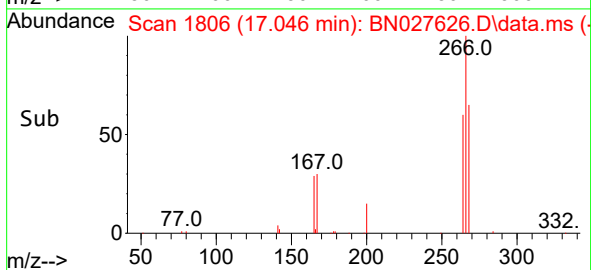

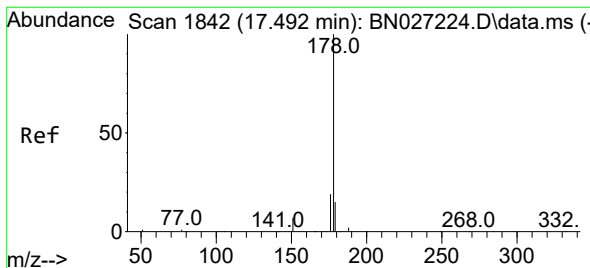

#25

Phenanthrene

Concen: 0.426 ng

RT: 17.443 min Scan# 1838

Delta R.T. -0.012 min

Lab File: BN027626.D

Acq: 13 Sep 2023 02:17

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:178 Resp: 22582

Ion Ratio Lower Upper

178 100

176 19.3 15.6 23.4

179 15.6 12.3 18.5

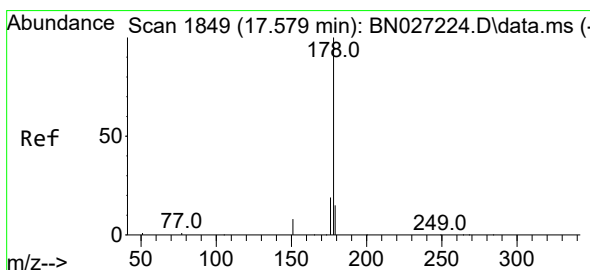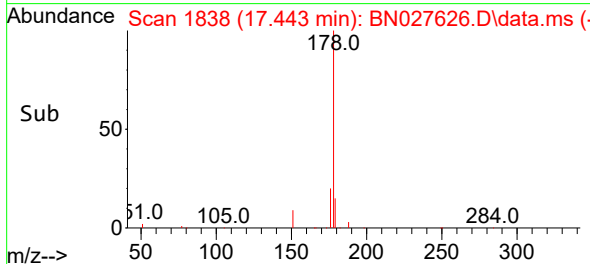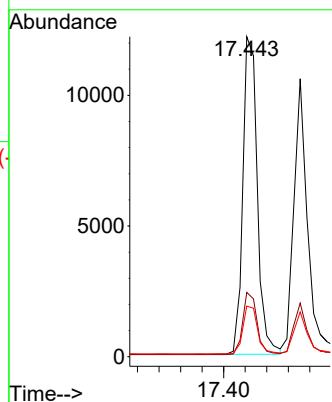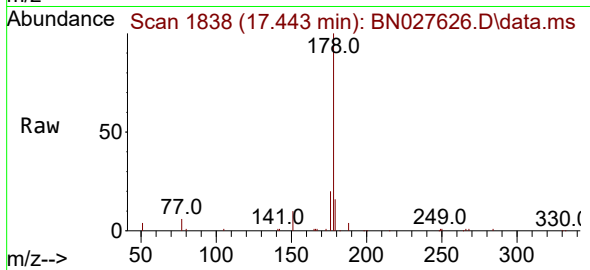

#26

Anthracene

Concen: 0.407 ng

RT: 17.542 min Scan# 1846

Delta R.T. 0.000 min

Lab File: BN027626.D

Acq: 13 Sep 2023 02:17




Tgt Ion:178 Resp: 18345


Ion Ratio Lower Upper

178 100

176 18.7 14.9 22.3

179 15.1 12.0 18.0


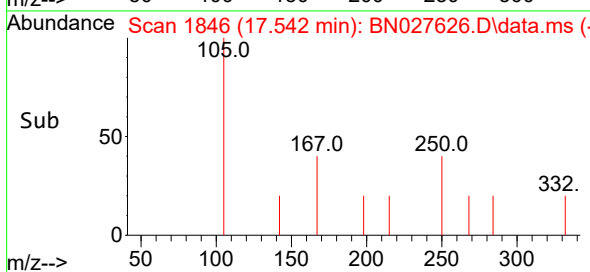
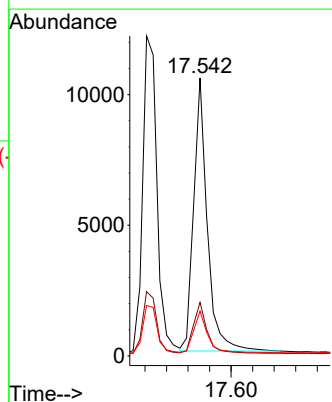
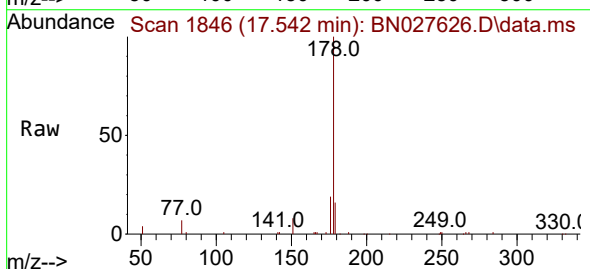




#27
Fluoranthene-d10
Concen: 0.390 ng
RT: 19.430 min Scan# 2129
Delta R.T. -0.005 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 17465
Ion Ratio Lower Upper
212 100
106 15.0 12.1 18.1
104 8.3 6.9 10.3

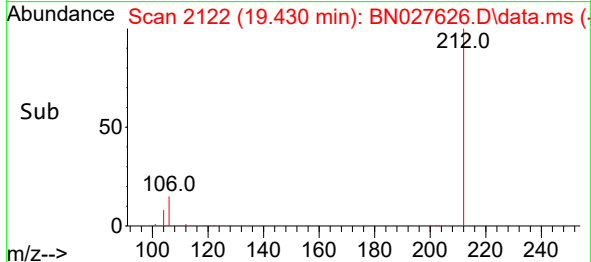

#28
Fluoranthene
Concen: 0.380 ng
RT: 19.463 min Scan# 2129
Delta R.T. -0.005 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17

Tgt Ion:202 Resp: 23681
Ion Ratio Lower Upper
202 100
101 11.9 9.6 14.4
203 17.0 13.6 20.4

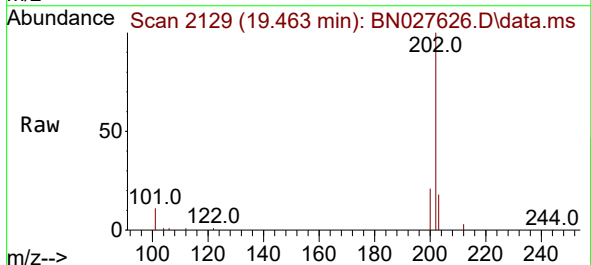

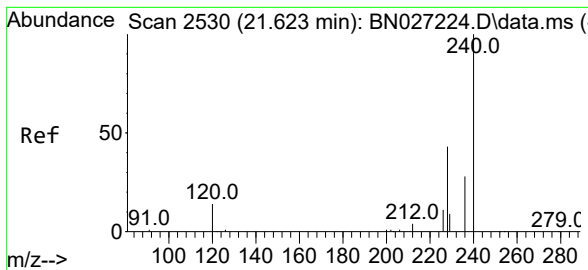

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.587 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN027626.D

Acq: 13 Sep 2023 02:17

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:240 Resp: 13167

Ion Ratio Lower Upper

240 100

120 13.8 14.2 21.4#

236 28.1 22.9 34.3

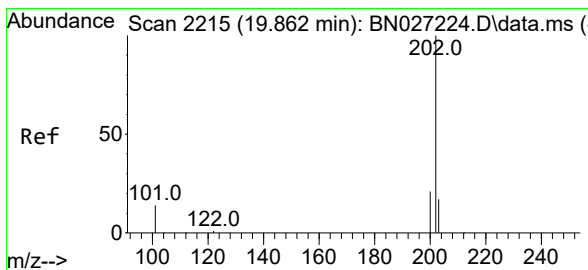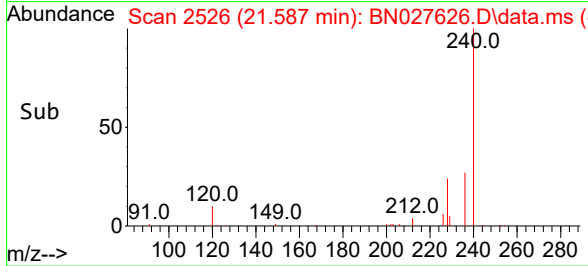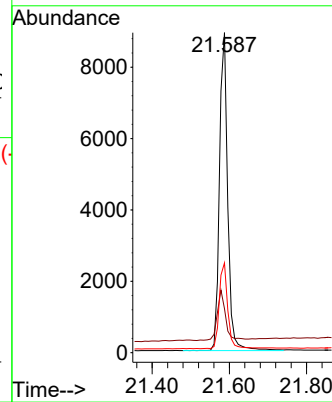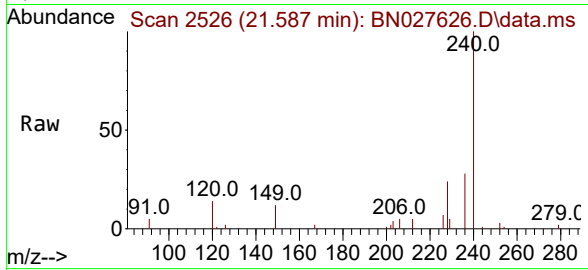

#30

Pyrene

Concen: 0.452 ng

RT: 19.825 min Scan# 2207

Delta R.T. -0.005 min

Lab File: BN027626.D

Acq: 13 Sep 2023 02:17




Tgt Ion:202 Resp: 23660


Ion Ratio Lower Upper

202 100

200 21.0 16.6 25.0

203 18.0 14.2 21.4


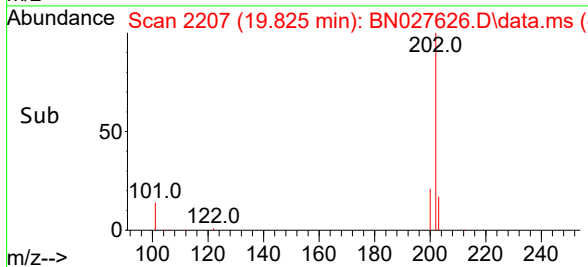

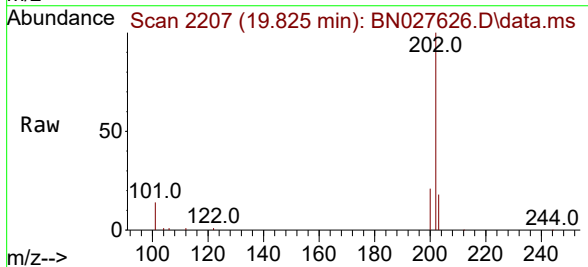




#31
 Terphenyl-d14
 Concen: 0.450 ng
 RT: 20.015 min Scan# 21
 Delta R.T. -0.005 min
 Lab File: BN027626.D
 Acq: 13 Sep 2023 02:17




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:244 Resp: 11893
 Ion Ratio Lower Upper
 244 100
 212 9.2 7.5 11.3
 122 16.5 14.0 21.0

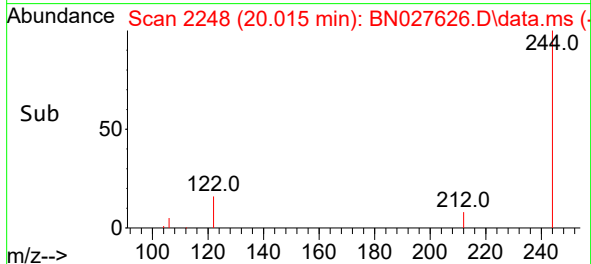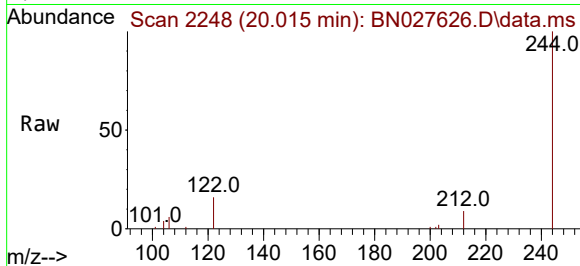

#32
 Benzo(a)anthracene
 Concen: 0.432 ng
 RT: 21.569 min Scan# 2524
 Delta R.T. 0.000 min
 Lab File: BN027626.D
 Acq: 13 Sep 2023 02:17

Tgt Ion:228 Resp: 19499
 Ion Ratio Lower Upper
 228 100
 226 27.2 21.9 32.9
 229 20.0 15.7 23.5

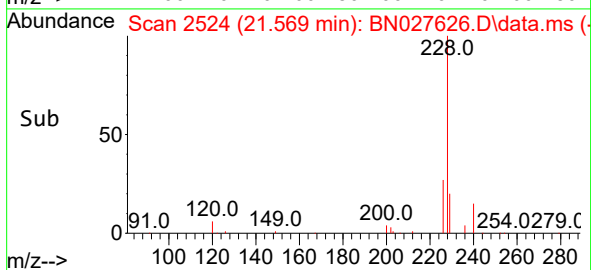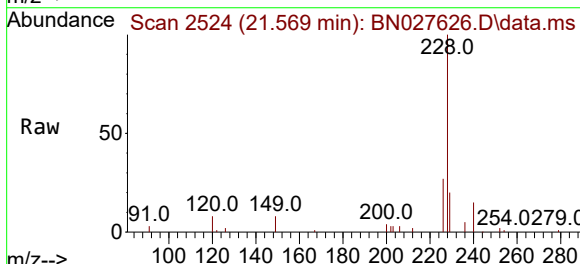

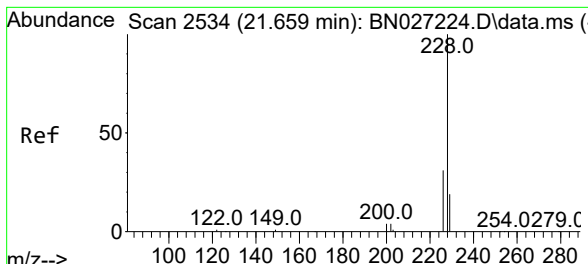

#33

Chrysene

Concen: 0.435 ng

RT: 21.623 min Scan# 21580

Delta R.T. 0.000 min

Lab File: BN027626.D

Acq: 13 Sep 2023 02:17

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:228 Resp: 21580

Ion Ratio Lower Upper

228 100

226 30.4 24.3 36.5

229 19.8 15.4 23.2

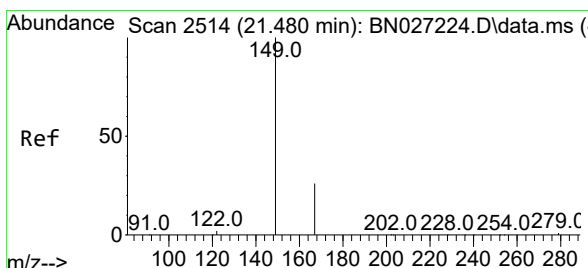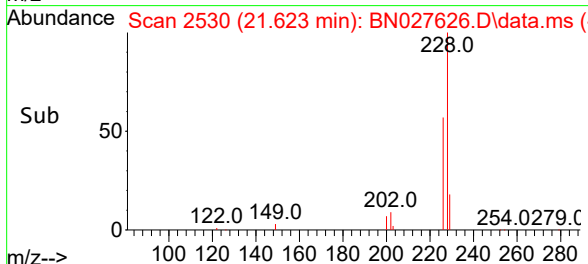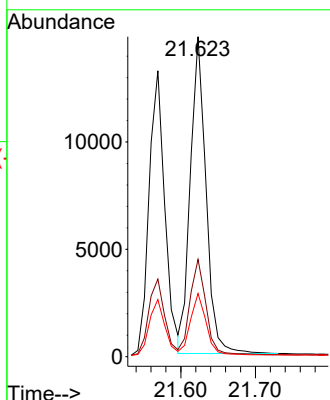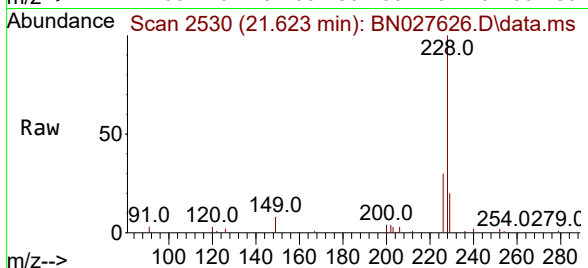

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.370 ng

RT: 21.444 min Scan# 2510

Delta R.T. 0.000 min

Lab File: BN027626.D

Acq: 13 Sep 2023 02:17




Tgt Ion:149 Resp: 8063


Ion Ratio Lower Upper

149 100

167 26.9 22.1 33.1

279 2.9 2.7 4.1


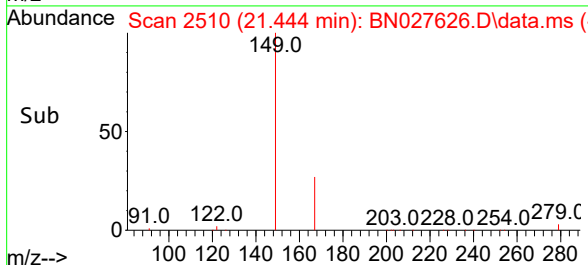
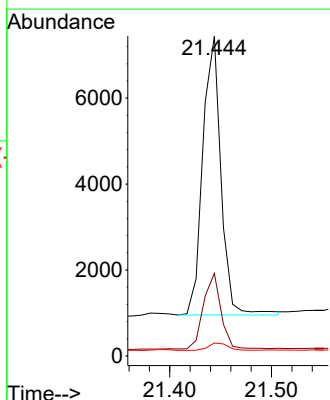
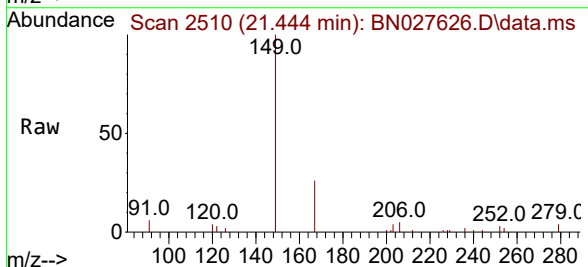




#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.089 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BN027626.D
 Acq: 13 Sep 2023 02:17




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:264 Resp: 12129
 Ion Ratio Lower Upper
 264 100
 260 26.0 20.7 31.1
 265 74.0 53.3 79.9

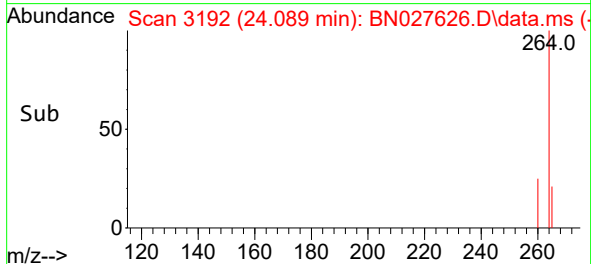

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.444 ng
 RT: 26.726 min Scan# 4094
 Delta R.T. -0.003 min
 Lab File: BN027626.D
 Acq: 13 Sep 2023 02:17

Tgt Ion:276 Resp: 21851
 Ion Ratio Lower Upper
 276 100
 138 29.4 23.4 35.2
 277 25.0 19.8 29.8


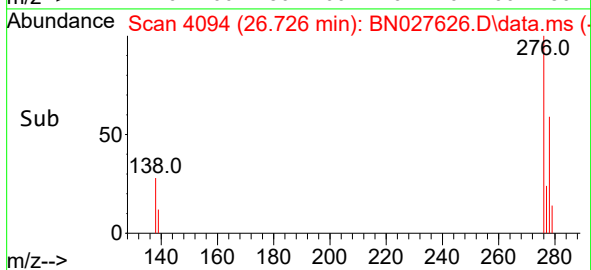






#37
Benzo(b)fluoranthene
Concen: 0.425 ng
RT: 23.309 min Scan# 2943
Delta R.T. -0.006 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 19952
Ion Ratio Lower Upper
252 100
253 25.6 19.9 29.9
125 16.7 13.8 20.6

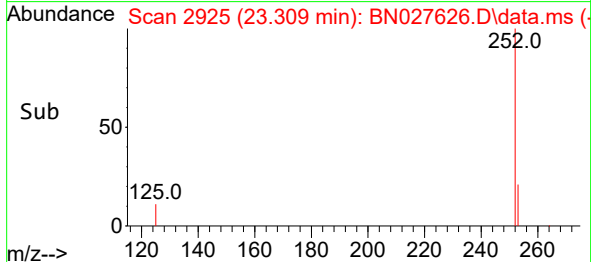

#38
Benzo(k)fluoranthene
Concen: 0.411 ng
RT: 23.361 min Scan# 2943
Delta R.T. -0.006 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17

Tgt Ion:252 Resp: 19839
Ion Ratio Lower Upper
252 100
253 26.2 20.2 30.2
125 16.5 14.1 21.1


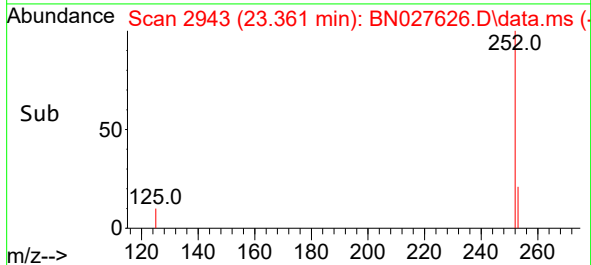






#39
Benzo(a)pyrene
Concen: 0.397 ng
RT: 23.972 min Scan# 31
Delta R.T. -0.009 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252	Resp:	17413
Ion Ratio	Lower	Upper
252	100	
253	28.3	21.4 32.0
125	20.3	16.5 24.7

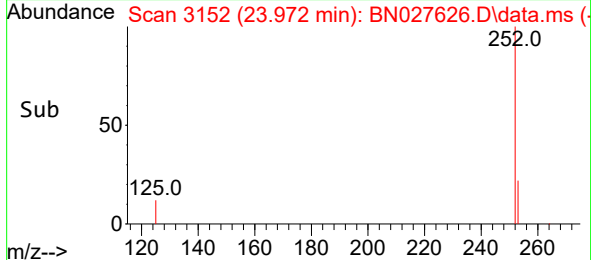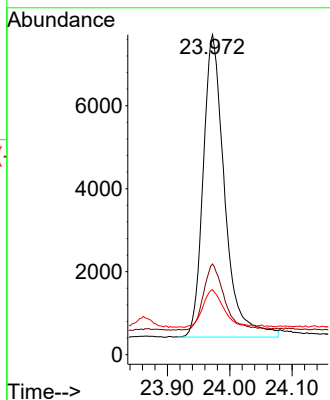

#40
Dibenzo(a,h)anthracene
Concen: 0.465 ng
RT: 26.747 min Scan# 4101
Delta R.T. -0.009 min
Lab File: BN027626.D
Acq: 13 Sep 2023 02:17


Tgt Ion:278	Resp:	17951
Ion Ratio	Lower	Upper
278	100	
139	21.1	17.9 26.9
279	26.7	21.8 32.6

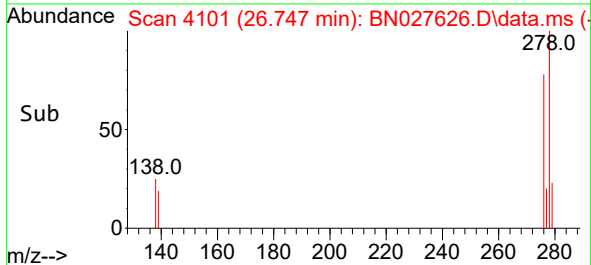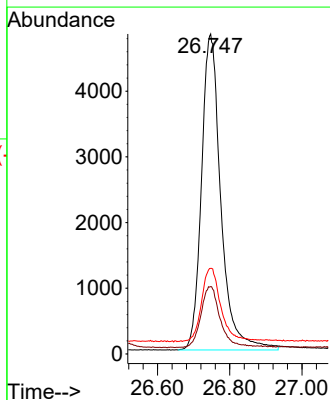

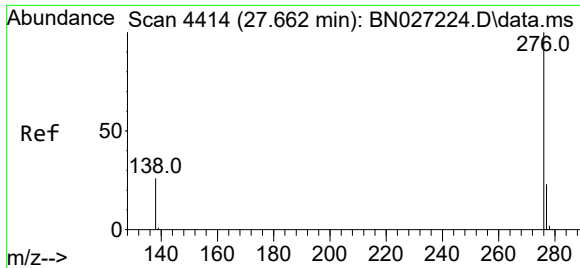

#41
 Benzo(g,h,i)perylene
 Concen: 0.444 ng
 RT: 27.545 min Scan# 41
 Delta R.T. -0.009 min
 Lab File: BN027626.D
 Acq: 13 Sep 2023 02:17

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

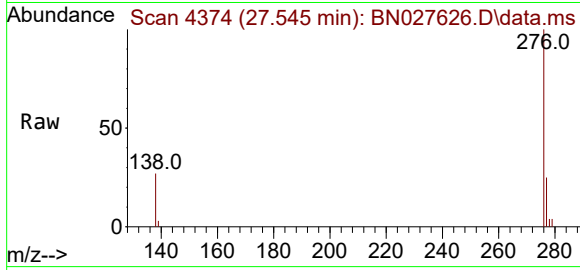

Tgt Ion:276 Resp: 19875
 Ion Ratio Lower Upper
 276 100
 277 24.9 19.6 29.4
 138 26.7 22.1 33.1

