
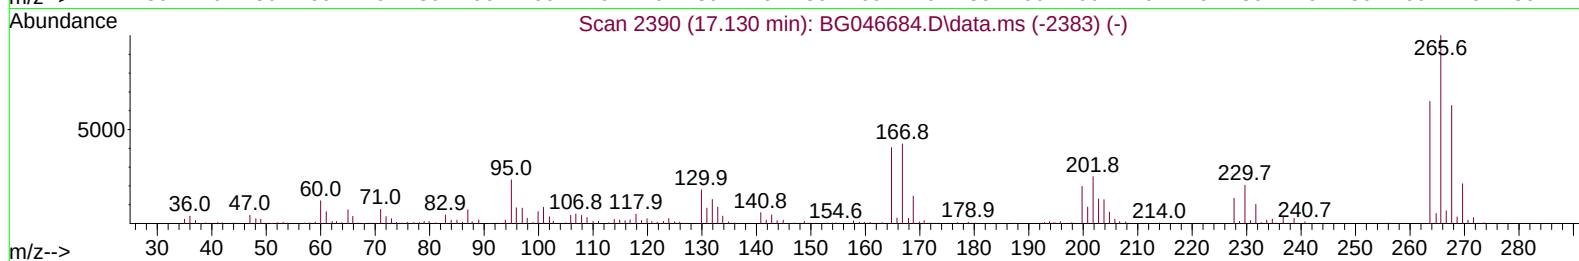
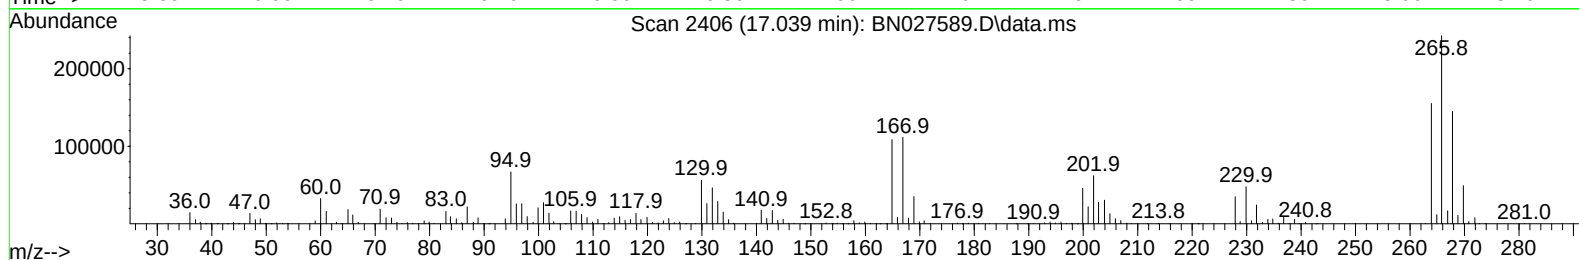


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027589.D
Acq On : 12 Sep 2023 00:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 90 Sample Multiplier: 1

Quant Time: Sep 12 02:39:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:39:44 2023
Response via : Initial Calibration

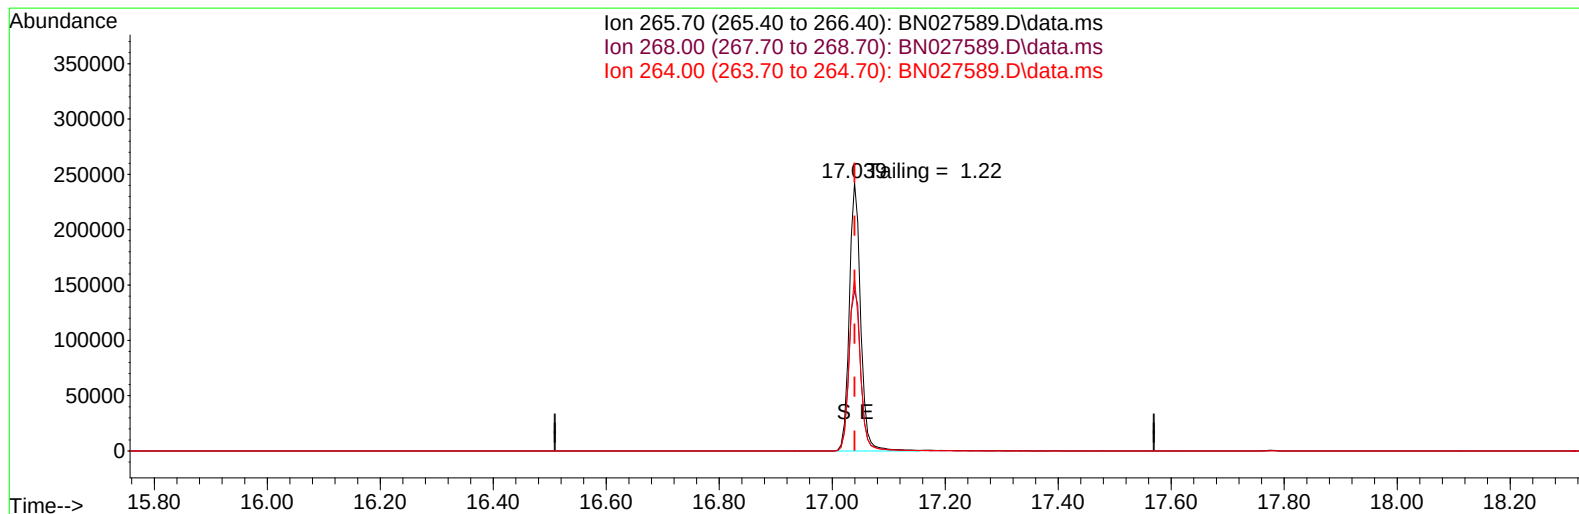

TIC: BN027589.D\data.ms

(70) Pentachlorophenol (C)




17.039min (0.000) 20906.42 ng

response 338637

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.79
264.00	61.60	63.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027589.D
Acq On : 12 Sep 2023 00:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 90 Sample Multiplier: 1

Quant Time: Sep 12 02:39:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:39:44 2023
Response via : Initial Calibration

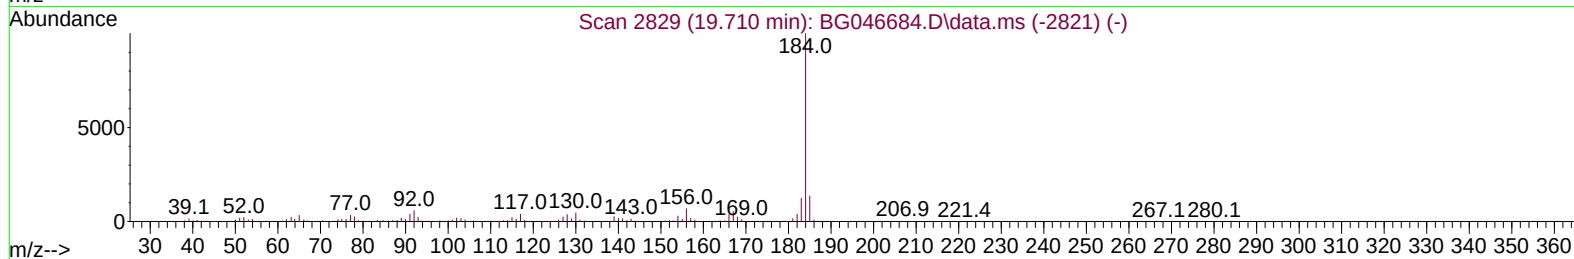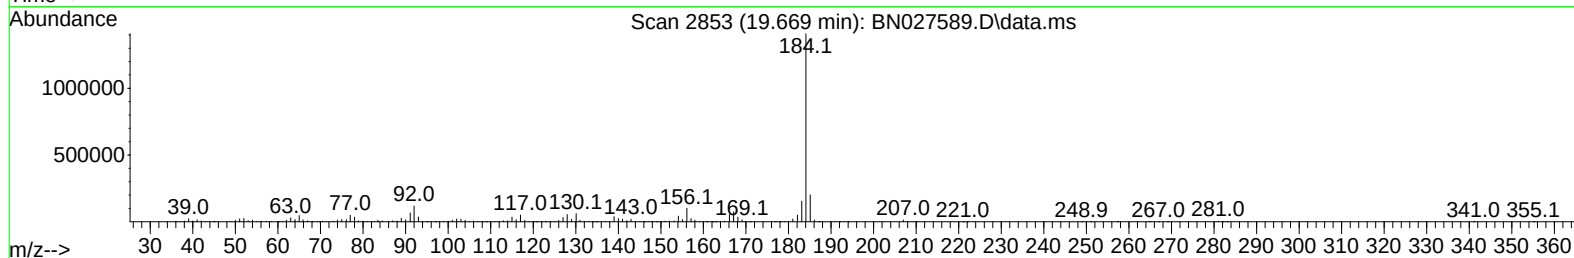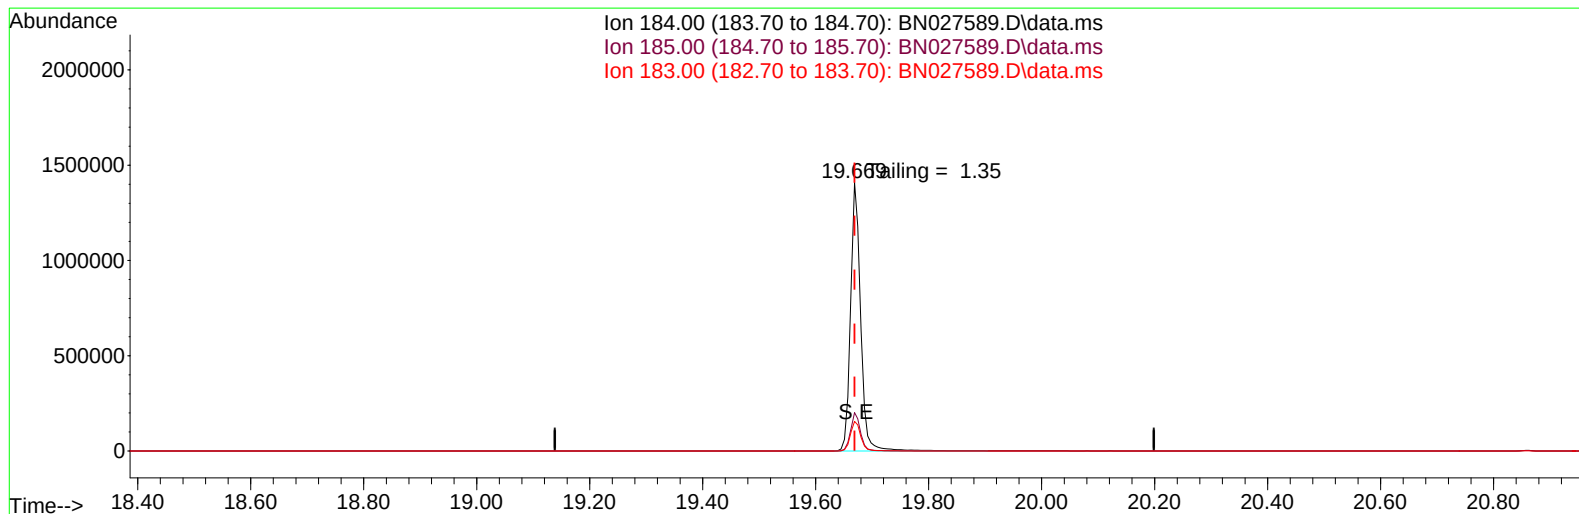

TIC: BN027589.D\data.ms

(77) Benzidine

19.669min (0.000) 0.00 ng

response 1761177

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.31
183.00	13.20	11.03
0.00	0.00	0.00