
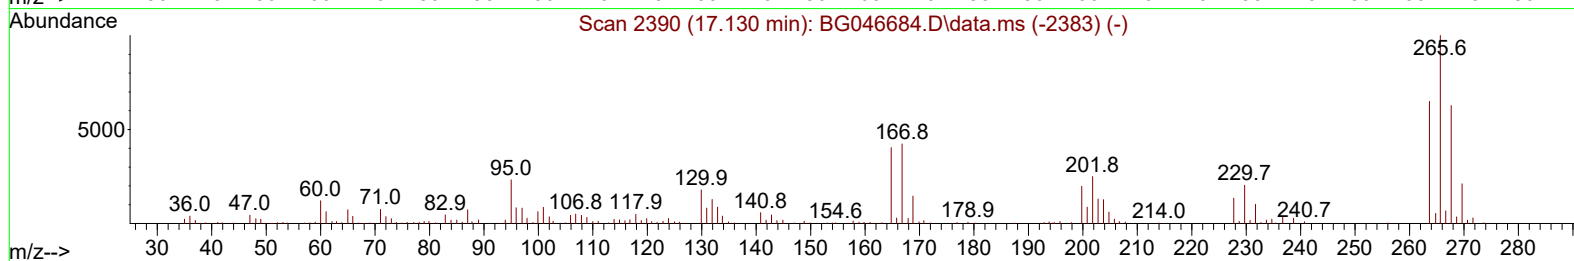
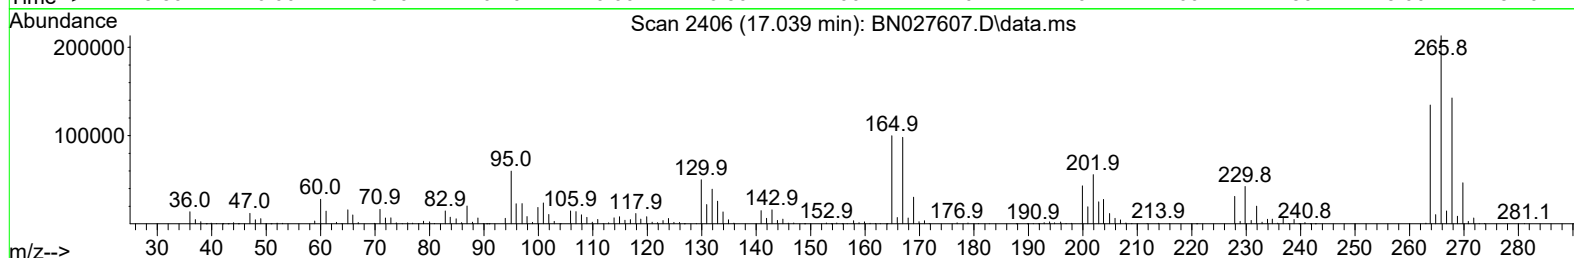


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027607.D
Acq On : 12 Sep 2023 13:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 109 Sample Multiplier: 1

Quant Time: Sep 13 07:58:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 13 07:57:09 2023
Response via : Initial Calibration

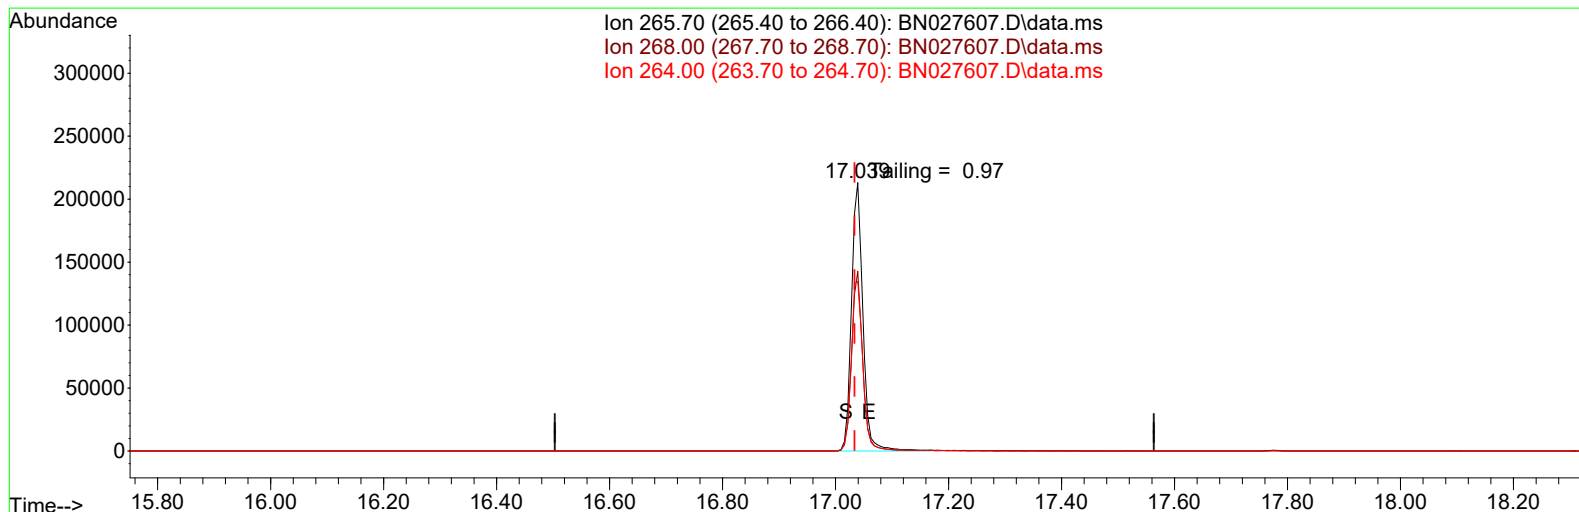

TIC: BN027607.D\data.ms

(70) Pentachlorophenol (C)




17.039min (+ 0.006) 19477.36 ng

response 300357

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.94
264.00	61.60	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027607.D
Acq On : 12 Sep 2023 13:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 109 Sample Multiplier: 1

Quant Time: Sep 13 07:58:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 13 07:57:09 2023
Response via : Initial Calibration

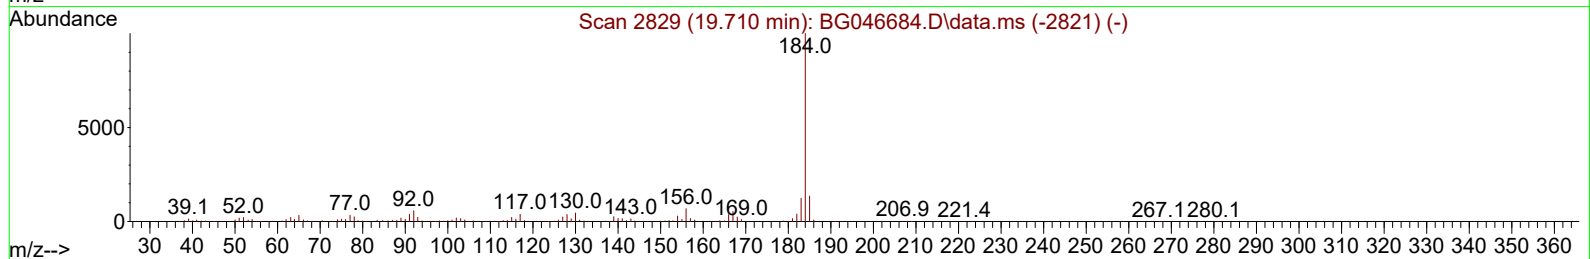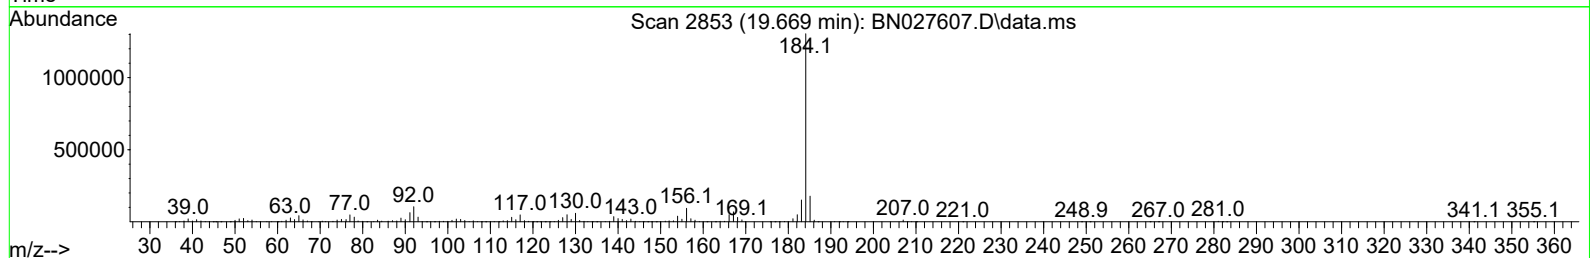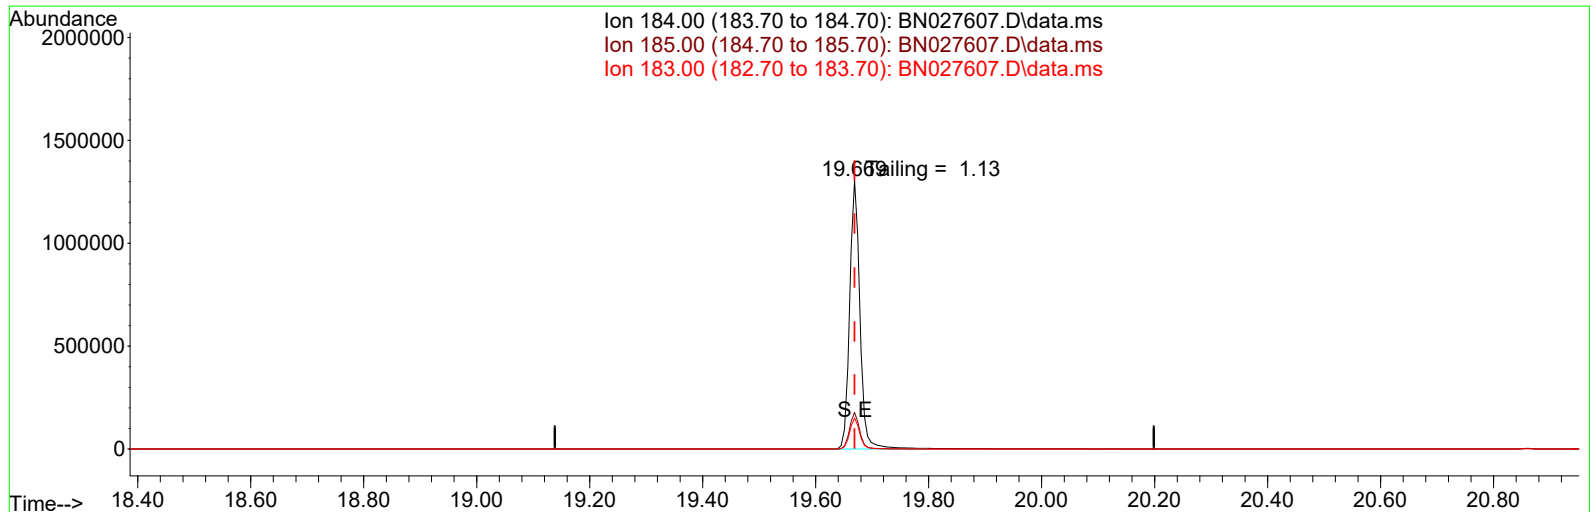

TIC: BN027607.D\data.ms

(77) Benzidine

19.669min (+ 0.000) 0.00 ng

response 1663408

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.65
183.00	13.20	11.56
0.00	0.00	0.00