
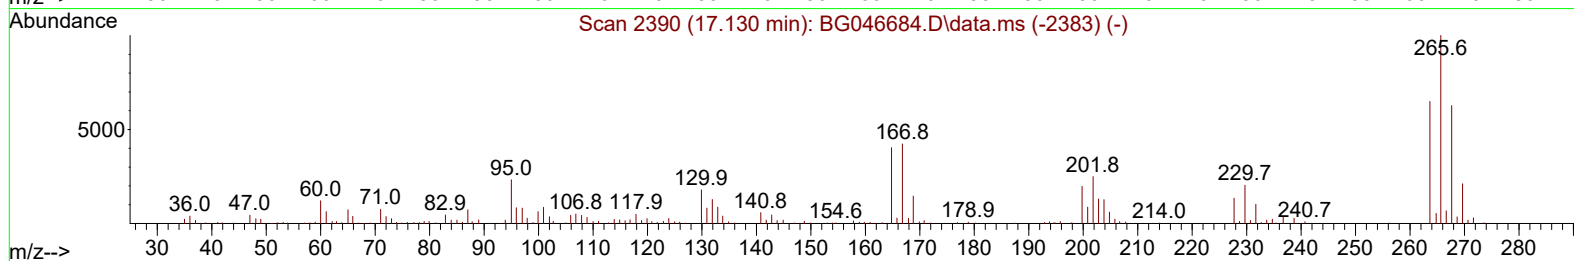
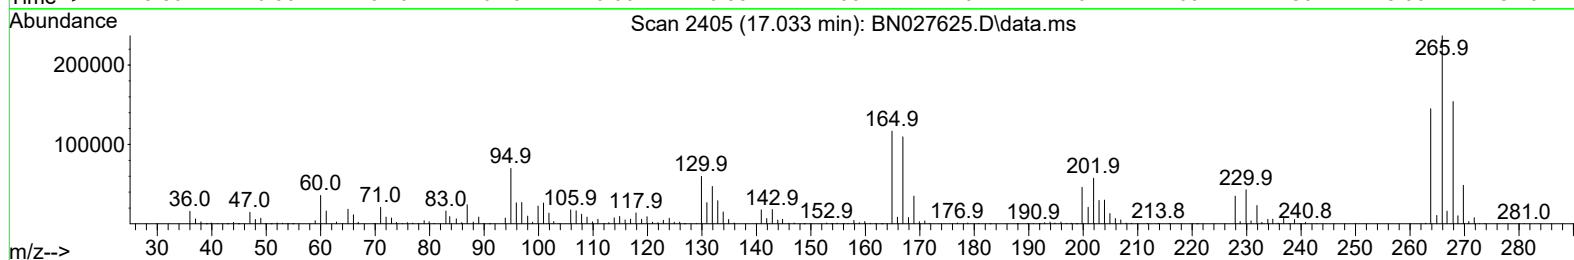


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027625.D
Acq On : 13 Sep 2023 01:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 128 Sample Multiplier: 1

Quant Time: Sep 13 07:57:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 13 07:57:09 2023
Response via : Initial Calibration

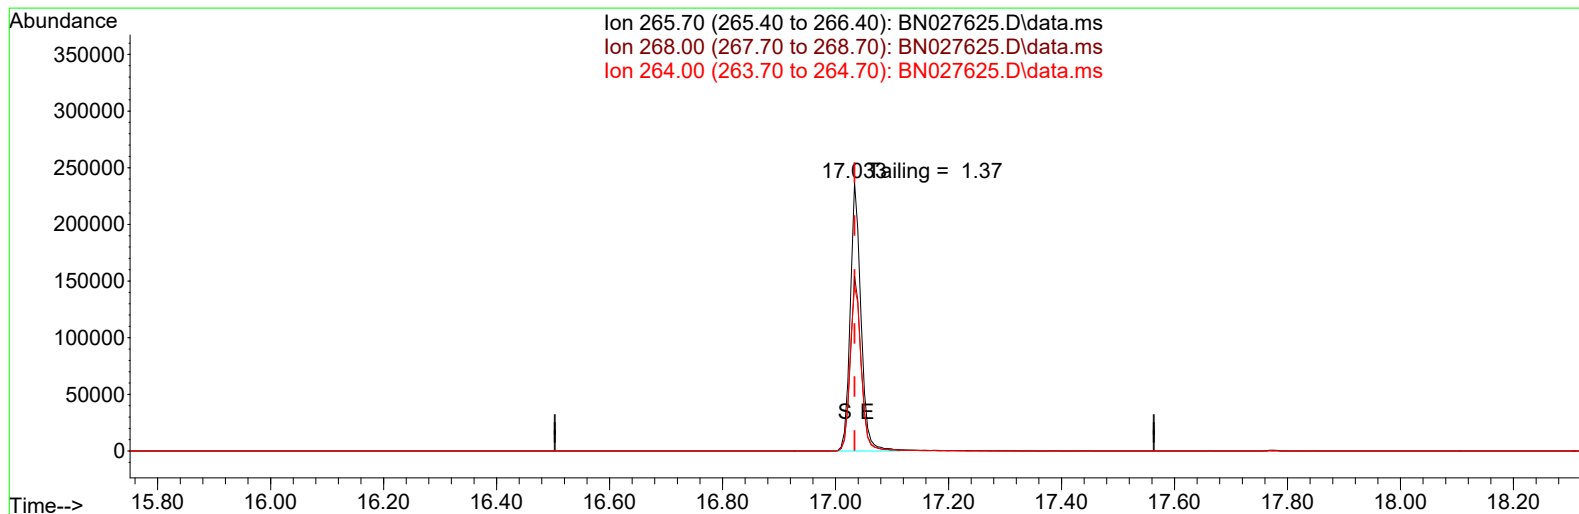

TIC: BN027625.D\data.ms

(70) Pentachlorophenol (C)




17.033min (0.000) 17754.77 ng

response 316569

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.06
264.00	61.60	61.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027625.D
Acq On : 13 Sep 2023 01:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 128 Sample Multiplier: 1

Quant Time: Sep 13 07:57:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 13 07:57:09 2023
Response via : Initial Calibration

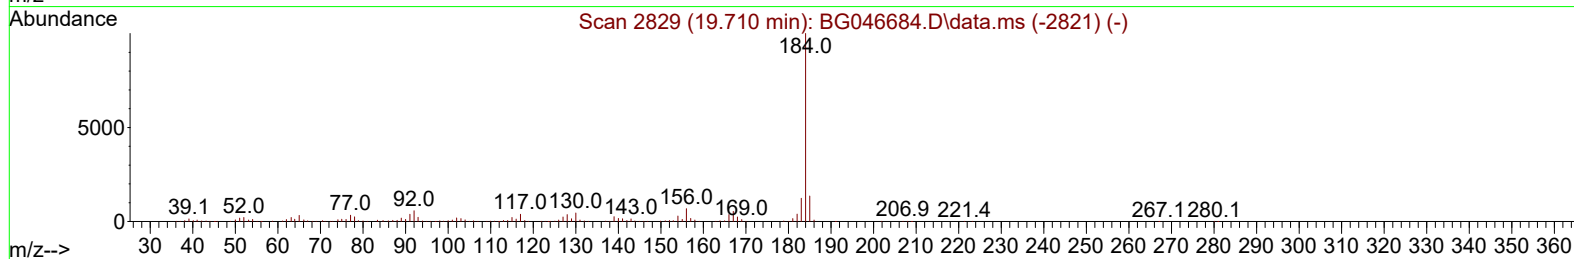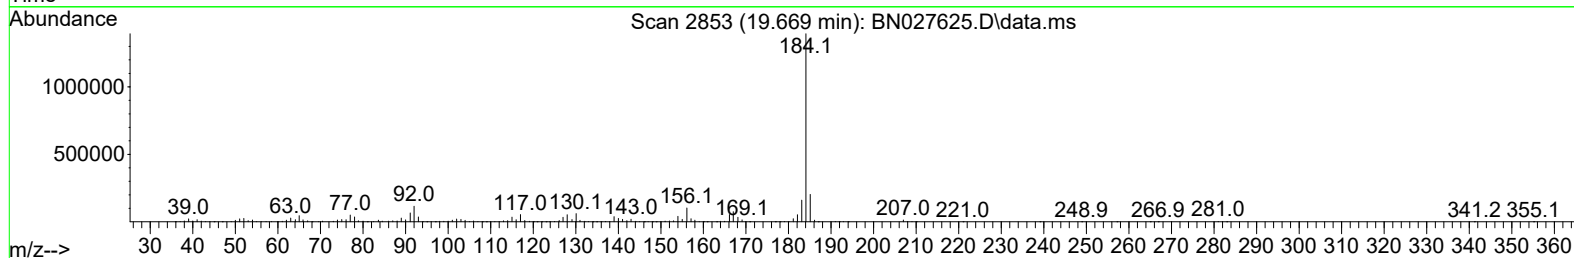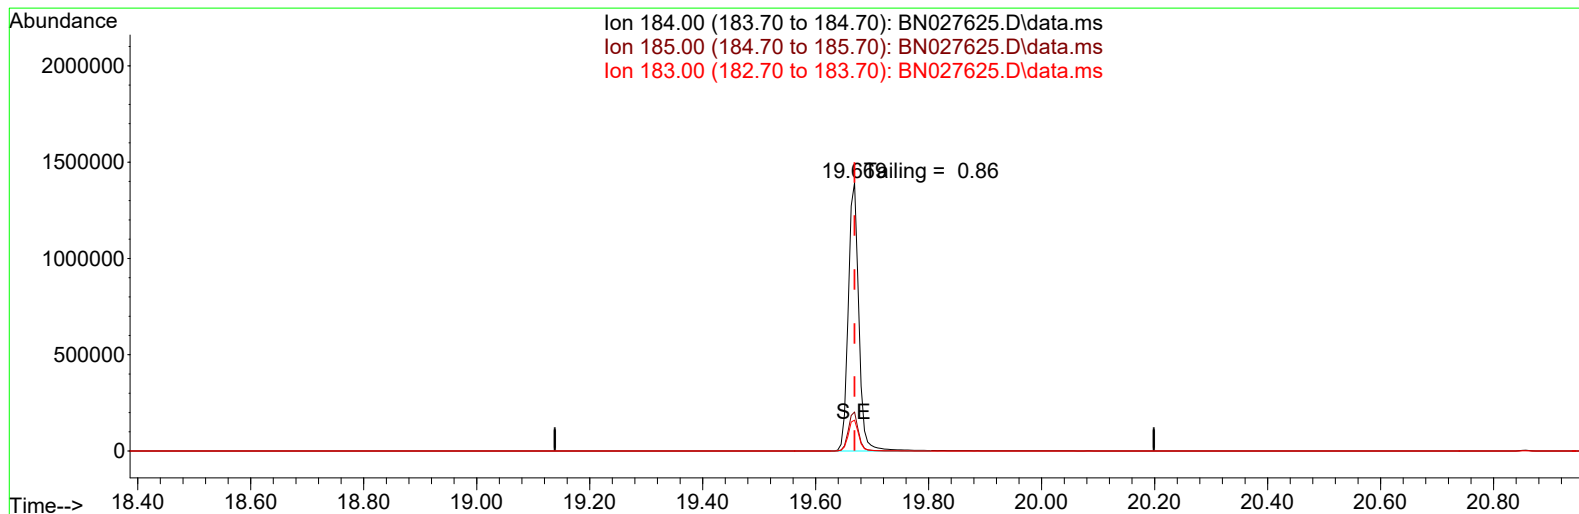

TIC: BN027625.D\data.ms

(77) Benzidine

19.669min (0.000) 0.00 ng

response 1822835

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.57
183.00	13.20	11.52
0.00	0.00	0.00