

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
 Data File : BN027598.D
 Acq On : 12 Sep 2023 06:13
 Operator : MA/JU
 Sample : 04269-02
 Misc :
 ALS Vial : 99 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW-14B-45.5-083123

Quant Time: Sep 12 08:12:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 02:45:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.037	152	6233	0.400	ng	0.00
7) Naphthalene-d8	10.853	136	16273	0.400	ng	0.00
13) Acenaphthene-d10	14.662	164	7759	0.400	ng	0.00
19) Phenanthrene-d10	17.406	188	15660	0.400	ng	0.00
29) Chrysene-d12	21.587	240	12273	0.400	ng	0.00
35) Perylene-d12	24.089	264	12097	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.574	112	3542	0.218	ng	0.00
5) Phenol-d6	7.185	99	2423	0.123	ng	0.00
8) Nitrobenzene-d5	9.230	82	5176	0.436	ng	0.00
11) 2-Methylnaphthalene-d10	12.427	152	7766	0.325	ng	0.00
14) 2,4,6-Tribromophenol	16.152	330	1354	0.471	ng	0.00
15) 2-Fluorobiphenyl	13.283	172	13852	0.470	ng	-0.01
27) Fluoranthene-d10	19.430	212	15684	0.403	ng	0.00
31) Terphenyl-d14	20.015	244	13042	0.529	ng	0.00
Target Compounds						Qvalue
34) Bis(2-ethylhexyl)phtha...	21.444	149	4157	0.205	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027598.D
Acq On : 12 Sep 2023 06:13
Operator : MA/JU
Sample : 04269-02
Misc :
ALS Vial : 99 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MW-14B-45.5-083123


Quant Time: Sep 12 08:12:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:45:58 2023
Response via : Initial Calibration

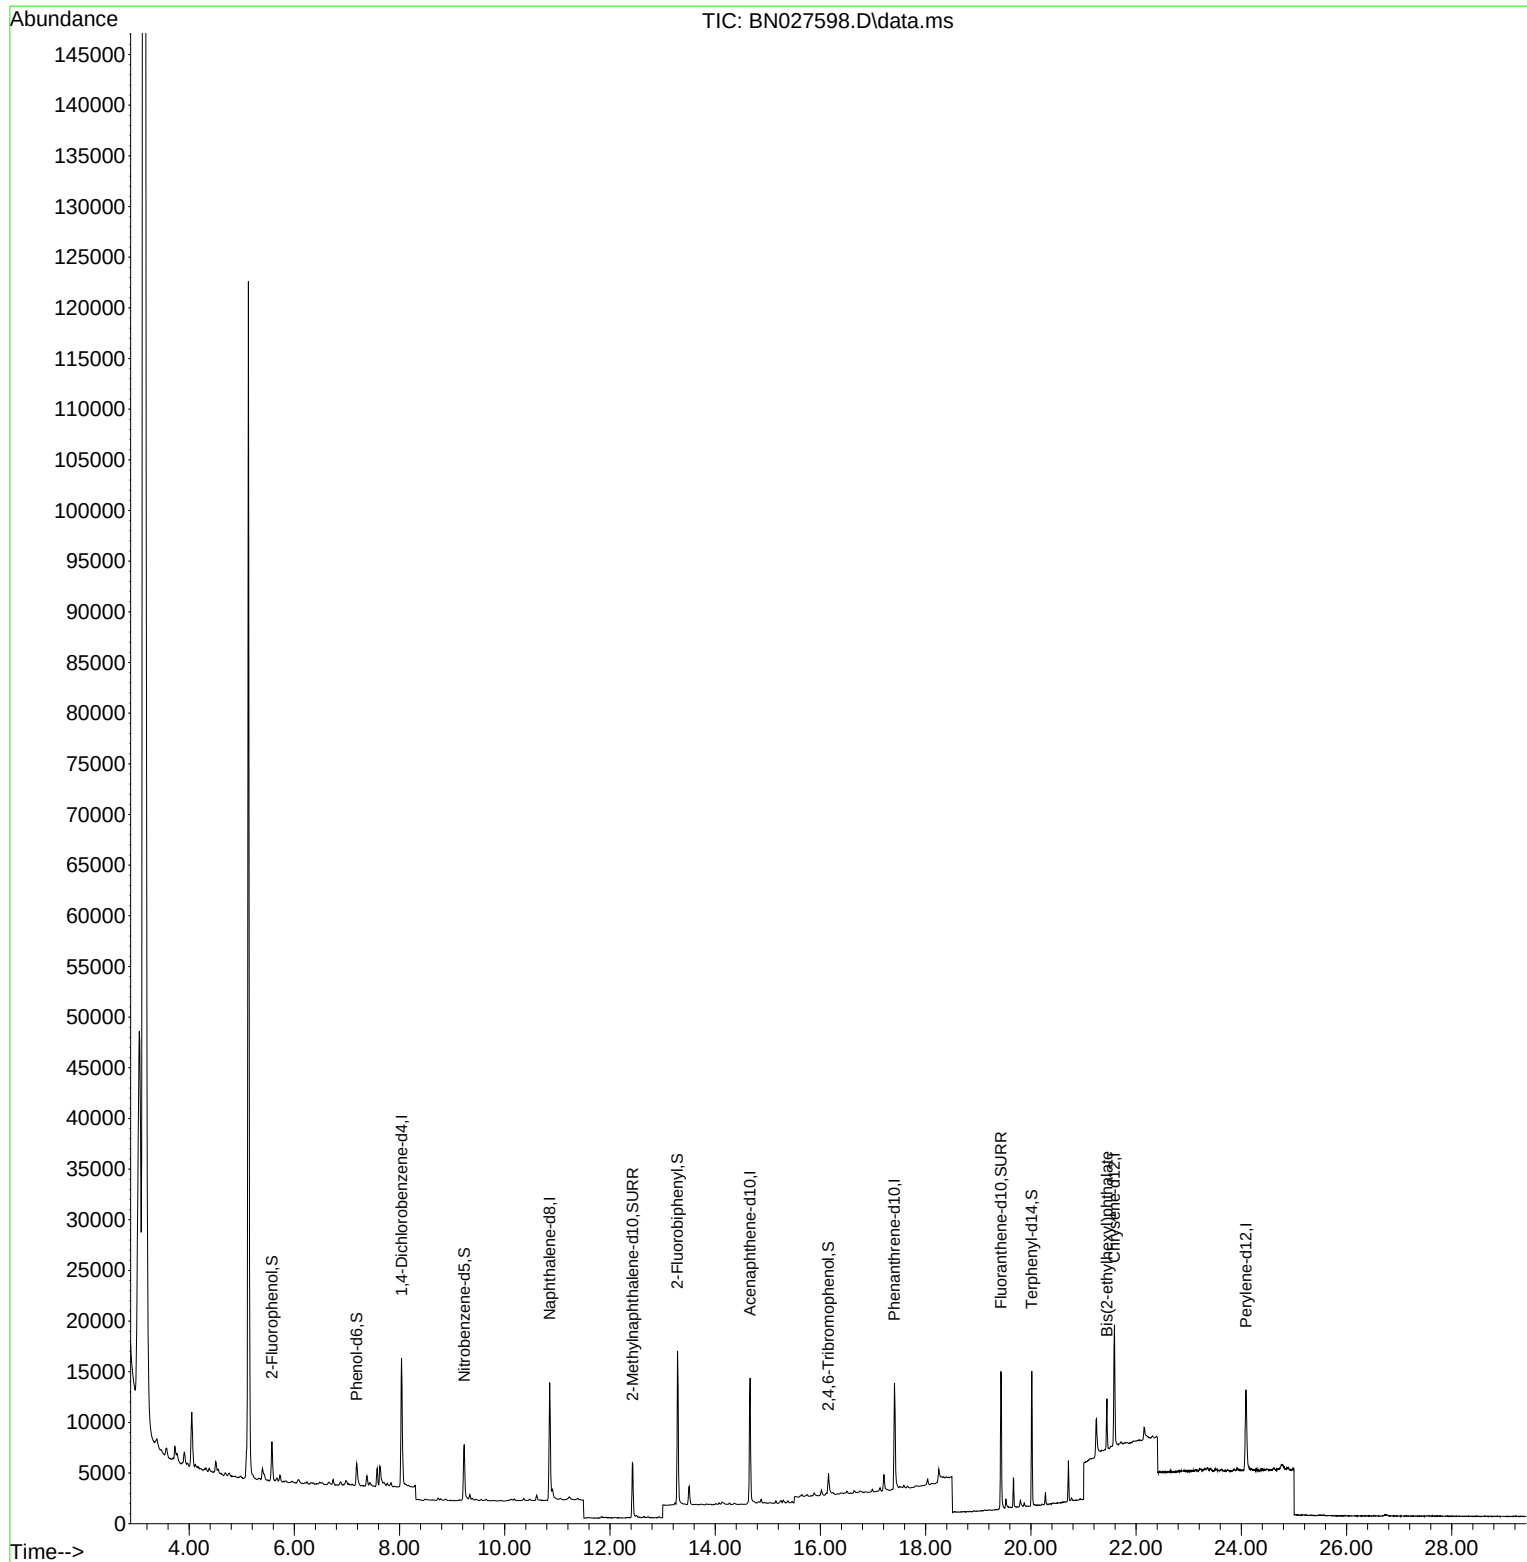



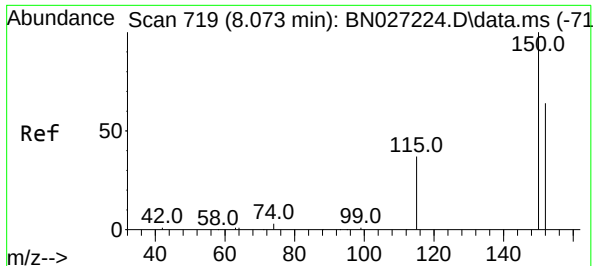


#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.037 min Scan# 719
Delta R.T. 0.000 min
Lab File: BN027598.D
Acq: 12 Sep 2023 06:13

Instrument :
BNA_N
ClientSampleId :
MW-14B-45.5-083123



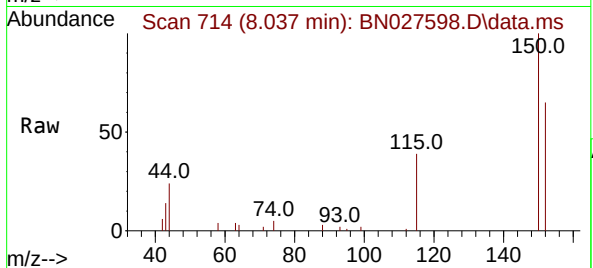



Tgt Ion:152 Resp: 6233
Ion Ratio Lower Upper
152 100
150 153.3 122.7 184.1
115 60.4 48.6 73.0

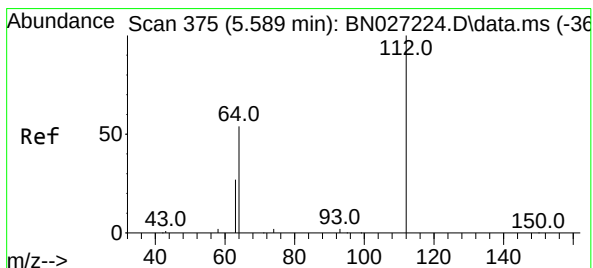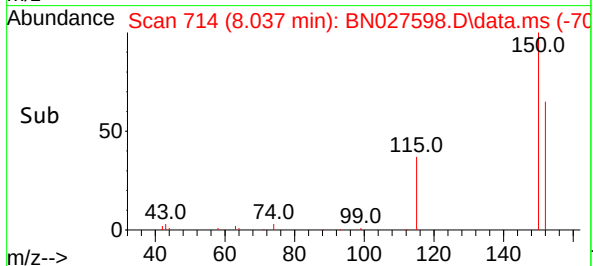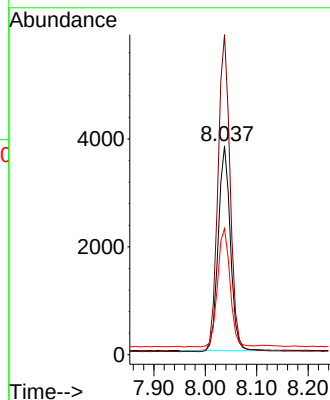

#4
2-Fluorophenol
Concen: 0.218 ng
RT: 5.574 min Scan# 373
Delta R.T. 0.000 min
Lab File: BN027598.D
Acq: 12 Sep 2023 06:13


Tgt Ion:112 Resp: 3542
Ion Ratio Lower Upper
112 100
64 54.5 44.4 66.6
63 29.1 23.1 34.7

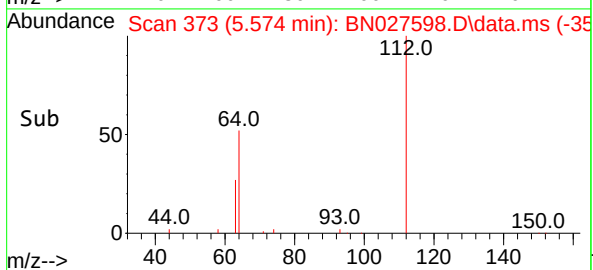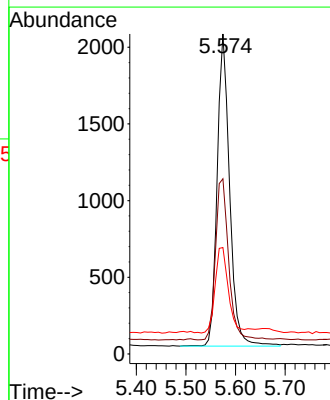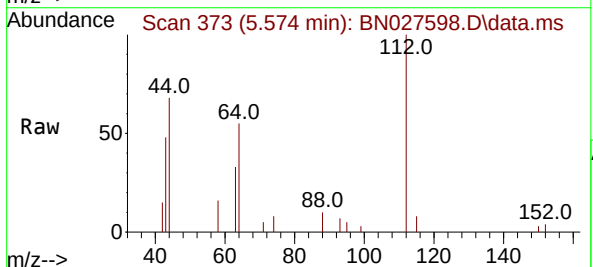



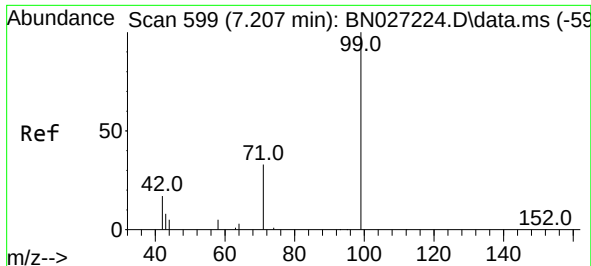


#5
Phenol-d6
Concen: 0.123 ng
RT: 7.185 min Scan# 599
Delta R.T. 0.000 min
Lab File: BN027598.D
Acq: 12 Sep 2023 06:13

Instrument :
BNA_N
ClientSampleId :
MW-14B-45.5-083123



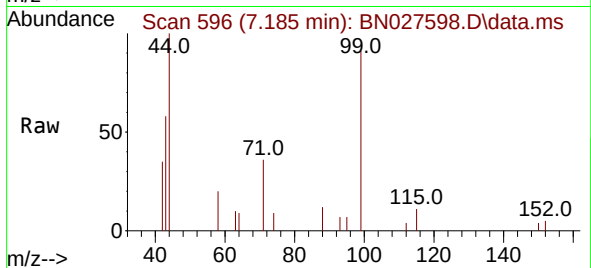



Tgt Ion	Ratio	Lower	Upper
99	100		
42	19.7	14.5	21.7
71	34.7	25.8	38.6

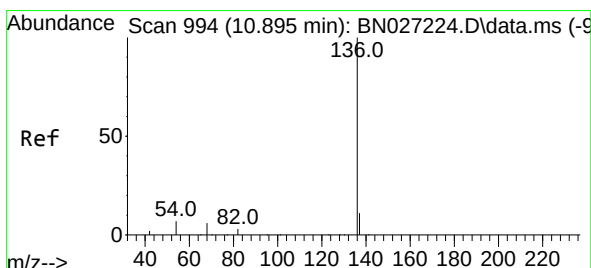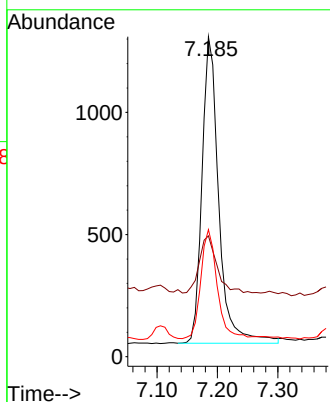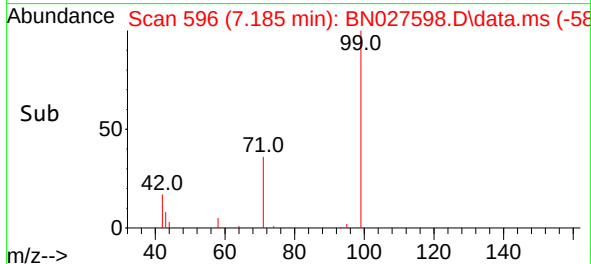

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.853 min Scan# 990
Delta R.T. 0.000 min
Lab File: BN027598.D
Acq: 12 Sep 2023 06:13

Tgt Ion	Ratio	Lower	Upper
136	100		
137	11.3	9.3	13.9
54	8.0	6.7	10.1
68	6.9	6.1	9.1


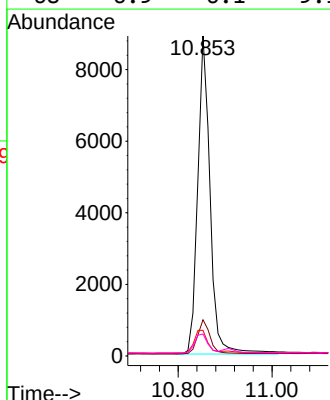
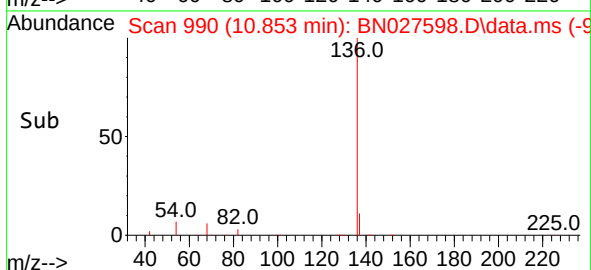
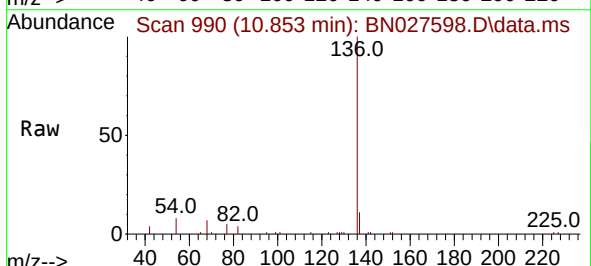


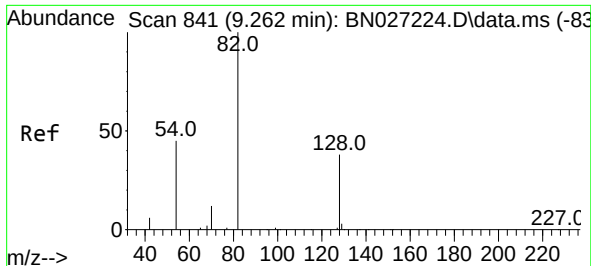

#8
Nitrobenzene-d5
Concen: 0.436 ng
RT: 9.230 min Scan# 81
Delta R.T. 0.000 min
Lab File: BN027598.D
Acq: 12 Sep 2023 06:13




Instrument :
BNA_N
ClientSampleId :
MW-14B-45.5-083123


Tgt Ion: 82 Resp: 5176
Ion Ratio Lower Upper
82 100
128 44.9 33.4 50.0
54 44.9 37.7 56.5

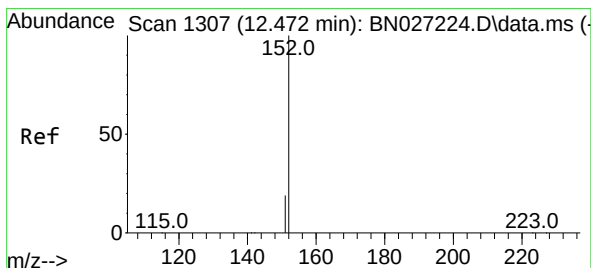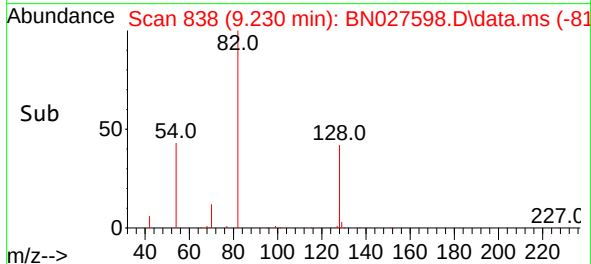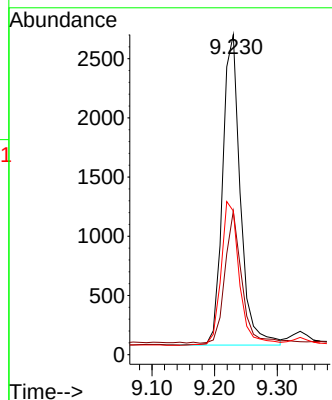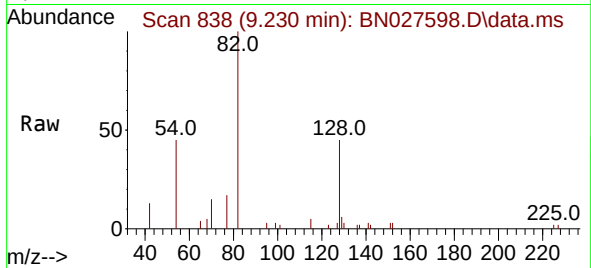

#11
2-Methylnaphthalene-d10
Concen: 0.325 ng
RT: 12.427 min Scan# 1295
Delta R.T. -0.004 min
Lab File: BN027598.D
Acq: 12 Sep 2023 06:13

Tgt Ion: 152 Resp: 7766
Ion Ratio Lower Upper
152 100
151 21.2 16.6 25.0

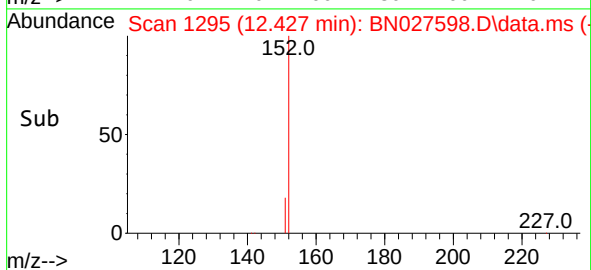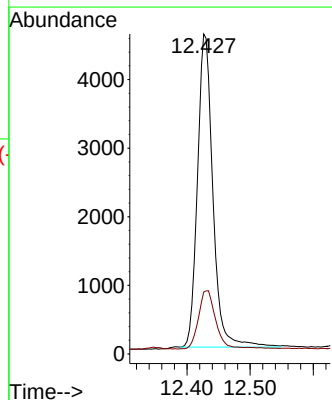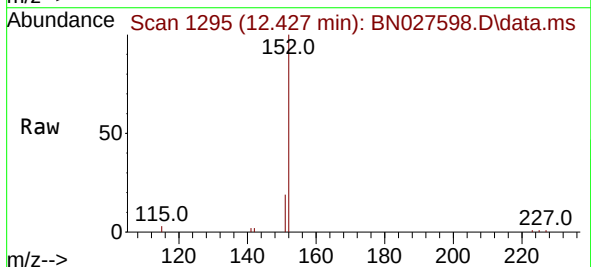

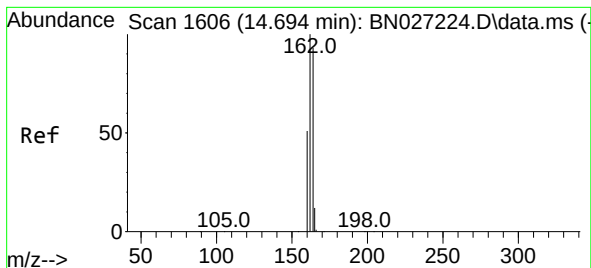

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.662 min Scan# 1603

Delta R.T. 0.000 min

Lab File: BN027598.D

Acq: 12 Sep 2023 06:13

Instrument :

BNA_N

ClientSampleId :

MW-14B-45.5-083123





Tgt Ion:164 Resp: 7759

Ion Ratio Lower Upper

164 100

162 101.7 85.8 128.8

160 49.6 44.2 66.2

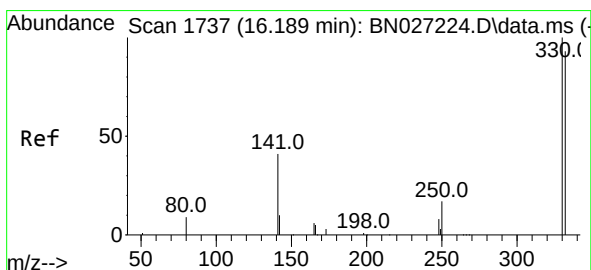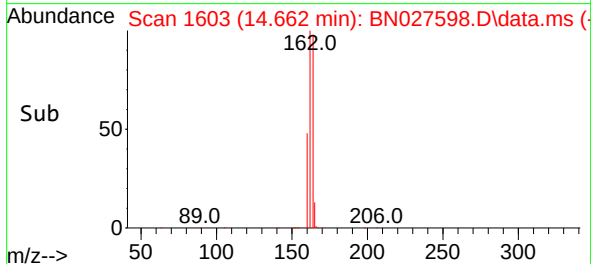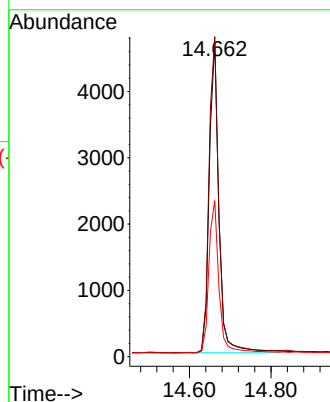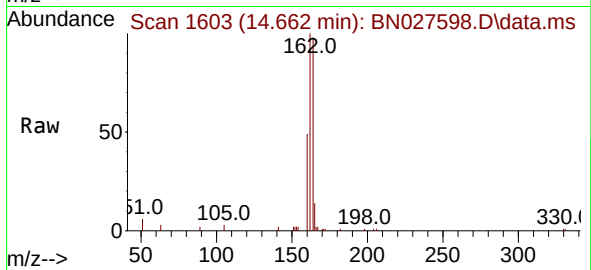

#14

2,4,6-Tribromophenol

Concen: 0.471 ng

RT: 16.152 min Scan# 1734

Delta R.T. 0.000 min

Lab File: BN027598.D

Acq: 12 Sep 2023 06:13




Tgt Ion:330 Resp: 1354


Ion Ratio Lower Upper

330 100

332 96.9 75.2 112.8

141 45.0 36.2 54.4


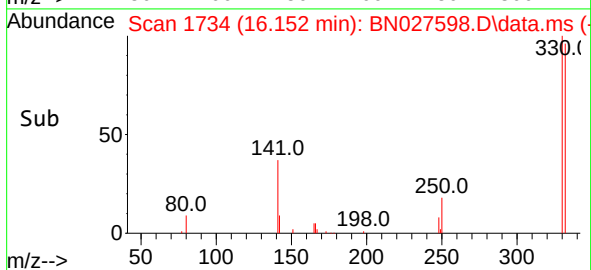
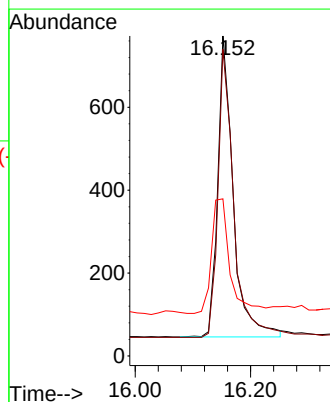
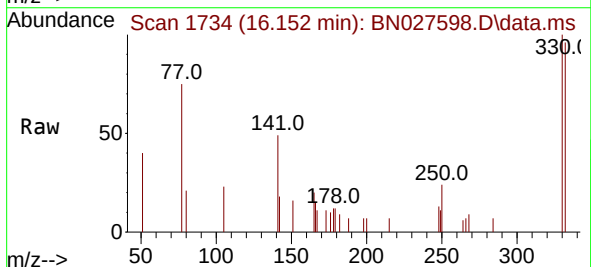


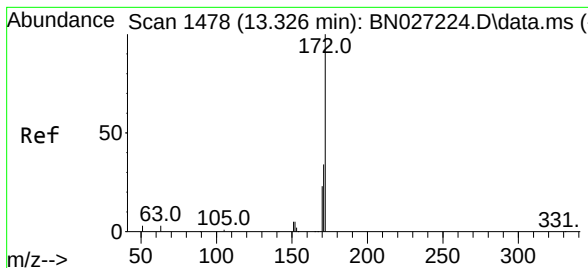

#15
2-Fluorobiphenyl
Concen: 0.470 ng
RT: 13.283 min Scan# 1478
Delta R.T. -0.011 min
Lab File: BN027598.D
Acq: 12 Sep 2023 06:13




Instrument :
BNA_N
ClientSampleId :
MW-14B-45.5-083123


Tgt Ion:172 Resp: 13852
Ion Ratio Lower Upper
172 100
171 35.3 27.8 41.8
170 24.0 19.3 28.9

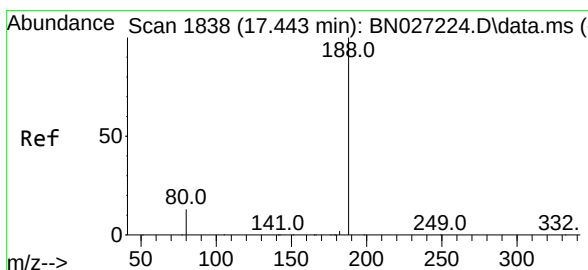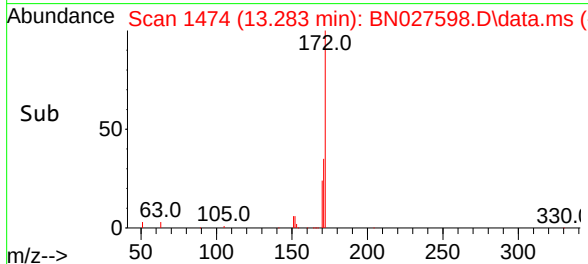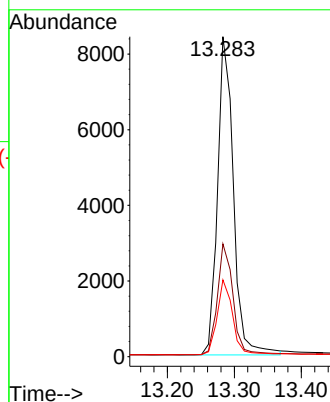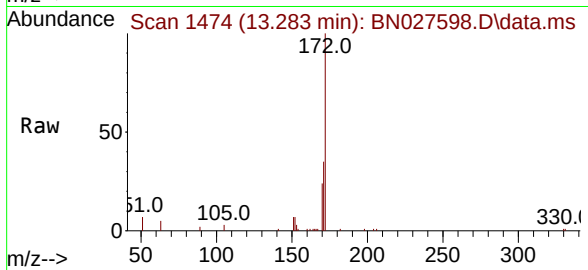

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.406 min Scan# 1835
Delta R.T. 0.000 min
Lab File: BN027598.D
Acq: 12 Sep 2023 06:13

Tgt Ion:188 Resp: 15660
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 13.9 11.0 16.6


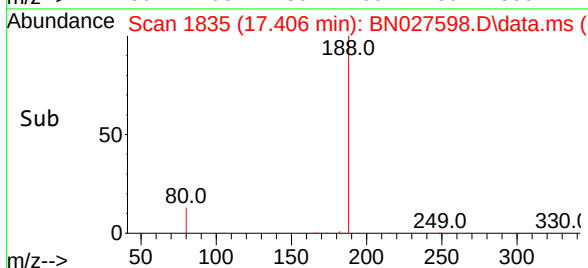
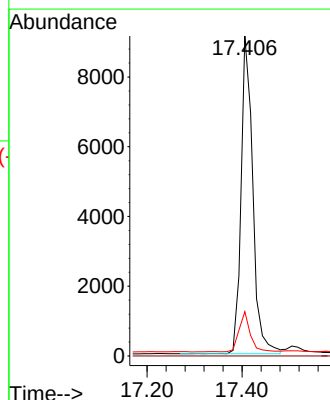
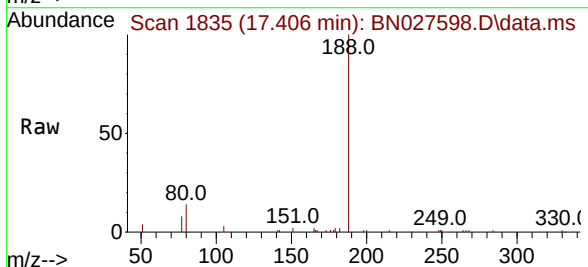


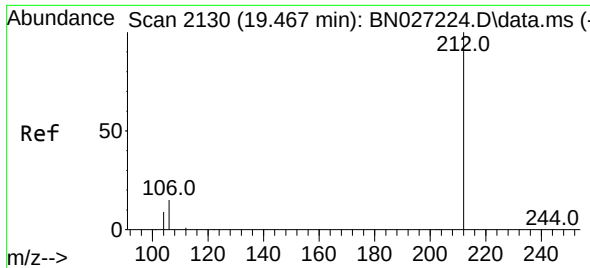

#27
Fluoranthene-d10
Concen: 0.403 ng
RT: 19.430 min Scan# 2130
Delta R.T. -0.005 min
Lab File: BN027598.D
Acq: 12 Sep 2023 06:13




Instrument :
BNA_N
ClientSampleId :
MW-14B-45.5-083123


Tgt Ion:212 Resp: 15684
Ion Ratio Lower Upper
212 100
106 14.4 12.1 18.1
104 8.3 6.9 10.3

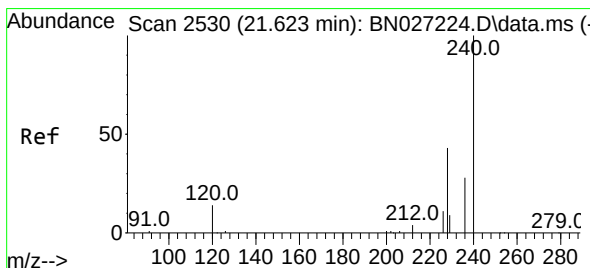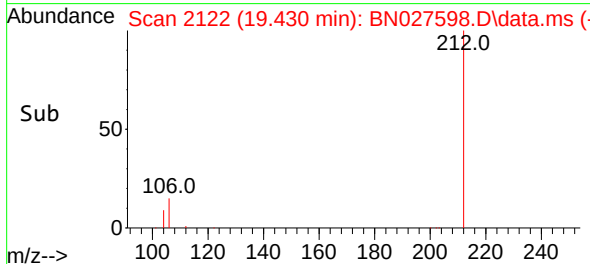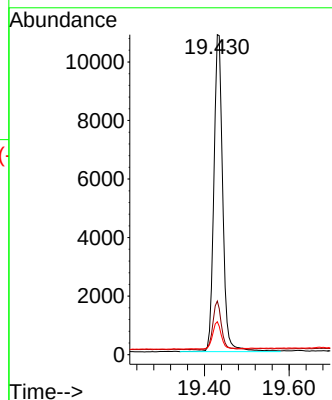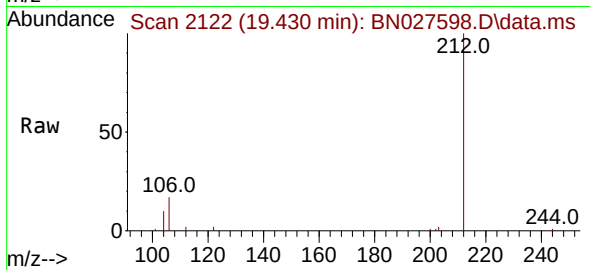

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.587 min Scan# 2526
Delta R.T. 0.000 min
Lab File: BN027598.D
Acq: 12 Sep 2023 06:13

Tgt Ion:240 Resp: 12273
Ion Ratio Lower Upper
240 100
120 16.3 14.2 21.4
236 28.8 22.9 34.3


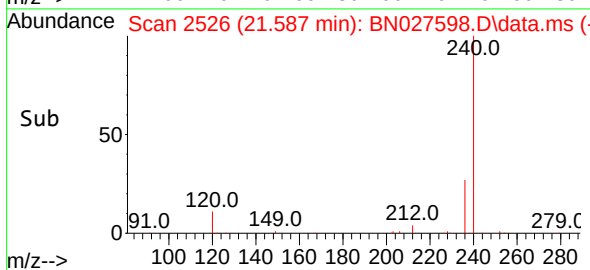
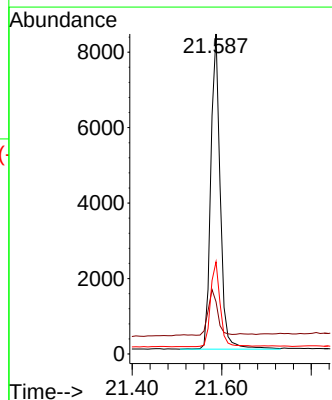
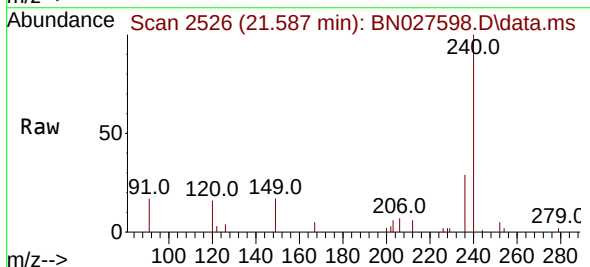


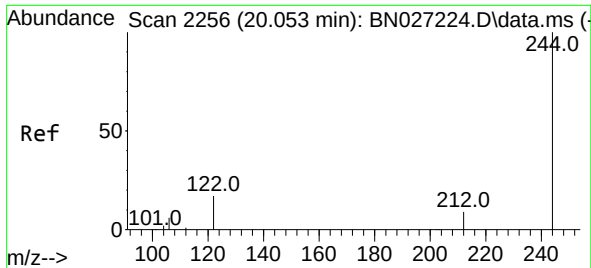

#31
 Terphenyl-d14
 Concen: 0.529 ng
 RT: 20.015 min Scan# 21
 Delta R.T. -0.005 min
 Lab File: BN027598.D
 Acq: 12 Sep 2023 06:13




Instrument :
 BNA_N
 ClientSampleId :
 MW-14B-45.5-083123


Tgt Ion:244 Resp: 13042
 Ion Ratio Lower Upper
 244 100
 212 9.9 7.5 11.3
 122 18.3 14.0 21.0

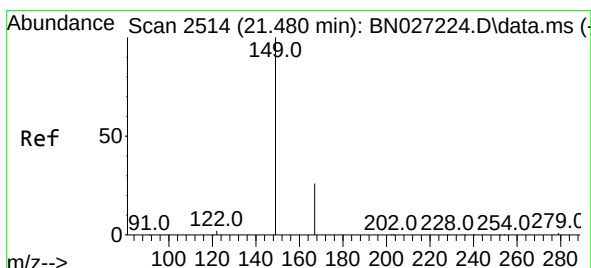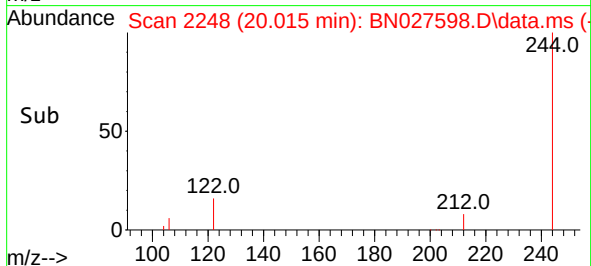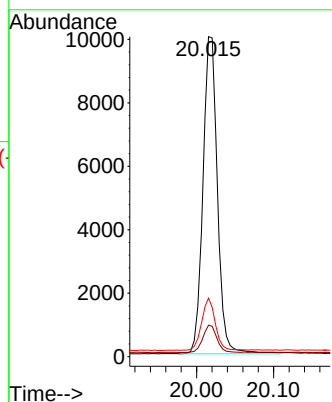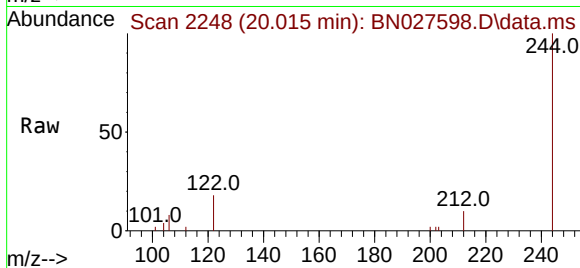

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.205 ng
 RT: 21.444 min Scan# 2510
 Delta R.T. 0.000 min
 Lab File: BN027598.D
 Acq: 12 Sep 2023 06:13

Tgt Ion:149 Resp: 4157
 Ion Ratio Lower Upper
 149 100
 167 27.4 22.1 33.1
 279 3.5 2.7 4.1

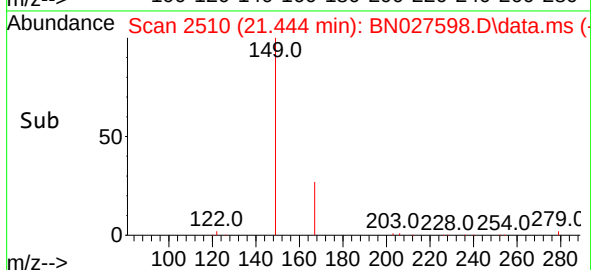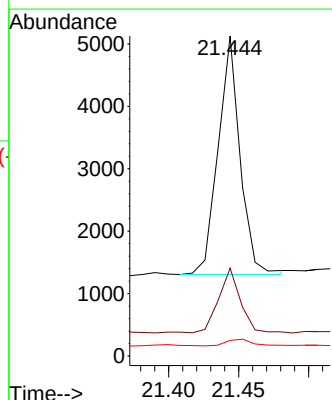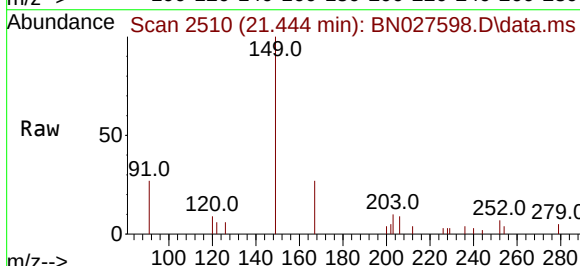

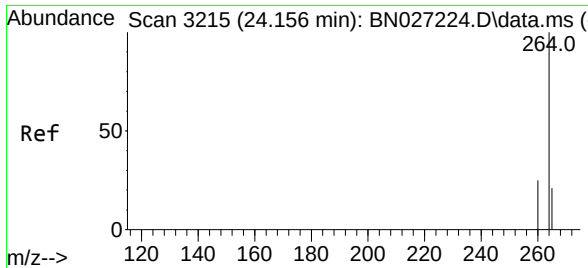

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.089 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BN027598.D
 Acq: 12 Sep 2023 06:13

Instrument :
 BNA_N
 ClientSampleId :
 MW-14B-45.5-083123

Tgt Ion:264	Resp:	12097
Ion	Ratio	Lower Upper
264	100	
260	26.0	20.7 31.1
265	74.1	53.3 79.9

