

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
 Data File : BN027611.D
 Acq On : 12 Sep 2023 15:41
 Operator : MA/JU
 Sample : PB155426BL
 Misc :
 ALS Vial : 113 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB155426BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

Quant Time: Sep 12 16:53:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 02:45:58 2023
 Response via : Initial Calibration

09/13/2023
 Supervised By :mohammad
 ahmed

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.037	152	5025	0.400	ng	0.00
7) Naphthalene-d8	10.853	136	12840	0.400	ng	0.00
13) Acenaphthene-d10	14.662	164	5791	0.400	ng	0.00
19) Phenanthrene-d10	17.418	188	11586	0.400	ng	0.01
29) Chrysene-d12	21.596	240	8408	0.400	ng	0.00
35) Perylene-d12	24.107	264	7819	0.400	ng	# 0.01

09/13/2023
 Supervised By :mohammad
 ahmed

System Monitoring Compounds						
4) 2-Fluorophenol	5.574	112	5892	0.450	ng	0.00
5) Phenol-d6	7.185	99	6071	0.381	ng	0.00
8) Nitrobenzene-d5	9.230	82	5095	0.544	ng	0.00
11) 2-Methylnaphthalene-d10	12.434	152	7456	0.395	ng	0.00
14) 2,4,6-Tribromophenol	16.177	330	674m	0.314	ng	0.02
15) 2-Fluorobiphenyl	13.293	172	12009m	0.545	ng	0.00
27) Fluoranthene-d10	19.439	212	12180	0.423	ng	0.00
31) Terphenyl-d14	20.025	244	10593	0.627	ng	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027611.D
Acq On : 12 Sep 2023 15:41
Operator : MA/JU
Sample : PB155426BL
Misc :
ALS Vial : 113 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB155426BL

Quant Time: Sep 12 16:53:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:45:58 2023
Response via : Initial Calibration


Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

09/13/2023
Supervised By :mohammad
ahmed

~~09/13/2023~~
Supervised By :mohammad
ahmed


09/14/2023

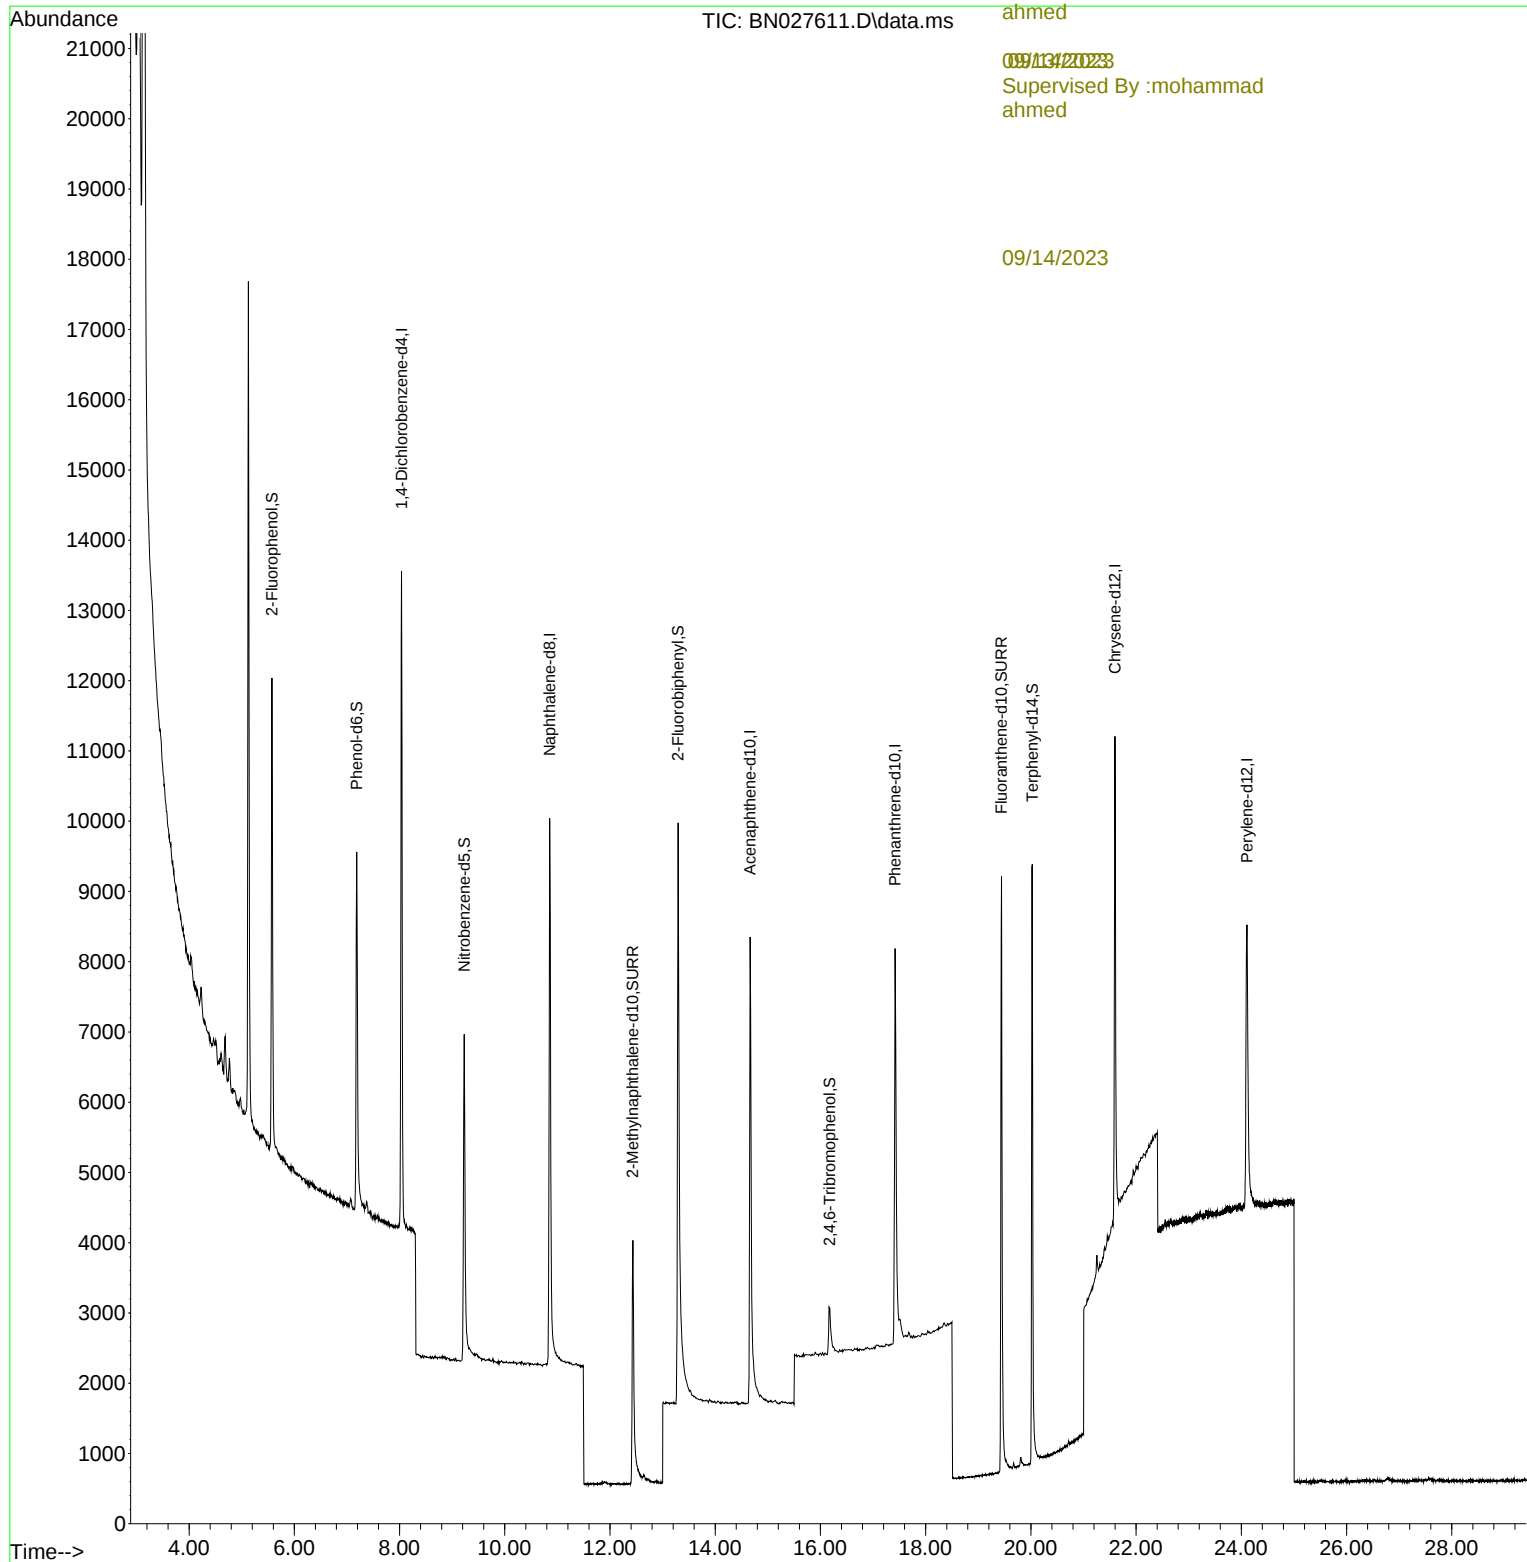



#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.037 min Scan# 719
Delta R.T. 0.000 min
Lab File: BN027611.D
Acq: 12 Sep 2023 15:41

Instrument :
BNA_N
ClientSampleId :
PB155426BL

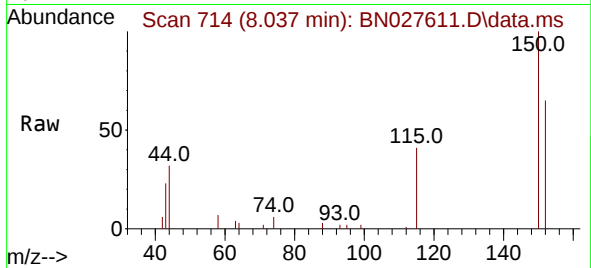



Tgt Ion:152 Resp: 502
Ion Ratio Lower Upper
152 100
150 153.7 122.7 184.1
115 63.1 48.6 73.0

Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel

09/13/2023
Supervised By :mohammad
ahmed

09/13/2023
Supervised By :mohammad
ahmed


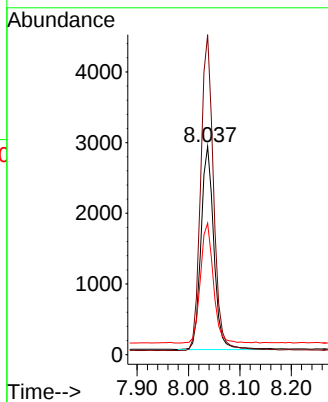
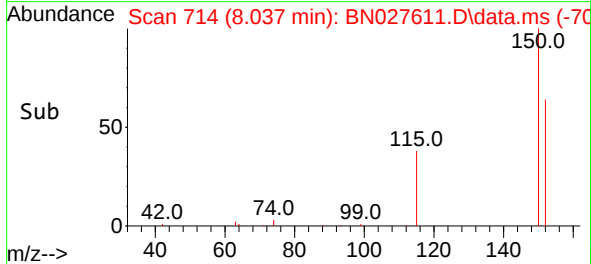


09/14/2023

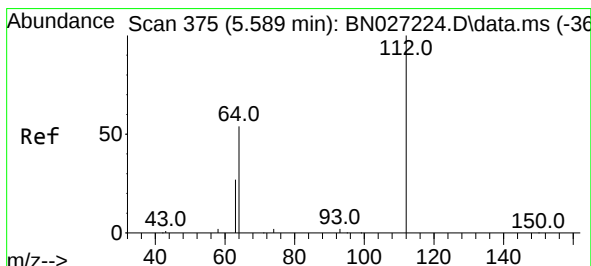

#4
2-Fluorophenol
Concen: 0.450 ng
RT: 5.574 min Scan# 373
Delta R.T. 0.000 min
Lab File: BN027611.D
Acq: 12 Sep 2023 15:41


Tgt Ion:112 Resp: 5892
Ion Ratio Lower Upper
112 100
64 56.1 44.4 66.6
63 29.4 23.1 34.7

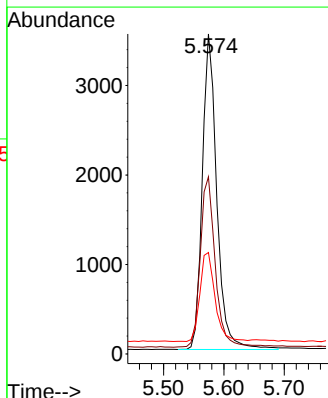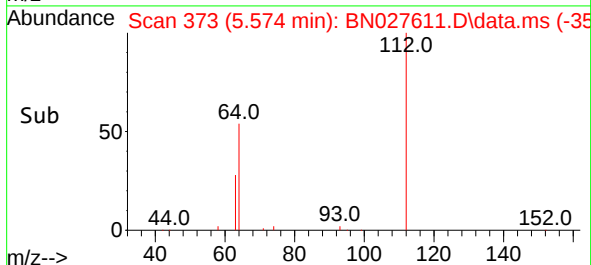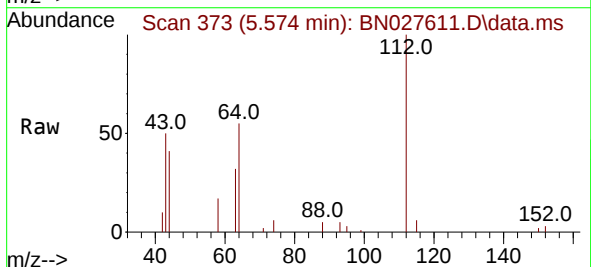



#5
Phenol-d6
Concen: 0.381 ng
RT: 7.185 min Scan# 599
Delta R.T. 0.000 min
Lab File: BN027611.D
Acq: 12 Sep 2023 15:41

Instrument :
BNA_N
ClientSampleId :
PB155426BL

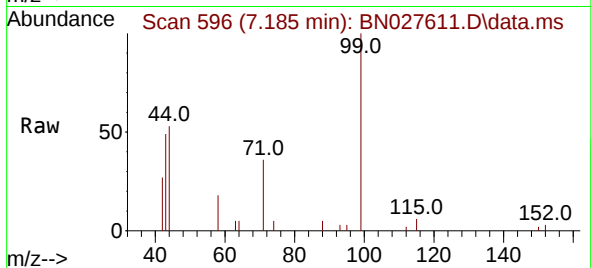



Tgt Ion: 99 Resp: 607
Ion Ratio Lower Upper
99 100
42 19.1 14.5 21.7
71 34.0 25.8 38.6

Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel

09/13/2023
Supervised By :mohammad
ahmed

09/13/2023
Supervised By :mohammad
ahmed


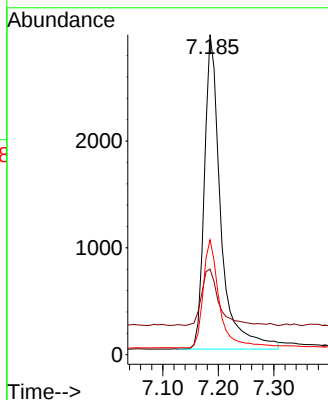
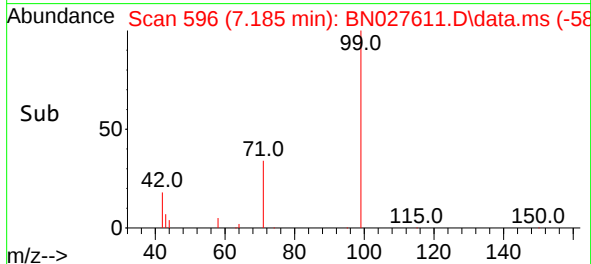


09/14/2023

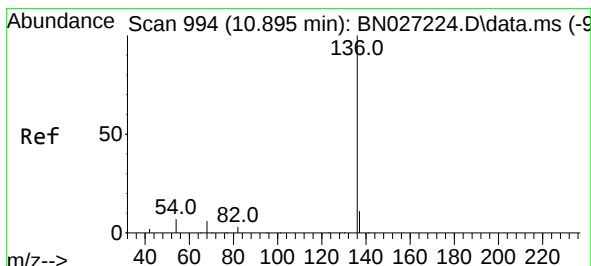

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.853 min Scan# 990
Delta R.T. 0.000 min
Lab File: BN027611.D
Acq: 12 Sep 2023 15:41


Tgt Ion:136 Resp: 12840
Ion Ratio Lower Upper
136 100
137 11.7 9.3 13.9
54 9.0 6.7 10.1
68 7.9 6.1 9.1

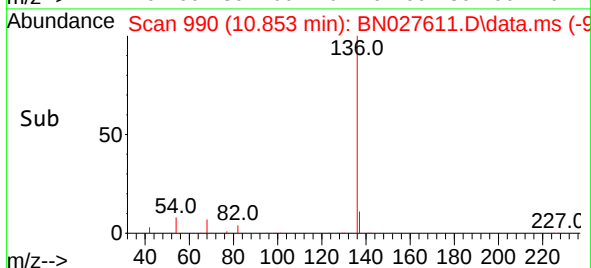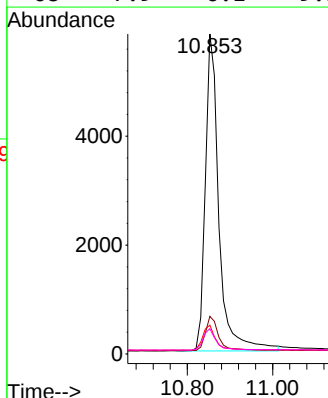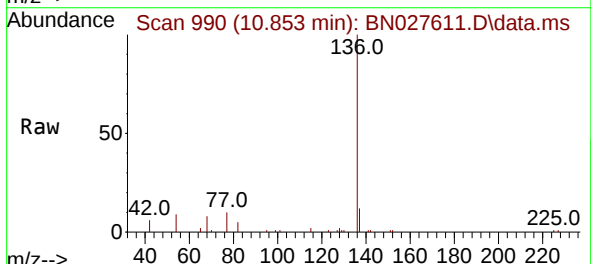



#8
Nitrobenzene-d5
Concen: 0.544 ng
RT: 9.230 min Scan# 81
Delta R.T. 0.000 min
Lab File: BN027611.D
Acq: 12 Sep 2023 15:41

Instrument :
BNA_N
ClientSampleId :
PB155426BL

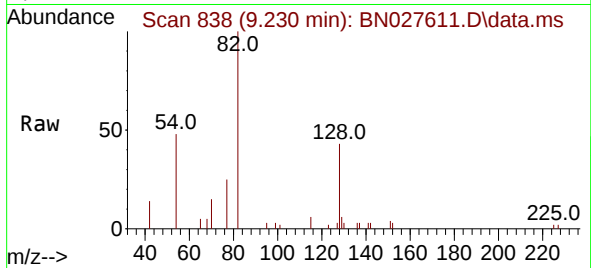



Tgt Ion: 82 Resp: 509
Ion Ratio Lower Upper
82 100
128 43.0 33.4 50.0
54 48.0 37.7 56.5

Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel

09/13/2023
Supervised By :mohammad
ahmed

09/13/2023
Supervised By :mohammad
ahmed


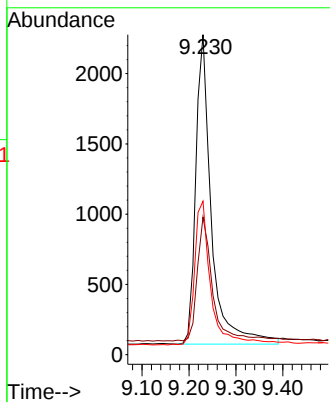
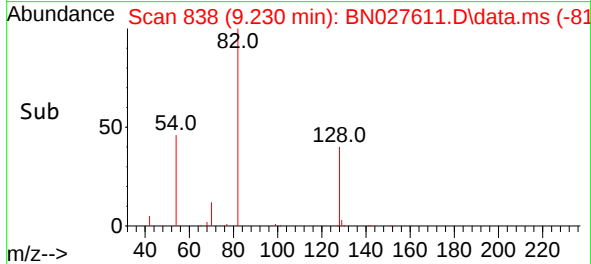



09/14/2023

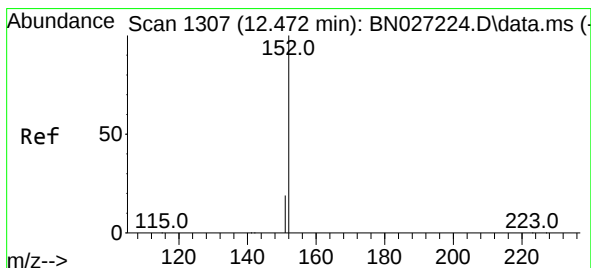

#11
2-Methylnaphthalene-d10
Concen: 0.395 ng
RT: 12.434 min Scan# 1297
Delta R.T. 0.004 min
Lab File: BN027611.D
Acq: 12 Sep 2023 15:41


Tgt Ion:152 Resp: 7456
Ion Ratio Lower Upper
152 100
151 19.4 16.6 25.0

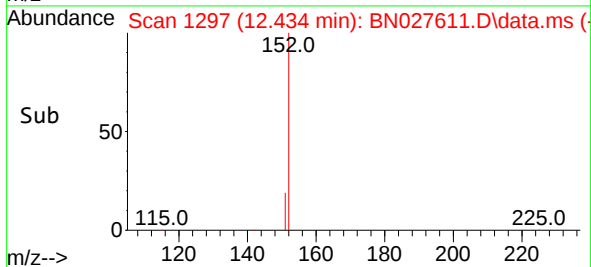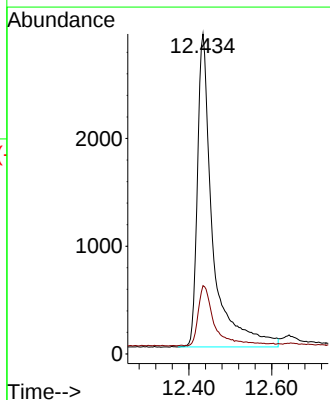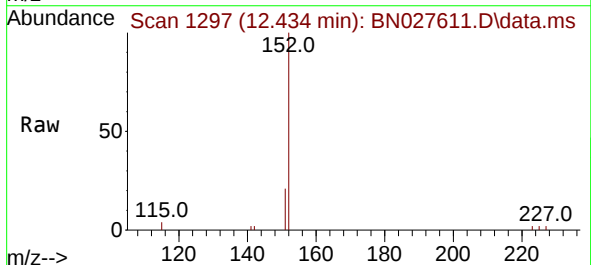

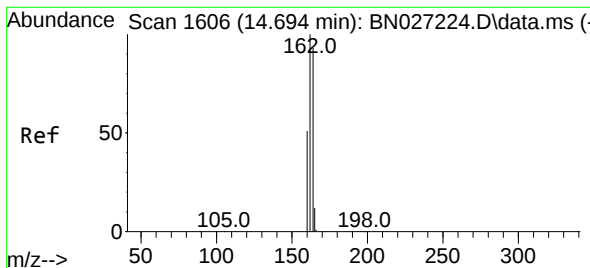

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.662 min Scan# 1603
Delta R.T. 0.000 min
Lab File: BN027611.D
Acq: 12 Sep 2023 15:41

Instrument :
BNA_N
ClientSampleId :
PB155426BL

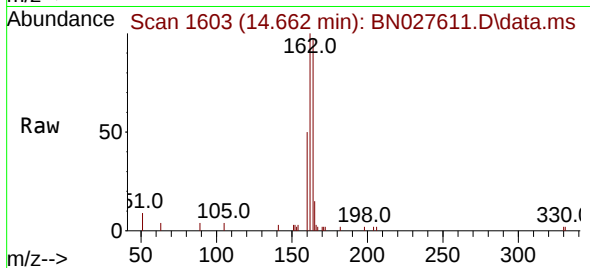



Tgt Ion:164 Resp: 579
Ion Ratio Lower Upper
164 100
162 103.5 85.8 128.8
160 51.8 44.2 66.2

Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel

09/13/2023
Supervised By :mohammad
ahmed


09/13/2023
Supervised By :mohammad
ahmed

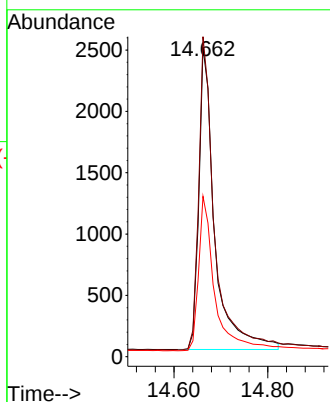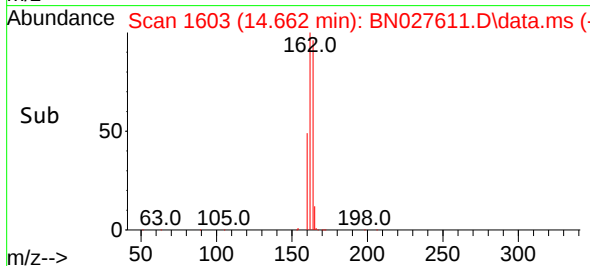



09/14/2023

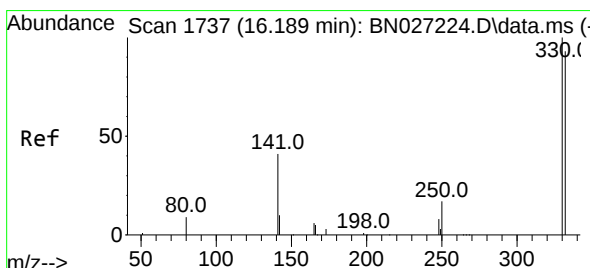


#14
2,4,6-Tribromophenol
Concen: 0.314 ng m
RT: 16.177 min Scan# 1736
Delta R.T. 0.025 min
Lab File: BN027611.D
Acq: 12 Sep 2023 15:41

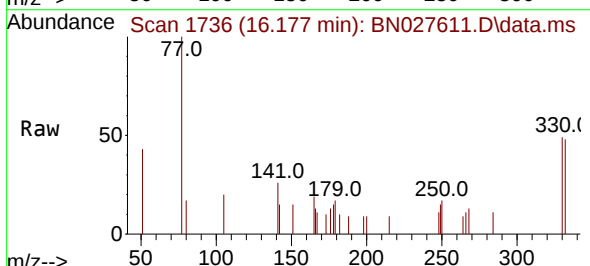


Tgt Ion:330 Resp: 674
Ion Ratio Lower Upper
330 100
332 88.4 75.2 112.8
141 45.0 36.2 54.4

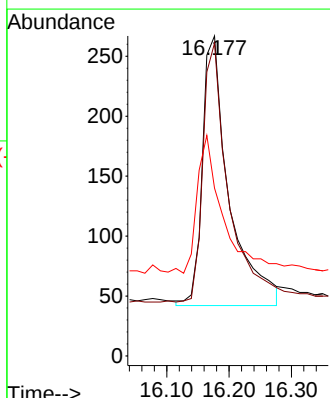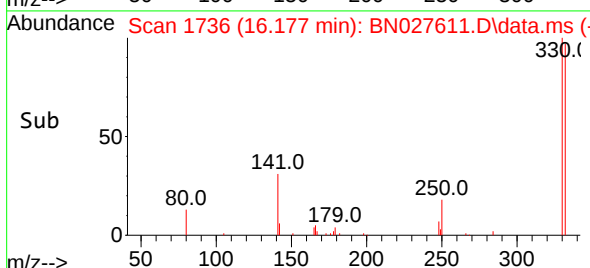

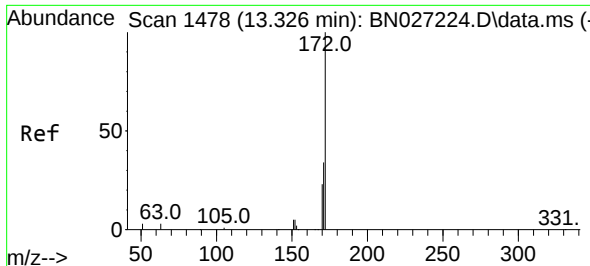

#15
2-Fluorobiphenyl
Concen: 0.545 ng m
RT: 13.293 min Scan# 1478
Delta R.T. 0.000 min
Lab File: BN027611.D
Acq: 12 Sep 2023 15:41

Instrument :
BNA_N
ClientSampleId :
PB155426BL

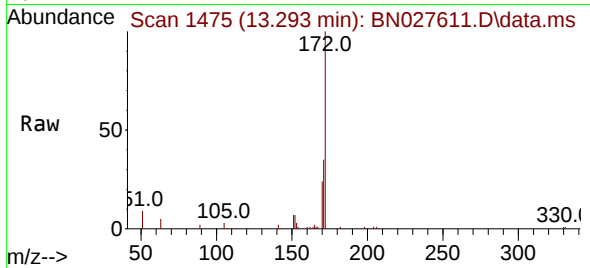



Tgt Ion:172 Resp: 12009
Ion Ratio Lower Upper
172 100
171 35.0 27.8 41.8
170 24.2 19.3 28.9

Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel

09/13/2023
Supervised By :mohammad
ahmed

09/13/2023
Supervised By :mohammad
ahmed


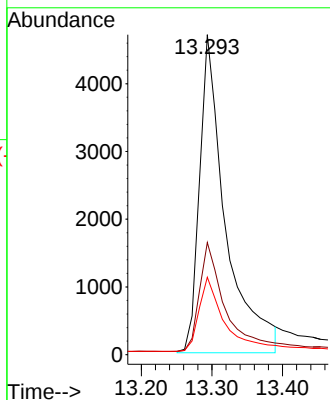
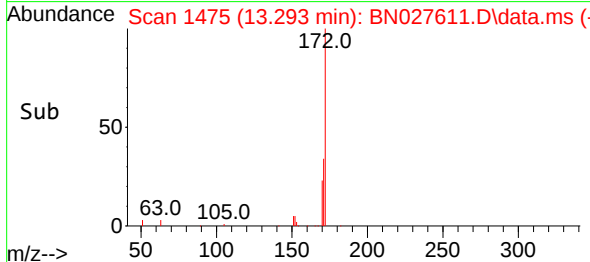



09/14/2023

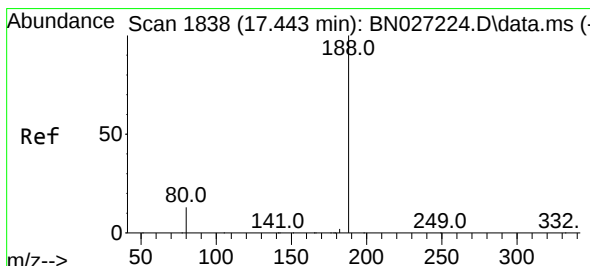

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.418 min Scan# 1836
Delta R.T. 0.012 min
Lab File: BN027611.D
Acq: 12 Sep 2023 15:41


Tgt Ion:188 Resp: 11586
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 13.4 11.0 16.6

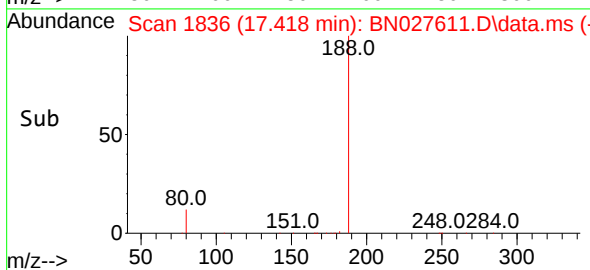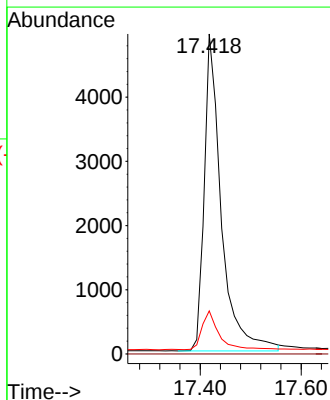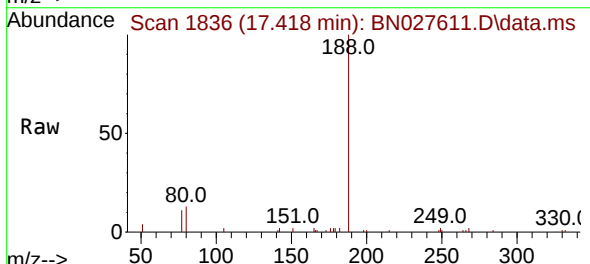

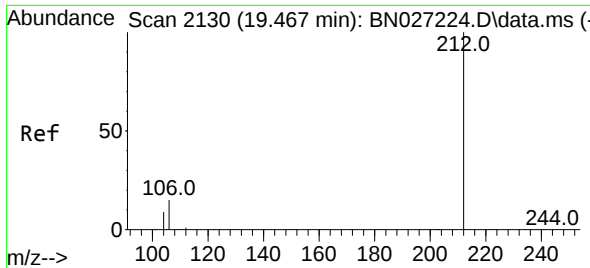

#27
Fluoranthene-d10
Concen: 0.423 ng
RT: 19.439 min Scan# 2118
Delta R.T. 0.005 min
Lab File: BN027611.D
Acq: 12 Sep 2023 15:41



Instrument :
BNA_N
ClientSampleId :
PB155426BL

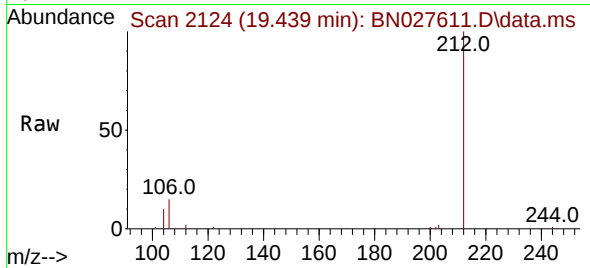

Tgt Ion:212 Resp: 12180
Ion Ratio Lower Upper
212 100
106 14.4 12.1 18.1
104 8.3 6.9 10.3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/13/2023
Supervised By :mohammad ahmed 09/14/2023

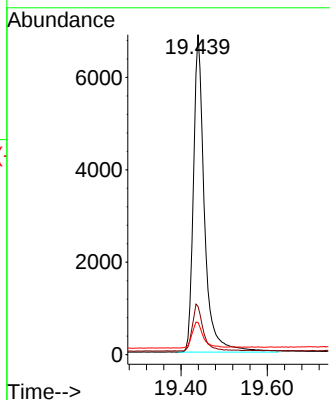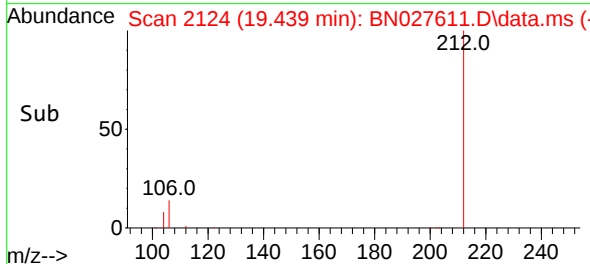




09/13/2023
Supervised By :mohammad
ahmed


09/14/2023

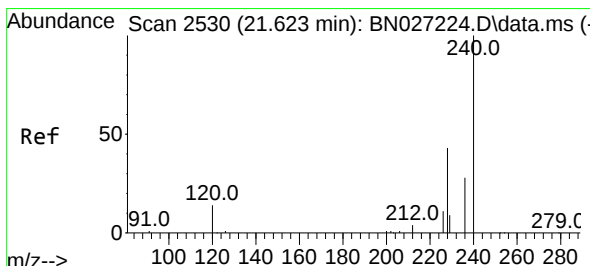

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.596 min Scan# 2527
Delta R.T. 0.009 min
Lab File: BN027611.D
Acq: 12 Sep 2023 15:41

Tgt Ion:240 Resp: 8408
Ion Ratio Lower Upper
240 100
120 20.7 14.2 21.4
236 29.9 22.9 34.3

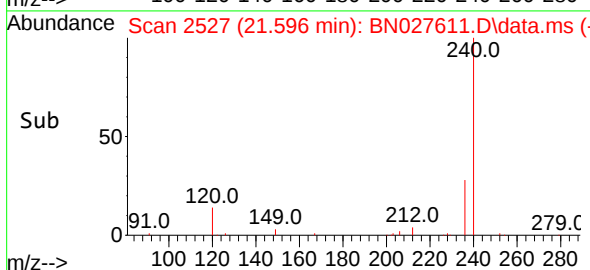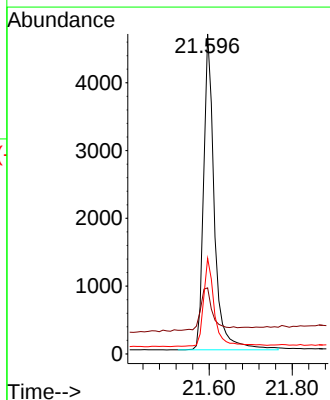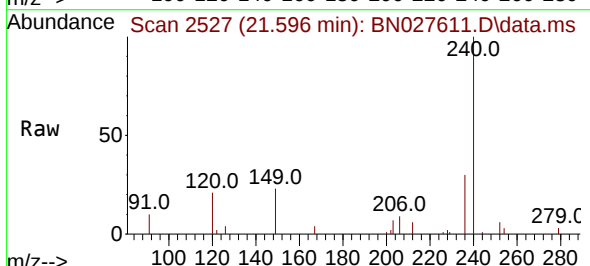

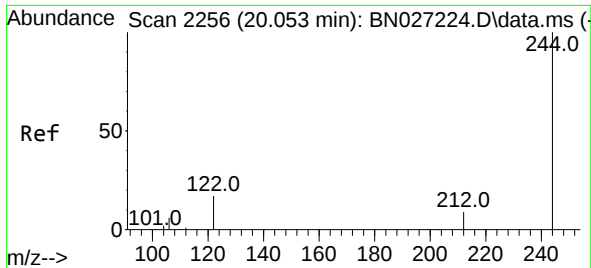

#31
Terphenyl-d14
Concen: 0.627 ng
RT: 20.025 min Scan# 21
Delta R.T. 0.005 min
Lab File: BN027611.D
Acq: 12 Sep 2023 15:41

Instrument :

BNA_N

ClientSampleId :

PB155426BL



Tgt Ion:244 Resp: 1059
Ion Ratio Lower Upper
244 100
212 9.4 7.5 11.3
122 15.6 14.0 21.0

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 09/13/2023



Supervised By :mohammad ahmed 09/14/2023

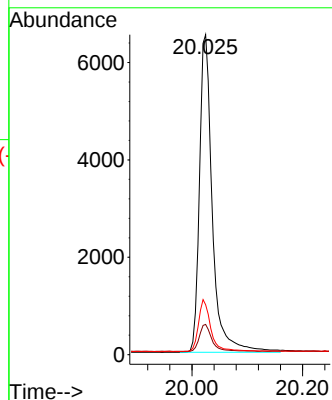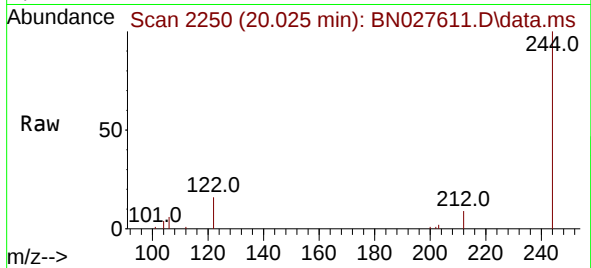

09/13/2023

Supervised By :mohammad
ahmed

09/14/2023

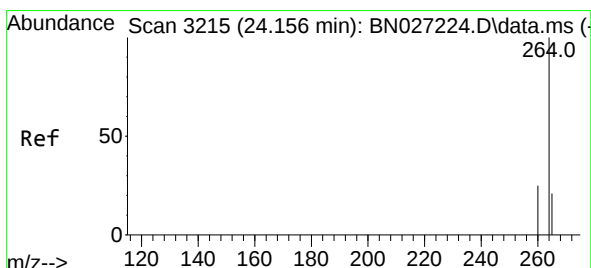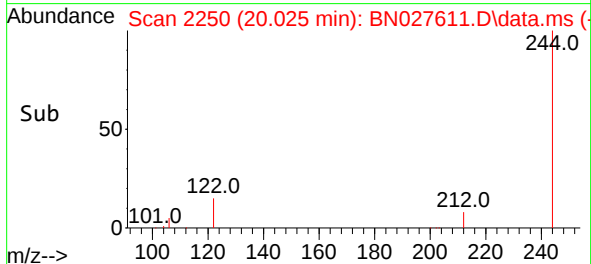

#35
Perylene-d12
Concen: 0.400 ng
RT: 24.107 min Scan# 3198
Delta R.T. 0.012 min
Lab File: BN027611.D
Acq: 12 Sep 2023 15:41

Tgt Ion:264 Resp: 7819
Ion Ratio Lower Upper
264 100
260 26.2 20.7 31.1
265 116.3 53.3 79.9#

