


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
 Data File : BN027589.D
 Acq On : 12 Sep 2023 00:41
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 02:45:58 2023

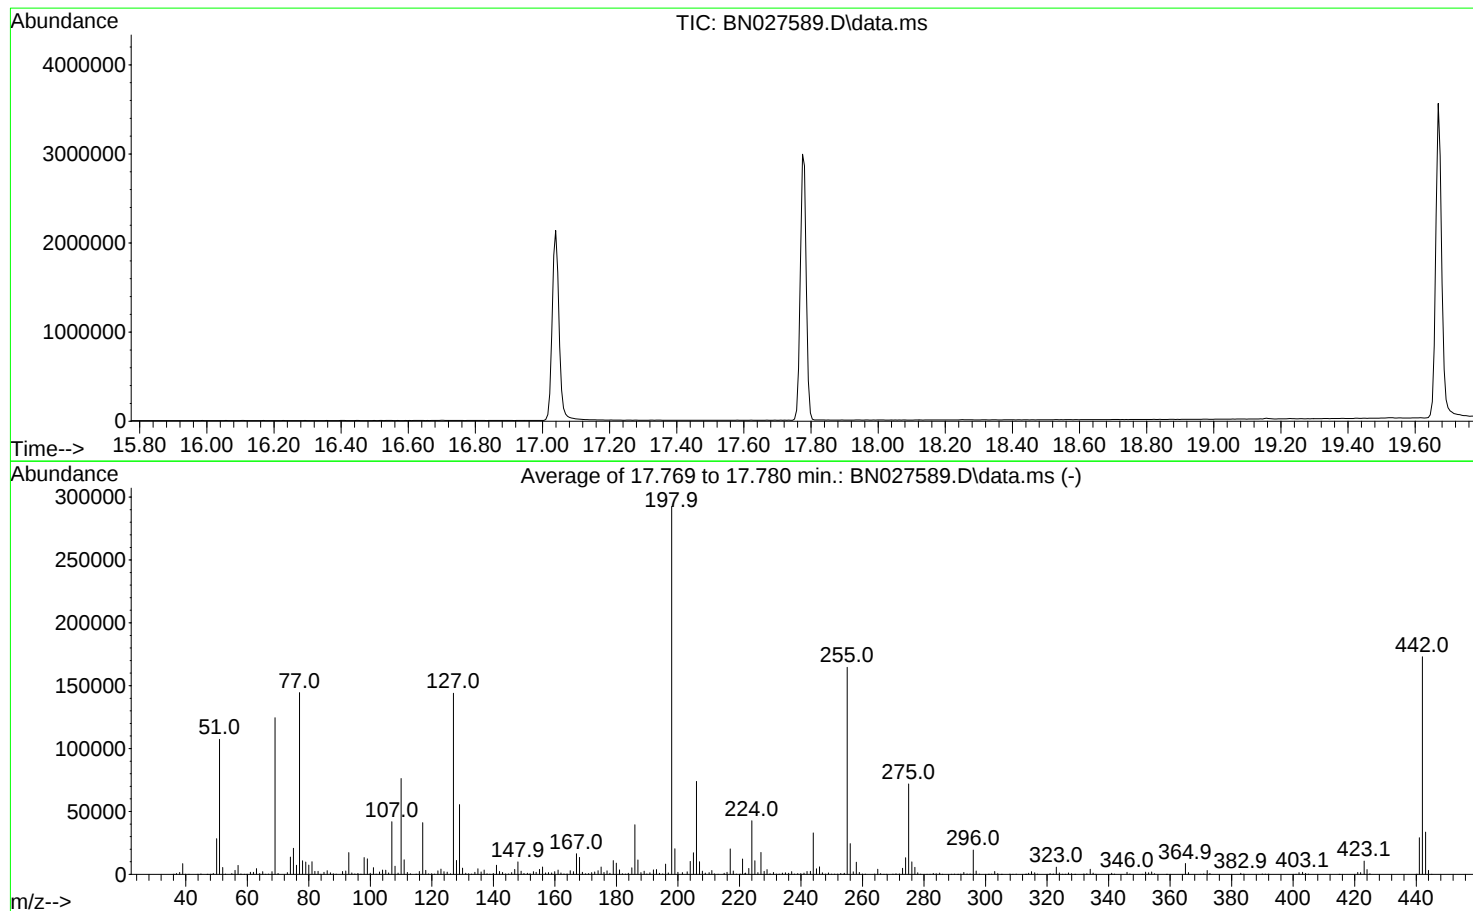




AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2524

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	107437	PASS
68	69	0.00	2	1.7	2150	PASS
69	198	0.00	100	42.6	124549	PASS
70	69	0.00	2	0.6	747	PASS
127	198	10	80	49.2	144059	PASS
197	198	0.00	2	0.4	1174	PASS
198	198	100	100	100.0	292523	PASS
199	198	5	9	7.0	20387	PASS
275	198	10	60	24.6	71877	PASS
365	198	1	100	3.0	8646	PASS
441	198	0.01	100	10.0	29185	PASS
442	442	50	100	100.0	173077	PASS
443	442	15	24	19.4	33626	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027589.D
Acq On : 12 Sep 2023 00:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 12 02:39:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:39:44 2023
Response via : Initial Calibration

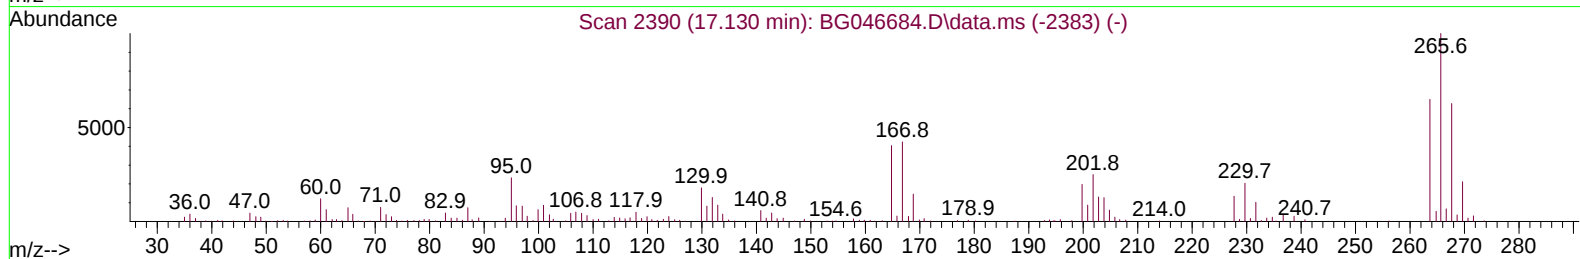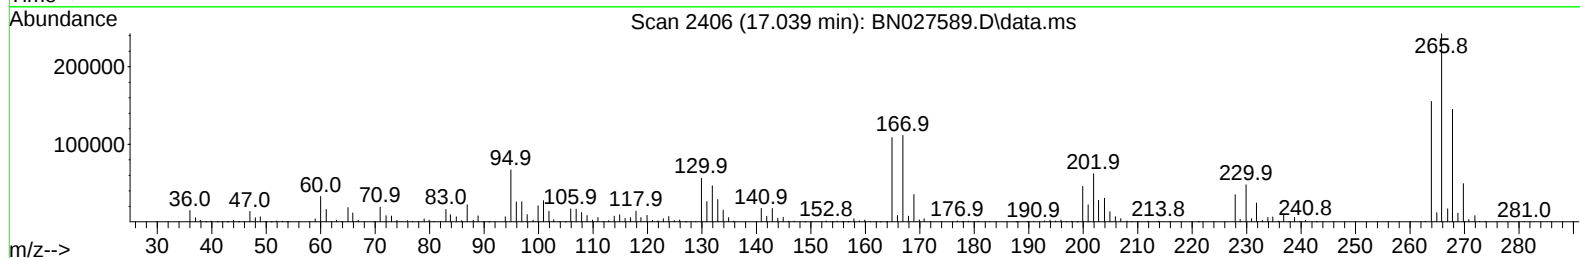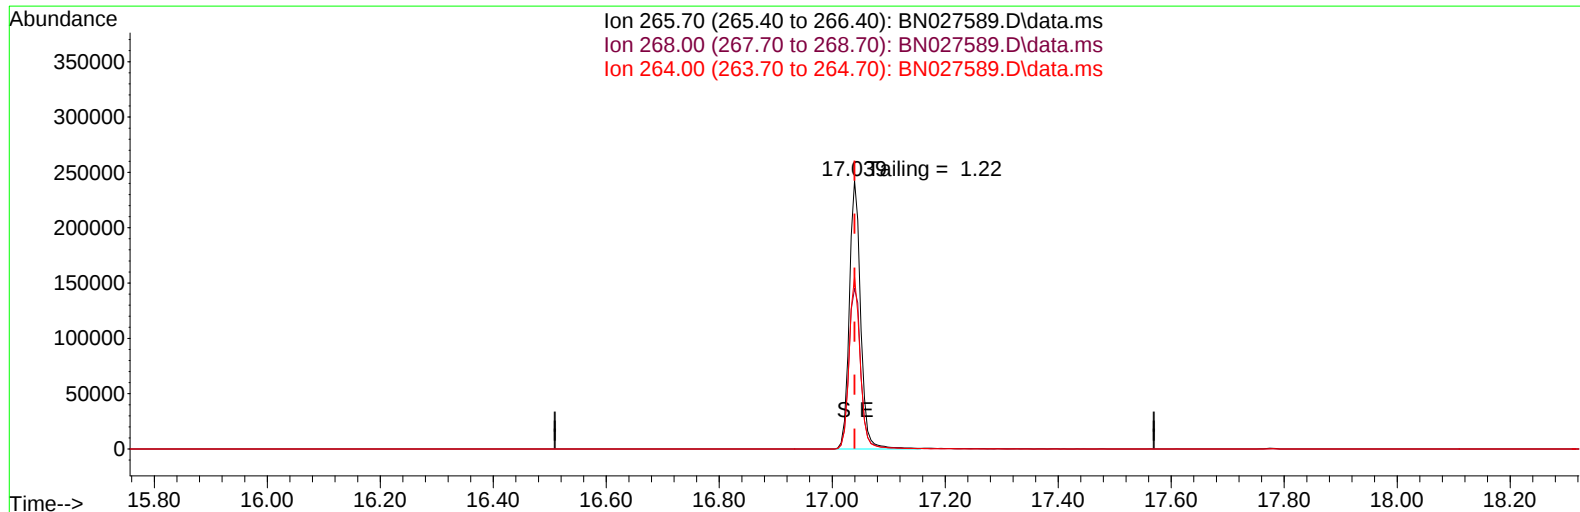

TIC: BN027589.D\data.ms

(70) Pentachlorophenol (C)

17.039min (0.000) 20906.42 ng




response 338637

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.79
264.00	61.60	63.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027589.D
Acq On : 12 Sep 2023 00:41
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTTP

Quant Time: Sep 12 02:39:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:39:44 2023
Response via : Initial Calibration

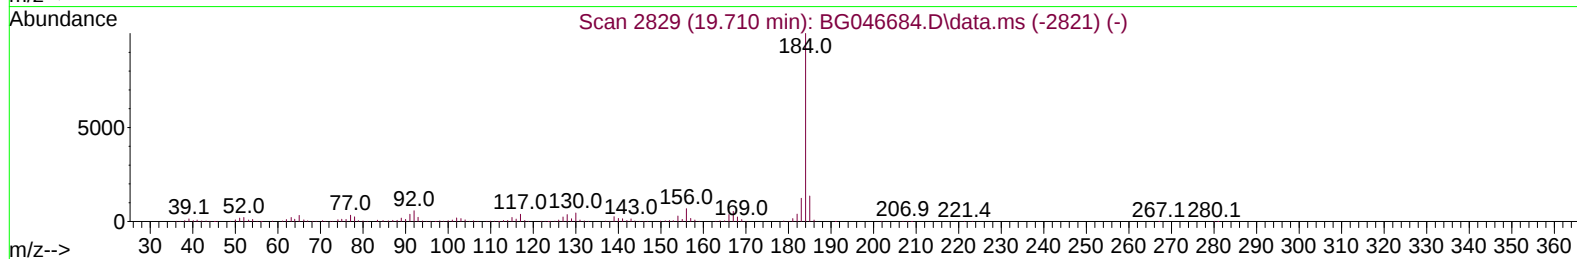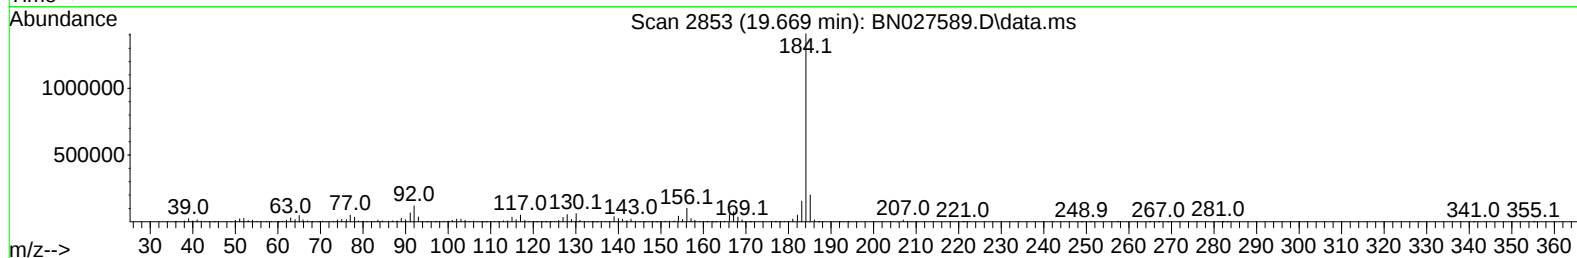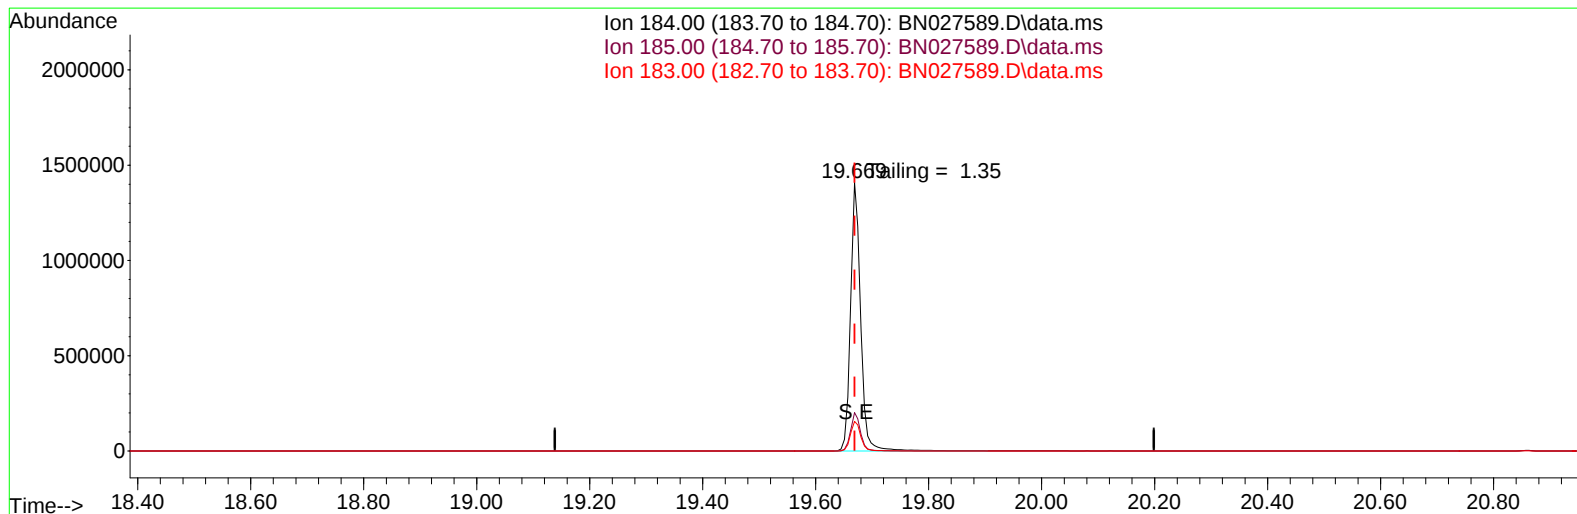

TIC: BN027589.D\data.ms

(77) Benzidine

19.669min (0.000) 0.00 ng

response 1761177

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.31
183.00	13.20	11.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/13/2023	BNA_N	<u>BN027589.D</u>
Compound Name	Response	Retention Time
DDT	901667	20.857
DDD	22822	20.421
DDE	1370	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24192	925859	2.61

Instrument :
BNA_N
ClientSampleId :
DFTPP