


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
 Data File : BN027607.D
 Acq On : 12 Sep 2023 13:11
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 109 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 02:45:58 2023

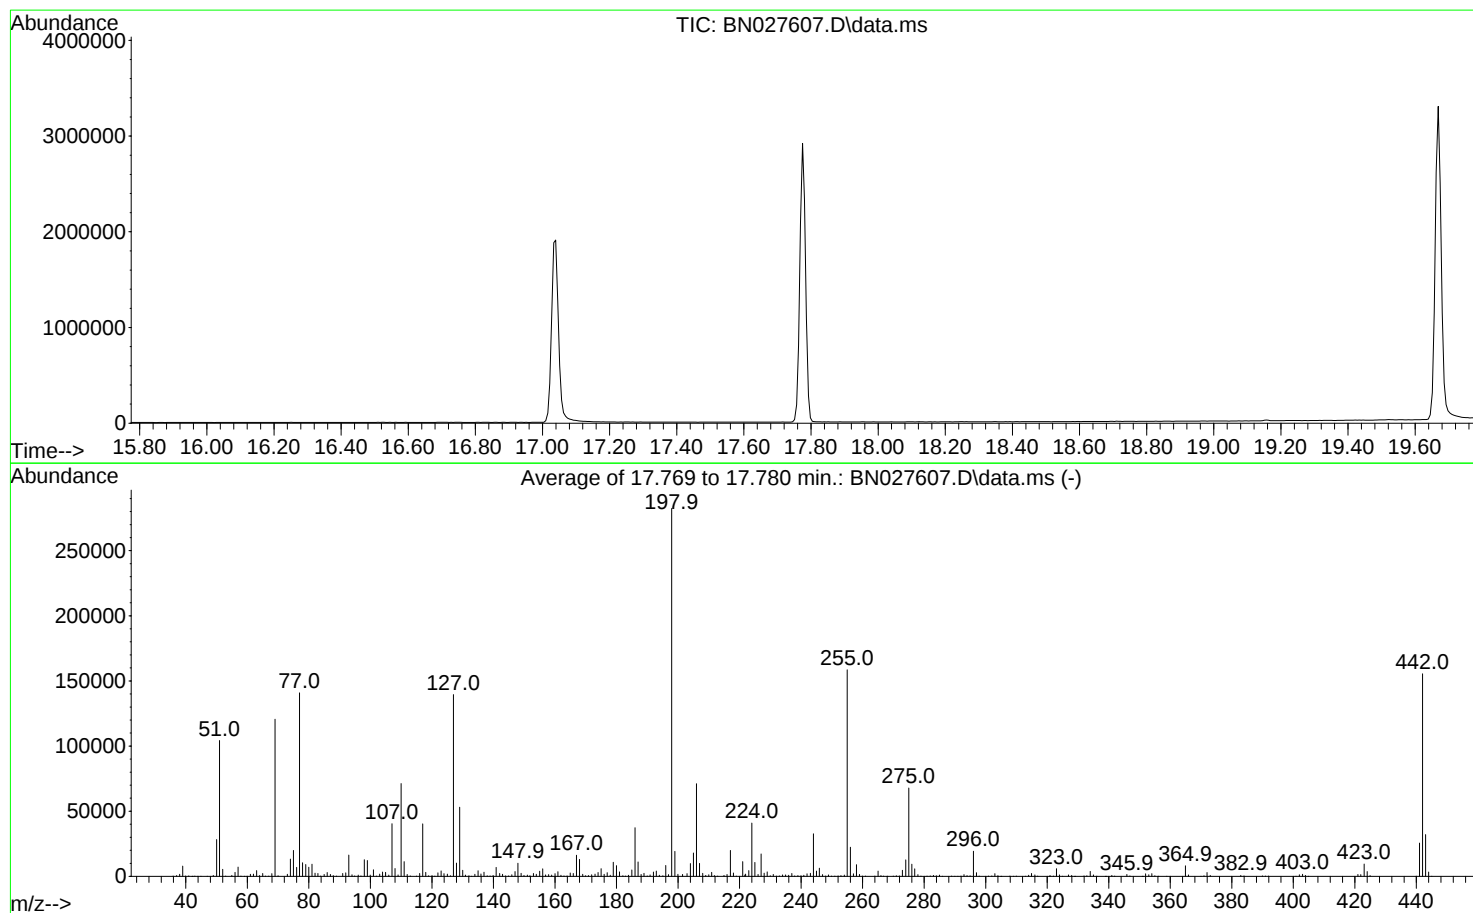




AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	104260	PASS
68	69	0.00	2	1.7	2059	PASS
69	198	0.00	100	42.7	120565	PASS
70	69	0.00	2	0.5	545	PASS
127	198	10	80	49.4	139501	PASS
197	198	0.00	2	0.5	1395	PASS
198	198	100	100	100.0	282368	PASS
199	198	5	9	6.8	19157	PASS
275	198	10	60	24.0	67845	PASS
365	198	1	100	2.9	8127	PASS
441	198	0.01	100	9.1	25598	PASS
442	442	50	100	100.0	155491	PASS
443	442	15	24	20.6	32097	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027607.D
Acq On : 12 Sep 2023 13:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 109 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 13 07:58:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 13 07:57:09 2023
Response via : Initial Calibration

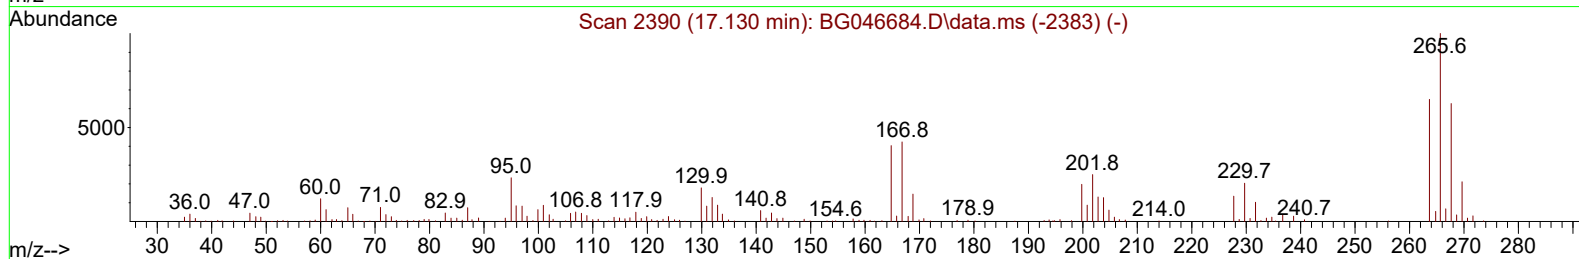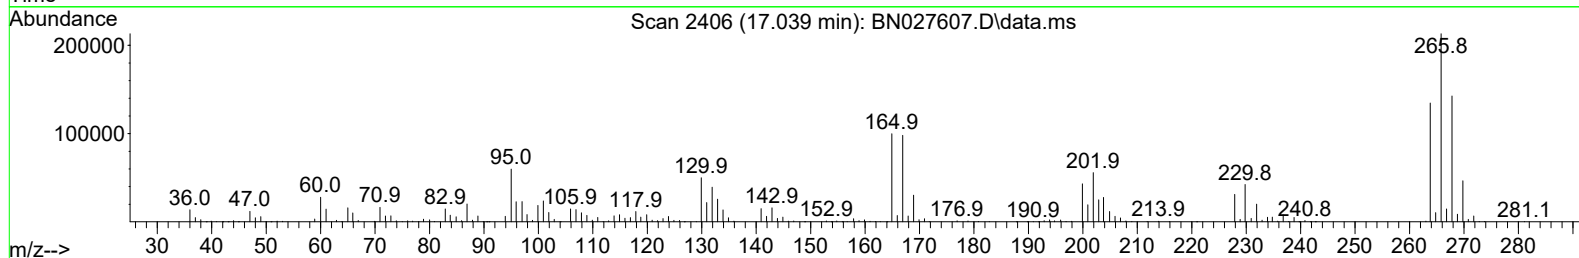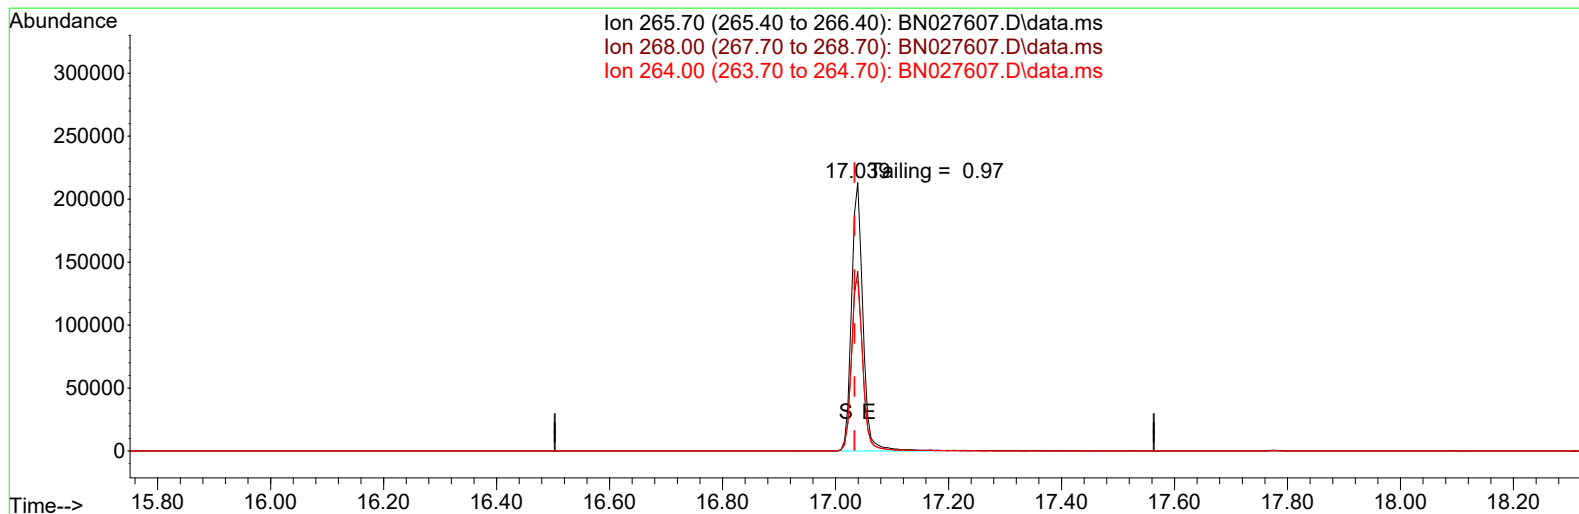

TIC: BN027607.D\data.ms

(70) Pentachlorophenol (C)

17.039min (+ 0.006) 19477.36 ng




response 300357

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.94
264.00	61.60	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027607.D
Acq On : 12 Sep 2023 13:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 109 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 13 07:58:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 13 07:57:09 2023
Response via : Initial Calibration

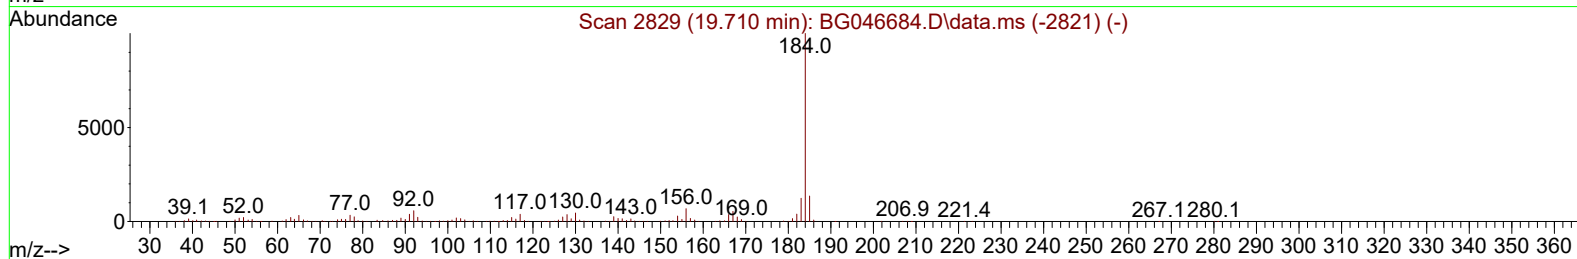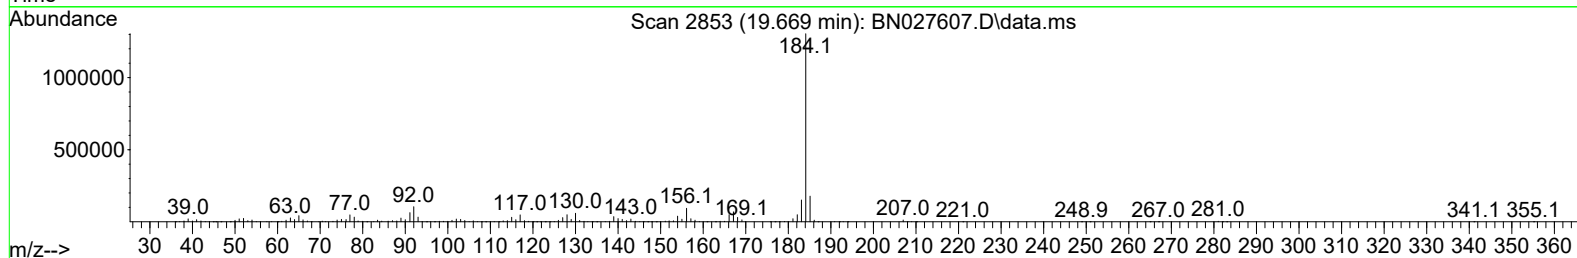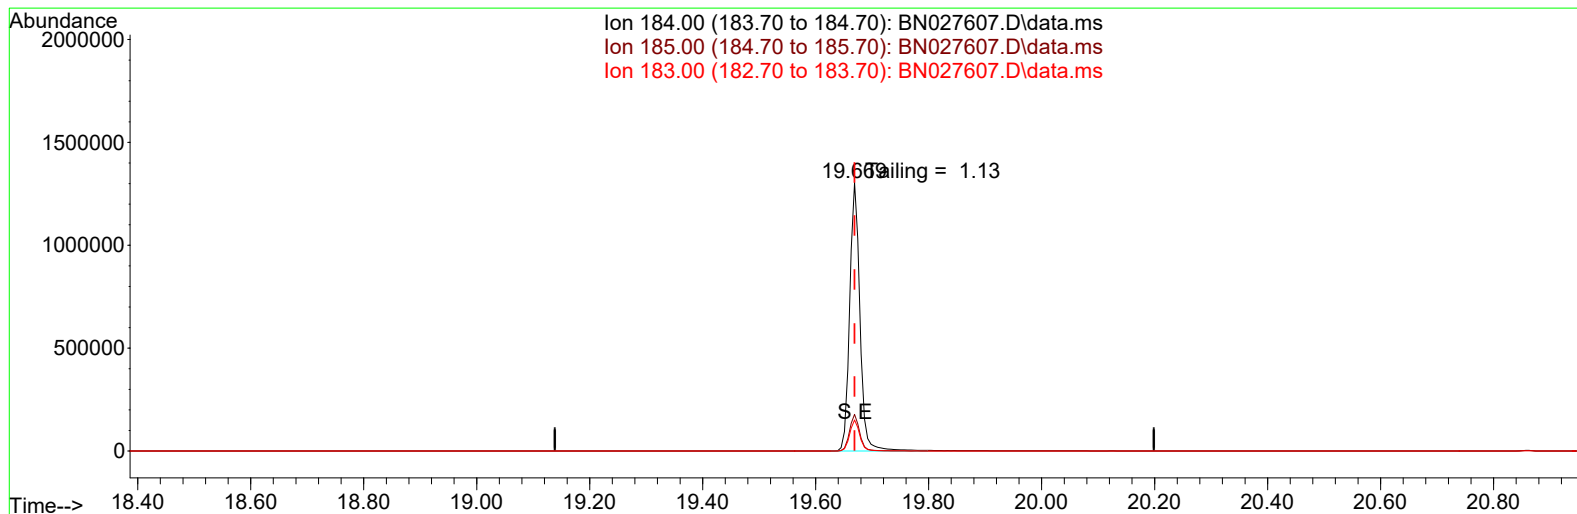

TIC: BN027607.D\data.ms

(77) Benzidine

19.669min (+ 0.000) 0.00 ng

response 1663408

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.65
183.00	13.20	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/13/2023	BNA_N	<u>BN027607.D</u>
Compound Name	Response	Retention Time
DDT	838046	20.863
DDD	22191	20.422
DDE	1479	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23670	861716	2.75

Instrument :
BNA_N
ClientSampleId :
DFTPP