


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027625.D
Acq On : 13 Sep 2023 01:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 128 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 12 02:45:58 2023

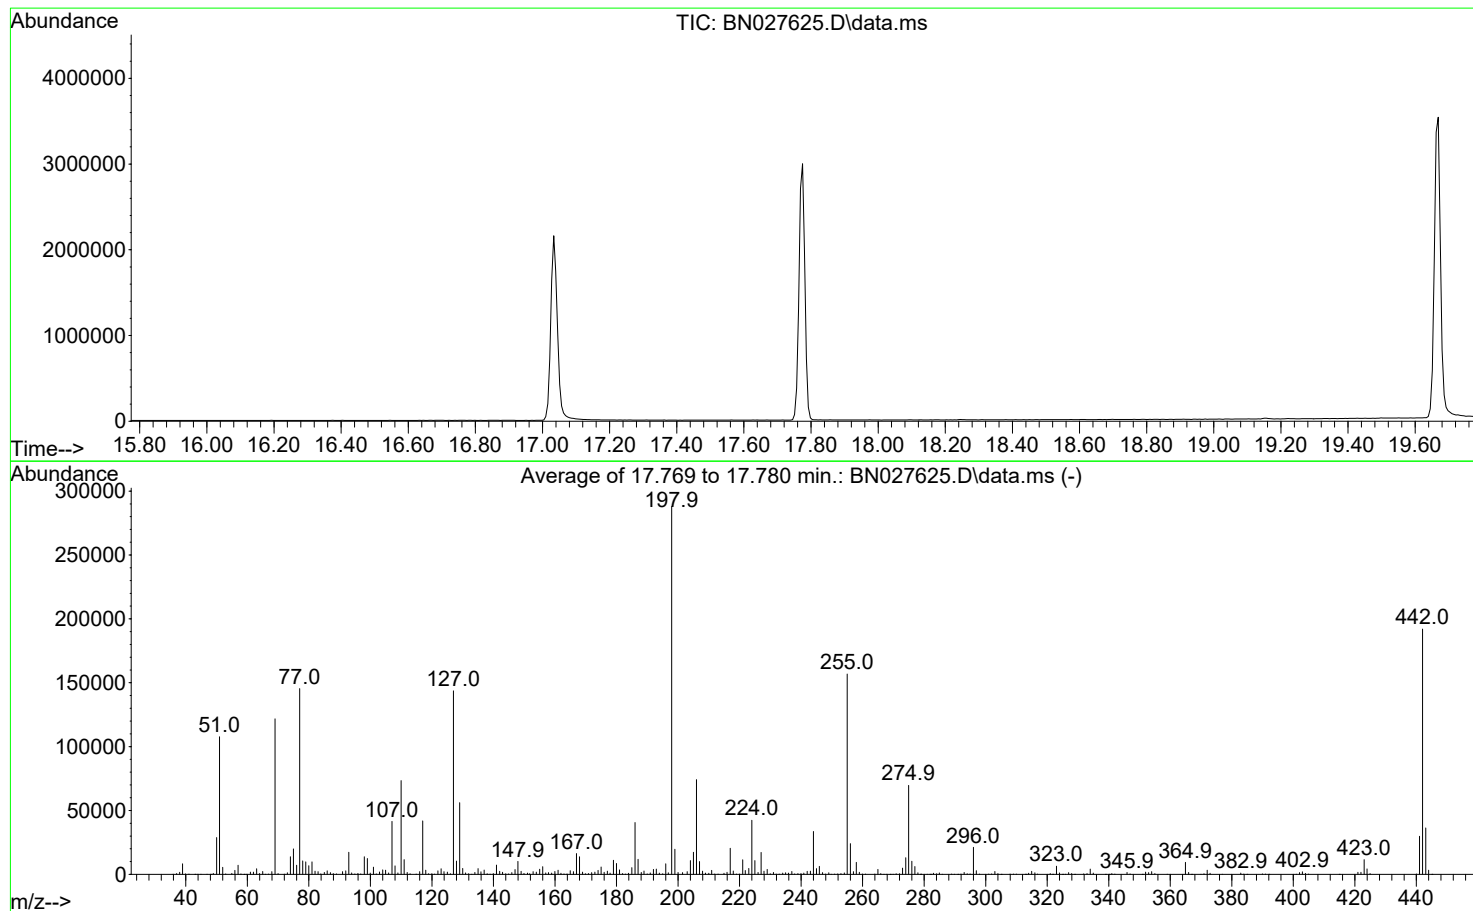




AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	107668	PASS
68	69	0.00	2	1.8	2195	PASS
69	198	0.00	100	42.3	121696	PASS
70	69	0.00	2	0.5	661	PASS
127	198	10	80	49.9	143672	PASS
197	198	0.00	2	0.4	1289	PASS
198	198	100	100	100.0	287957	PASS
199	198	5	9	6.8	19720	PASS
275	198	10	60	24.2	69653	PASS
365	198	1	100	3.3	9375	PASS
441	198	0.01	100	10.3	29781	PASS
442	442	50	100	100.0	191957	PASS
443	442	15	24	19.0	36379	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
 Data File : BN027625.D
 Acq On : 13 Sep 2023 01:03
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 128 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 13 07:57:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 13 07:57:09 2023
 Response via : Initial Calibration

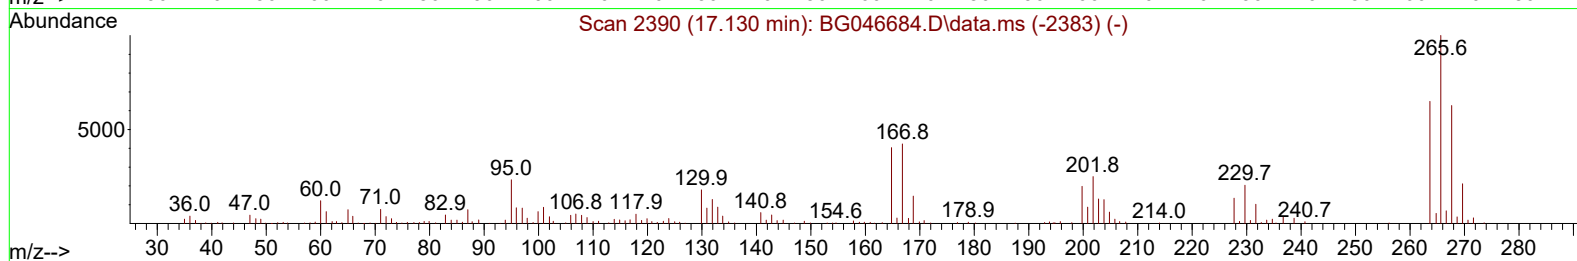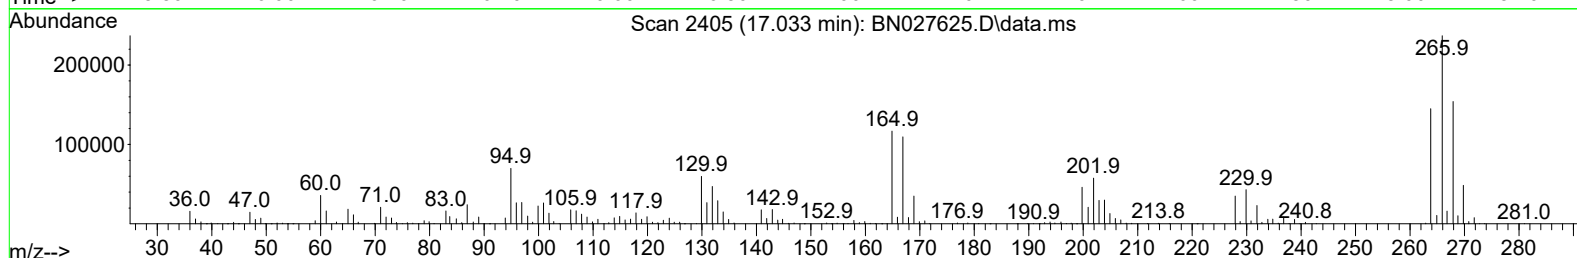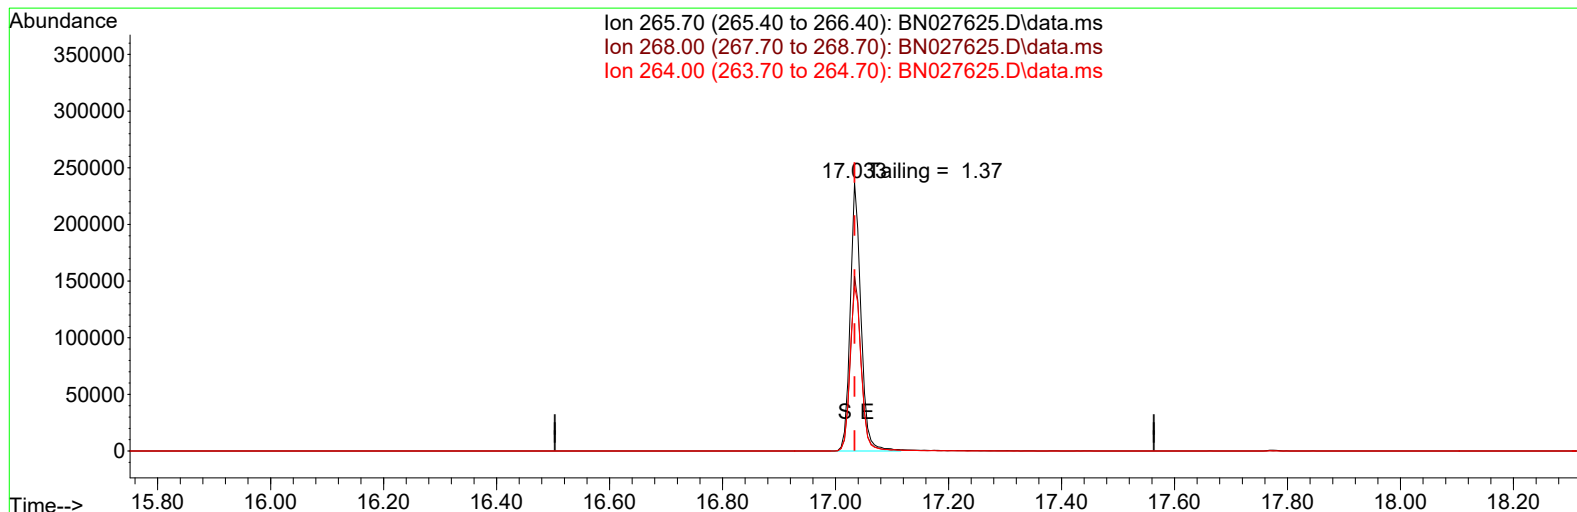

TIC: BN027625.D\data.ms

(70) Pentachlorophenol (C)

17.033min (0.000) 17754.77 ng




response 316569

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.06
264.00	61.60	61.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091323\
Data File : BN027625.D
Acq On : 13 Sep 2023 01:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 128 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 13 07:57:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 13 07:57:09 2023
Response via : Initial Calibration

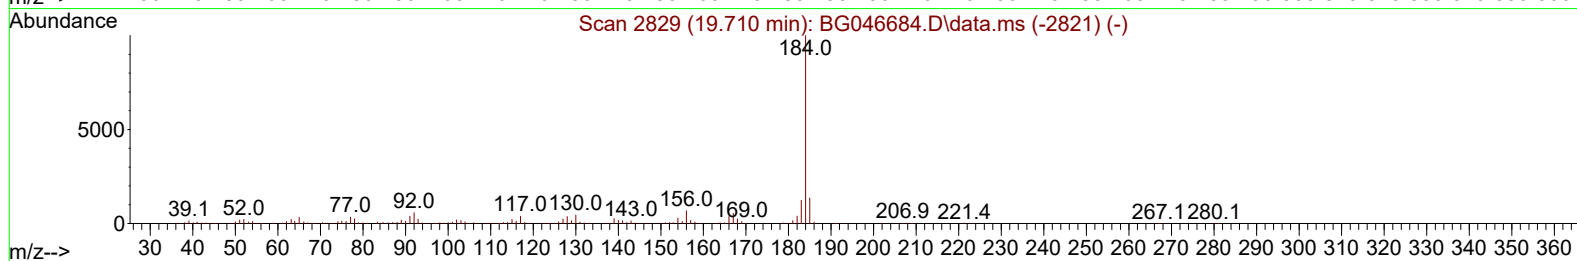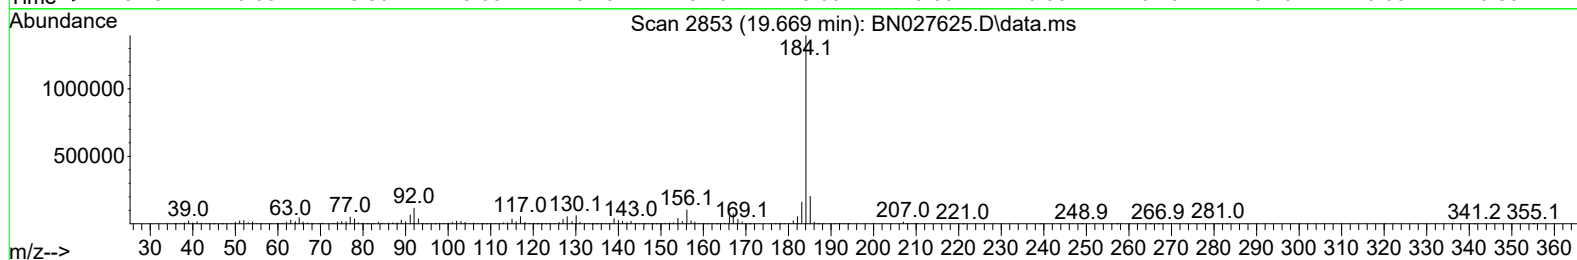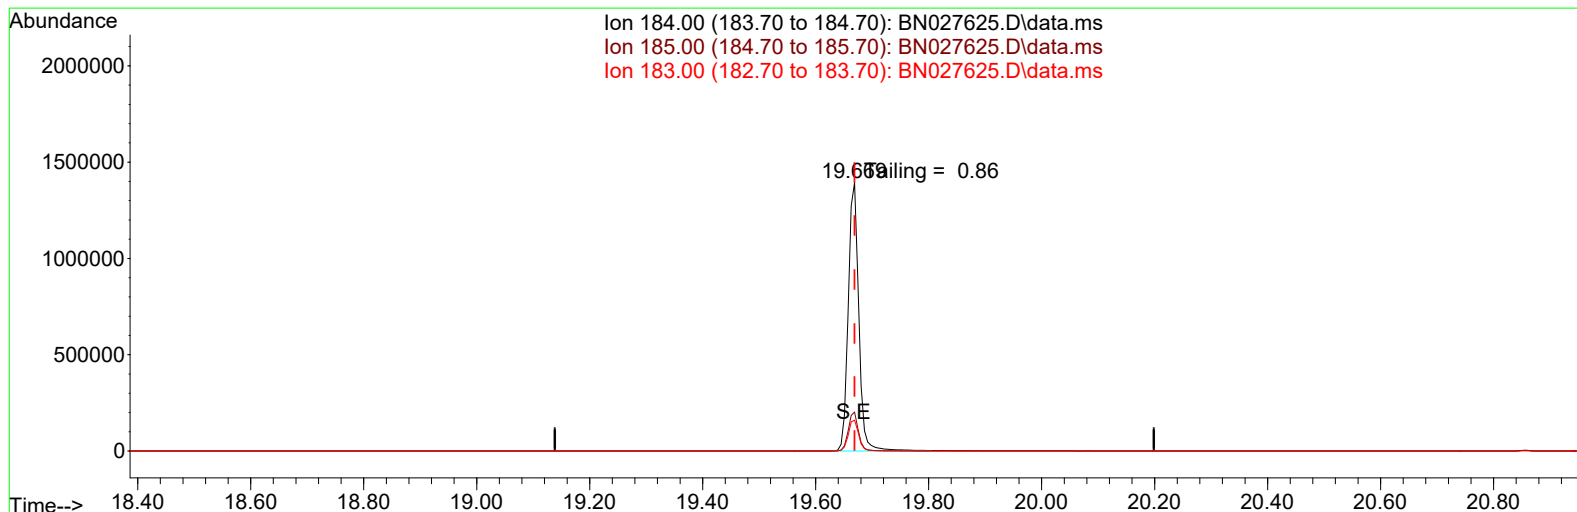

TIC: BN027625.D\data.ms

(77) Benzidine

19.669min (0.000) 0.00 ng

response 1822835

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.57
183.00	13.20	11.52
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/13/2023	BNA_N	<u>BN027625.D</u>
Compound Name	Response	Retention Time
DDT	874598	20.857
DDD	29196	20.421
DDE	1544	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30740	905338	3.40

Instrument :
BNA_N
ClientSampleId :
DFTPP