
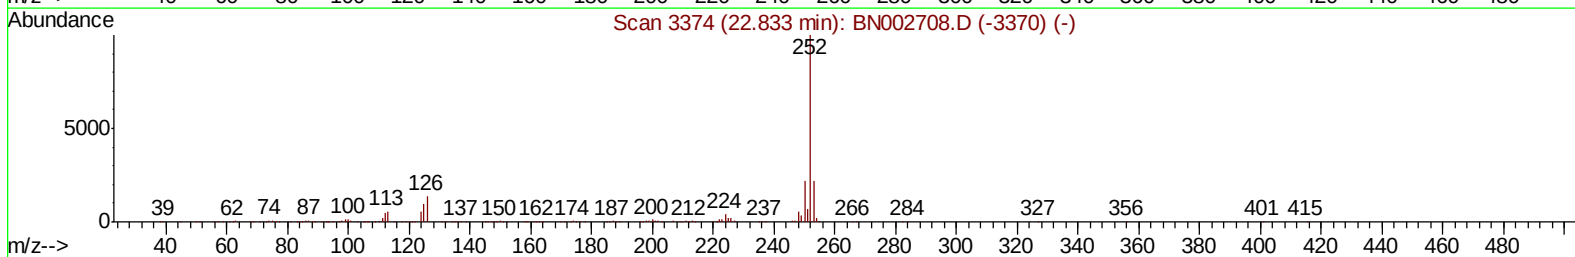
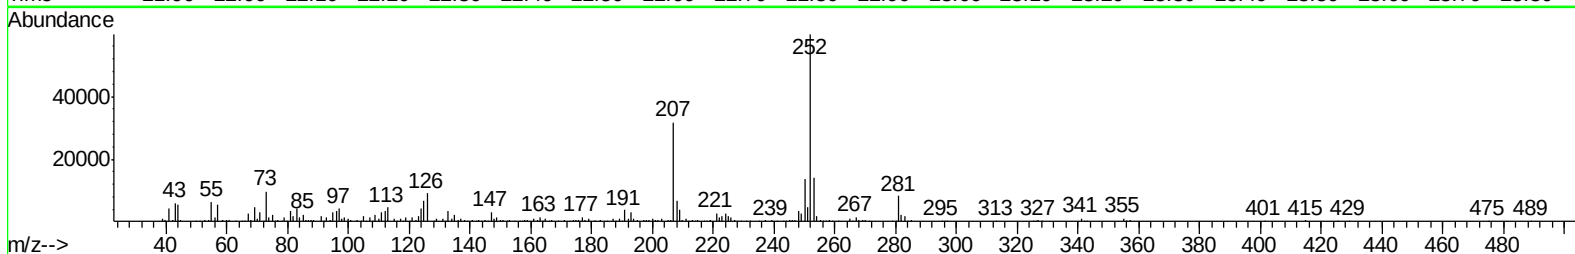


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091418\
Data File : BN002716.D
Acq On : 15 Sep 2018 07:11
Operator : JU/SJ
Sample : J4865-20
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Sep 17 02:20:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 15 04:34:35 2018
Response via : Initial Calibration

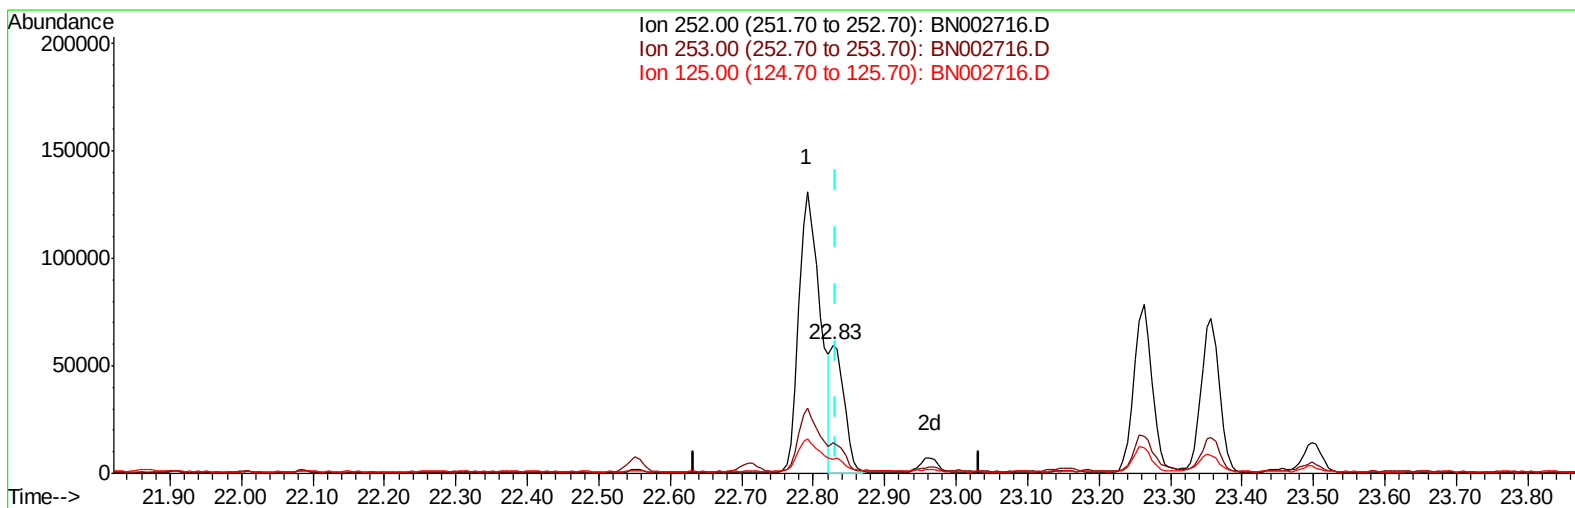

TIC: BN002716.D

(88) Benzo(k)fluoranthene

22.827min (-0.006) 1.55ng/ul m

response 75918

Ion	Exp%	Act%
252.00	100	100
253.00	22.30	23.92
125.00	10.40	11.45
0.00	0.00	0.00