

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091418\
 Data File : BN002711.D
 Acq On : 15 Sep 2018 04:14
 Operator : JU/SJ
 Sample : J4865-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 15 06:31:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 15 04:34:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	158817	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	652226	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.29	164	333376	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	670033	20.00	ng/ul	0.00
77) Chrysene-d12	21.24	240	665874	20.00	ng/ul	0.00
85) Perylene-d12	23.45	264	710402	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	9243	2.68	ng/uL	0.00
5) Phenol-d5	6.84	99	193885	14.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	125739	15.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	162761	14.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	119405	11.43	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	76318	15.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	86619	15.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	150883	14.62	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	192202	16.10	ng/ul	0.00
43) Dimethylphthalate-d6	13.70	166	452745	17.35	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	566478	16.62	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	52276	12.12	ng/ul	0.00
57) Fluorene-d10	15.28	176	390450	17.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	51978	12.40	ng/ul	0.00
70) Anthracene-d10	17.13	188	559506	17.49	ng/ul	0.00
78) Pyrene-d10	19.44	212	611128	17.39	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.31	264	684505	18.31	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.87	94	27817	2.045	ng/ul	99
44) Dimethylphthalate	13.75	163	115959	4.553	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091418\
Data File : BN002711.D
Acq On : 15 Sep 2018 04:14
Operator : JU/SJ
Sample : J4865-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 15 06:31:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 15 04:34:35 2018
Response via : Initial Calibration

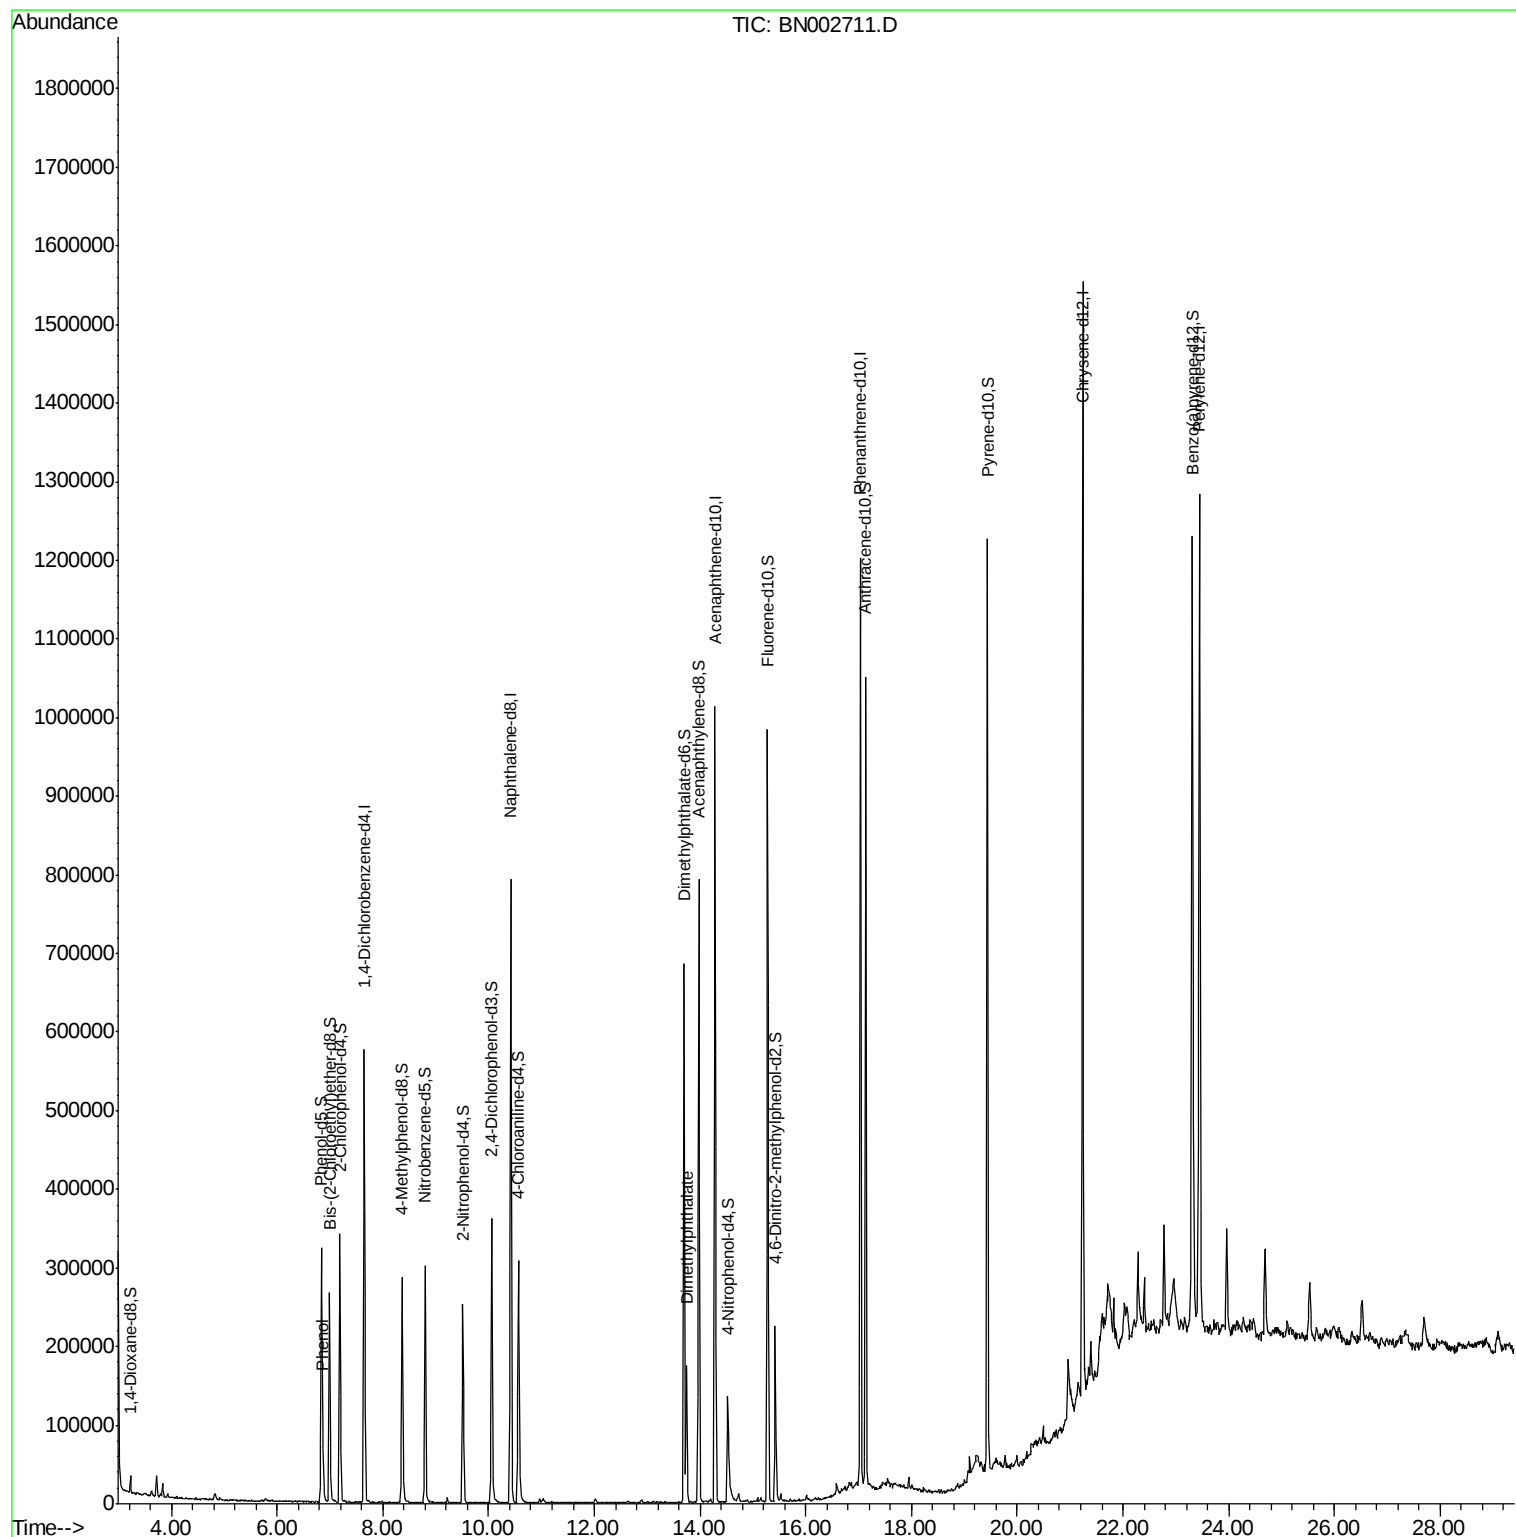

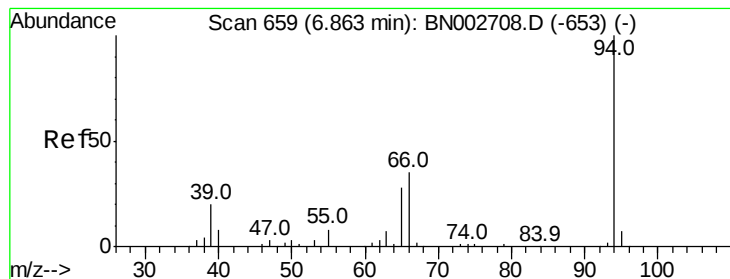


#6

Phenol




Concen: 2.045 ng/ul
 RT: 6.87 min Scan# 660
 Delta R.T. 0.01 min
 Lab File: BN002711.D
 Acq: 15 Sep 2018 04:14

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 94 Resp: 27817
 Ion Ratio Lower Upper
 94 100
 65 28.7 23.1 34.7
 66 38.4 29.8 44.6

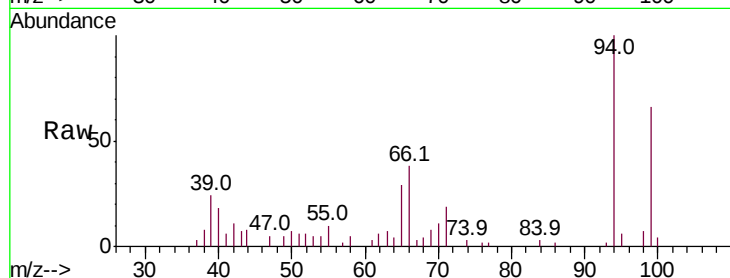

Abundance Ion 94.00 (93.70 to 94.70): BN0
 Ion 65.00 (64.70 to 65.70): BN0
 Ion 66.00 (65.70 to 66.70): BN0

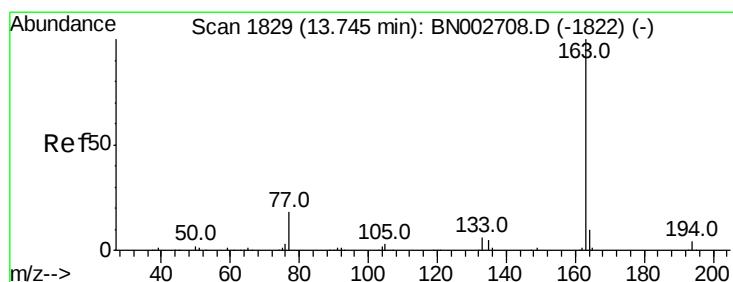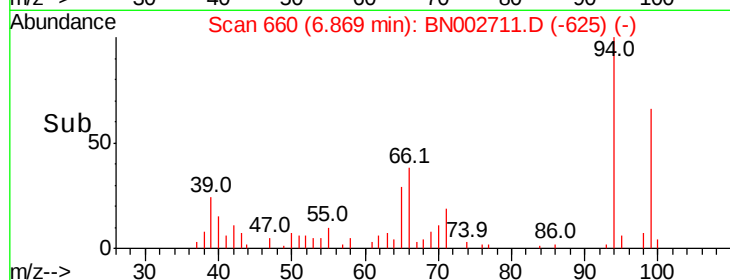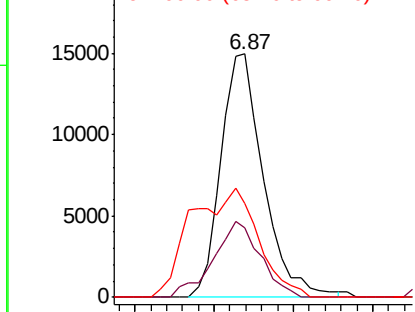


#44

Dimethylphthalate

Concen: 4.553 ng/ul
 RT: 13.75 min Scan# 1829
 Delta R.T. -0.00 min
 Lab File: BN002711.D
 Acq: 15 Sep 2018 04:14

Tgt Ion:163 Resp: 115959
 Ion Ratio Lower Upper
 163 100
 194 4.4 3.5 5.3
 164 10.2 8.1 12.1

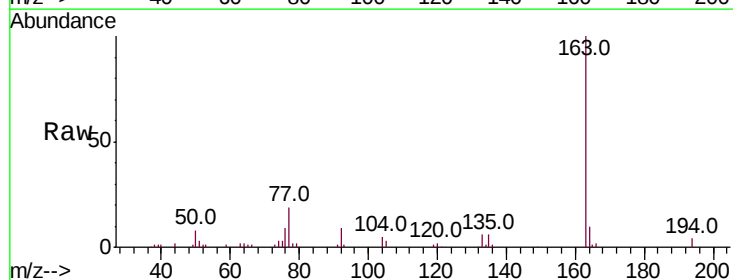

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

