

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091418\
 Data File : BN002715.D
 Acq On : 15 Sep 2018 06:35
 Operator : JU/SJ
 Sample : J4865-21
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB3P9

Quant Time: Sep 15 07:09:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 15 04:34:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	196970	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	844882	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.29	164	429891	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	826070	20.00	ng/ul	0.00
77) Chrysene-d12	21.24	240	736624	20.00	ng/ul	0.00
85) Perylene-d12	23.45	264	795050	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	11346	2.66	ng/uL	0.00
5) Phenol-d5	6.84	99	266550	15.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	174396	16.79	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	227122	16.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	224464	17.33	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	109487	16.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	130834	17.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	221593	16.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	241364	15.60	ng/ul	0.00
43) Dimethylphthalate-d6	13.70	166	647314	19.24	ng/ul	0.00
46) Acenaphthylene-d8	13.98	160	819993	18.66	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	75916	13.64	ng/ul	0.01
57) Fluorene-d10	15.29	176	541670	18.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	80351	15.55	ng/ul	0.00
70) Anthracene-d10	17.13	188	766528	19.44	ng/ul	0.00
78) Pyrene-d10	19.44	212	769010	19.78	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.31	264	834775	19.95	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	13.75	163	277076	8.437	ng/ul# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091418\
Data File : BN002715.D
Acq On : 15 Sep 2018 06:35
Operator : JU/SJ
Sample : J4865-21
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DB3P9

Quant Time: Sep 15 07:09:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 15 04:34:35 2018
Response via : Initial Calibration

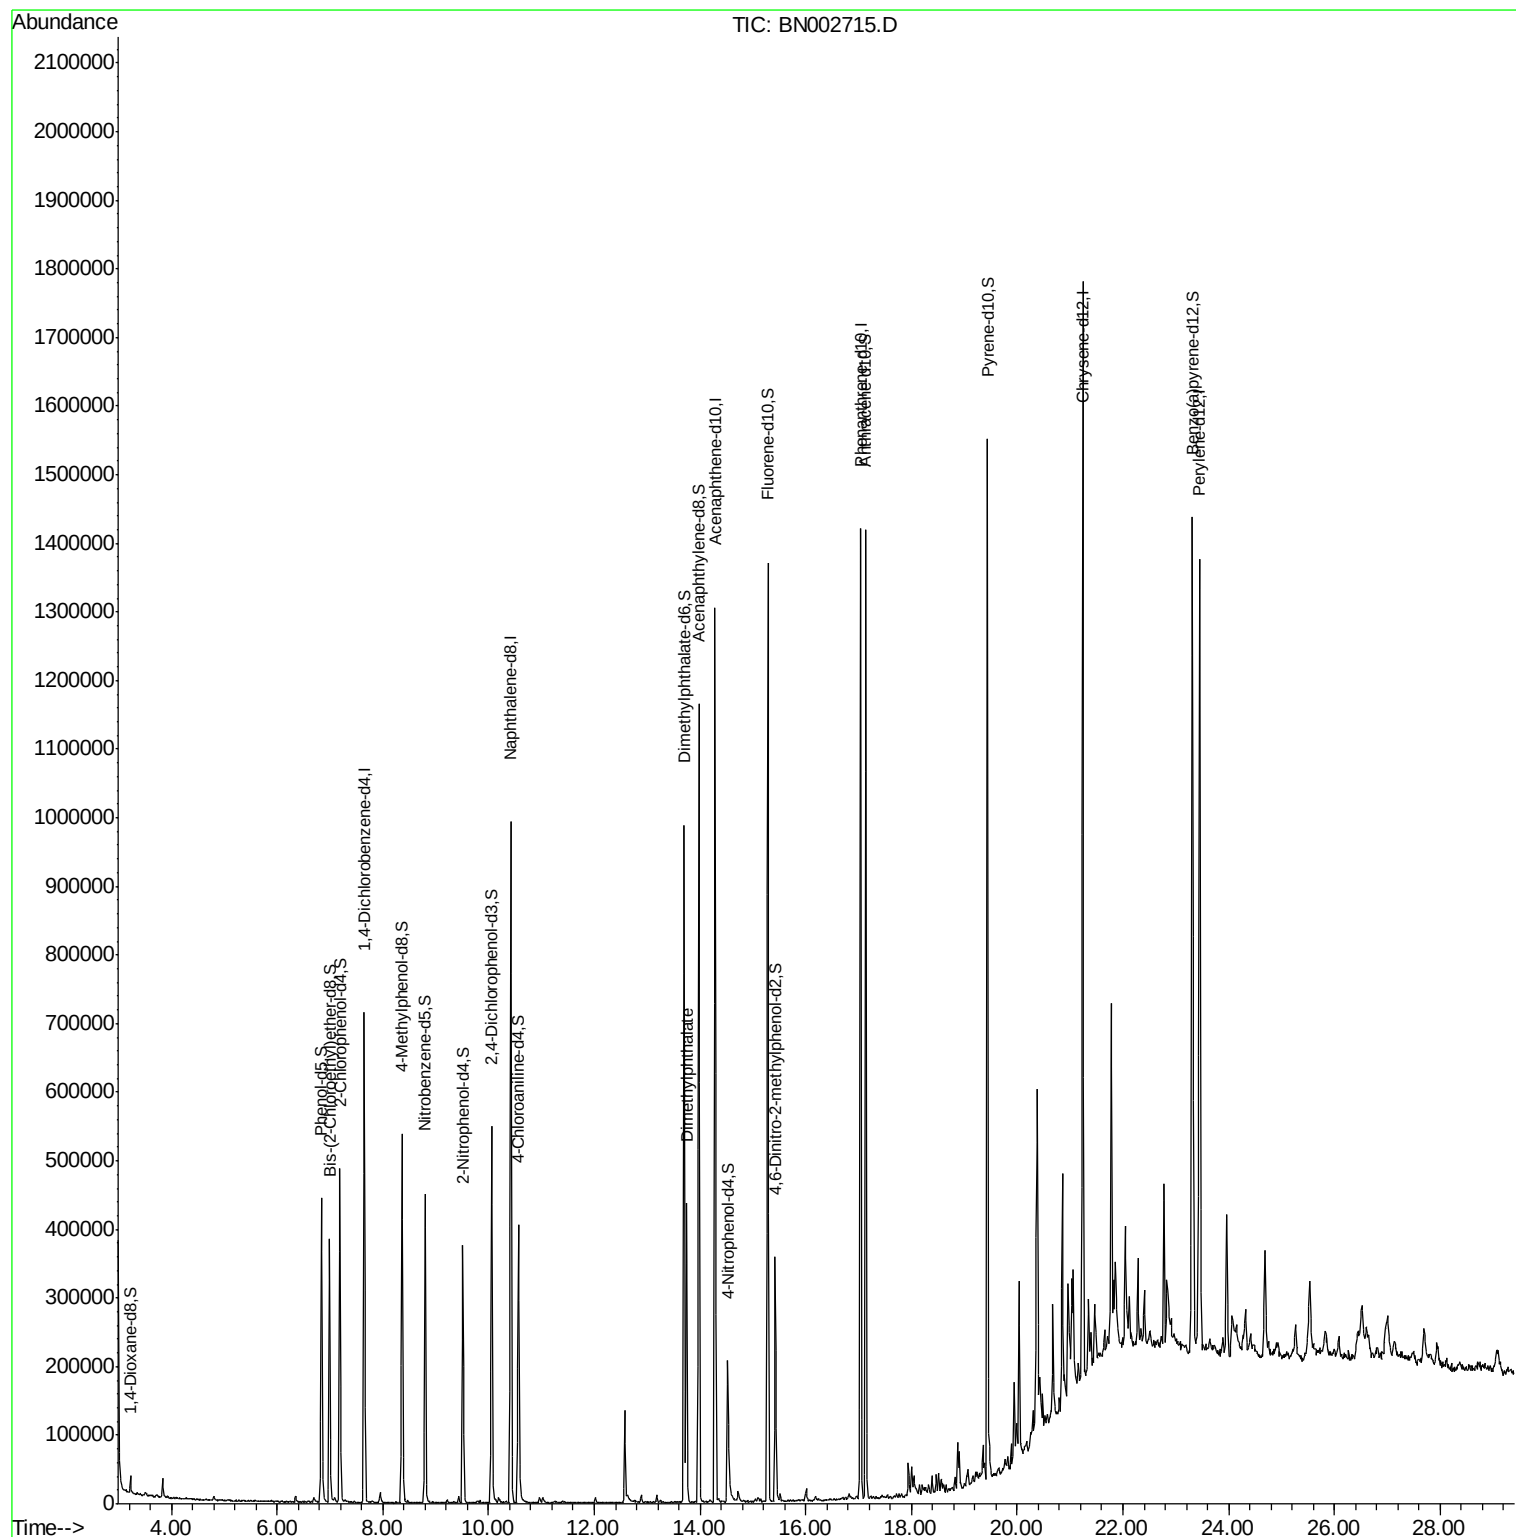

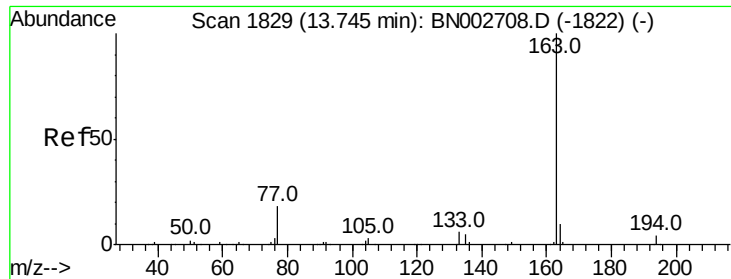

#44

Dimethylphthalate

Concen: 8.437 ng/ul

RT: 13.75 min Scan# 1829

Delta R.T. 0.00 min

Lab File: BN002715.D

Acq: 15 Sep 2018 06:35

Instrument :

BNA_N

ClientSampleId :

DB3P9

Tot Ion:163 Resp: 277076

Ion Ratio Lower Upper

163 100

194 3.5 3.5 5.3#

164 10.0 8.1 12.1

