
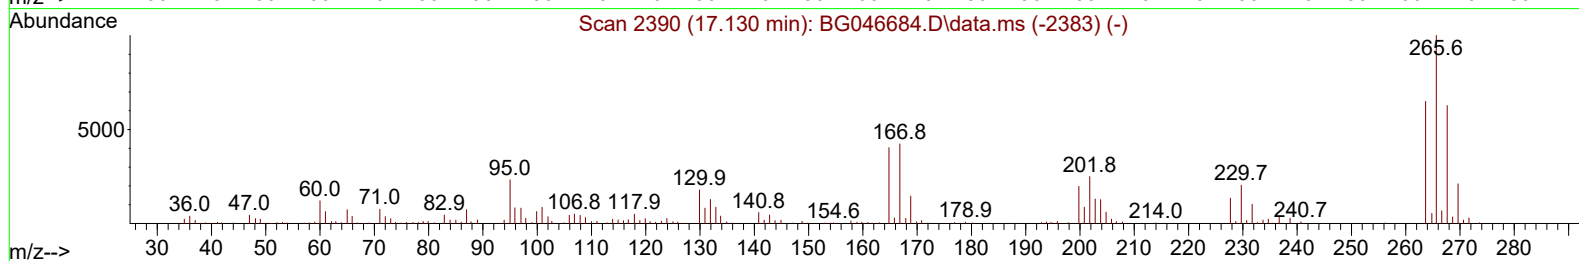
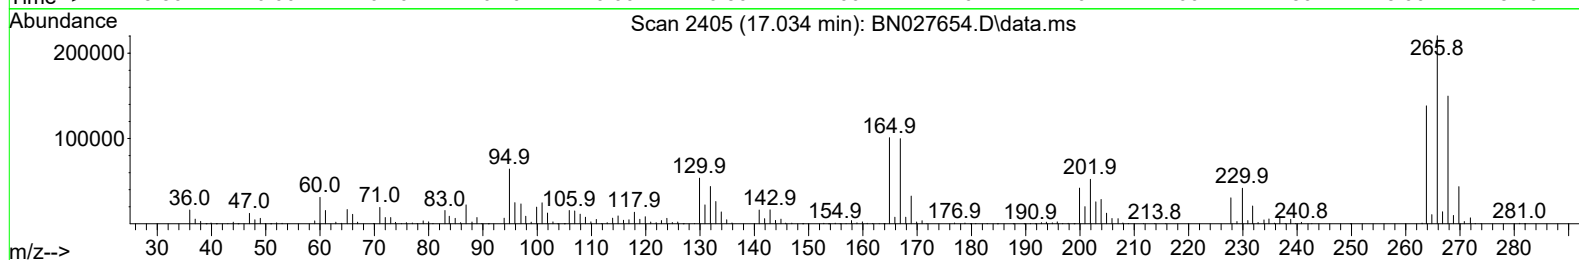


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091423\
Data File : BN027654.D
Acq On : 13 Sep 2023 21:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Sep 14 08:12:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 14 08:12:26 2023
Response via : Initial Calibration

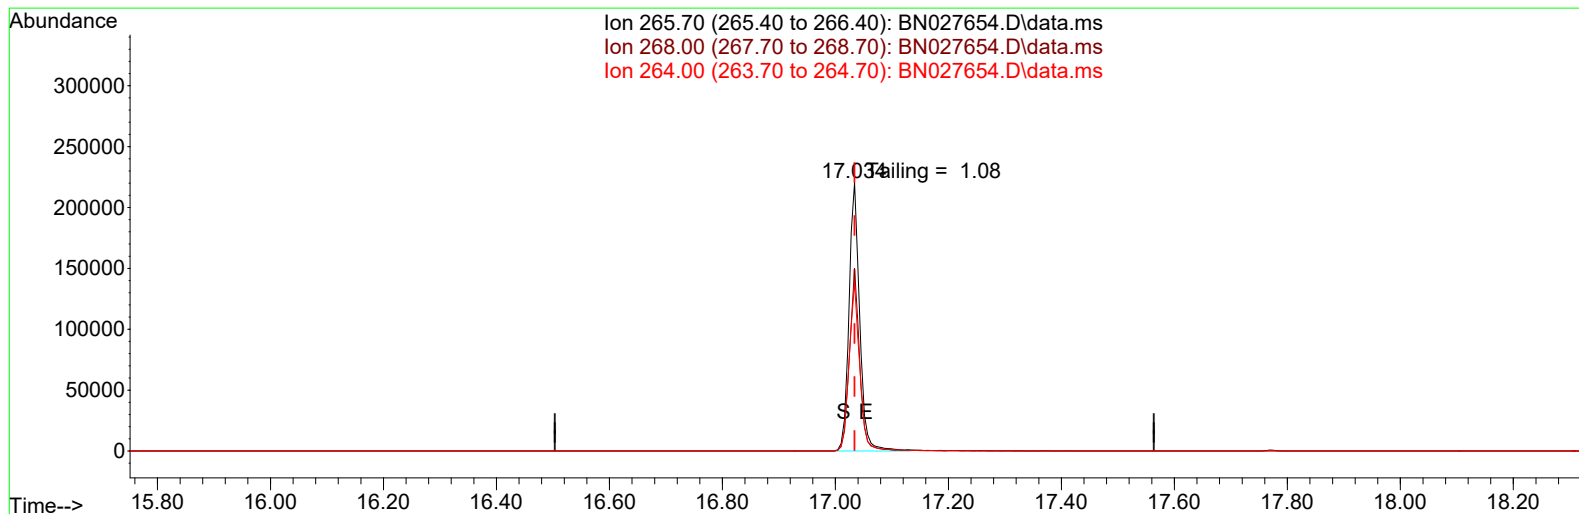

TIC: BN027654.D\data.ms

(70) Pentachlorophenol (C)




17.034min (0.000) 18028.00 ng

response 289608

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.97
264.00	61.60	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091423\
Data File : BN027654.D
Acq On : 13 Sep 2023 21:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Sep 14 08:12:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 14 08:12:26 2023
Response via : Initial Calibration

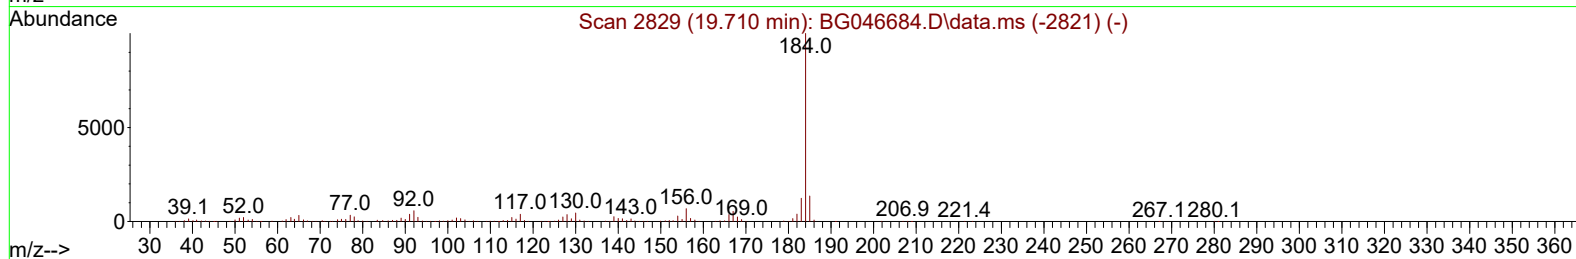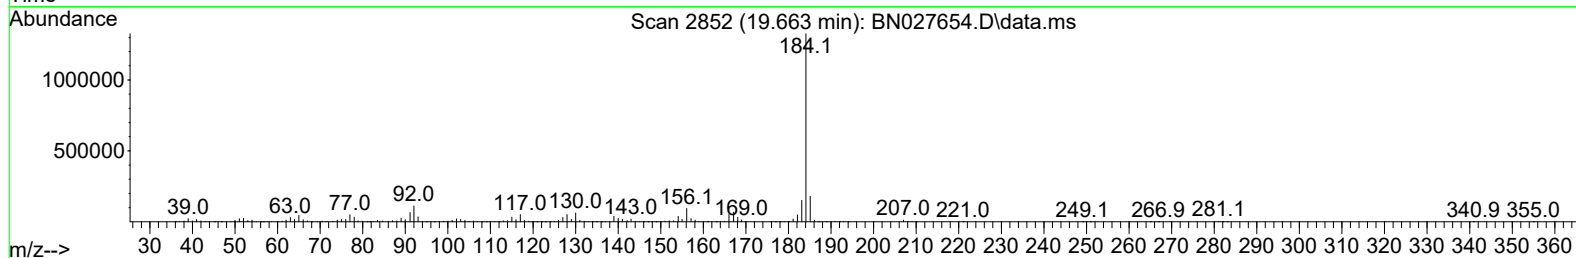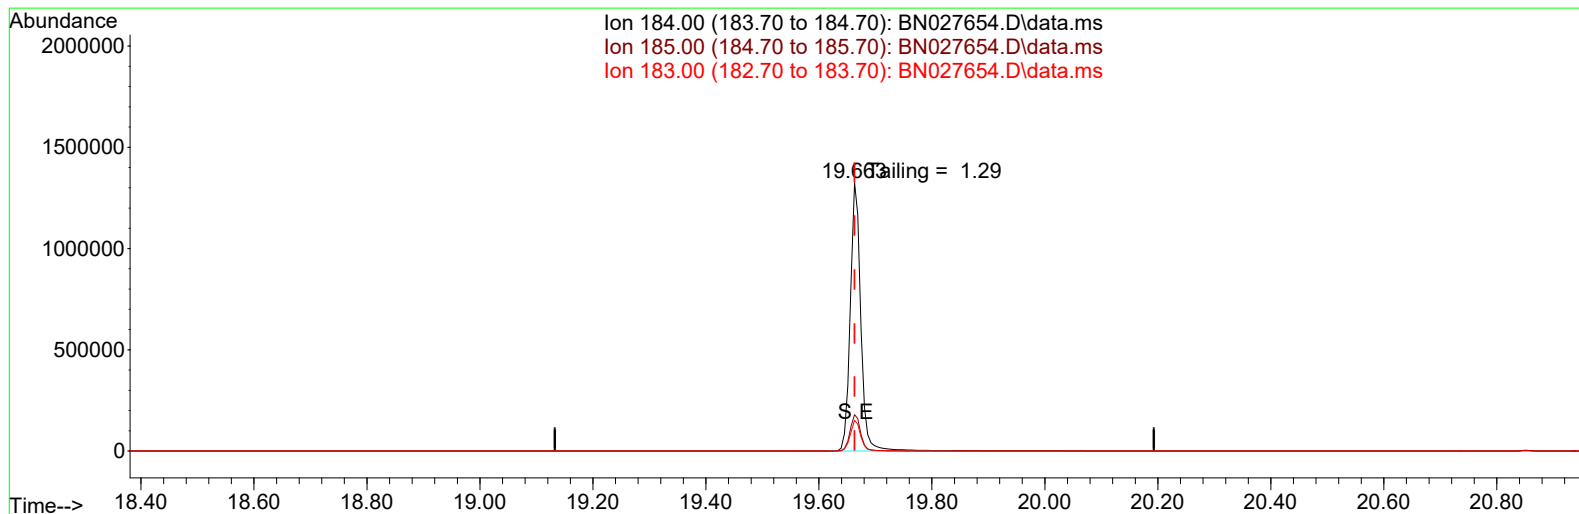

TIC: BN027654.D\data.ms

(77) Benzidine

19.663min (0.000) 0.00 ng

response 1720183

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.55
183.00	13.20	11.44
0.00	0.00	0.00