
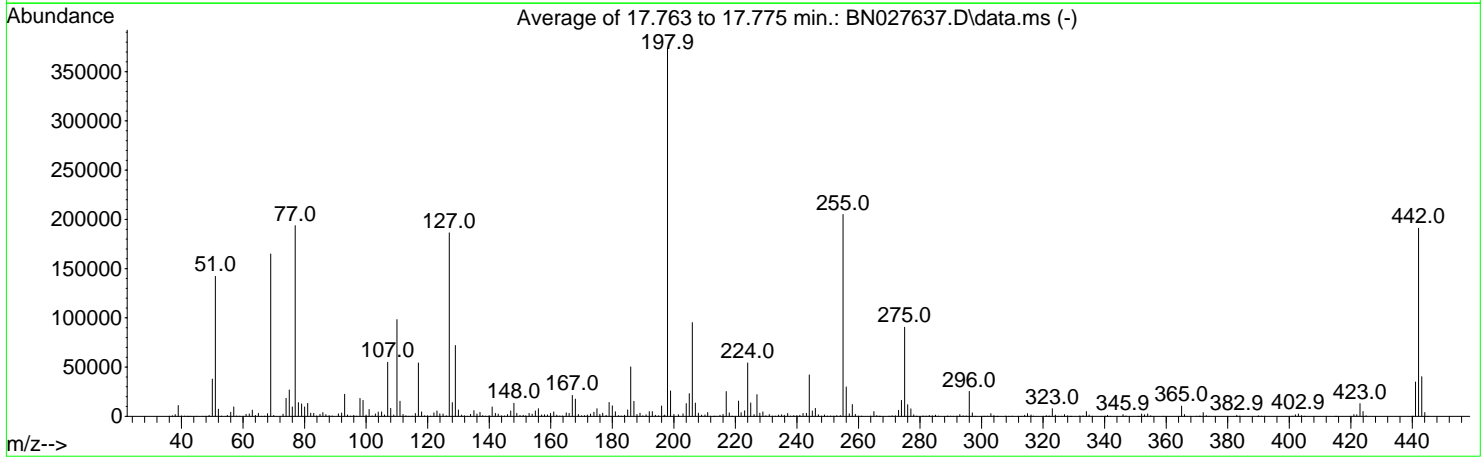


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN091423\  
 Data File : BN027637.D  
 Acq On : 13 Sep 2023 10:02  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN082923.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Sep 12 02:45:58 2023

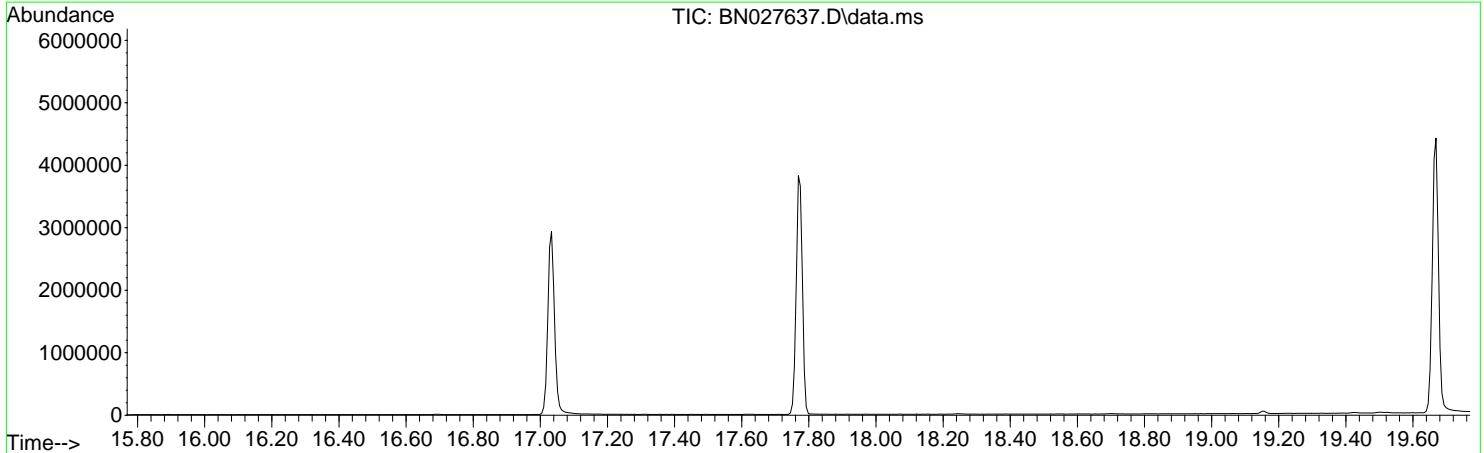




AutoFind: Scans 2529, 2530, 2531; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	142214	PASS
68	69	0.00	2	1.7	2794	PASS
69	198	0.00	100	44.2	164907	PASS
70	69	0.00	2	0.6	920	PASS
127	198	10	80	49.9	186389	PASS
197	198	0.00	2	0.3	1242	PASS
198	198	100	100	100.0	373504	PASS
199	198	5	9	6.9	25827	PASS
275	198	10	60	24.2	90440	PASS
365	198	1	100	2.8	10436	PASS
441	198	0.01	100	9.3	34881	PASS
442	442	50	100	100.0	191061	PASS
443	442	15	24	21.1	40288	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN091423\  
 Data File : BN027637.D  
 Acq On : 13 Sep 2023 10:02  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_N  
**ClientSampleId :**  
 DFTPP

Quant Time: Sep 14 00:05:38 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Sep 14 00:05:33 2023  
 Response via : Initial Calibration

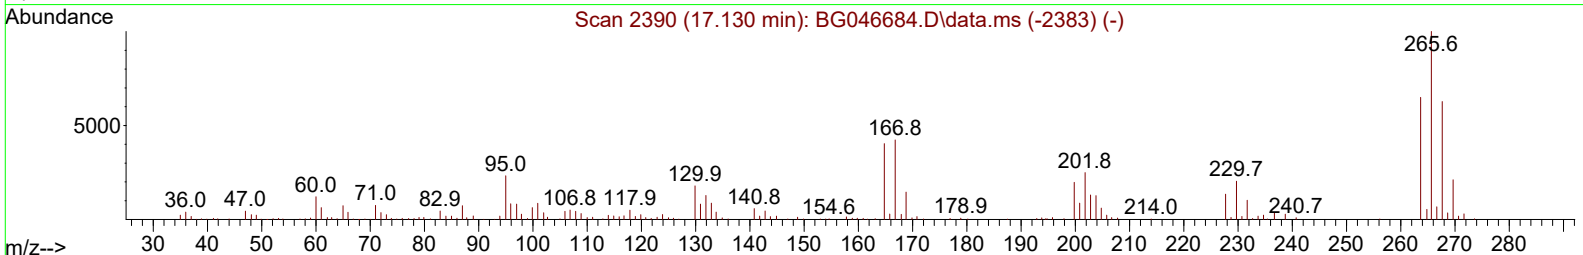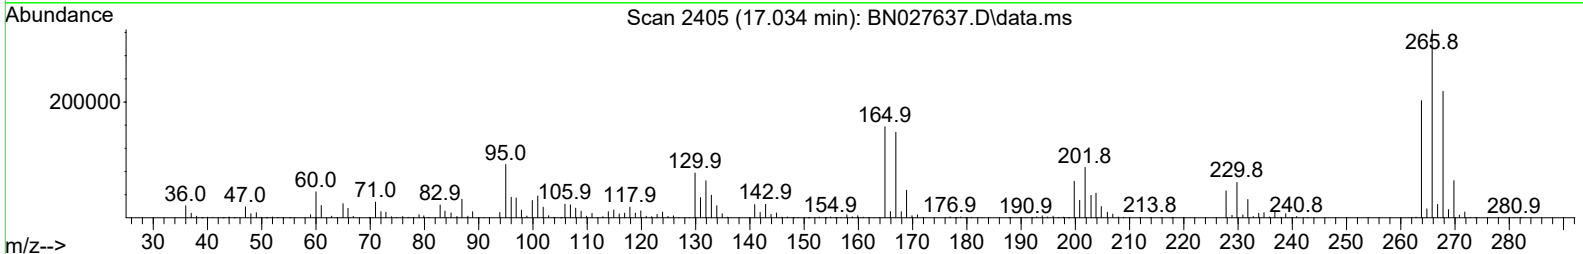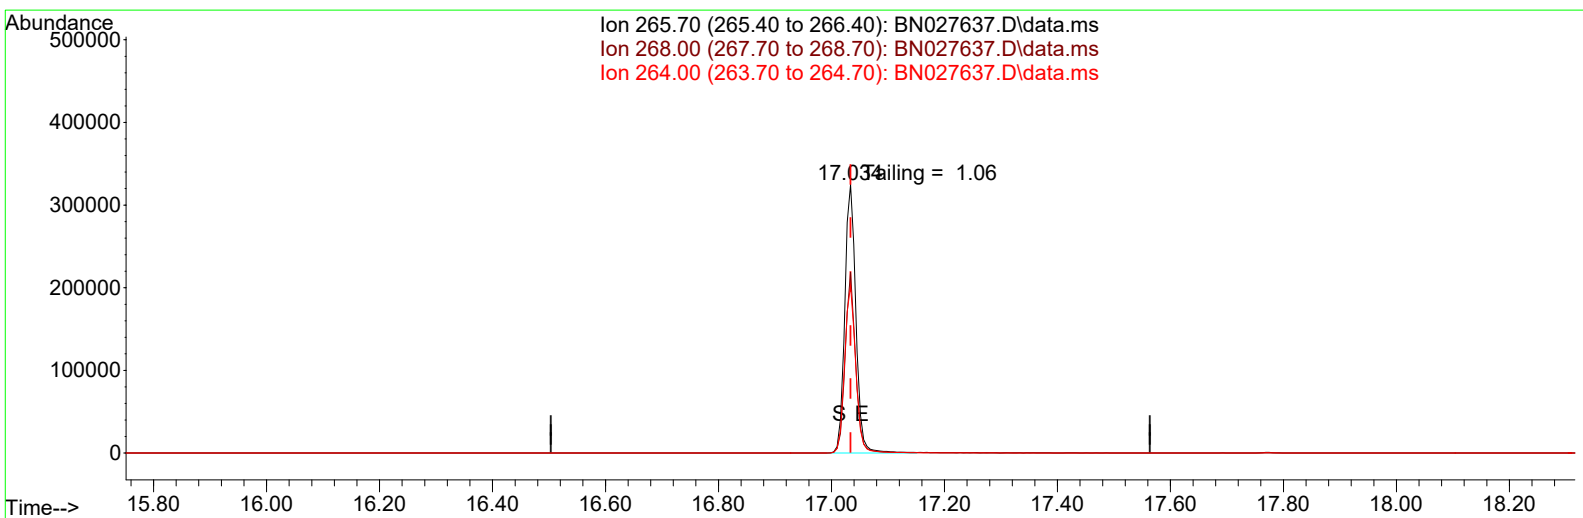

TIC: BN027637.D\data.ms

(70) Pentachlorophenol (C)

17.034min ( 0.000) 20839.64 ng




response 443859

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.26
264.00	61.60	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN091423\  
 Data File : BN027637.D  
 Acq On : 13 Sep 2023 10:02  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_N  
**ClientSampleId :**  
 DFTPP

Quant Time: Sep 14 00:05:38 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Sep 14 00:05:33 2023  
 Response via : Initial Calibration

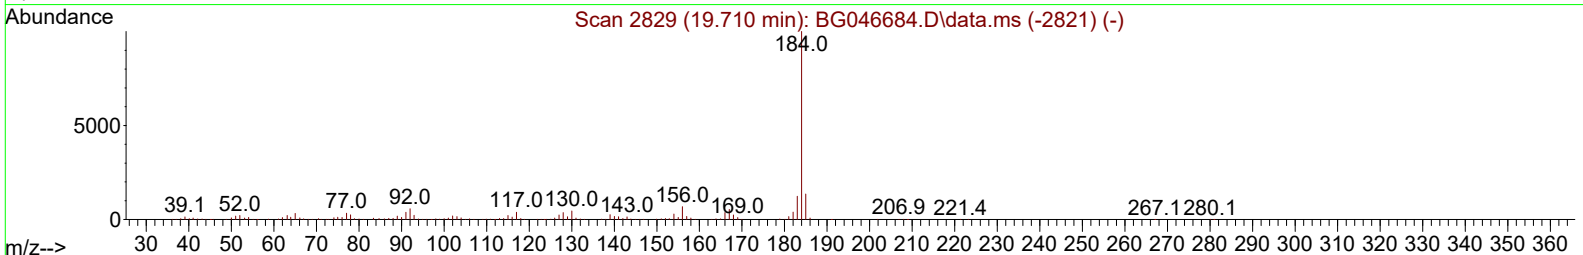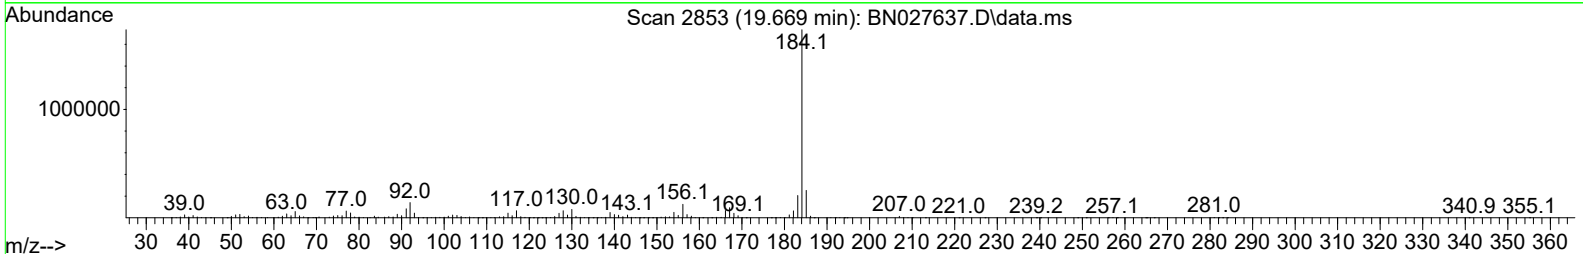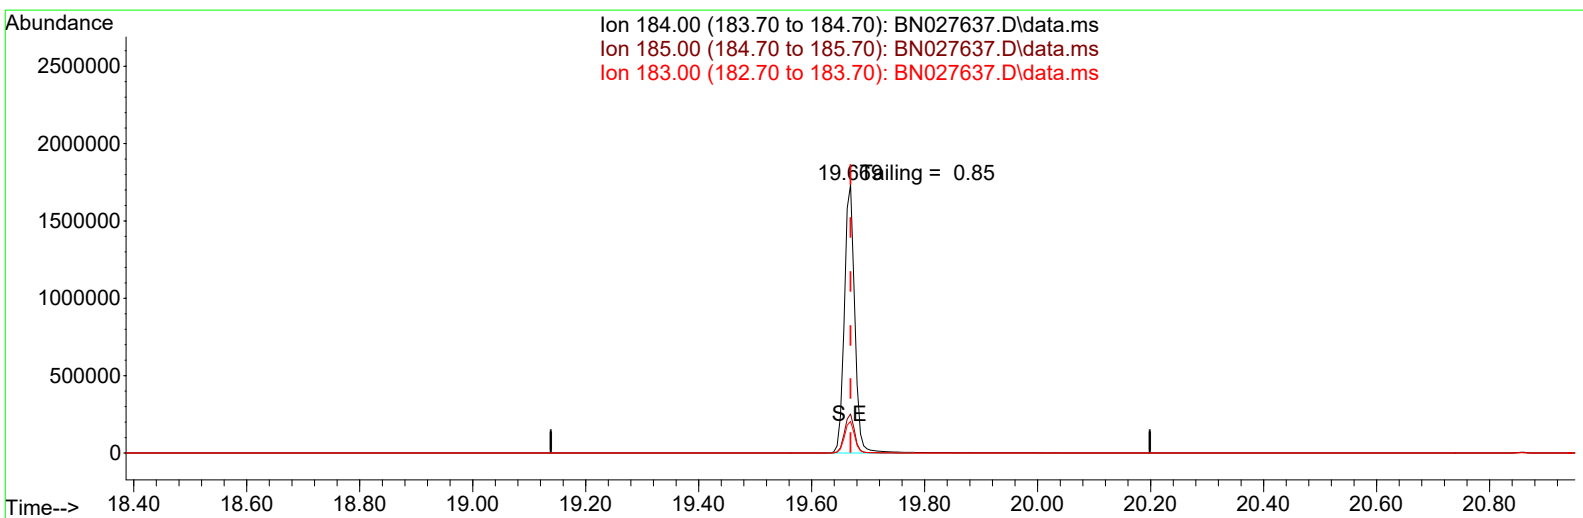

TIC: BN027637.D\data.ms

(77) Benzidine

19.669min ( 0.000) 0.00 ng

response 2232186

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.57
183.00	13.20	11.83
0.00	0.00	0.00

**DDT Breakdown**

Date	Instrument Name	DFTPP Data File
9/14/2023	BNA_N	<u>BN027637.D</u>
Compound Name	Response	Retention Time
DDT	1191127	20.857
DDD	42575	20.422
DDE	1829	19.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44404	1235531	3.59

Instrument :  
 BNA\_N  
 Client:Sampled :  
 DFTPP