


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091423\
 Data File : BN027654.D
 Acq On : 13 Sep 2023 21:55
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 02:45:58 2023

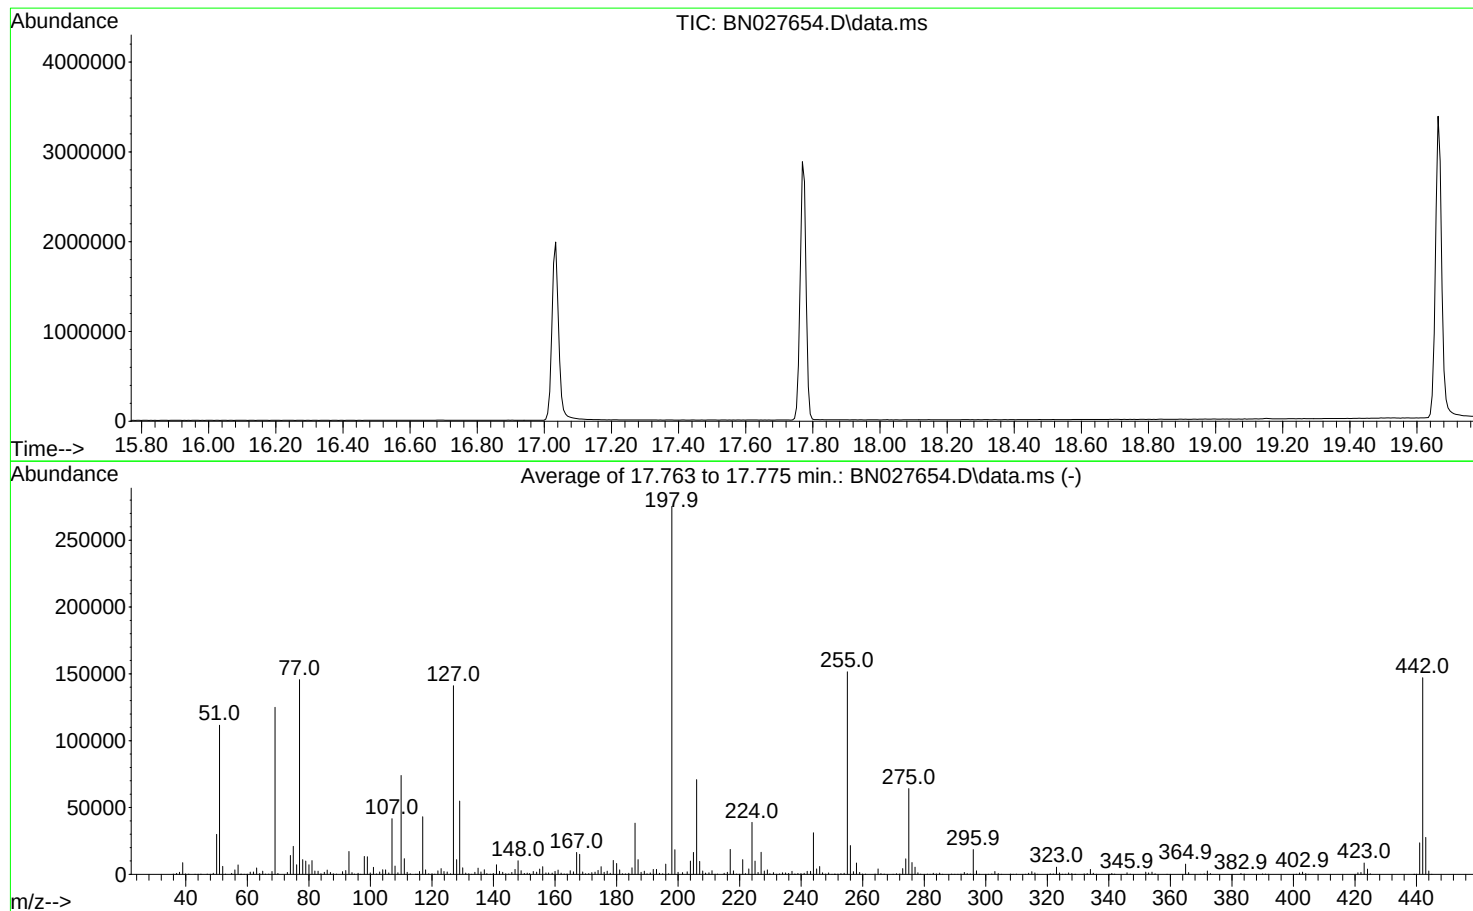




AutoFind: Scans 2529, 2530, 2531; Background Corrected with Scan 2522

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	111525	PASS
68	69	0.00	2	1.7	2131	PASS
69	198	0.00	100	45.4	124989	PASS
70	69	0.00	2	0.6	720	PASS
127	198	10	80	51.3	141187	PASS
197	198	0.00	2	0.2	466	PASS
198	198	100	100	100.0	275200	PASS
199	198	5	9	6.7	18448	PASS
275	198	10	60	23.3	64139	PASS
365	198	1	100	2.8	7640	PASS
441	198	0.01	100	8.6	23548	PASS
442	442	50	100	100.0	147117	PASS
443	442	15	24	18.8	27605	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091423\
Data File : BN027654.D
Acq On : 13 Sep 2023 21:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 14 08:12:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 14 08:12:26 2023
Response via : Initial Calibration

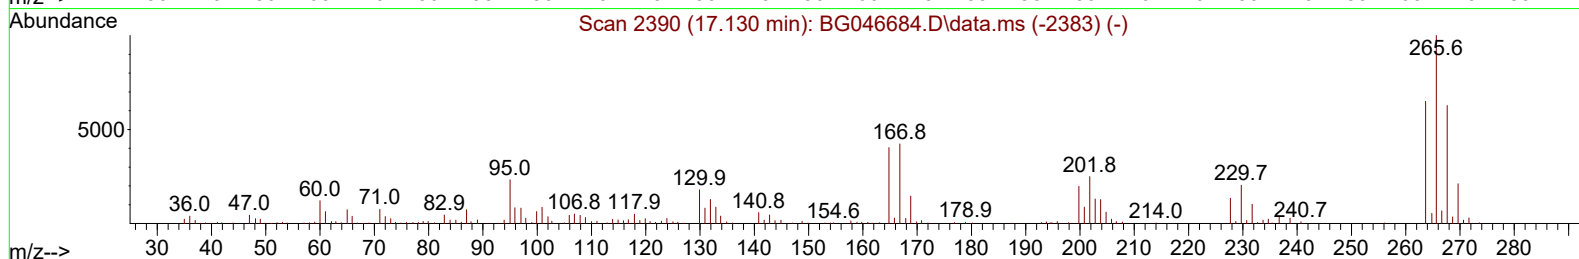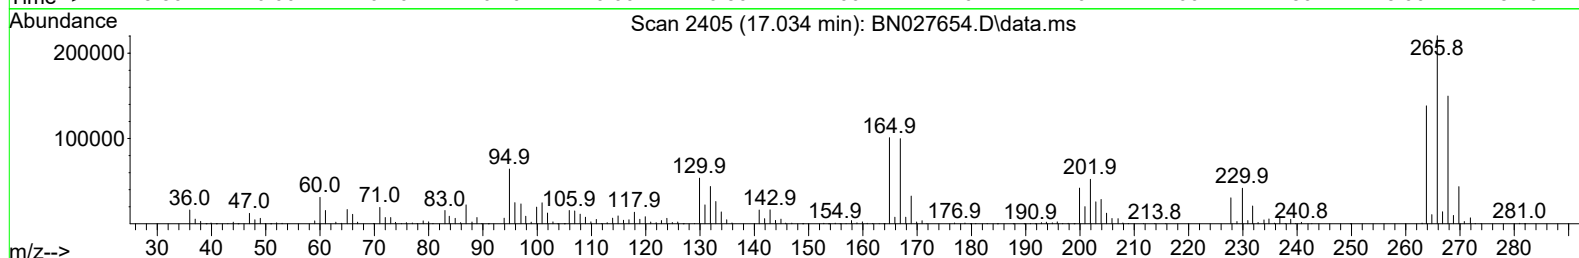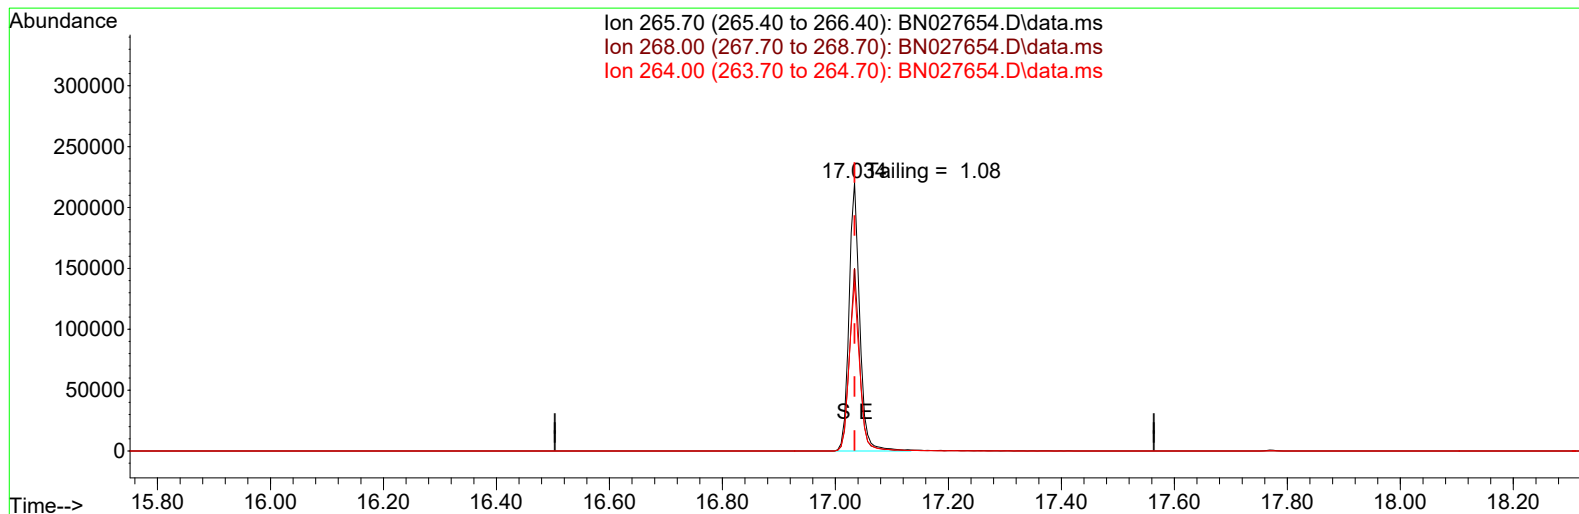

TIC: BN027654.D\data.ms

(70) Pentachlorophenol (C)

17.034min (0.000) 18028.00 ng




response 289608

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.97
264.00	61.60	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091423\
Data File : BN027654.D
Acq On : 13 Sep 2023 21:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 14 08:12:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 14 08:12:26 2023
Response via : Initial Calibration

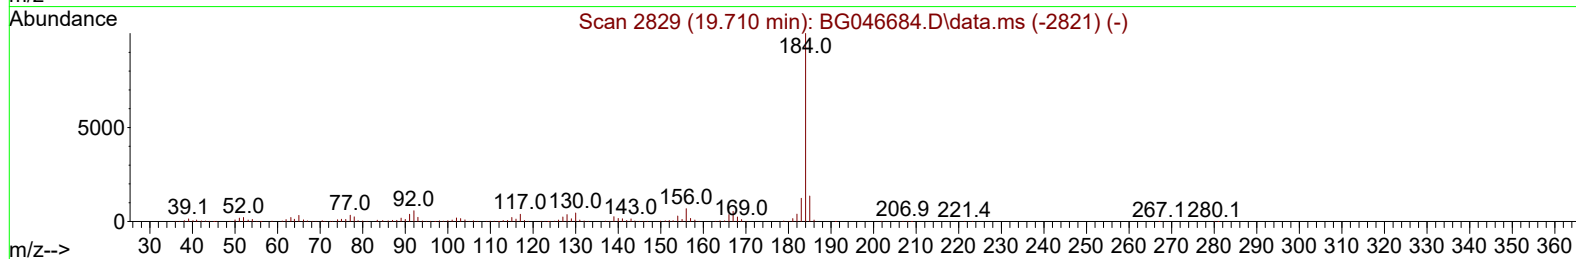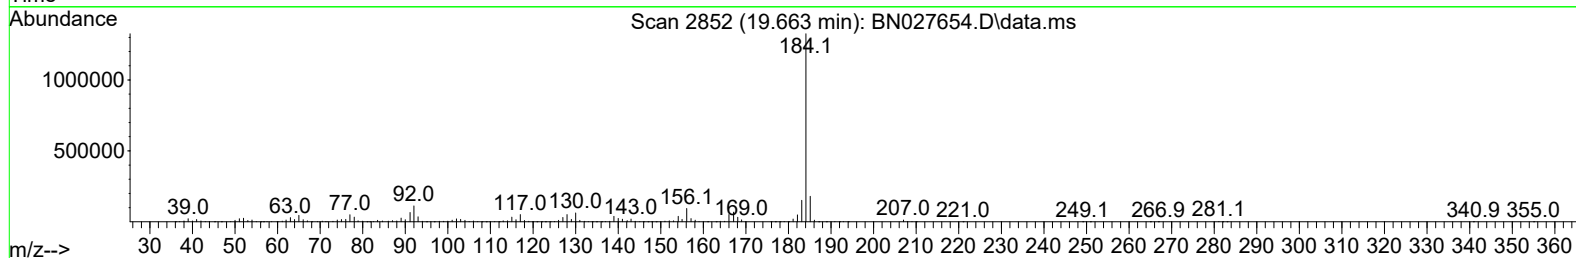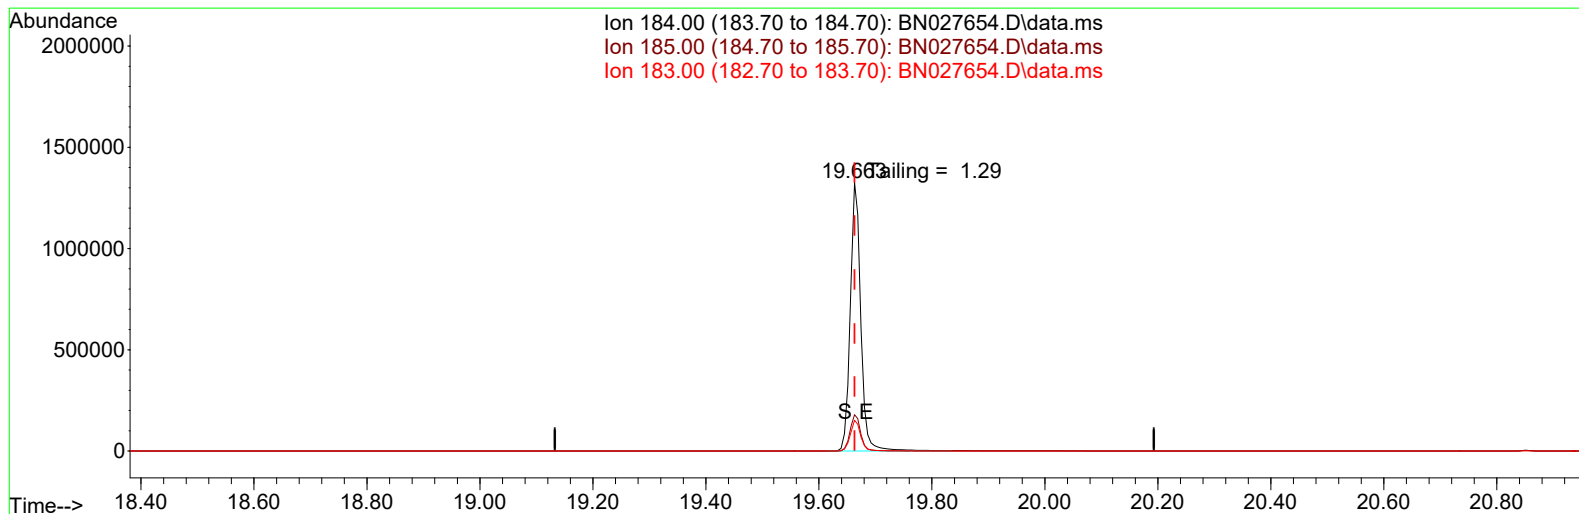

TIC: BN027654.D\data.ms

(77) Benzidine

19.663min (0.000) 0.00 ng

response 1720183

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.55
183.00	13.20	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/14/2023	BNA_N	<u>BN027654.D</u>
Compound Name	Response	Retention Time
DDT	795890	20.851
DDD	27566	20.416
DDE	1789	19.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29355	825245	3.56

Instrument :
BNA_N
ClientSampleId :
DFTPP