


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091423\
 Data File : BN027673.D
 Acq On : 14 Sep 2023 10:12
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 02:45:58 2023

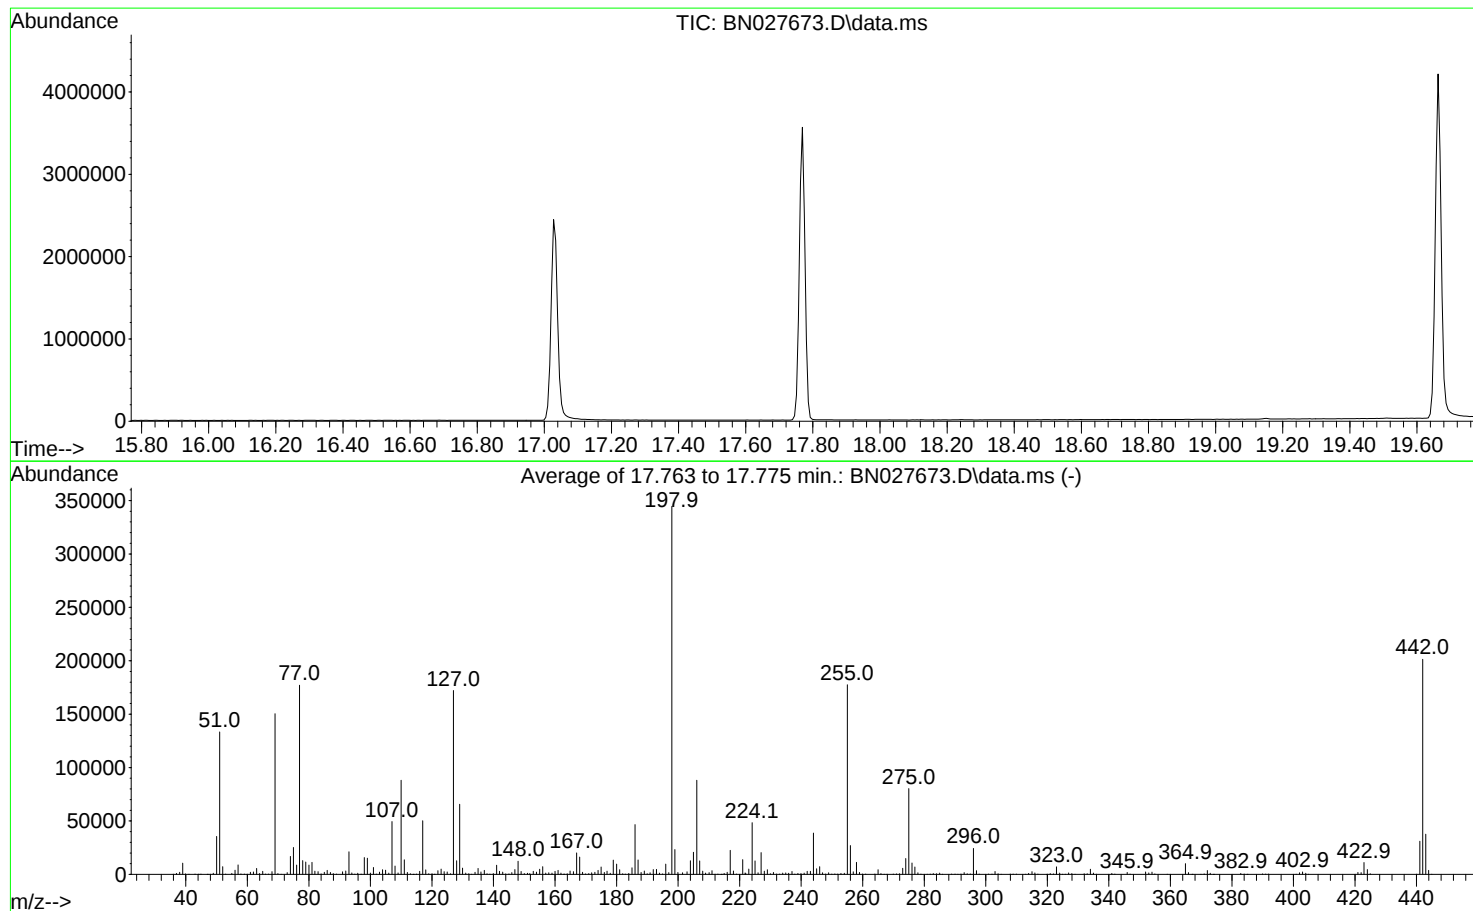




AutoFind: Scans 2529, 2530, 2531; Background Corrected with Scan 2522

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	133396	PASS
68	69	0.00	2	1.7	2591	PASS
69	198	0.00	100	43.7	150403	PASS
70	69	0.00	2	0.5	797	PASS
127	198	10	80	50.0	172139	PASS
197	198	0.00	2	0.5	1617	PASS
198	198	100	100	100.0	344427	PASS
199	198	5	9	6.7	23171	PASS
275	198	10	60	23.3	80341	PASS
365	198	1	100	2.9	9972	PASS
441	198	0.01	100	9.0	30981	PASS
442	442	50	100	100.0	201365	PASS
443	442	15	24	18.7	37597	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091423\
 Data File : BN027673.D
 Acq On : 14 Sep 2023 10:12
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 15 07:46:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 15 07:46:30 2023
 Response via : Initial Calibration

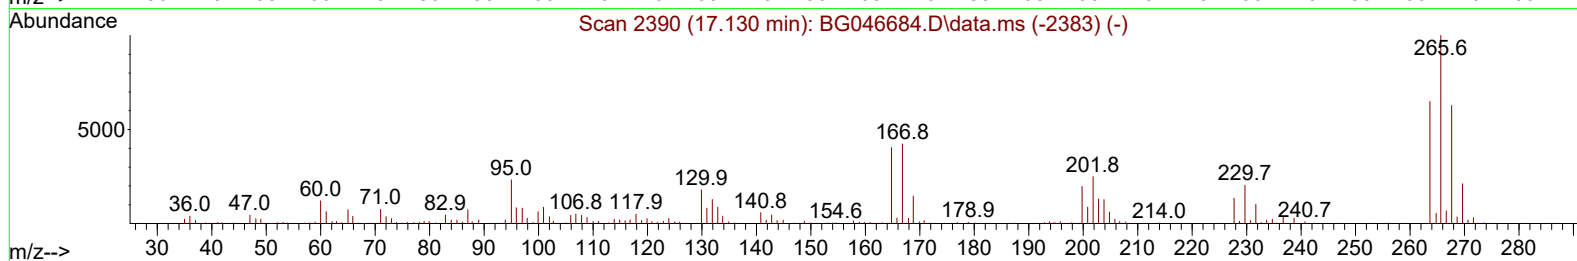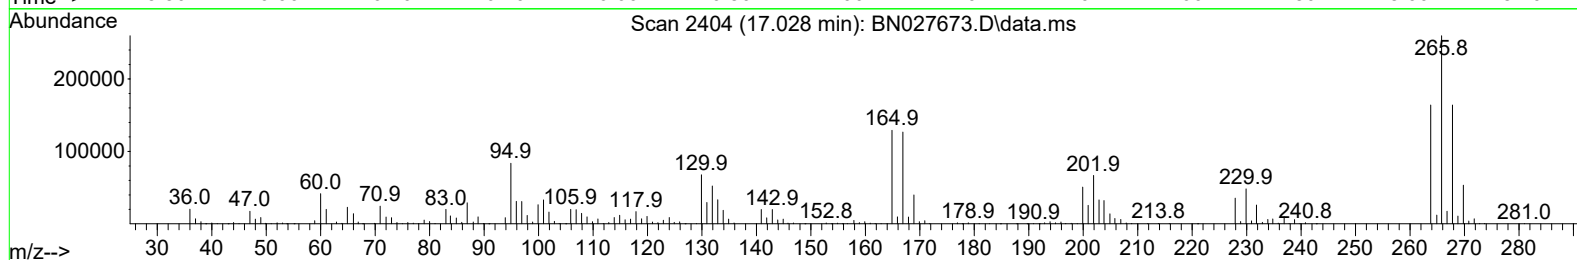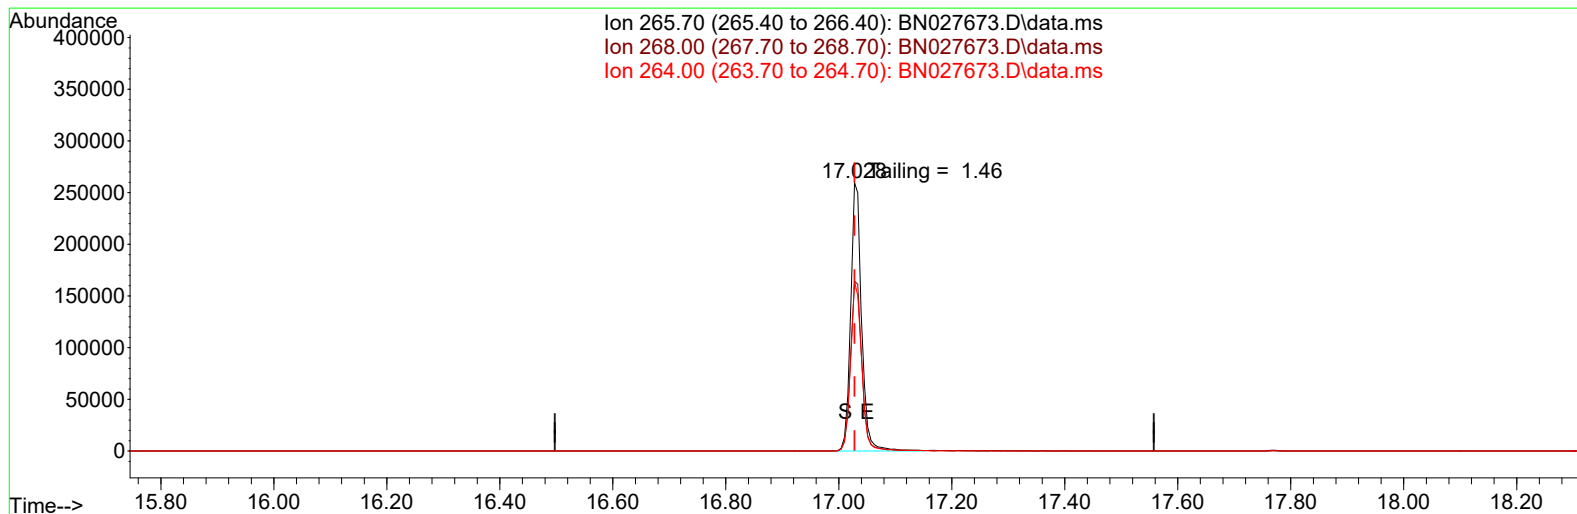

TIC: BN027673.D\data.ms

(70) Pentachlorophenol (C)

17.028min (0.000) 18461.90 ng




response 350765

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.18
264.00	61.60	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091423\
Data File : BN027673.D
Acq On : 14 Sep 2023 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 15 07:46:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 15 07:46:30 2023
Response via : Initial Calibration

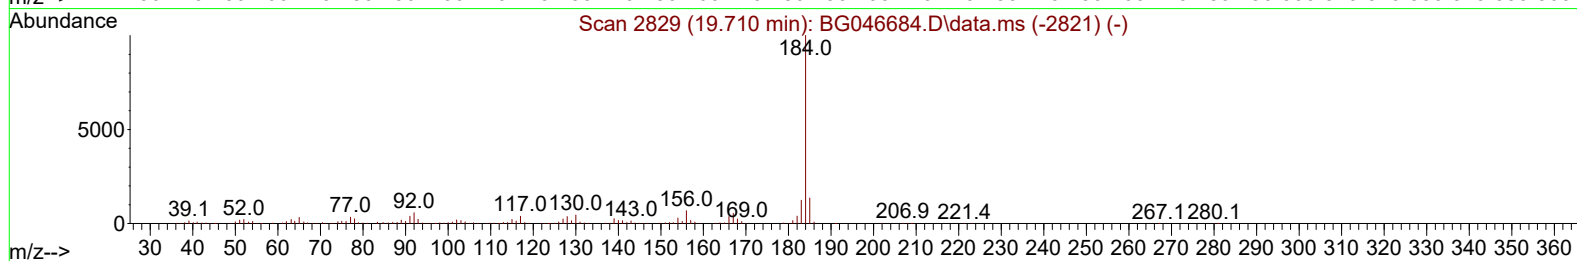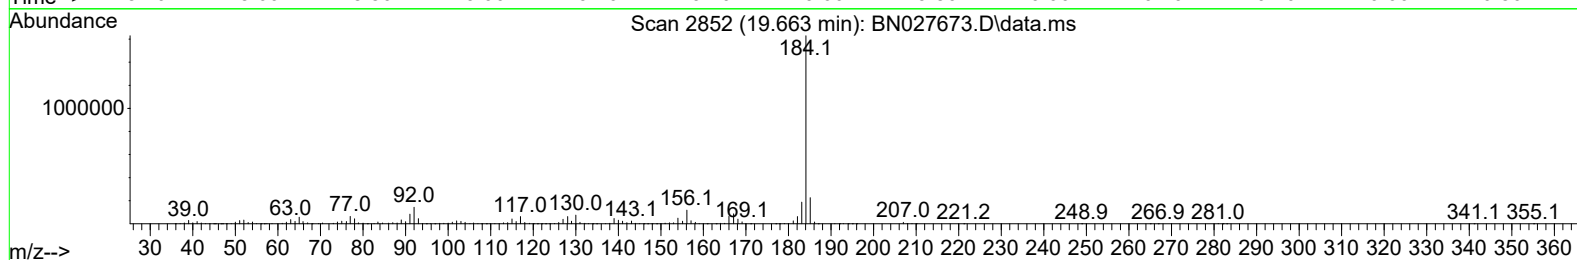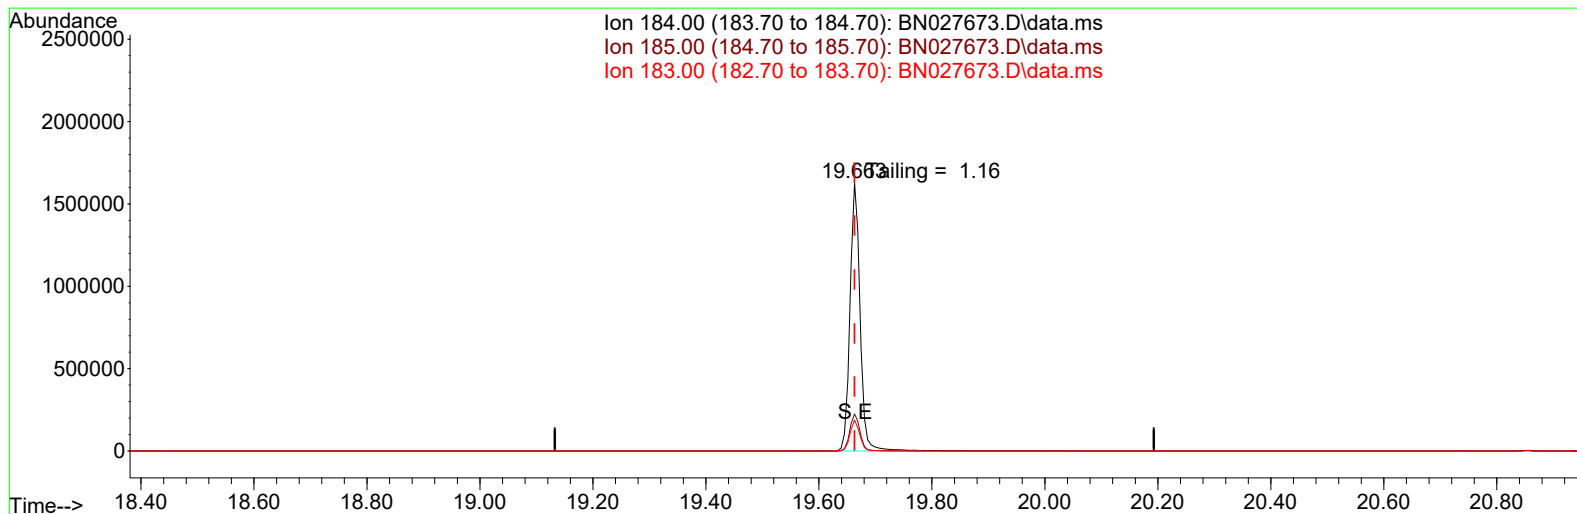

TIC: BN027673.D\data.ms

(77) Benzidine

19.663min (0.000) 0.00 ng

response 2033388

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.84
183.00	13.20	11.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/14/2023	BNA_N	<u>BN027673.D</u>
Compound Name	Response	Retention Time
DDT	954941	20.857
DDD	39755	20.416
DDE	2866	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
42621	997562	4.27

Instrument :
BNA_N
ClientSampleId :
DFTPP