

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033914.D
 Acq On : 14 Sep 2024 13:53
 Operator : JU/RC
 Sample : PB163391BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK391

Quant Time: Sep 15 01:58:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.485	152	3893	0.400	ng/ul	0.00
4) Naphthalene-d8	10.243	136	10703	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.132	164	5629	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.985	188	855565	0.400	ng/ul	0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.244	264	14494	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.101	96	26645	6.657	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.843	152	4837	0.315	ng/ul	0.00
18) Fluoranthene-d10	18.923	212	9789	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.135	88	131	0.029	ng/ul#	52
26) Benzo(a)pyrene	23.110	252	3855	0.085	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033914.D
Acq On : 14 Sep 2024 13:53
Operator : JU/RC
Sample : PB163391BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK391

Quant Time: Sep 15 01:58:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

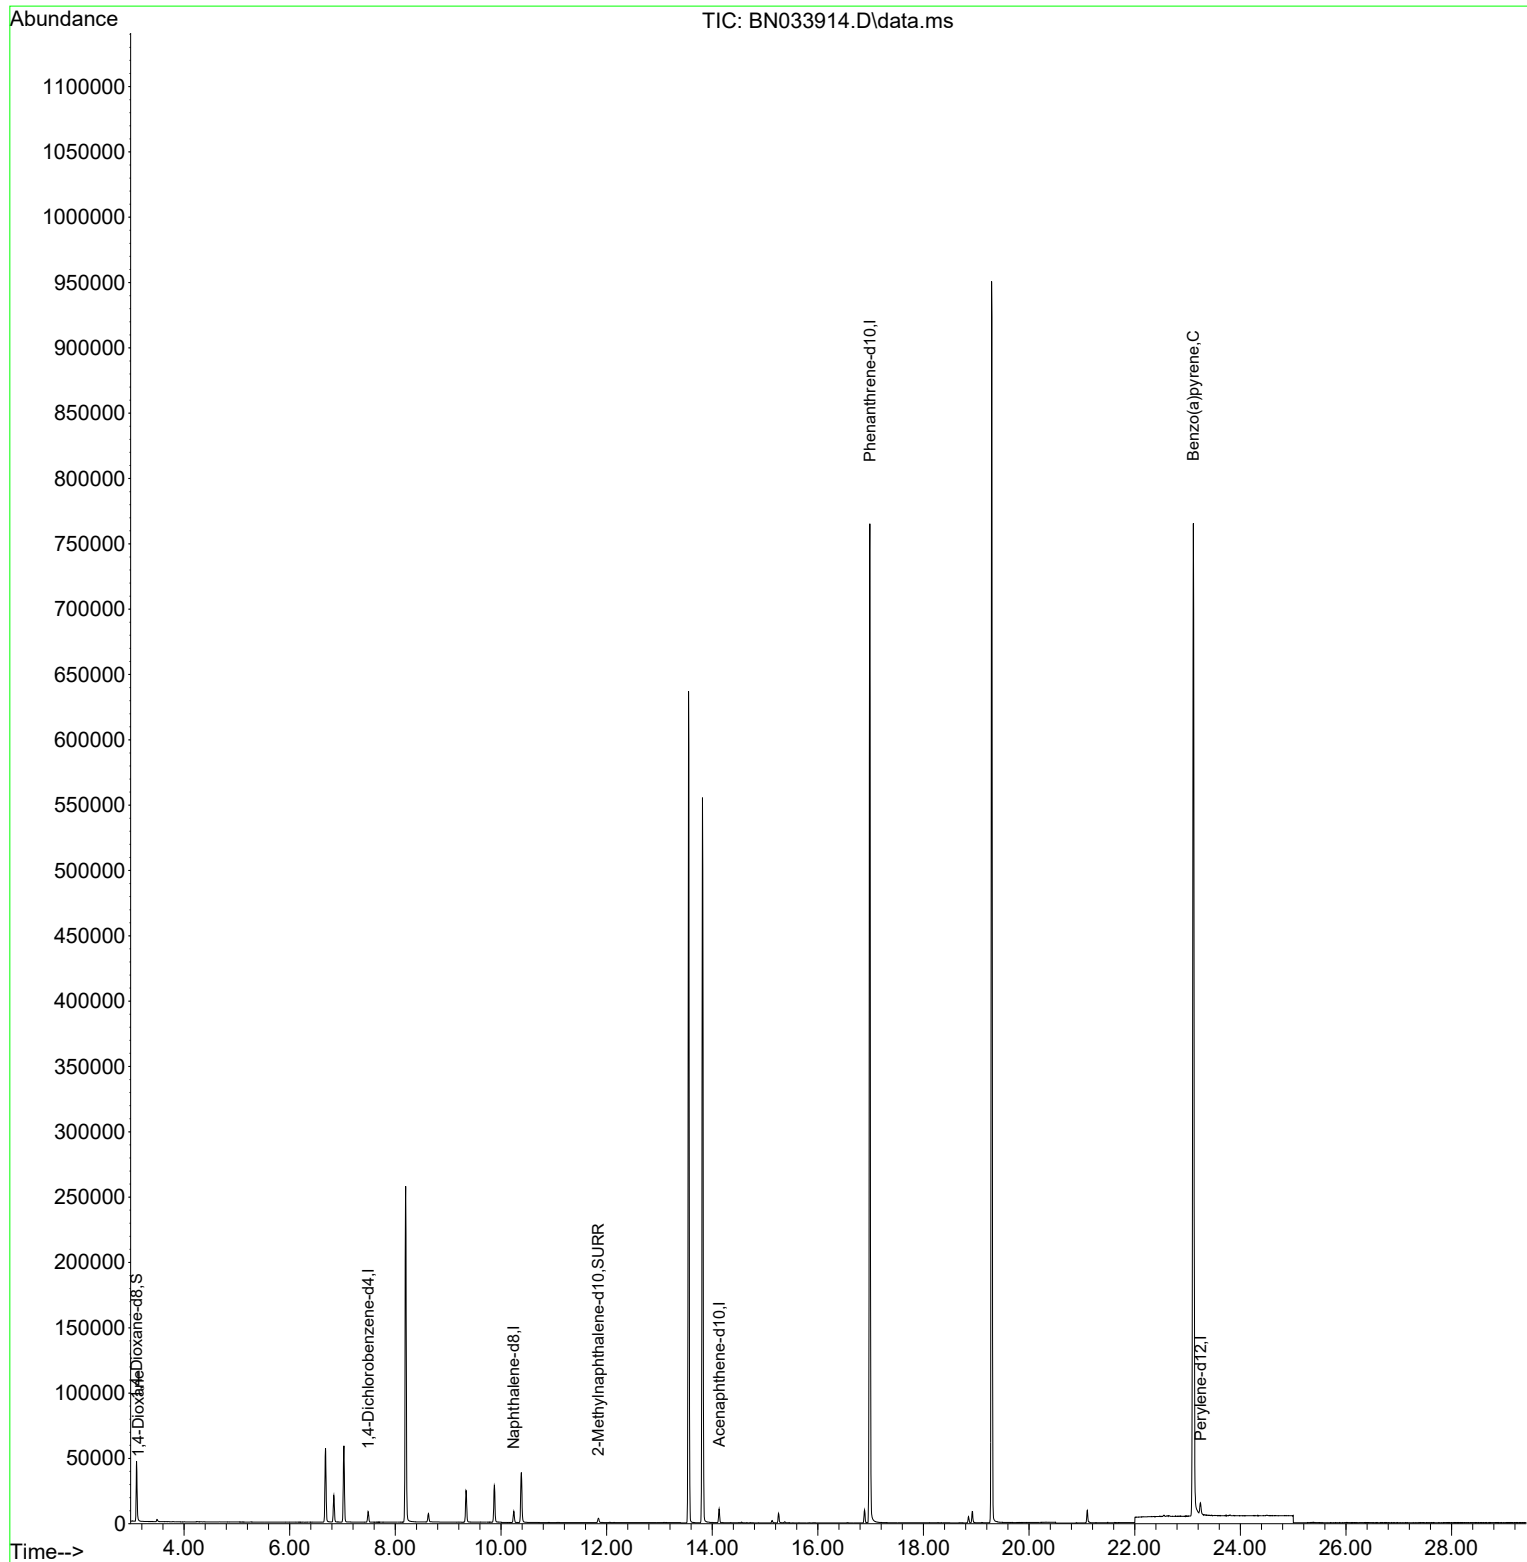

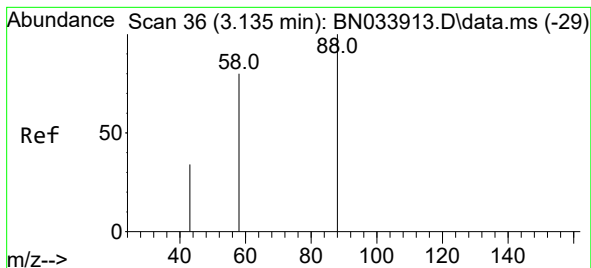

#2

1,4-Dioxane

Concen: 0.029 ng/ul

RT: 3.135 min Scan# 3

Delta R.T. -0.000 min

Lab File: BN033914.D

Acq: 14 Sep 2024 13:53

Instrument :

BNA_N

ClientSampleId :

SBLK391





Tgt Ion: 88 Resp: 131

Ion Ratio Lower Upper

88 100

43 90.8 47.0 70.4#

58 24.2 53.0 79.4#

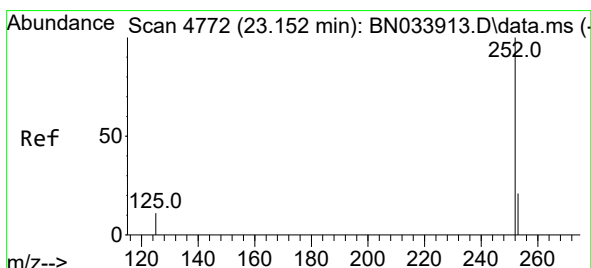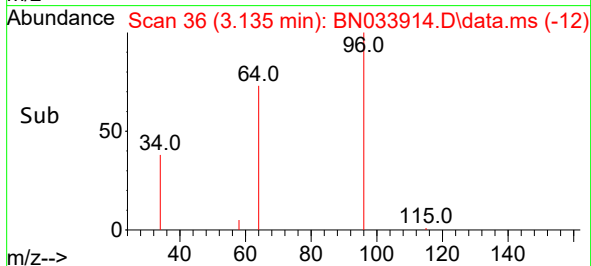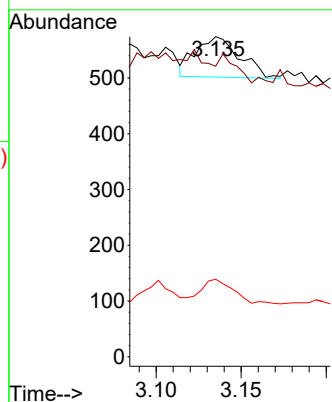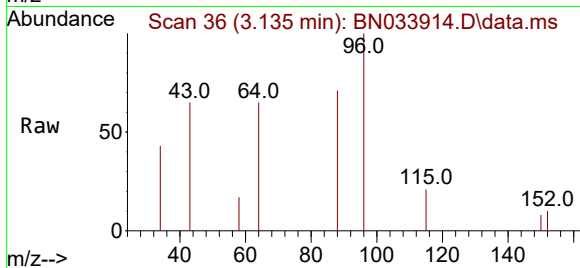

#26

Benzo(a)pyrene

Concen: 0.085 ng/ul

RT: 23.110 min Scan# 4758

Delta R.T. -0.042 min

Lab File: BN033914.D

Acq: 14 Sep 2024 13:53

Tgt Ion: 252 Resp: 3855

Ion Ratio Lower Upper

252 100

253 51.5 22.8 34.2#

125 49.0 18.0 27.0#

