

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033918.D
 Acq On : 14 Sep 2024 17:00
 Operator : JU/RC
 Sample : PB163194BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK194

Quant Time: Sep 15 01:59:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.485	152	4240	0.400	ng/ul	0.00
4) Naphthalene-d8	10.244	136	11801	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.128	164	6241	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.982	188	1003816	0.400	ng/ul	0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.245	264	16707	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.101	96	31236	7.166	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.845	152	5352	0.316	ng/ul	0.00
18) Fluoranthene-d10	18.924	212	11381	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.135	88	280	0.058	ng/ul#	63
26) Benzo(a)pyrene	23.111	252	4977	0.096	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033918.D
Acq On : 14 Sep 2024 17:00
Operator : JU/RC
Sample : PB163194BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK194

Quant Time: Sep 15 01:59:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

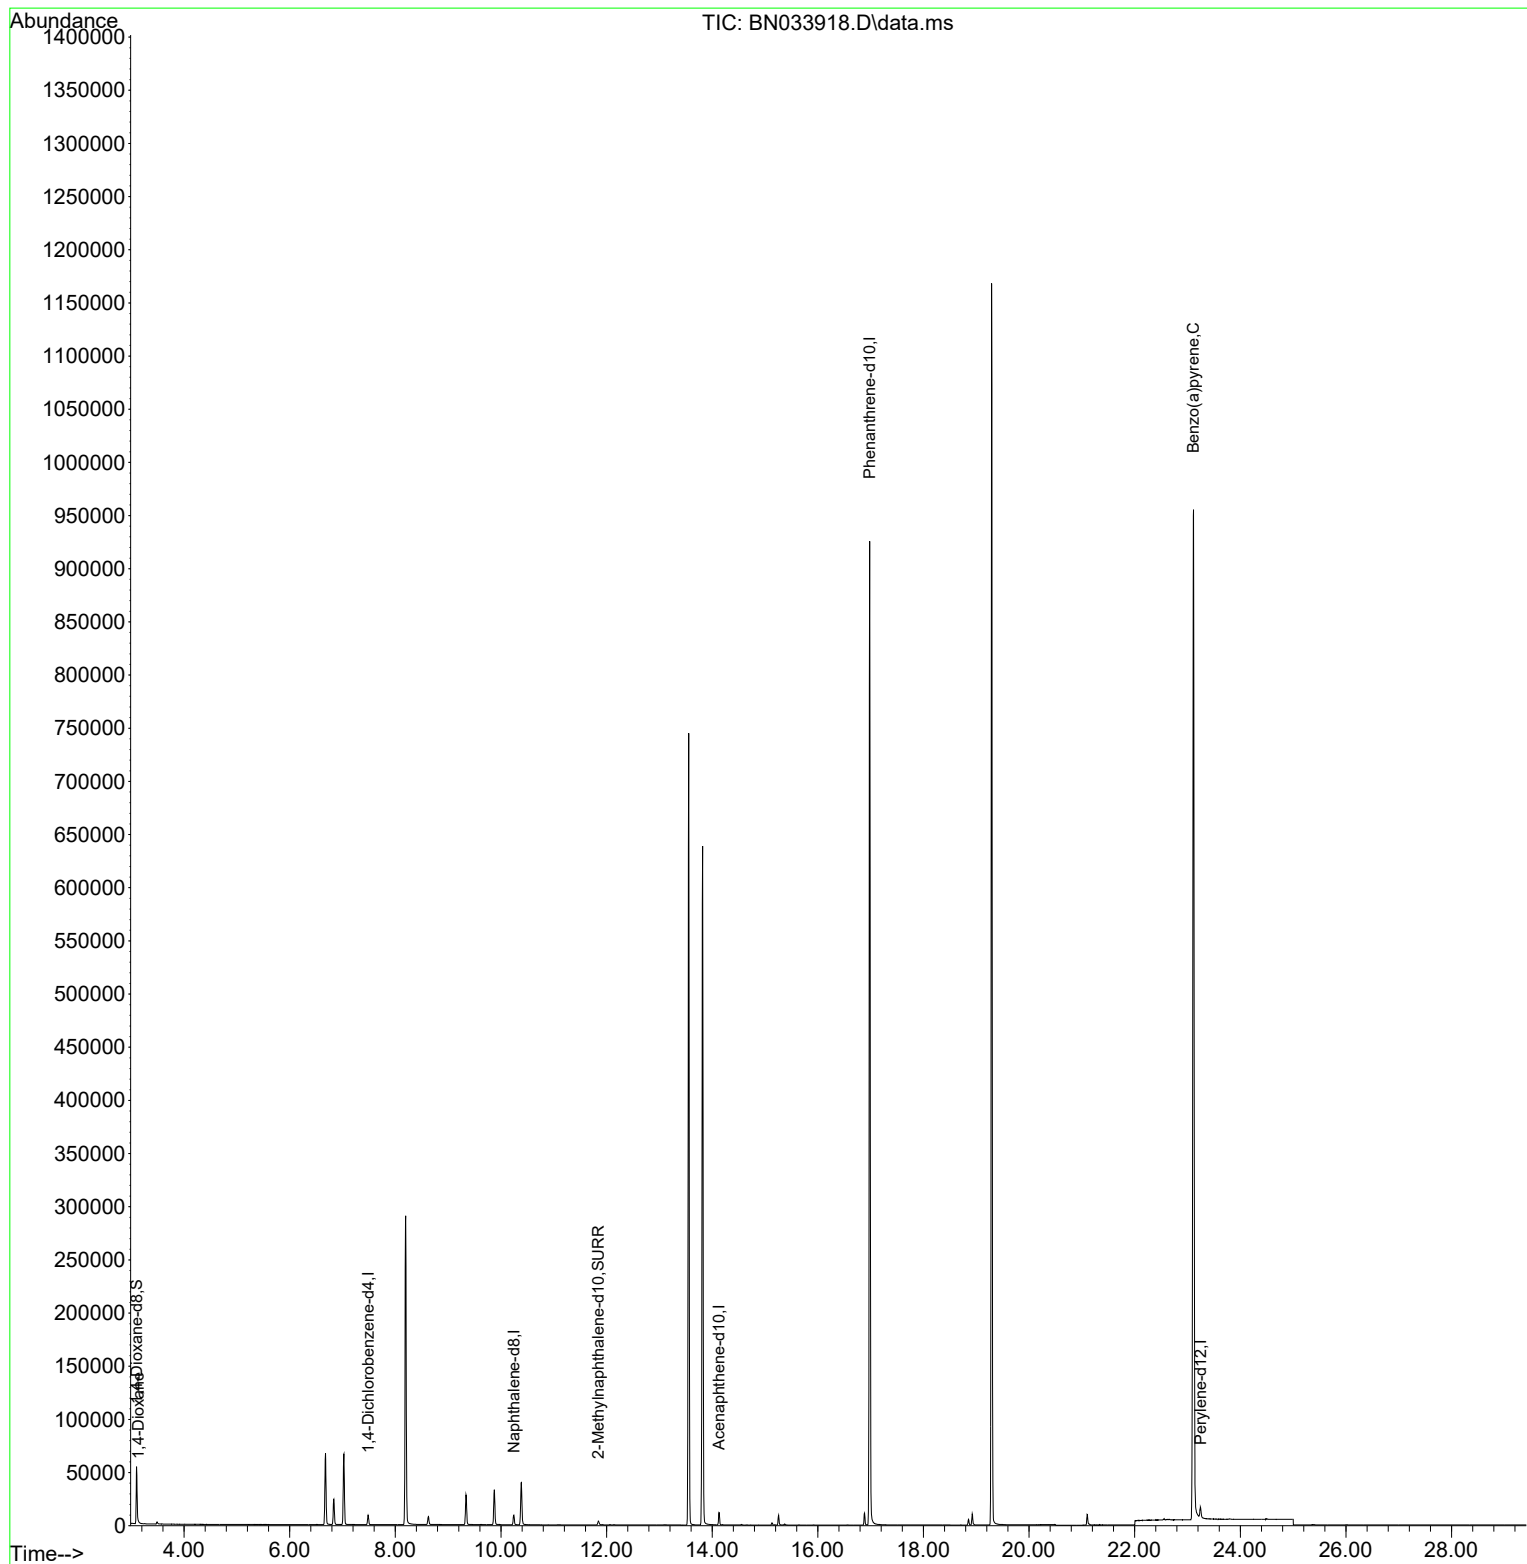

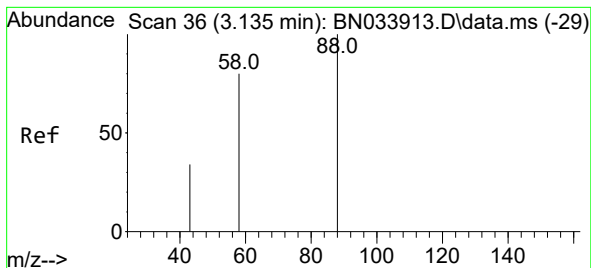

#2

1,4-Dioxane

Concen: 0.058 ng/ul

RT: 3.135 min Scan# 30

Delta R.T. -0.000 min

Lab File: BN033918.D

Acq: 14 Sep 2024 17:00

Instrument :

BNA_N

ClientSampleId :

SBLK194





Tgt Ion: 88 Resp: 280

Ion Ratio Lower Upper

88 100

43 48.1 47.0 70.4

58 20.5 53.0 79.4#

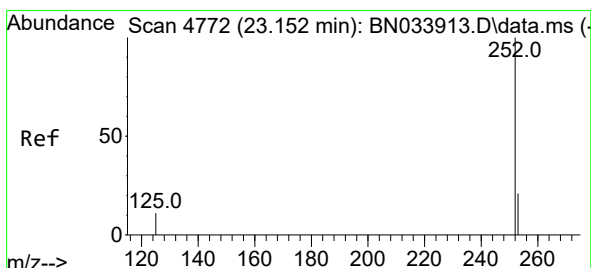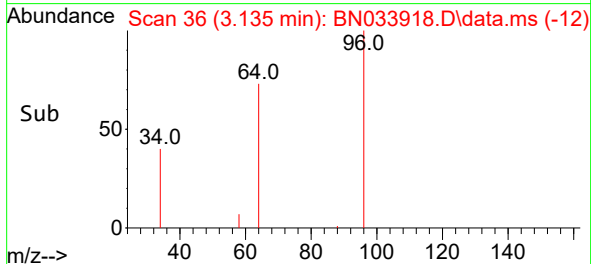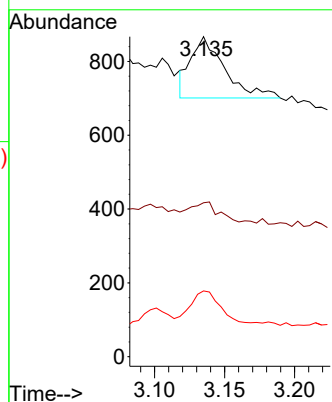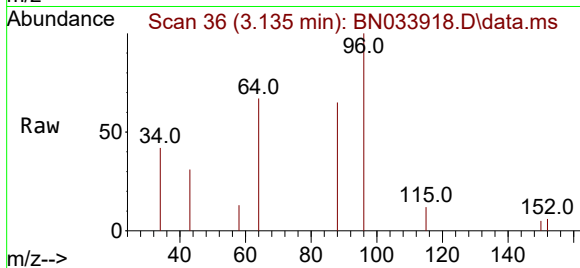

#26

Benzo(a)pyrene

Concen: 0.096 ng/ul

RT: 23.111 min Scan# 4758

Delta R.T. -0.041 min

Lab File: BN033918.D

Acq: 14 Sep 2024 17:00

Tgt Ion: 252 Resp: 4977

Ion Ratio Lower Upper

252 100

253 46.8 22.8 34.2#

125 43.7 18.0 27.0#

