

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033925.D
 Acq On : 14 Sep 2024 21:13
 Operator : JU/RC
 Sample : P3952-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B26

Quant Time: Sep 15 01:59:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.485	152	3642	0.400	ng/ul	0.00
4) Naphthalene-d8	10.243	136	10405	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.132	164	5571	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.981	188	1173172	0.400	ng/ul	0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.238	264	15854	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.101	96	24092	6.434	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.843	152	5747	0.385	ng/ul	0.00
18) Fluoranthene-d10	18.923	212	14386	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.135	88	6452	1.553	ng/ul#	84
24) Benzo(b)fluoranthene	22.604	252	1477	0.024	ng/ul#	7
26) Benzo(a)pyrene	23.104	252	4543	0.092	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033925.D
Acq On : 14 Sep 2024 21:13
Operator : JU/RC
Sample : P3952-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B26

Quant Time: Sep 15 01:59:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration




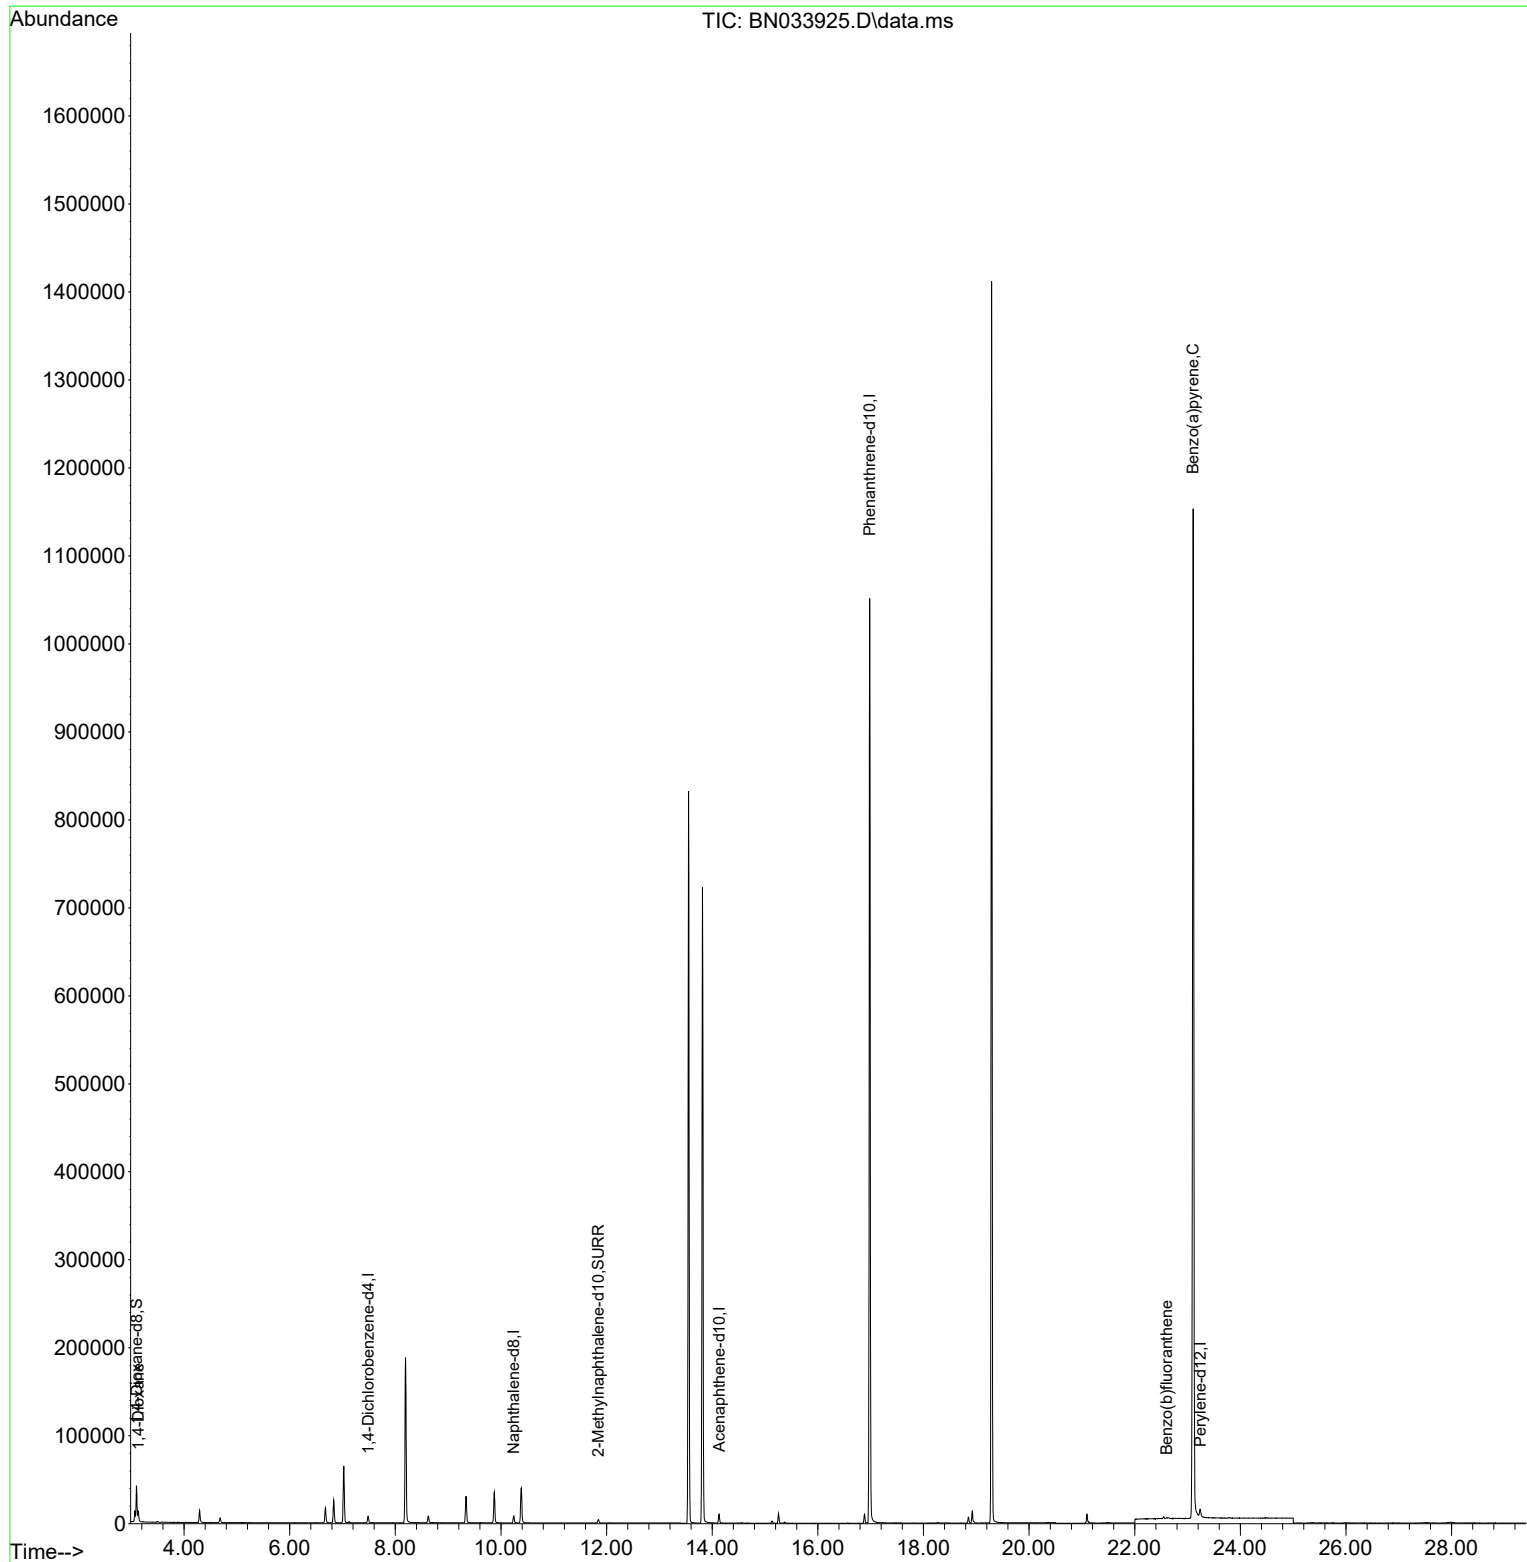


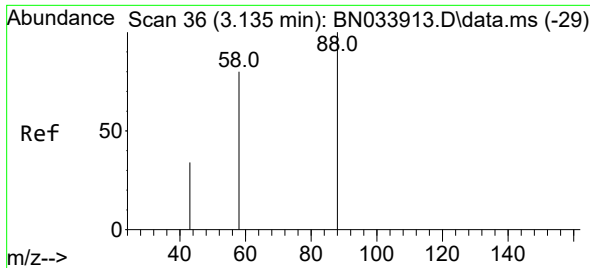

#2
1,4-Dioxane
Concen: 1.553 ng/ul
RT: 3.135 min Scan# 30
Delta R.T. 0.000 min
Lab File: BN033925.D
Acq: 14 Sep 2024 21:13




Instrument :
BNA_N
ClientSampleId :
C0B26


Tgt Ion: 88 Resp: 6452
Ion Ratio Lower Upper
88 100
43 34.5 47.0 70.4#
58 67.0 53.0 79.4

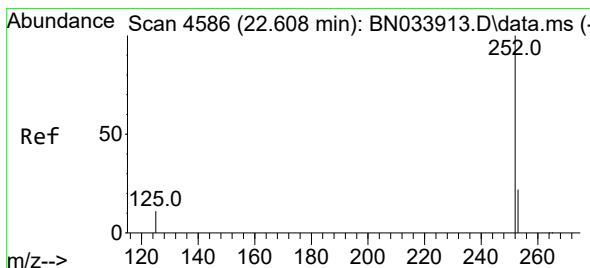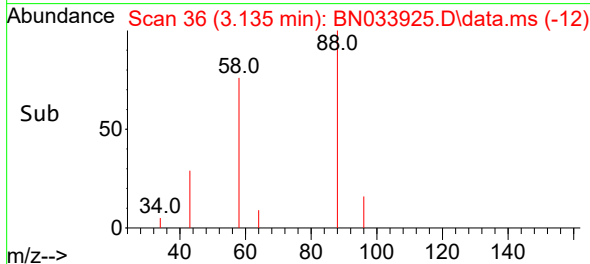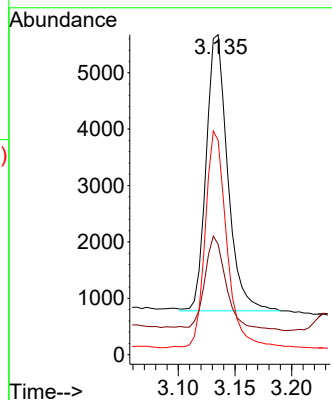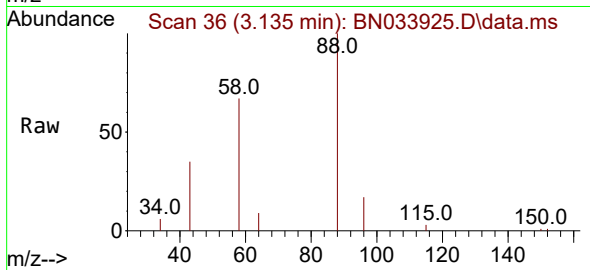

#24
Benzo(b)fluoranthene
Concen: 0.024 ng/ul
RT: 22.604 min Scan# 4585
Delta R.T. -0.004 min
Lab File: BN033925.D
Acq: 14 Sep 2024 21:13


Tgt Ion: 252 Resp: 1477
Ion Ratio Lower Upper
252 100
253 67.3 0.0 52.8#
125 67.7 0.0 36.4#

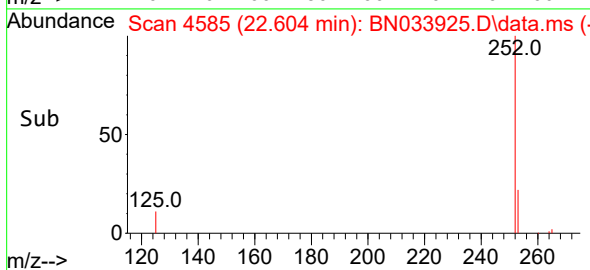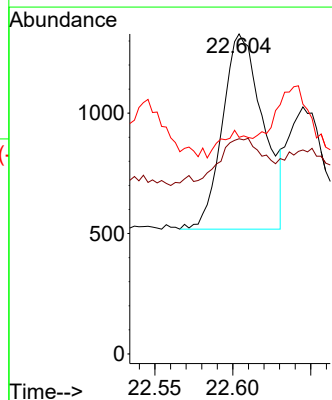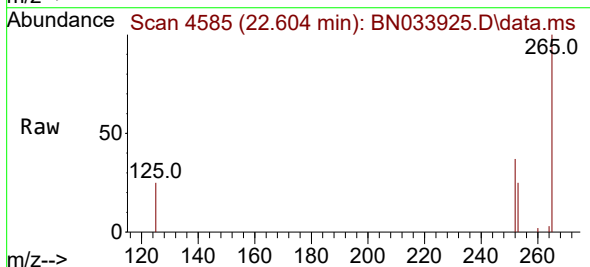

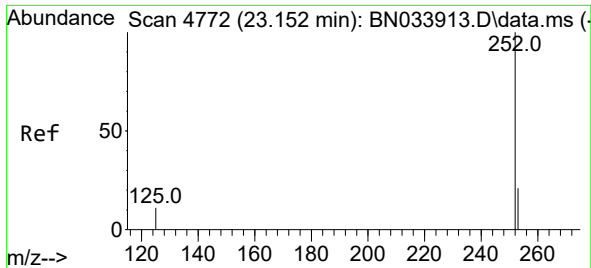

#26
Benzo(a)pyrene
Concen: 0.092 ng/ul
RT: 23.104 min Scan# 41
Delta R.T. -0.048 min
Lab File: BN033925.D
Acq: 14 Sep 2024 21:13

Instrument :
BNA_N
ClientSampleId :
C0B26

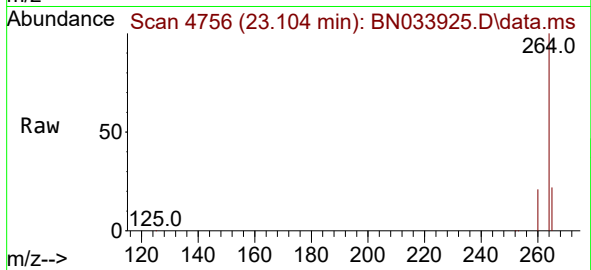

Tgt Ion:252 Resp: 4543
Ion Ratio Lower Upper
252 100
253 43.2 22.8 34.2#
125 40.9 18.0 27.0#

