

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033929.D
 Acq On : 15 Sep 2024 00:14
 Operator : JU/RC
 Sample : PB163194BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK194

Quant Time: Sep 15 02:00:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.485	152	4749	0.400	ng/ul	0.00
4) Naphthalene-d8	10.244	136	13308	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.128	164	6966	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.982	188	1103240	0.400	ng/ul	0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.243	264	17956	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.101	96	34432	7.052	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.845	152	6131	0.321	ng/ul	0.00
18) Fluoranthene-d10	18.924	212	12449	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.135	88	230	0.042	ng/ul#	69
26) Benzo(a)pyrene	23.111	252	5302	0.095	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033929.D
Acq On : 15 Sep 2024 00:14
Operator : JU/RC
Sample : PB163194BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK194

Quant Time: Sep 15 02:00:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration




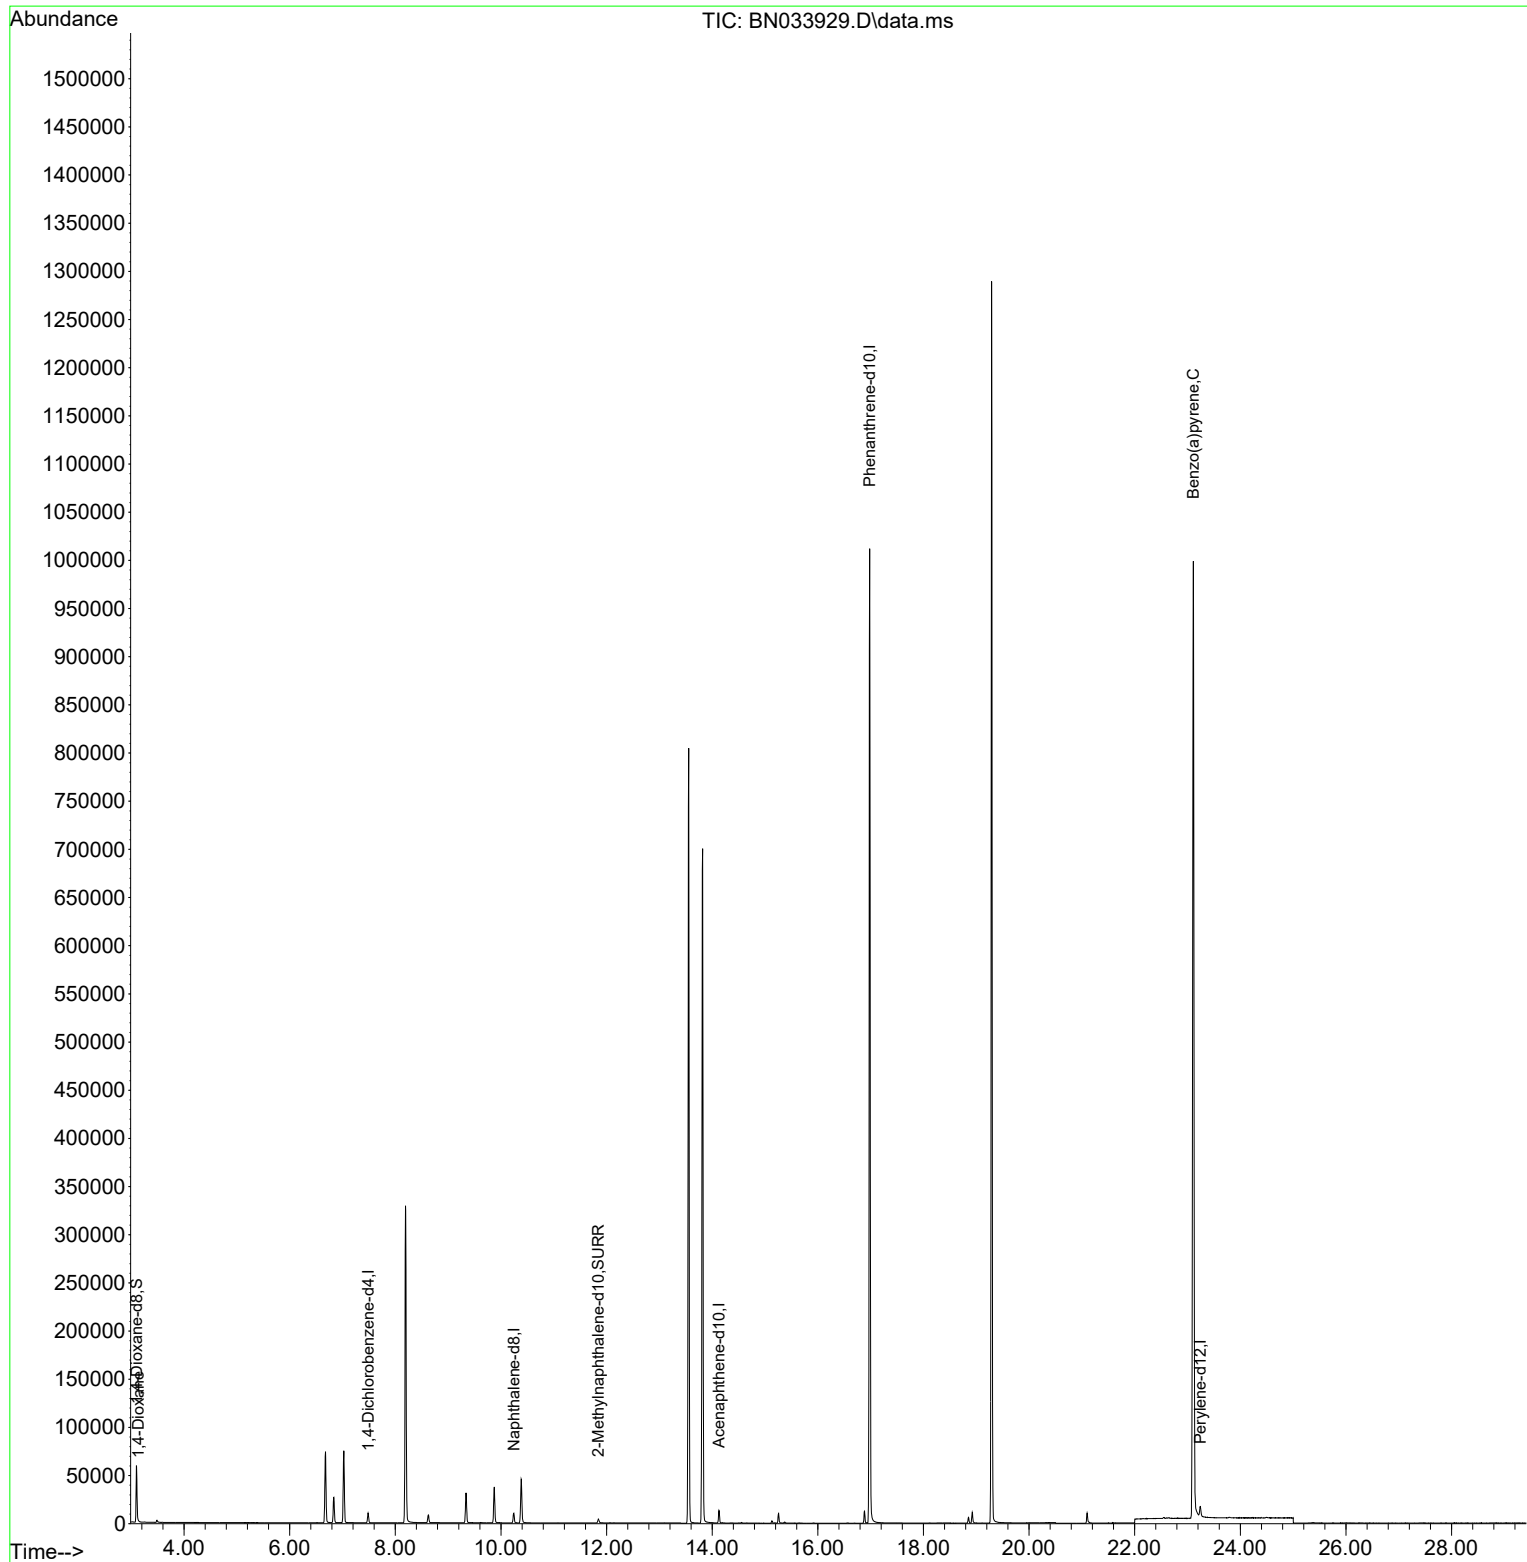


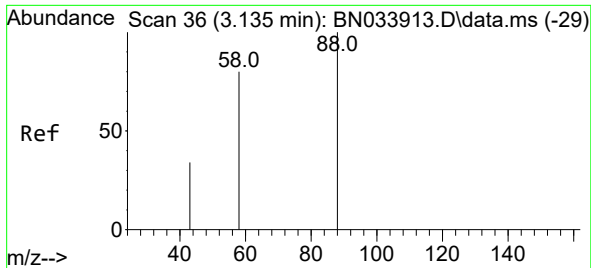

#2
1,4-Dioxane
Concen: 0.042 ng/ul
RT: 3.135 min Scan# 30
Delta R.T. -0.000 min
Lab File: BN033929.D
Acq: 15 Sep 2024 00:14

Instrument :
BNA_N
ClientSampleId :
SBLK194

Tgt Ion: 88 Resp: 230
Ion Ratio Lower Upper
88 100
43 52.1 47.0 70.4
58 26.3 53.0 79.4#

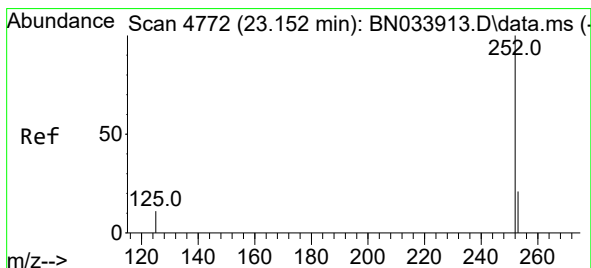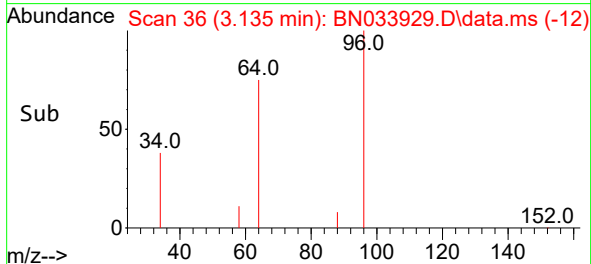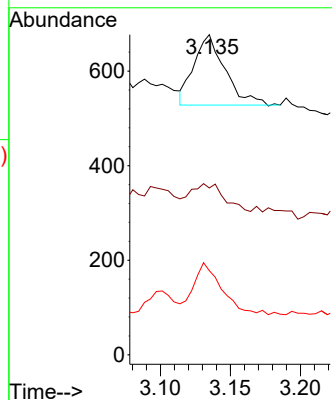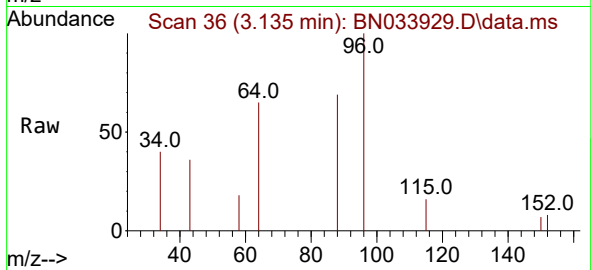

#26
Benzo(a)pyrene
Concen: 0.095 ng/ul
RT: 23.111 min Scan# 4758
Delta R.T. -0.041 min
Lab File: BN033929.D
Acq: 15 Sep 2024 00:14

Tgt Ion: 252 Resp: 5302
Ion Ratio Lower Upper
252 100
253 46.1 22.8 34.2#
125 43.4 18.0 27.0#

