

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033944.D
 Acq On : 15 Sep 2024 10:27
 Operator : JU/RC
 Sample : PB163352BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK352

Quant Time: Sep 16 00:12:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.481	152	3712	0.400	ng/ul	0.00
4) Naphthalene-d8	10.239	136	10229	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.128	164	5313	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.978	188	969927	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.240	264	15692	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	30402	7.967	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.845	152	5239	0.357	ng/ul	0.00
18) Fluoranthene-d10	18.924	212	11073	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.131	88	254	0.060	ng/ul#	71
26) Benzo(a)pyrene	23.111	252	4983	0.102	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033944.D
Acq On : 15 Sep 2024 10:27
Operator : JU/RC
Sample : PB163352BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK352

Quant Time: Sep 16 00:12:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration




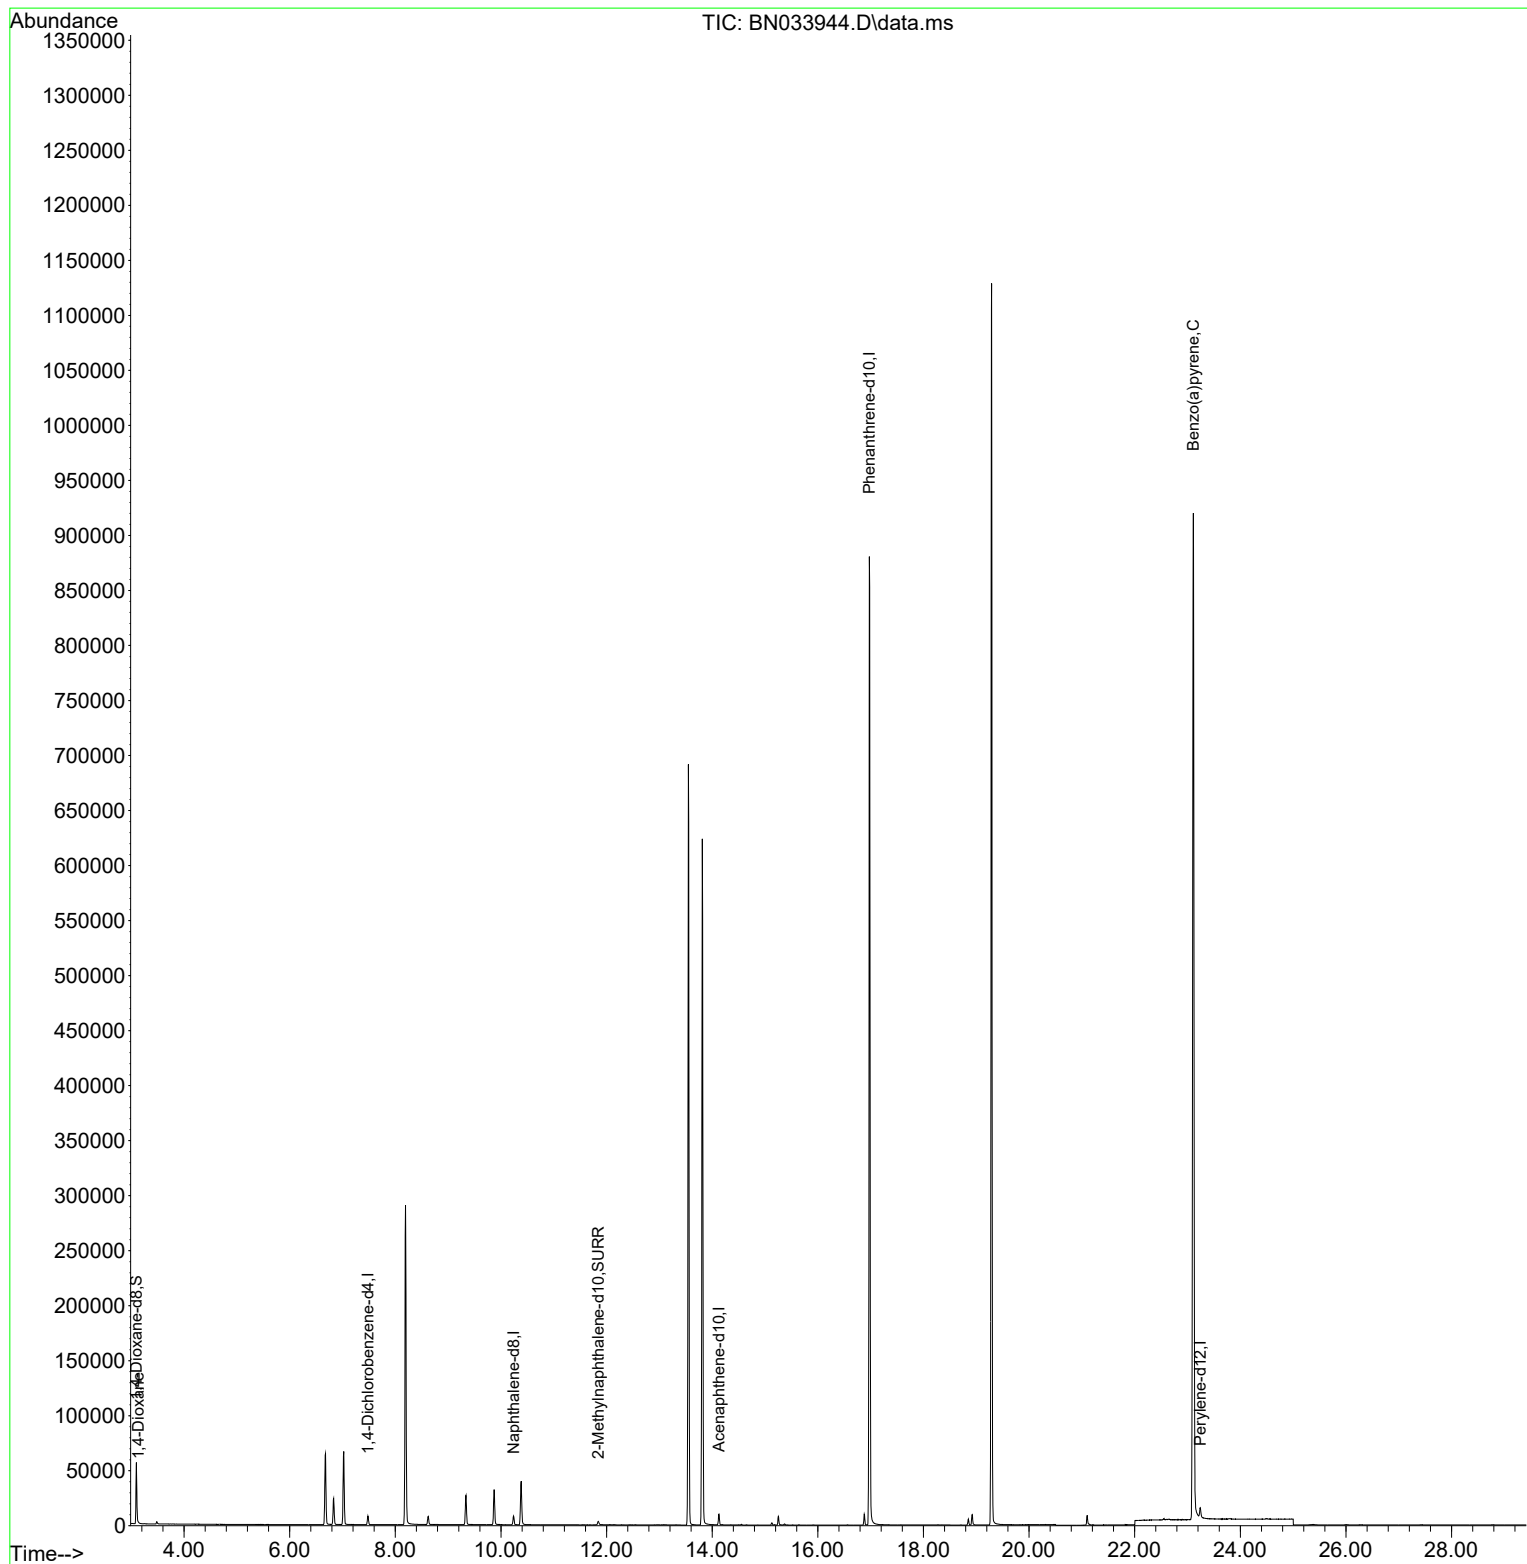


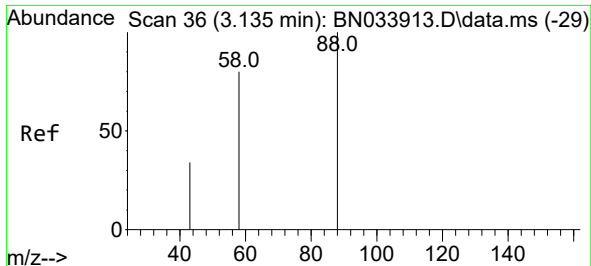

#2
1,4-Dioxane
Concen: 0.060 ng/ul
RT: 3.131 min Scan# 31
Delta R.T. -0.004 min
Lab File: BN033944.D
Acq: 15 Sep 2024 10:27

Instrument :
BNA_N
ClientSampleId :
SBLK352

Tgt Ion: 88 Resp: 254
Ion Ratio Lower Upper
88 100
43 52.9 47.0 70.4
58 28.1 53.0 79.4#

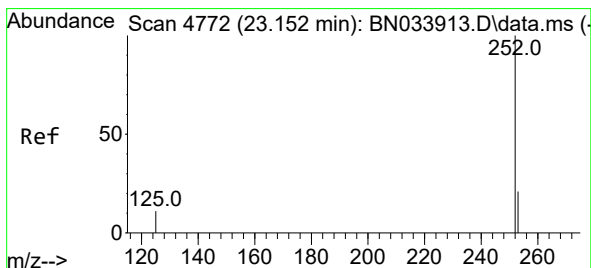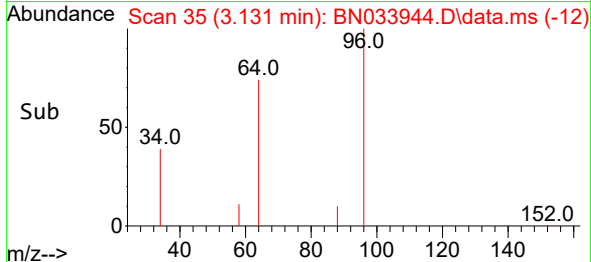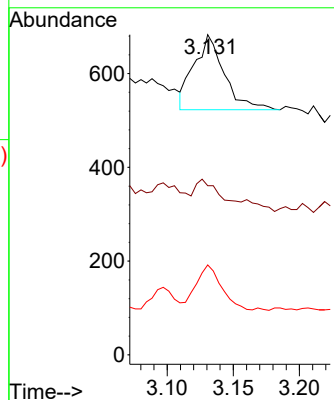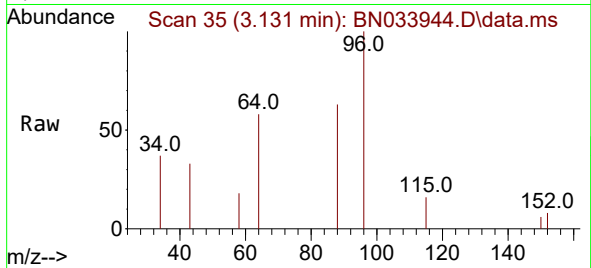

#26
Benzo(a)pyrene
Concen: 0.102 ng/ul
RT: 23.111 min Scan# 4758
Delta R.T. -0.041 min
Lab File: BN033944.D
Acq: 15 Sep 2024 10:27

Tgt Ion: 252 Resp: 4983
Ion Ratio Lower Upper
252 100
253 47.6 22.8 34.2#
125 43.5 18.0 27.0#

