

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033951.D
 Acq On : 15 Sep 2024 14:39
 Operator : JU/RC
 Sample : P3922-08
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AS9

Quant Time: Sep 16 00:13:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.481	152	4831	0.400	ng/ul	0.00
4) Naphthalene-d8	10.239	136	13838	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.128	164	7547	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.978	188	1368314	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.243	264	22068	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	24977	5.029	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.839	152	6100	0.307	ng/ul	0.00
18) Fluoranthene-d10	18.920	212	17625	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
26) Benzo(a)pyrene	23.108	252	6265	0.091	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033951.D
Acq On : 15 Sep 2024 14:39
Operator : JU/RC
Sample : P3922-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AS9

Quant Time: Sep 16 00:13:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

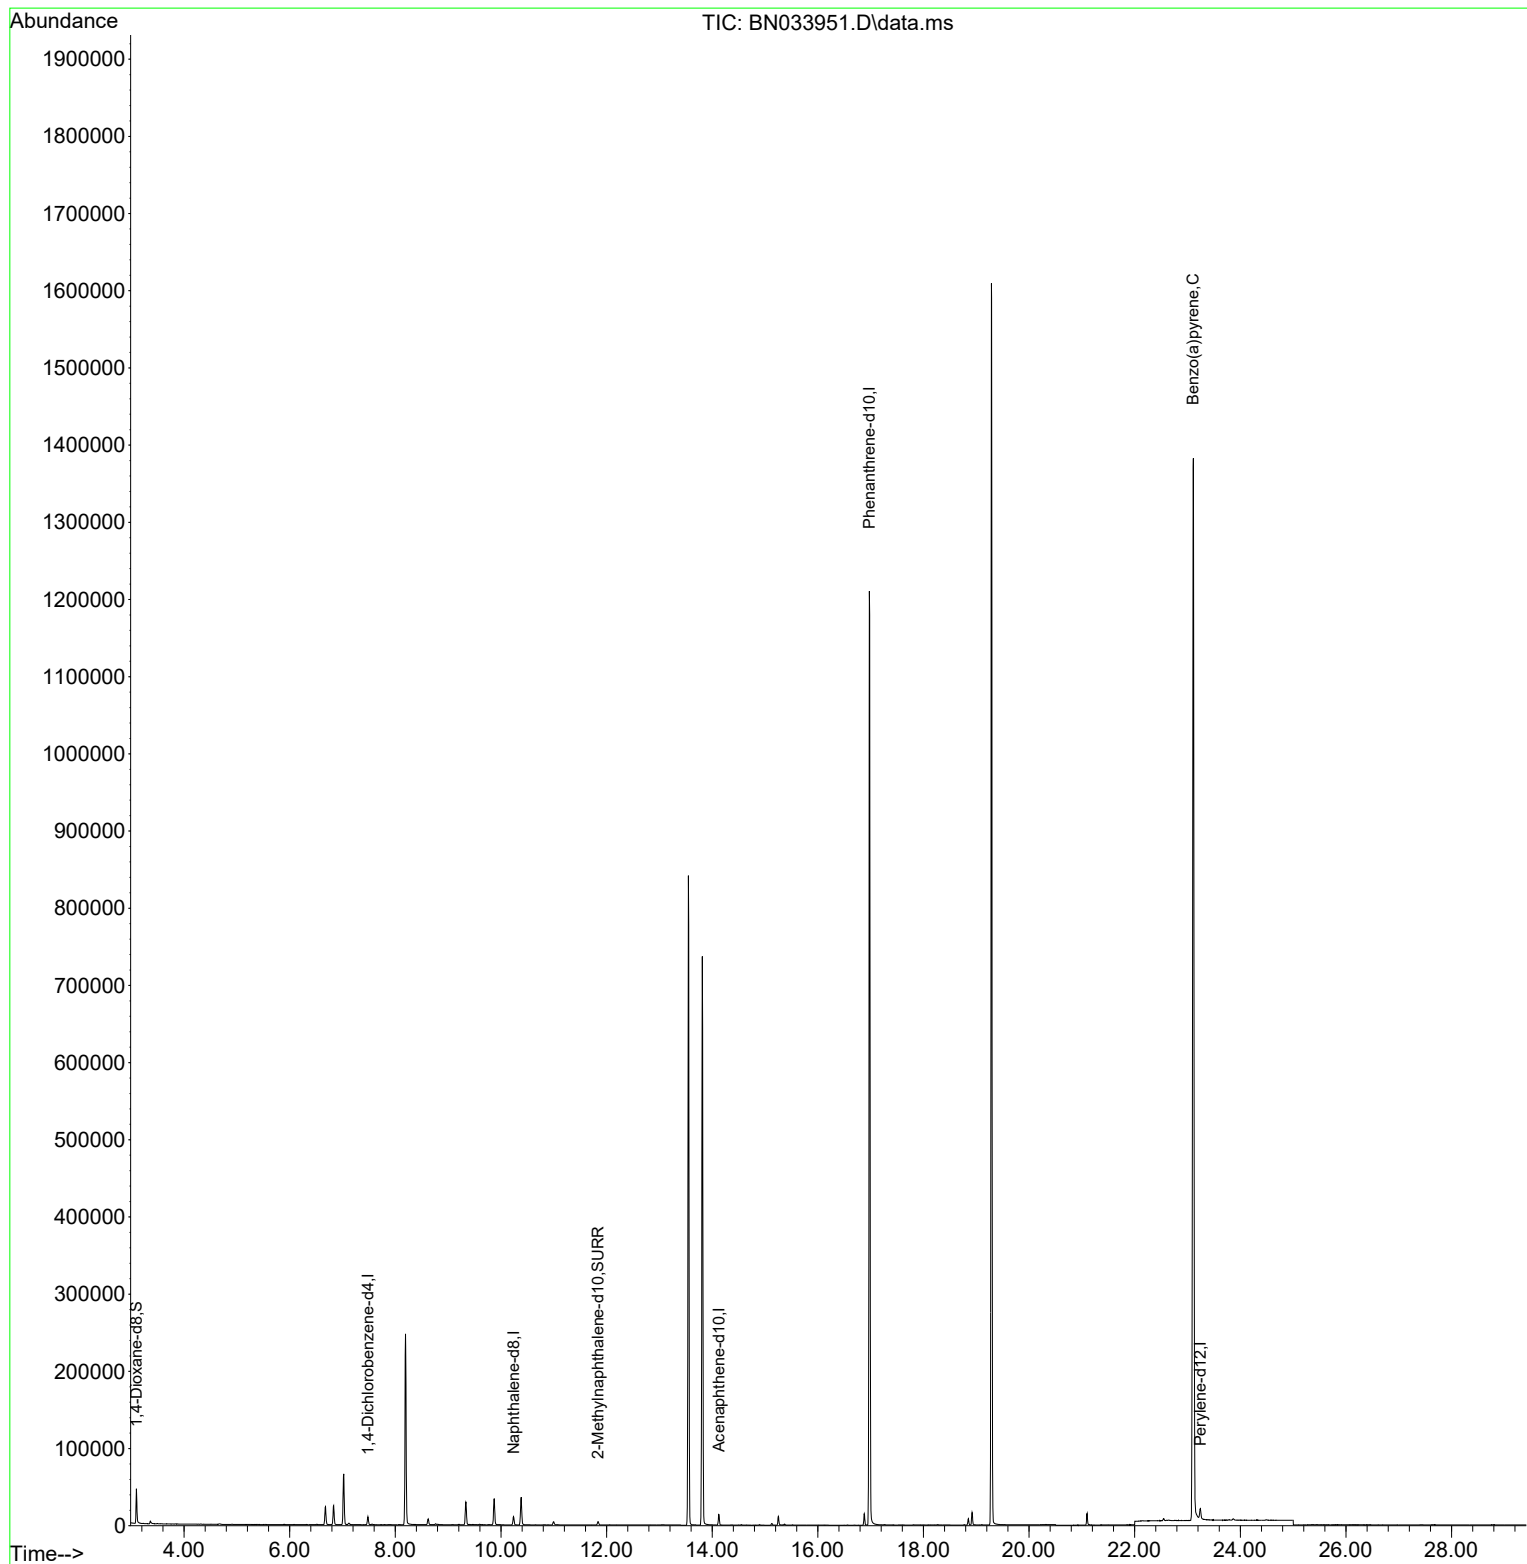

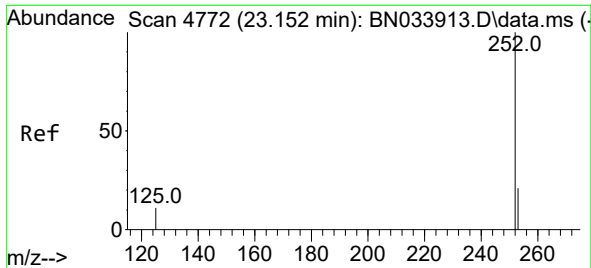

#26

Benzo(a)pyrene

Concen: 0.091 ng/ul

RT: 23.108 min Scan# 41

Delta R.T. -0.044 min

Lab File: BN033951.D


Acq: 15 Sep 2024 14:39

Instrument :

BNA_N

ClientSampleId :

C0AS9

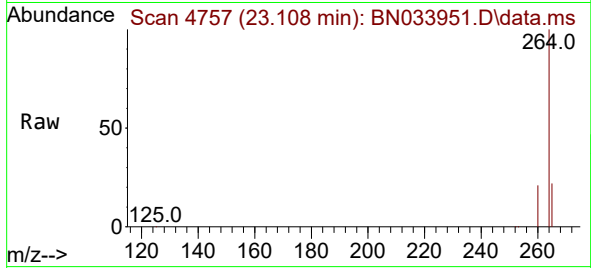

Tgt Ion:252 Resp: 6265

Ion Ratio Lower Upper

252 100

253 42.1 22.8 34.2#

125 41.5 18.0 27.0#

