

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033952.D
 Acq On : 15 Sep 2024 15:15
 Operator : JU/RC
 Sample : P3922-09
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AT3

Quant Time: Sep 16 00:13:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.481	152	4461	0.400	ng/ul	0.00
4) Naphthalene-d8	10.239	136	12562	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.124	164	6699	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.978	188	1188708	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.240	264	19178	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	25276	5.511	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.839	152	5605	0.311	ng/ul	0.00
18) Fluoranthene-d10	18.920	212	15160	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.131	88	248	0.049	ng/ul#	49
26) Benzo(a)pyrene	23.108	252	5460	0.091	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033952.D
Acq On : 15 Sep 2024 15:15
Operator : JU/RC
Sample : P3922-09
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AT3

Quant Time: Sep 16 00:13:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

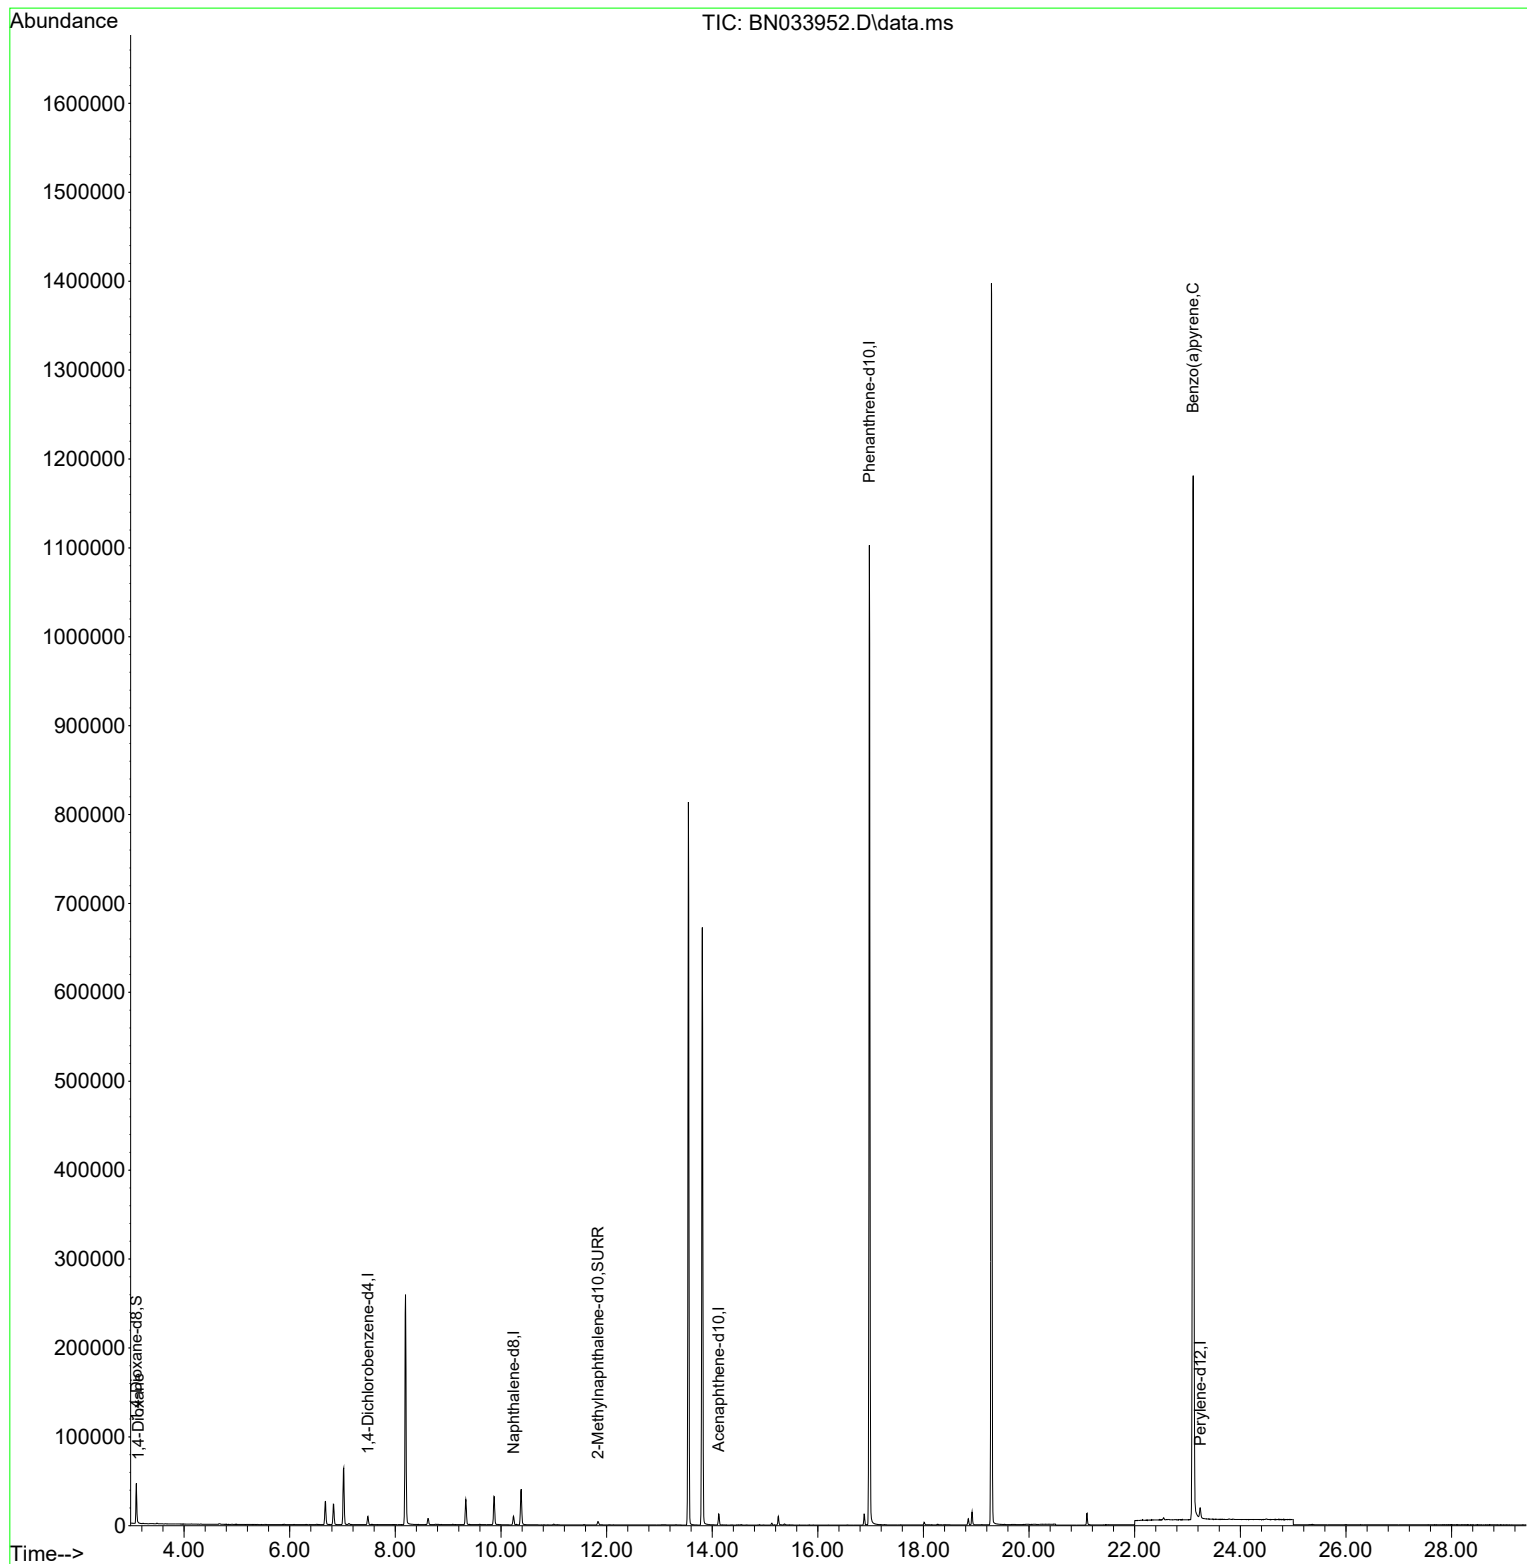

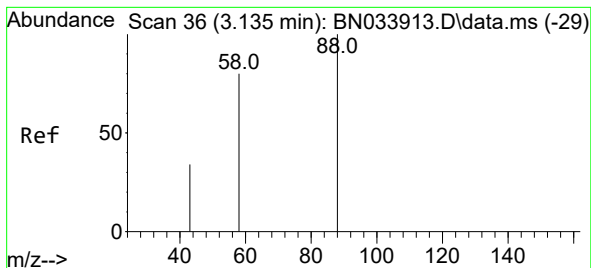

#2

1,4-Dioxane

Concen: 0.049 ng/ul

RT: 3.131 min Scan# 31

Delta R.T. -0.004 min

Lab File: BN033952.D

Acq: 15 Sep 2024 15:15

Instrument :

BNA_N

ClientSampleId :

COAT3





Tgt Ion: 88 Resp: 248

Ion Ratio Lower Upper

88 100

43 117.7 47.0 70.4#

58 45.7 53.0 79.4#

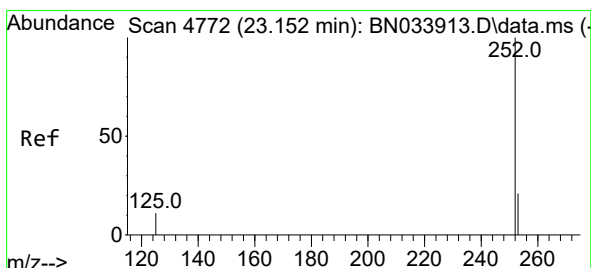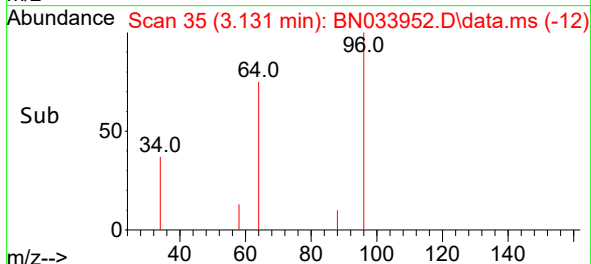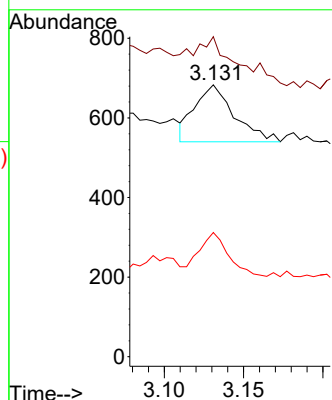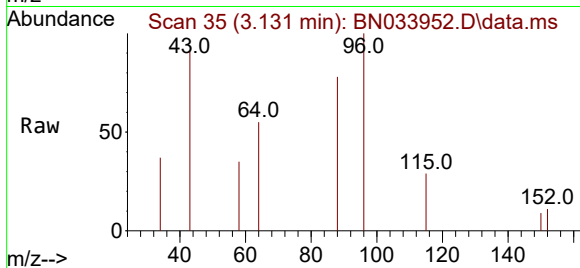

#26

Benzo(a)pyrene

Concen: 0.091 ng/ul

RT: 23.108 min Scan# 4757

Delta R.T. -0.044 min

Lab File: BN033952.D

Acq: 15 Sep 2024 15:15

Tgt Ion: 252 Resp: 5460

Ion Ratio Lower Upper

252 100

253 45.0 22.8 34.2#

125 45.6 18.0 27.0#

