

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033953.D
 Acq On : 15 Sep 2024 15:51
 Operator : JU/RC
 Sample : P3922-10
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AW5

Quant Time: Sep 16 00:13:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.481	152	4318	0.400	ng/ul	0.00
4) Naphthalene-d8	10.239	136	12404	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.124	164	6687	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.978	188	1230319	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.240	264	18878	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	24797	5.586	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.839	152	6084	0.342	ng/ul	0.00
18) Fluoranthene-d10	18.920	212	15371	0.000	ng/ul	0.00
Target Compounds						
26) Benzo(a)pyrene	23.108	252	5516	0.094	ng/ul#	Qvalue 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033953.D
Acq On : 15 Sep 2024 15:51
Operator : JU/RC
Sample : P3922-10
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5


Quant Time: Sep 16 00:13:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

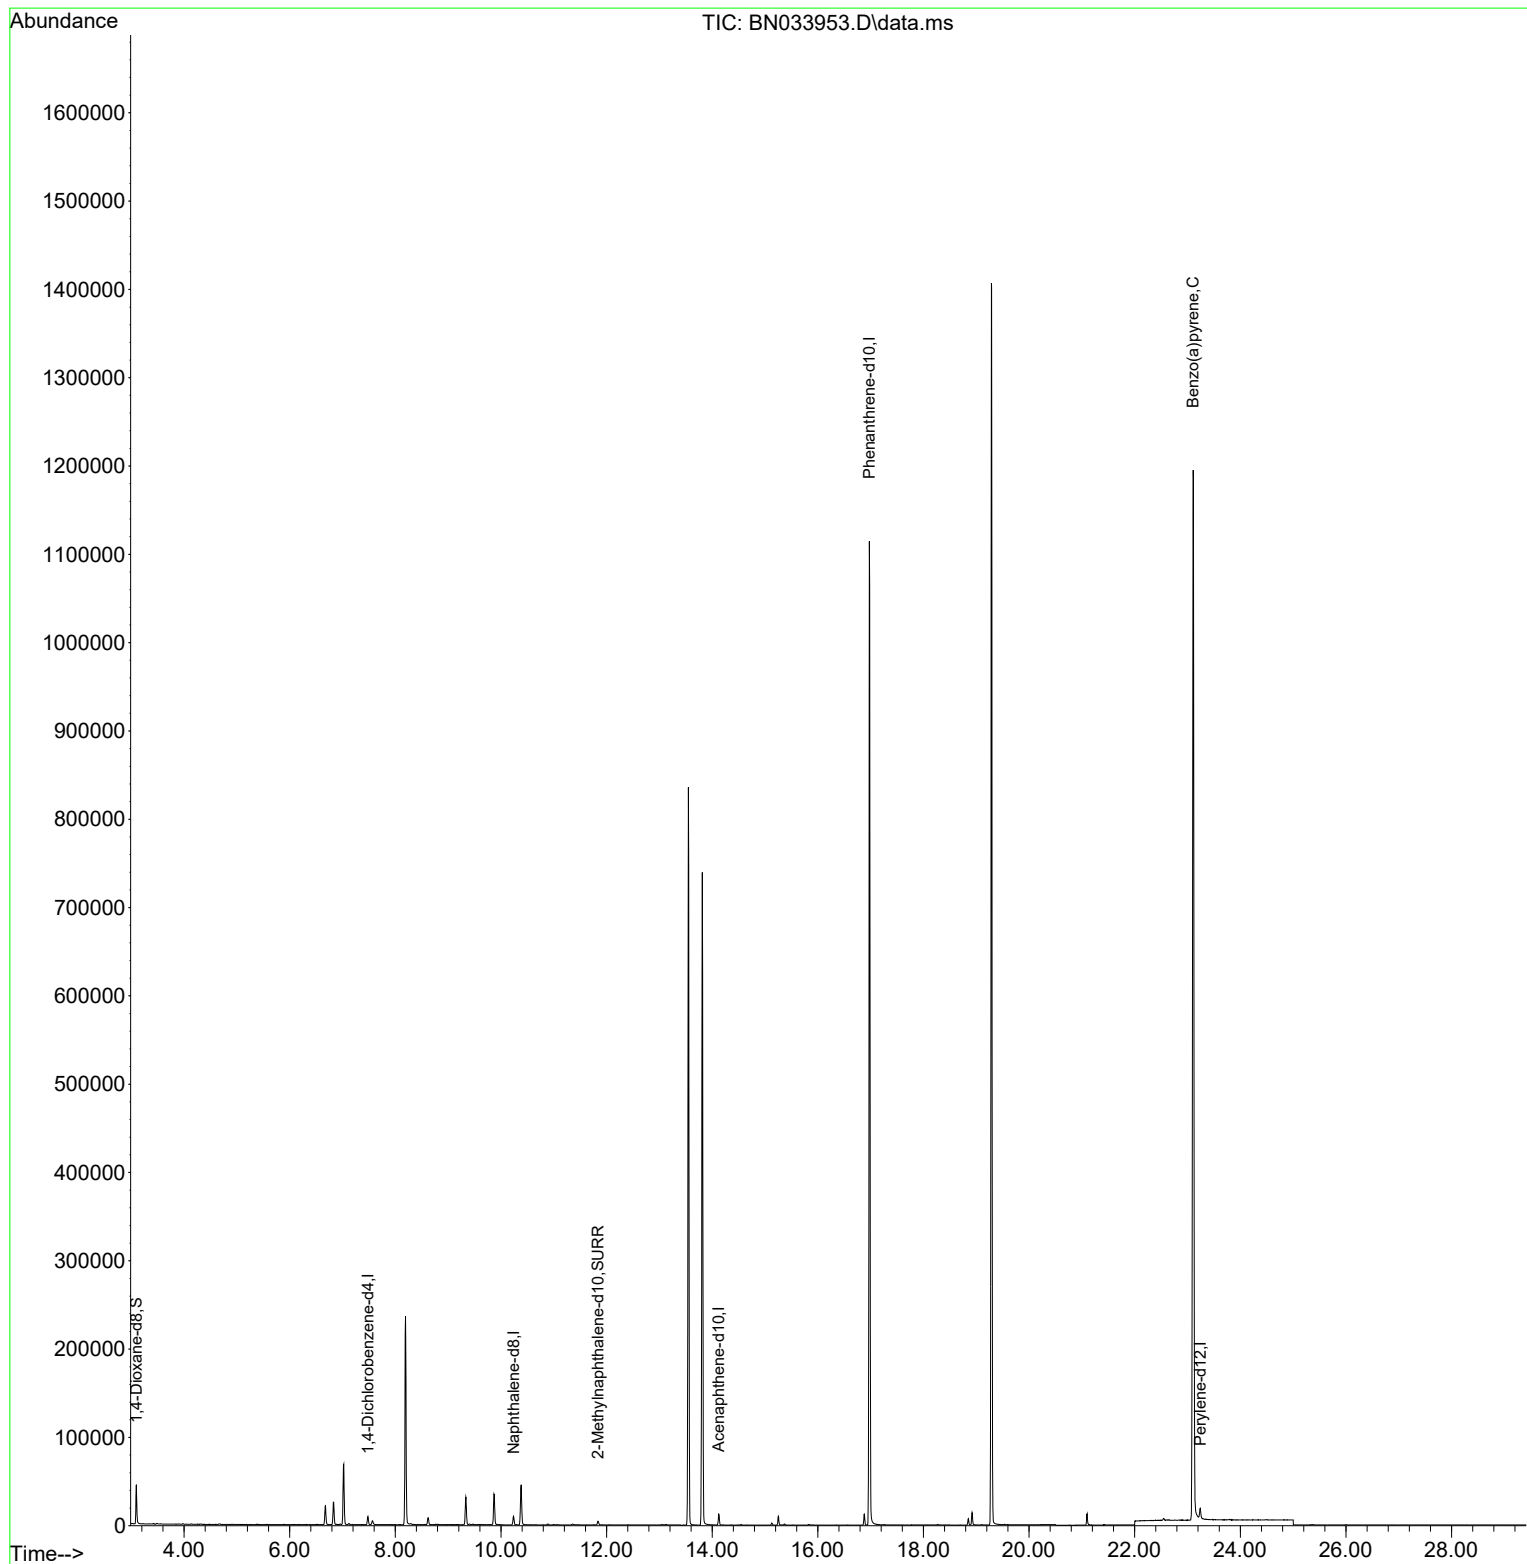

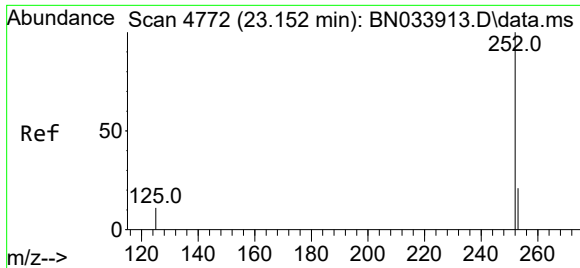

#26
Benzo(a)pyrene
Concen: 0.094 ng/ul
RT: 23.108 min Scan# 41
Delta R.T. -0.044 min
Lab File: BN033953.D
Acq: 15 Sep 2024 15:51

Instrument :
BNA_N
ClientSampleId :
C0AW5

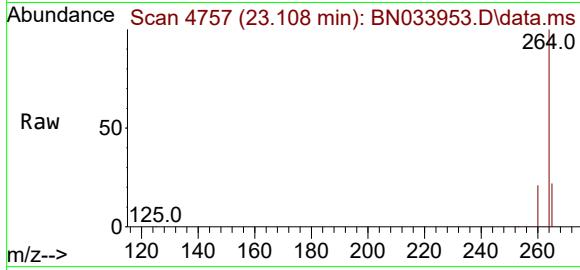

Tgt Ion:252 Resp: 5516
Ion Ratio Lower Upper
252 100
253 44.2 22.8 34.2#
125 42.1 18.0 27.0#

