

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033954.D
 Acq On : 15 Sep 2024 16:27
 Operator : JU/RC
 Sample : P3922-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AW4

Quant Time: Sep 16 00:13:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.481	152	4760	0.400	ng/ul	0.00
4) Naphthalene-d8	10.239	136	13766	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.123	164	7483	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.978	188	1420897	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.242	264	20747	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	27802	5.681	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.839	152	6997	0.354	ng/ul	0.00
18) Fluoranthene-d10	18.920	212	18212	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.135	88	148	0.027	ng/ul#	63
12) Fluorene	15.127	166	2337	0.085	ng/ul#	14
26) Benzo(a)pyrene	23.111	252	6530	0.101	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033954.D
Acq On : 15 Sep 2024 16:27
Operator : JU/RC
Sample : P3922-11
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW4


Quant Time: Sep 16 00:13:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

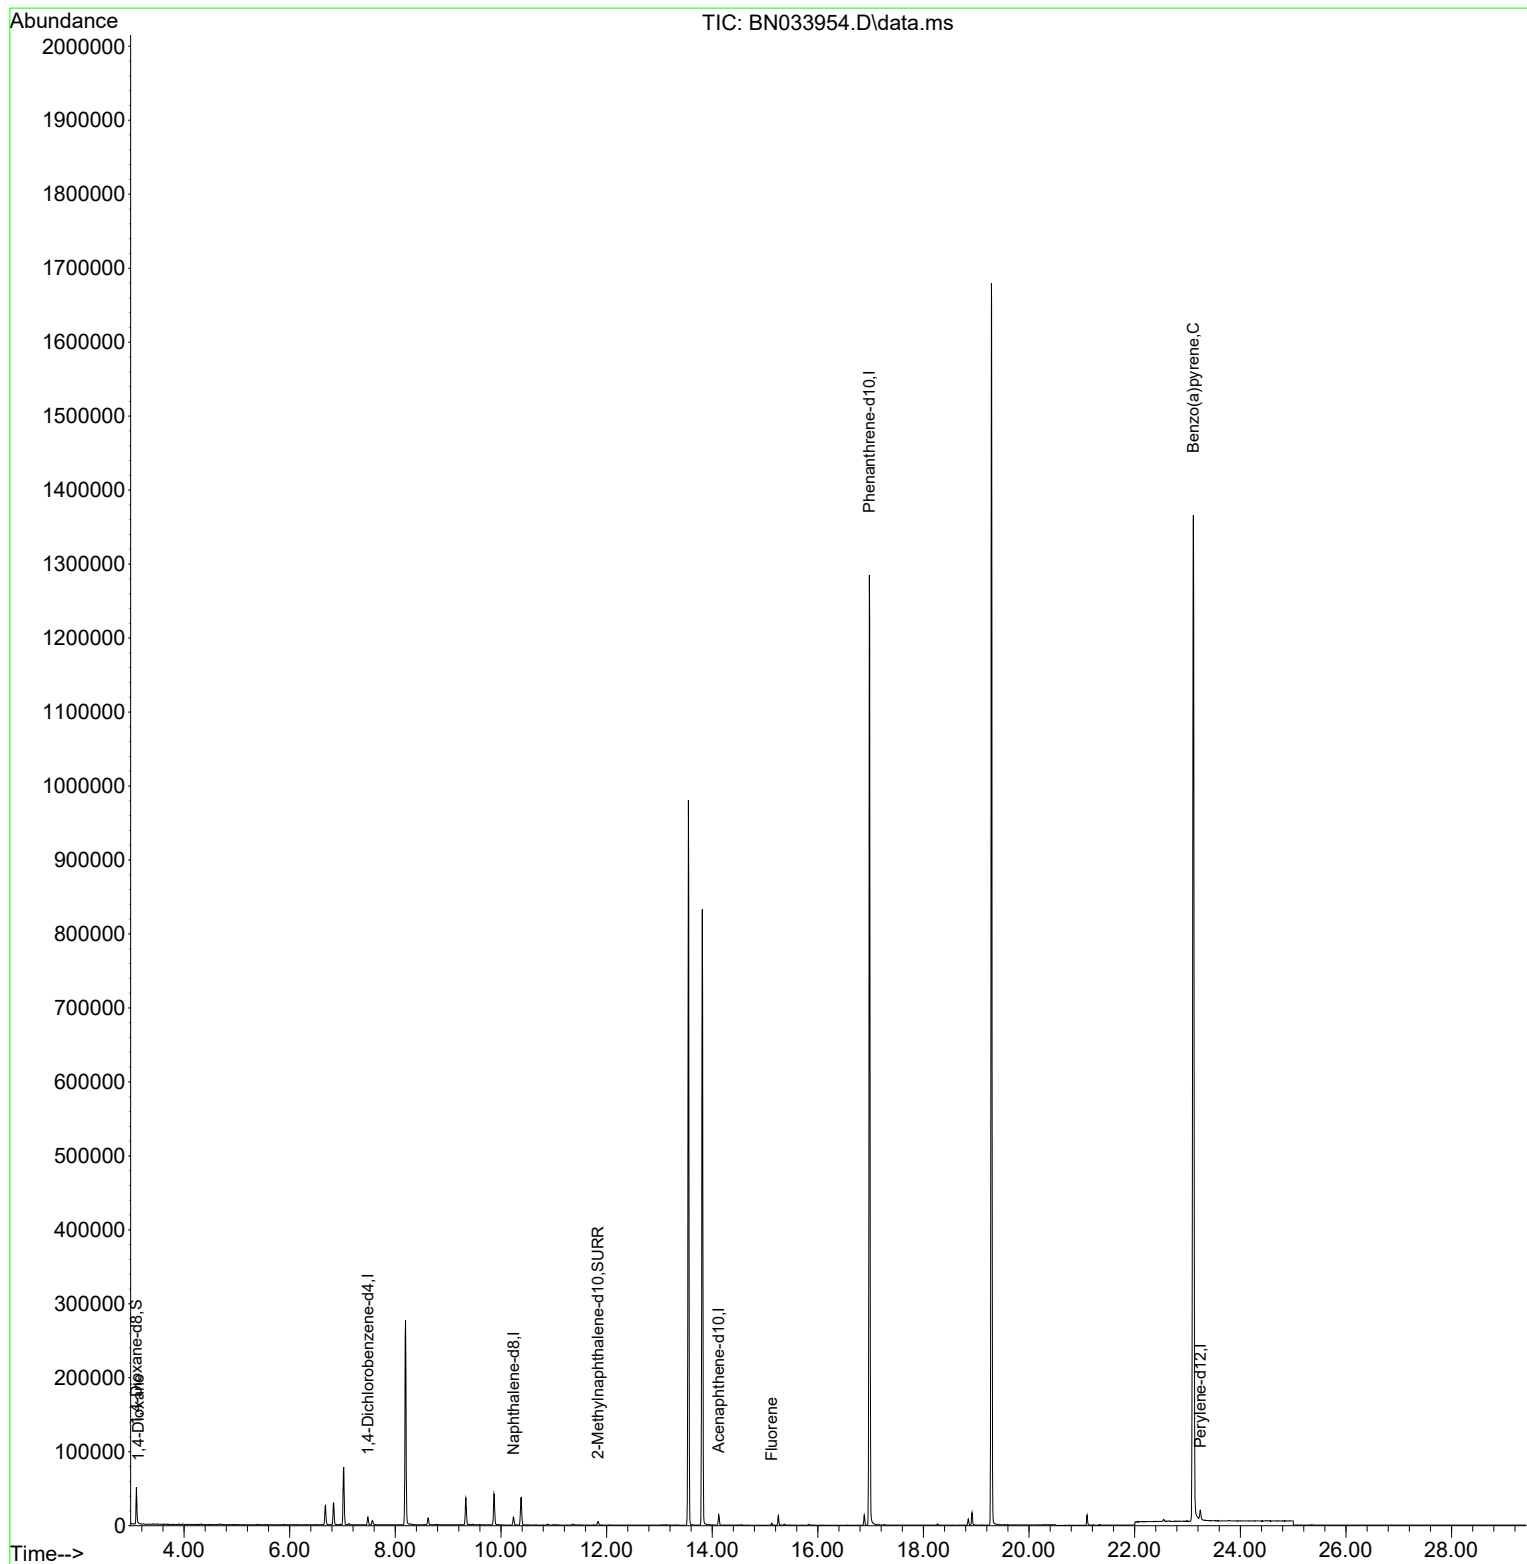



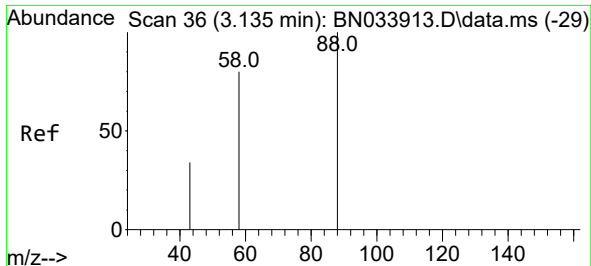


#2
1,4-Dioxane
Concen: 0.027 ng/ul
RT: 3.135 min Scan# 30
Delta R.T. -0.000 min
Lab File: BN033954.D
Acq: 15 Sep 2024 16:27

Instrument :
BNA_N
ClientSampleId :
C0AW4



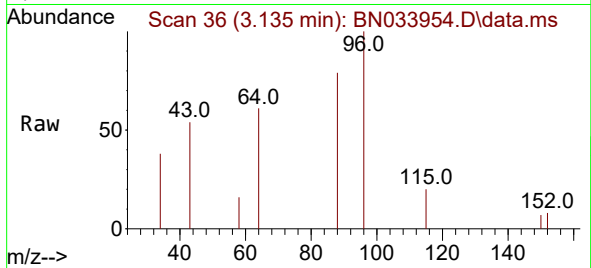



Tgt Ion: 88 Resp: 148
Ion Ratio Lower Upper
88 100
43 68.3 47.0 70.4
58 19.7 53.0 79.4#

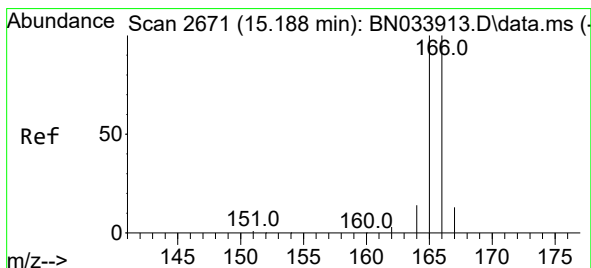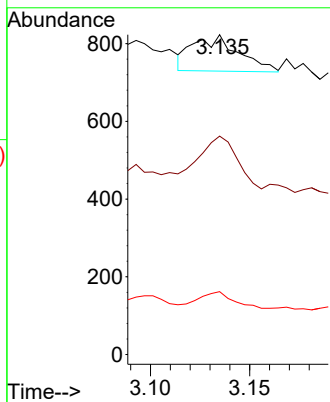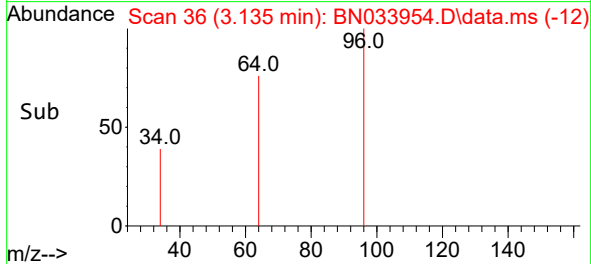

#12
Fluorene
Concen: 0.085 ng/ul
RT: 15.127 min Scan# 2658
Delta R.T. -0.060 min
Lab File: BN033954.D
Acq: 15 Sep 2024 16:27

Tgt Ion:166 Resp: 2337
Ion Ratio Lower Upper
166 100
165 8.2 79.1 118.7#
167 33.5 11.4 17.0#

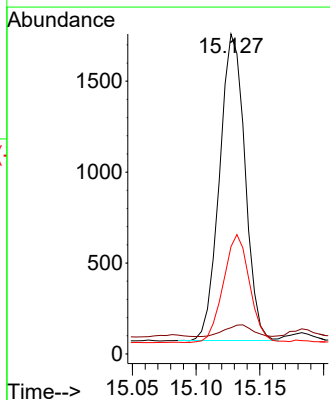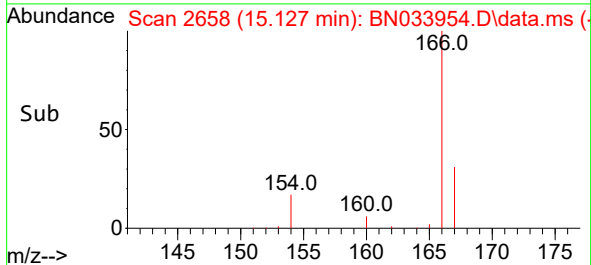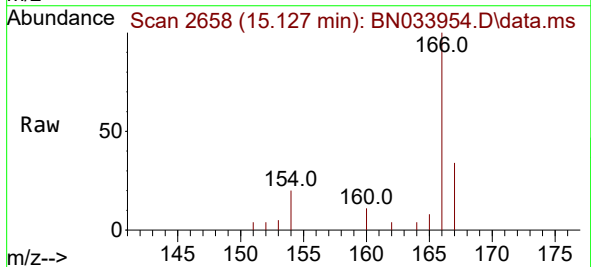

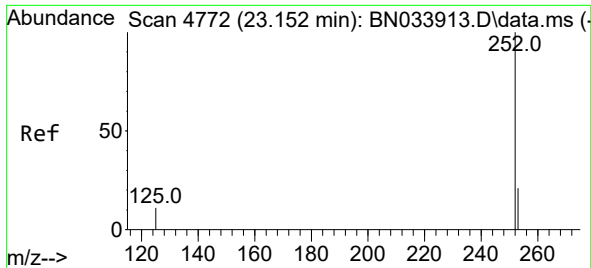

#26

Benzo(a)pyrene

Concen: 0.101 ng/ul

RT: 23.111 min Scan# 41

Delta R.T. -0.041 min

Lab File: BN033954.D


Acq: 15 Sep 2024 16:27

Instrument :

BNA_N

ClientSampleId :

C0AW4

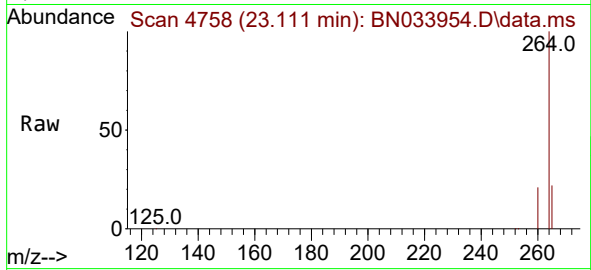

Tgt Ion:252 Resp: 6530

Ion Ratio Lower Upper

252 100

253 40.9 22.8 34.2#

125 37.7 18.0 27.0#

