

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033960.D
 Acq On : 15 Sep 2024 20:39
 Operator : JU/RC
 Sample : PB163195BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK195

Quant Time: Sep 16 00:14:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.481	152	4551	0.400	ng/ul	0.00
4) Naphthalene-d8	10.239	136	12963	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.123	164	6974	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.978	188	1276482	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.234	264	19865	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	37636	8.044	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.839	152	6803	0.366	ng/ul	0.00
18) Fluoranthene-d10	18.920	212	14799	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.131	88	275	0.053	ng/ul#	62
26) Benzo(a)pyrene	23.105	252	6402	0.103	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033960.D
Acq On : 15 Sep 2024 20:39
Operator : JU/RC
Sample : PB163195BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK195

Quant Time: Sep 16 00:14:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration




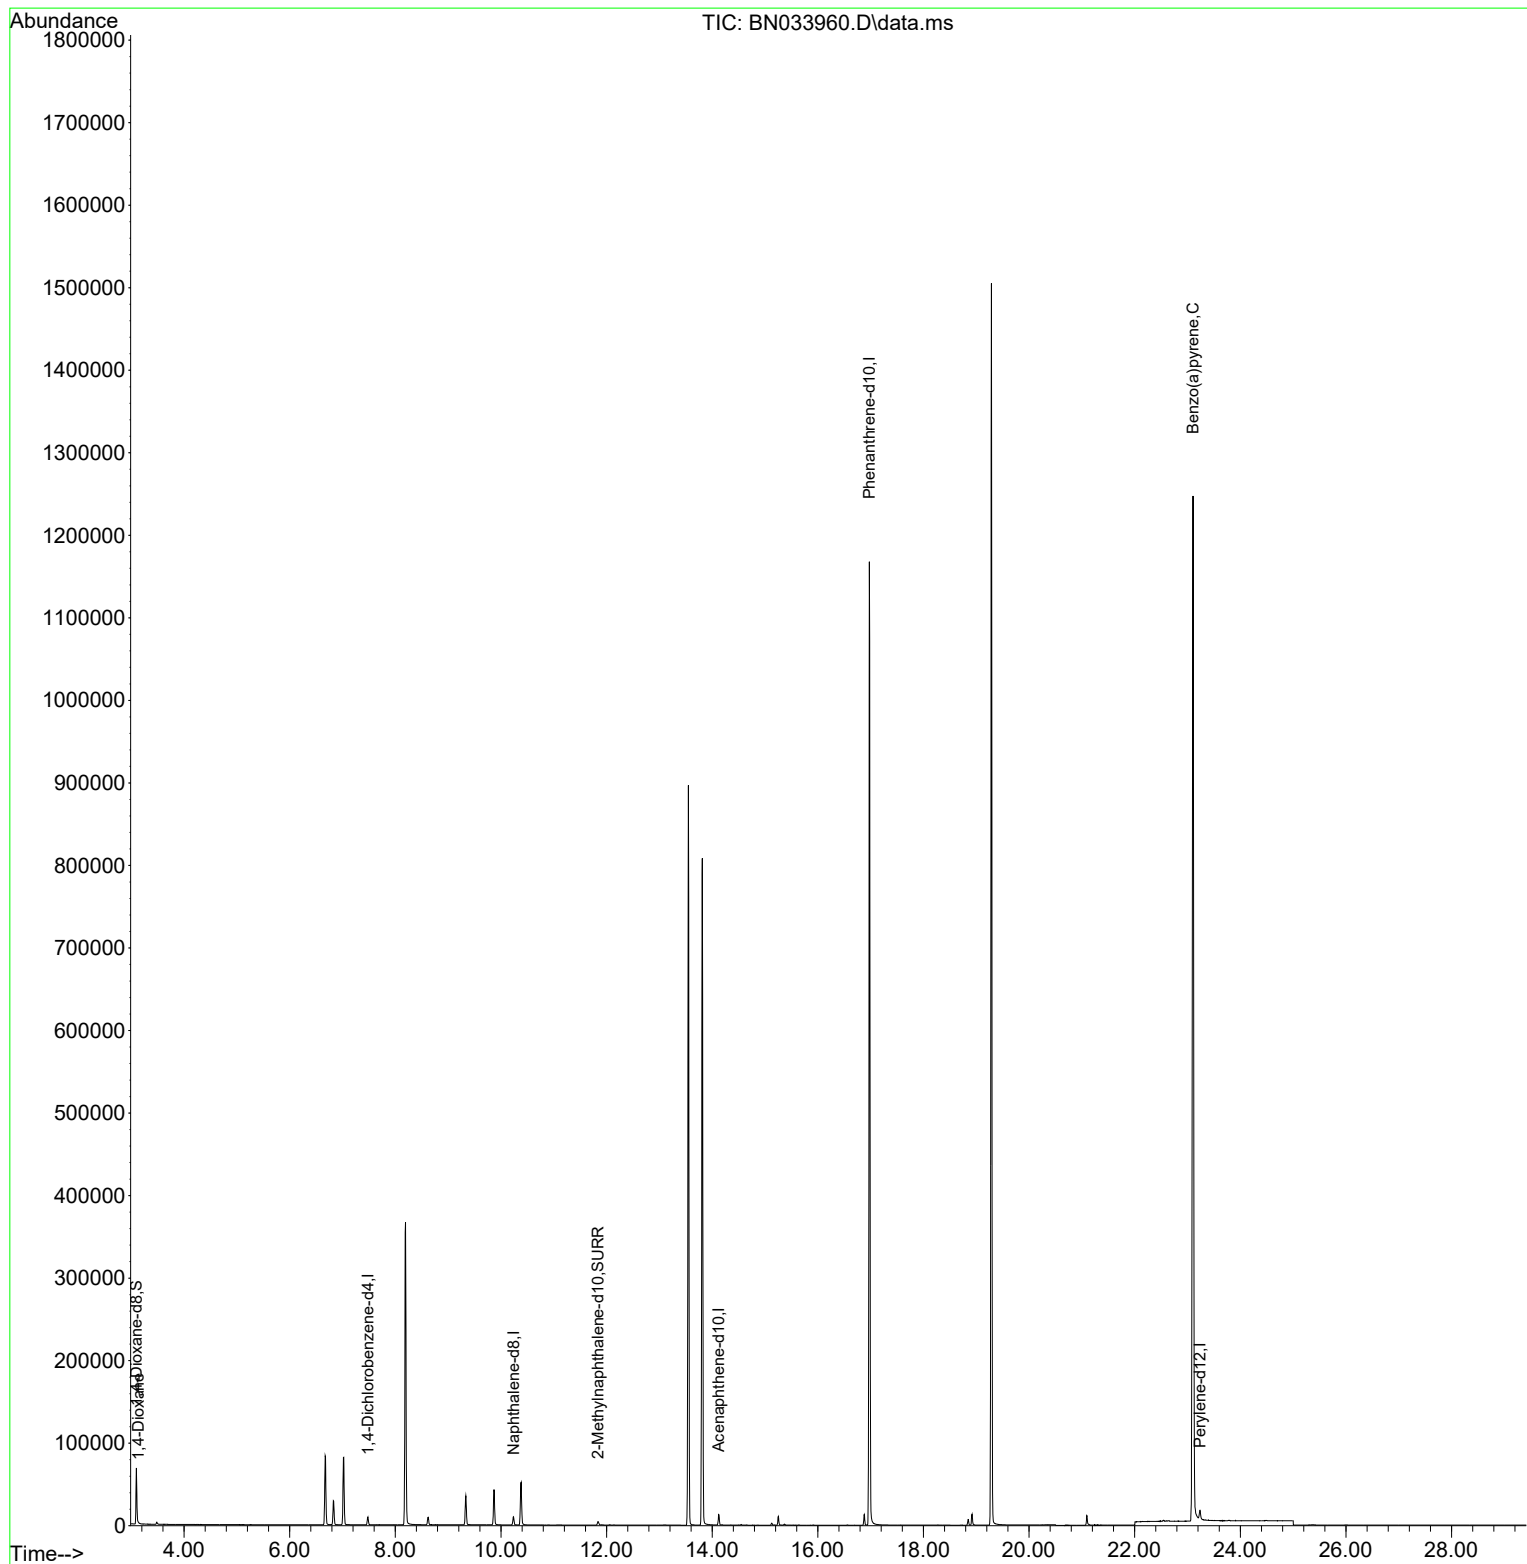


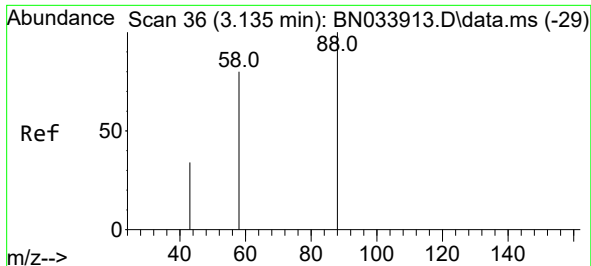

#2
1,4-Dioxane
Concen: 0.053 ng/ul
RT: 3.131 min Scan# 31
Delta R.T. -0.004 min
Lab File: BN033960.D
Acq: 15 Sep 2024 20:39

Instrument :
BNA_N
ClientSampleId :
SBLK195

Tgt Ion: 88 Resp: 275
Ion Ratio Lower Upper
88 100
43 44.1 47.0 70.4#
58 22.7 53.0 79.4#

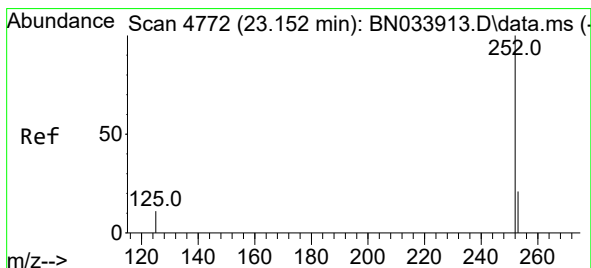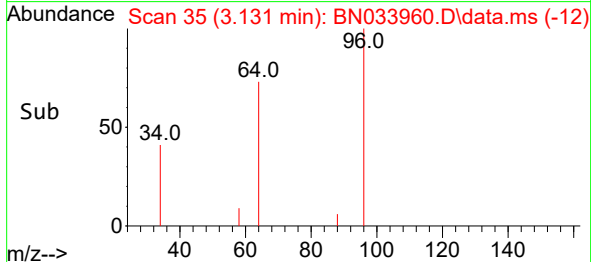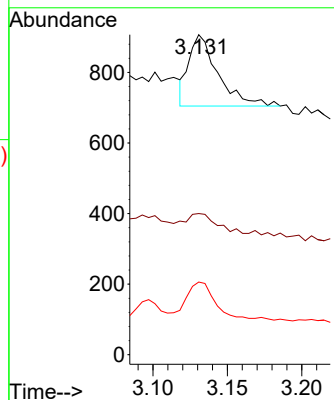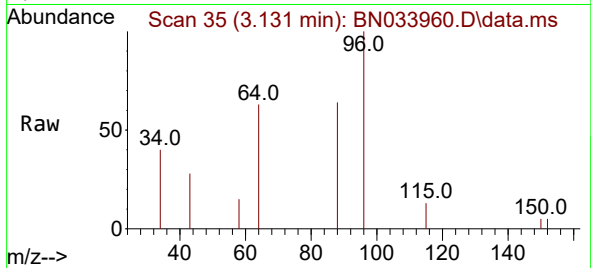

#26
Benzo(a)pyrene
Concen: 0.103 ng/ul
RT: 23.105 min Scan# 4756
Delta R.T. -0.047 min
Lab File: BN033960.D
Acq: 15 Sep 2024 20:39

Tgt Ion: 252 Resp: 6402
Ion Ratio Lower Upper
252 100
253 43.8 22.8 34.2#
125 39.5 18.0 27.0#

