

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033961.D
 Acq On : 15 Sep 2024 21:15
 Operator : JU/RC
 Sample : PB163312BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK312

Quant Time: Sep 16 00:15:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.481	152	5281	0.400	ng/ul	0.00
4) Naphthalene-d8	10.237	136	14600	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.127	164	7552	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.977	188	1134711	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.235	264	20737	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	36085	6.646	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.838	152	6311	0.301	ng/ul	0.00
18) Fluoranthene-d10	18.918	212	12793	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.135	88	294	0.049	ng/ul#	70
26) Benzo(a)pyrene	23.101	252	5562	0.086	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033961.D
Acq On : 15 Sep 2024 21:15
Operator : JU/RC
Sample : PB163312BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK312

Quant Time: Sep 16 00:15:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

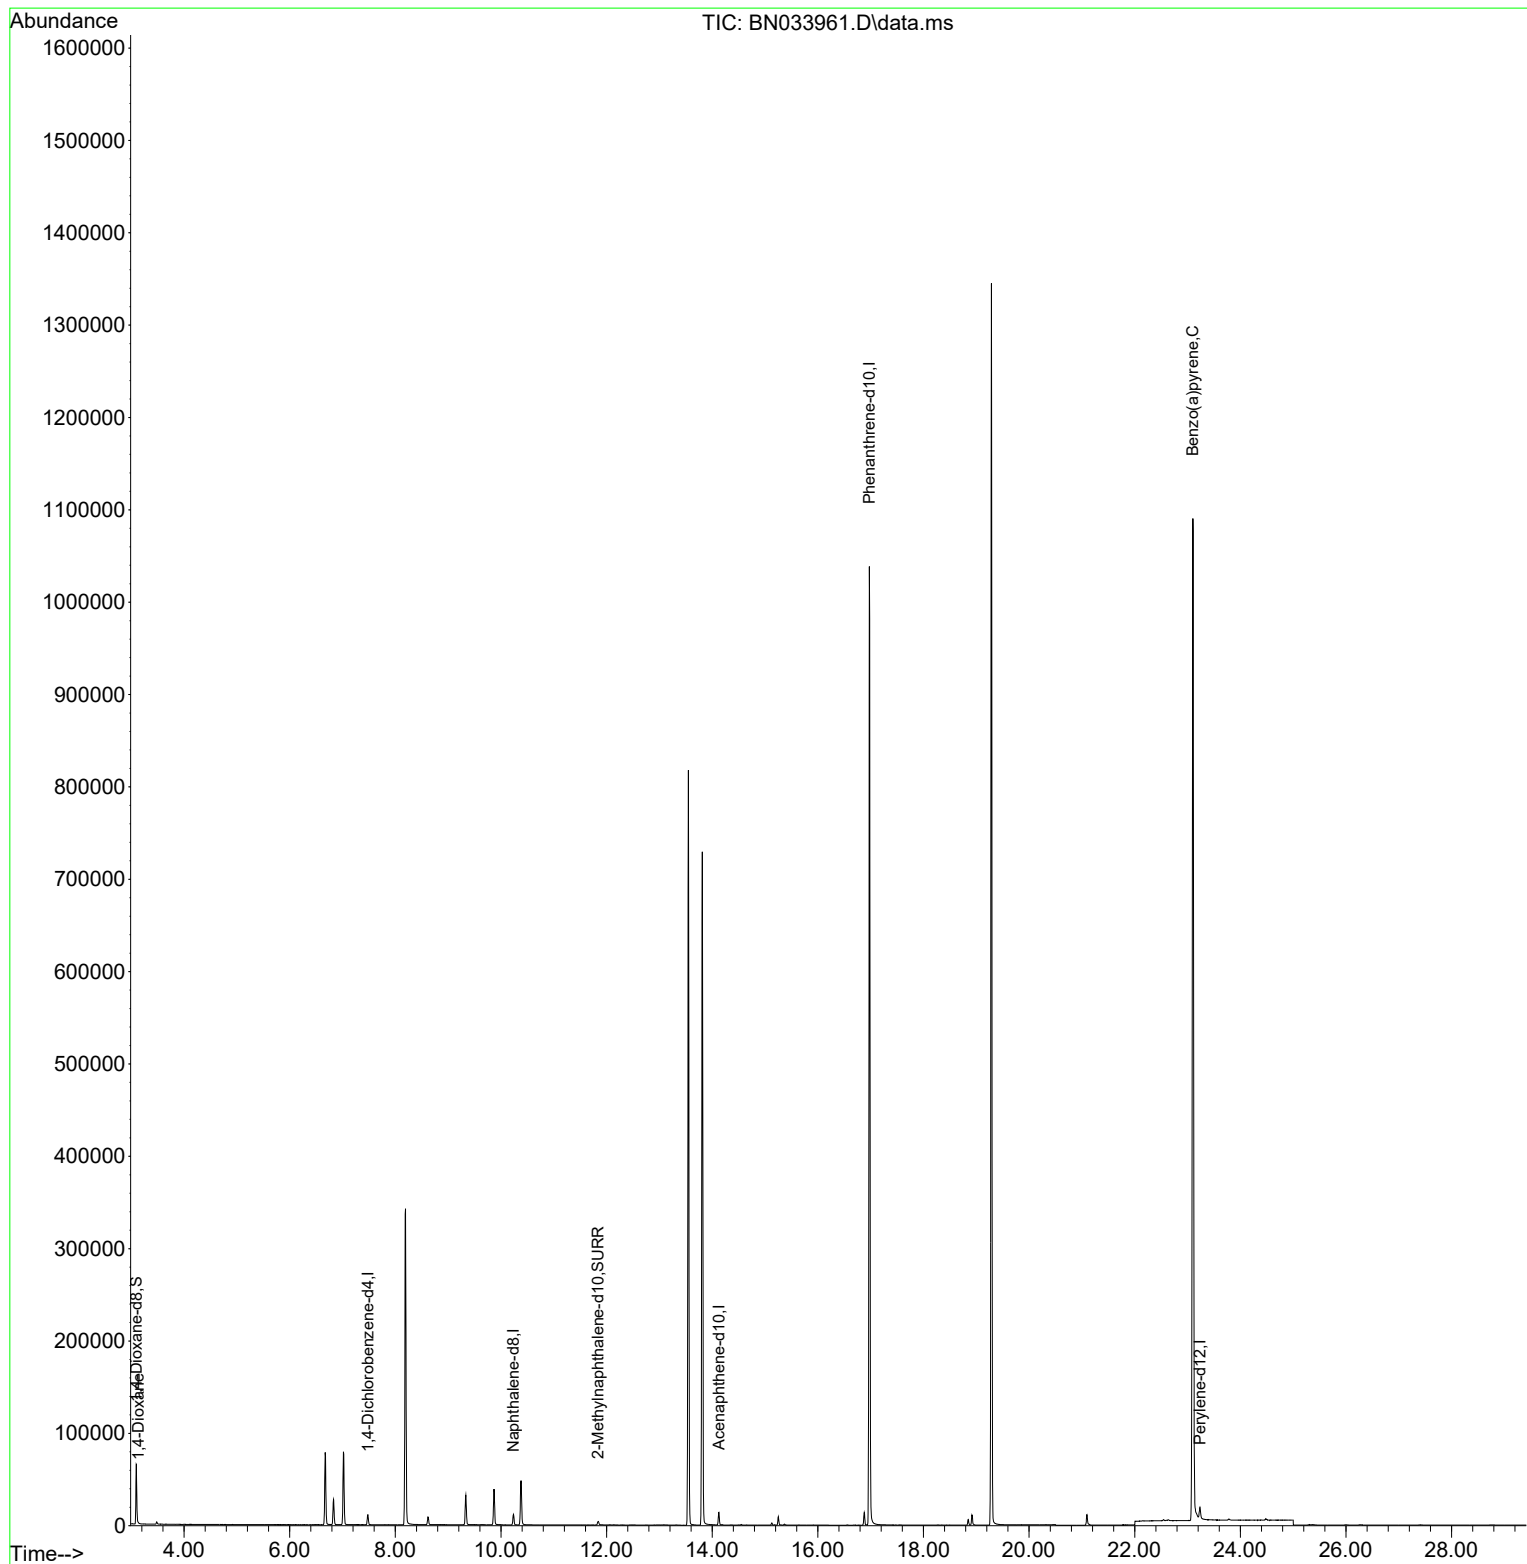

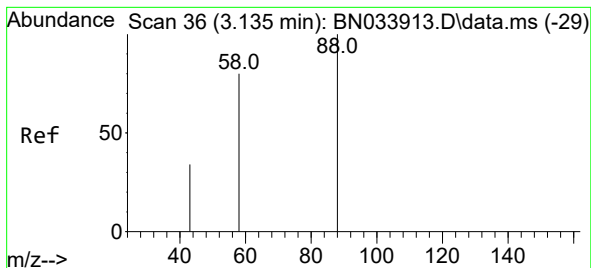

#2

1,4-Dioxane

Concen: 0.049 ng/ul

RT: 3.135 min Scan# 30

Delta R.T. -0.000 min

Lab File: BN033961.D

Acq: 15 Sep 2024 21:15

Instrument :

BNA_N

ClientSampleId :

SBLK312





Tgt Ion: 88 Resp: 294

Ion Ratio Lower Upper

88 100

43 51.1 47.0 70.4

58 28.2 53.0 79.4#

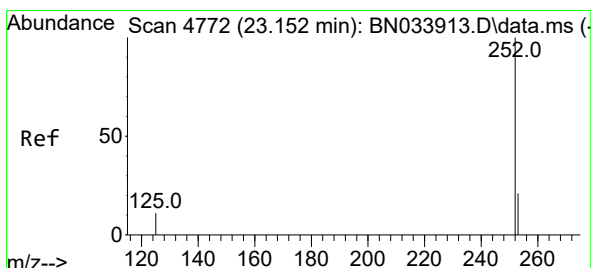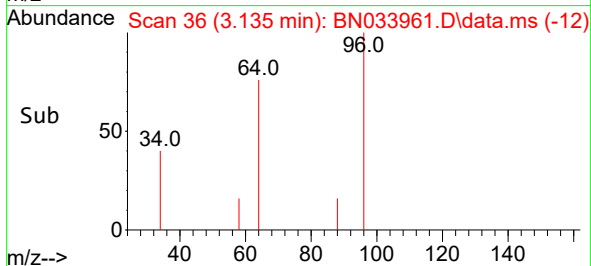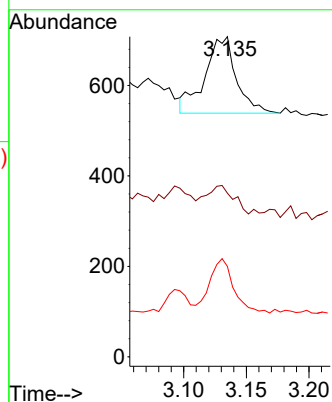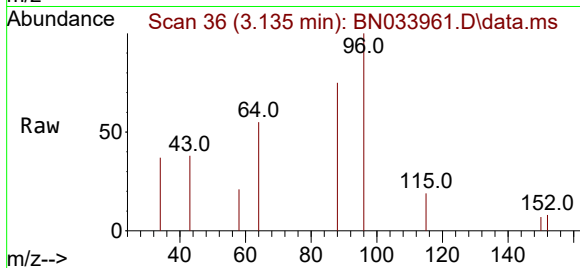

#26

Benzo(a)pyrene

Concen: 0.086 ng/ul

RT: 23.101 min Scan# 4755

Delta R.T. -0.051 min

Lab File: BN033961.D

Acq: 15 Sep 2024 21:15

Tgt Ion: 252 Resp: 5562

Ion Ratio Lower Upper

252 100

253 45.1 22.8 34.2#

125 41.0 18.0 27.0#

