

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033962.D
 Acq On : 15 Sep 2024 21:51
 Operator : JU/RC
 Sample : P3997-05
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AX1

Quant Time: Sep 16 00:15:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.481	152	4976	0.400	ng/ul	0.00
4) Naphthalene-d8	10.239	136	14008	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.124	164	7390	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.978	188	1397392	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.234	264	20017	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	29846	5.834	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.839	152	7399	0.368	ng/ul	0.00
18) Fluoranthene-d10	18.920	212	16777	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.127	166	2415	0.089	ng/ul#	14
26) Benzo(a)pyrene	23.102	252	6108	0.098	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033962.D
Acq On : 15 Sep 2024 21:51
Operator : JU/RC
Sample : P3997-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX1

Quant Time: Sep 16 00:15:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration




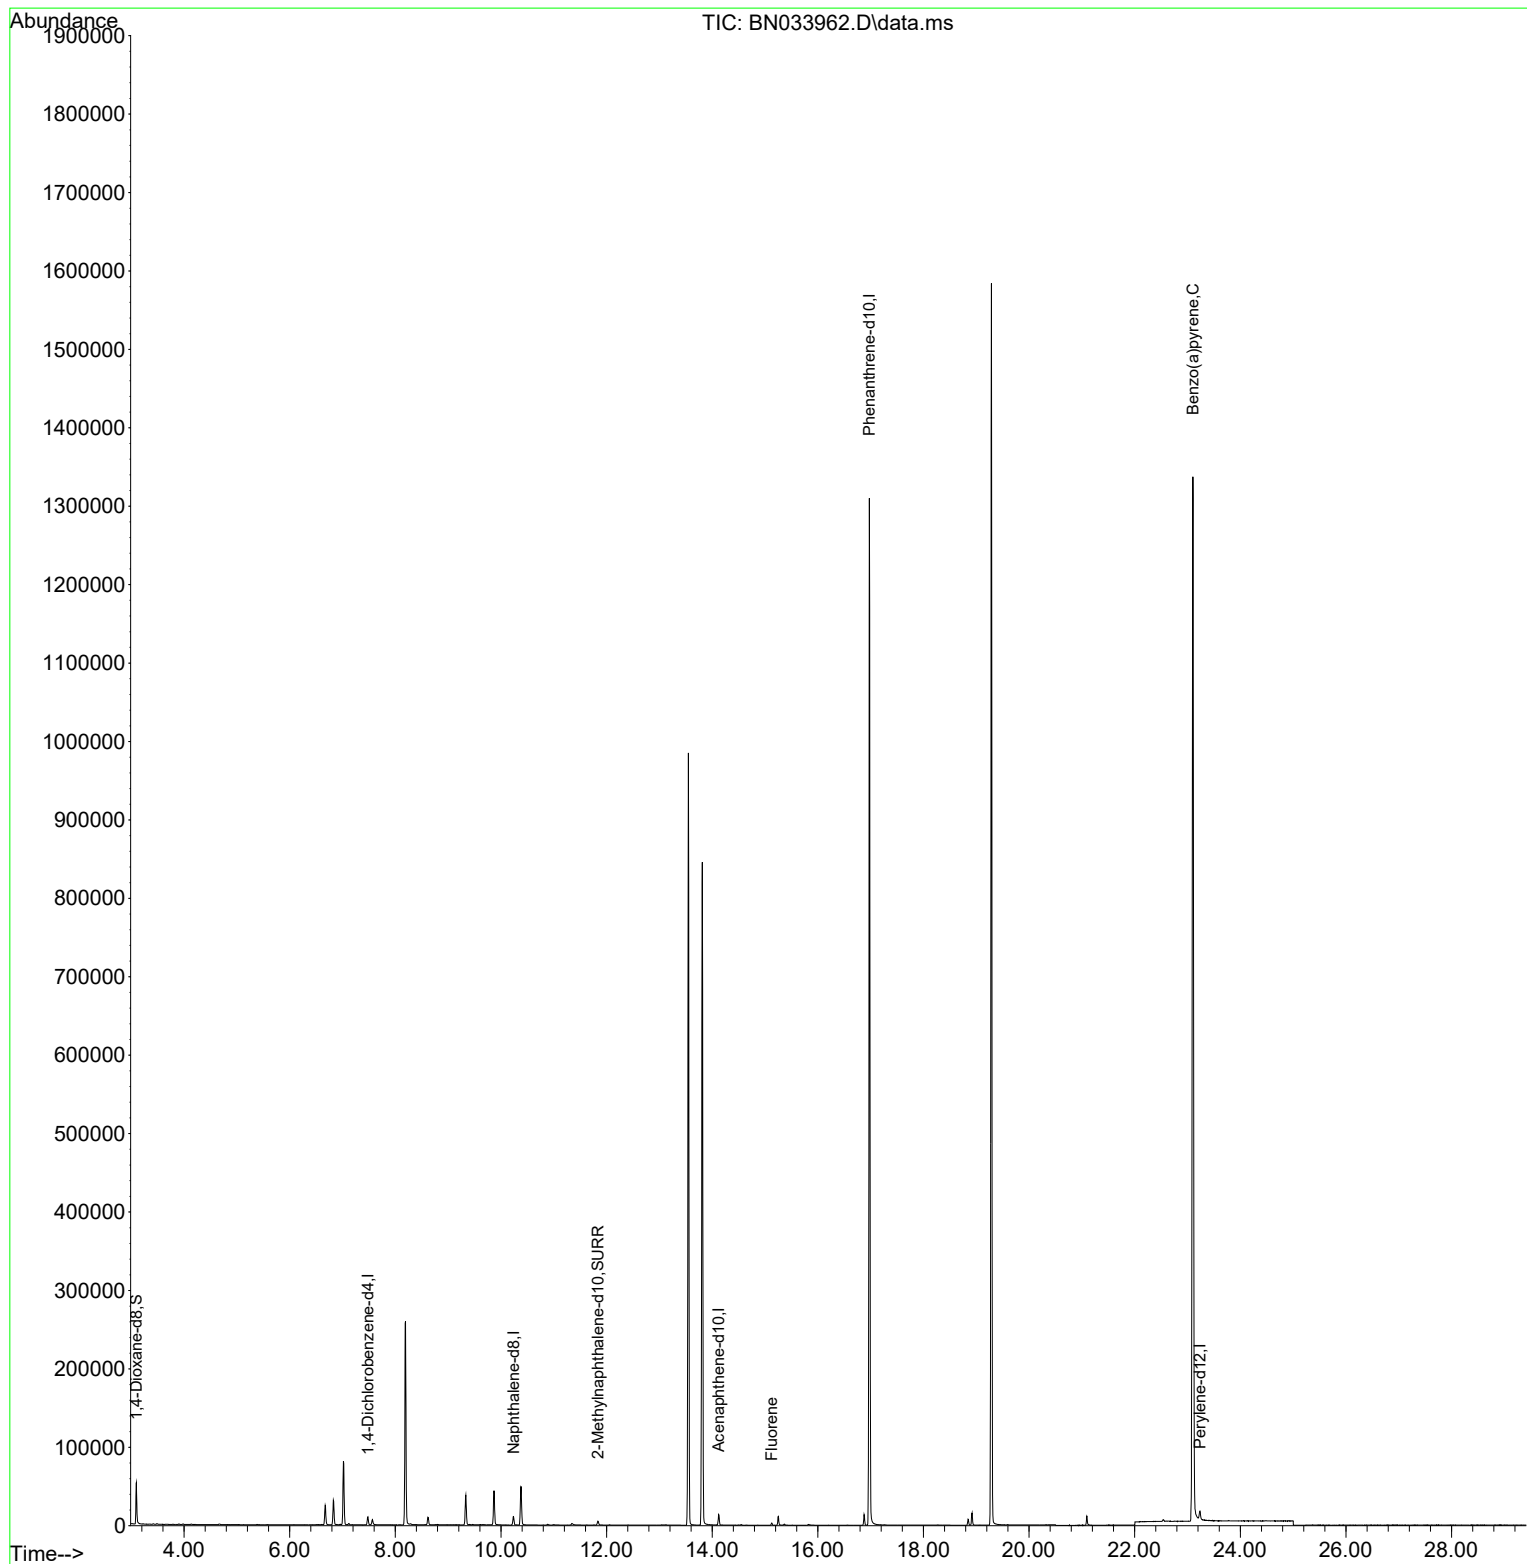


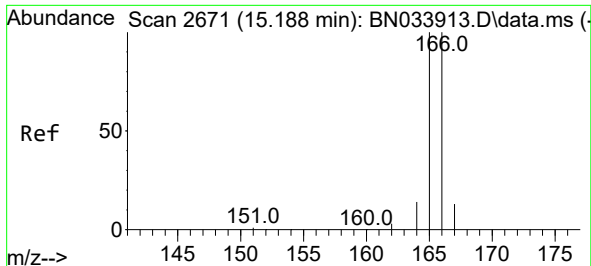

#12
Fluorene
Concen: 0.089 ng/ul
RT: 15.127 min Scan# 2
Delta R.T. -0.060 min
Lab File: BN033962.D
Acq: 15 Sep 2024 21:51

Instrument :
BNA_N
ClientSampleId :
C0AX1

Tgt Ion:166 Resp: 2415
Ion Ratio Lower Upper
166 100
165 7.8 79.1 118.7#
167 34.0 11.4 17.0#

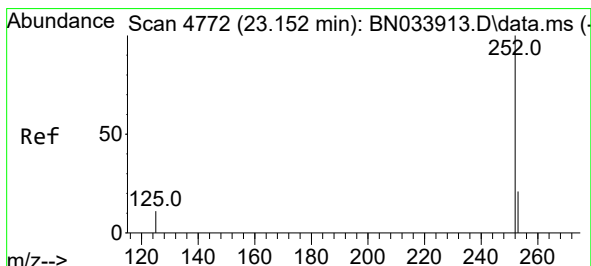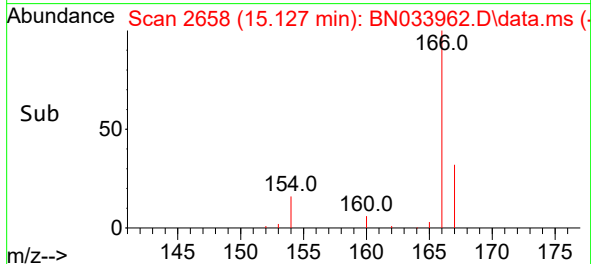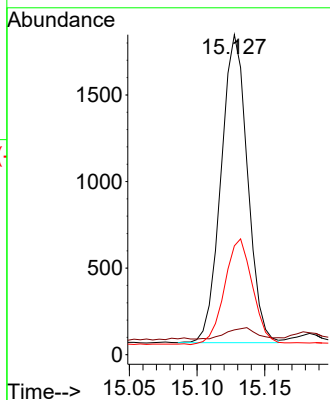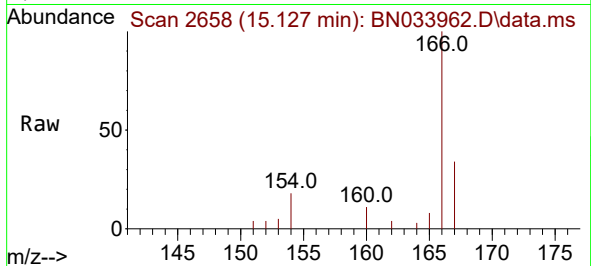

#26
Benzo(a)pyrene
Concen: 0.098 ng/ul
RT: 23.102 min Scan# 4755
Delta R.T. -0.050 min
Lab File: BN033962.D
Acq: 15 Sep 2024 21:51

Tgt Ion:252 Resp: 6108
Ion Ratio Lower Upper
252 100
253 39.5 22.8 34.2#
125 37.3 18.0 27.0#

