

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033963.D
 Acq On : 15 Sep 2024 22:27
 Operator : JU/RC
 Sample : P3997-06
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AP1

Quant Time: Sep 16 00:15:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.481	152	5015	0.400	ng/ul	0.00
4) Naphthalene-d8	10.239	136	14067	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.123	164	7451	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.978	188	1300039	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.231	264	20497	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	26524	5.145	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.839	152	6564	0.325	ng/ul	0.00
18) Fluoranthene-d10	18.920	212	15827	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
26) Benzo(a)pyrene	23.099	252	5788	0.091	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033963.D
Acq On : 15 Sep 2024 22:27
Operator : JU/RC
Sample : P3997-06
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP1


Quant Time: Sep 16 00:15:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

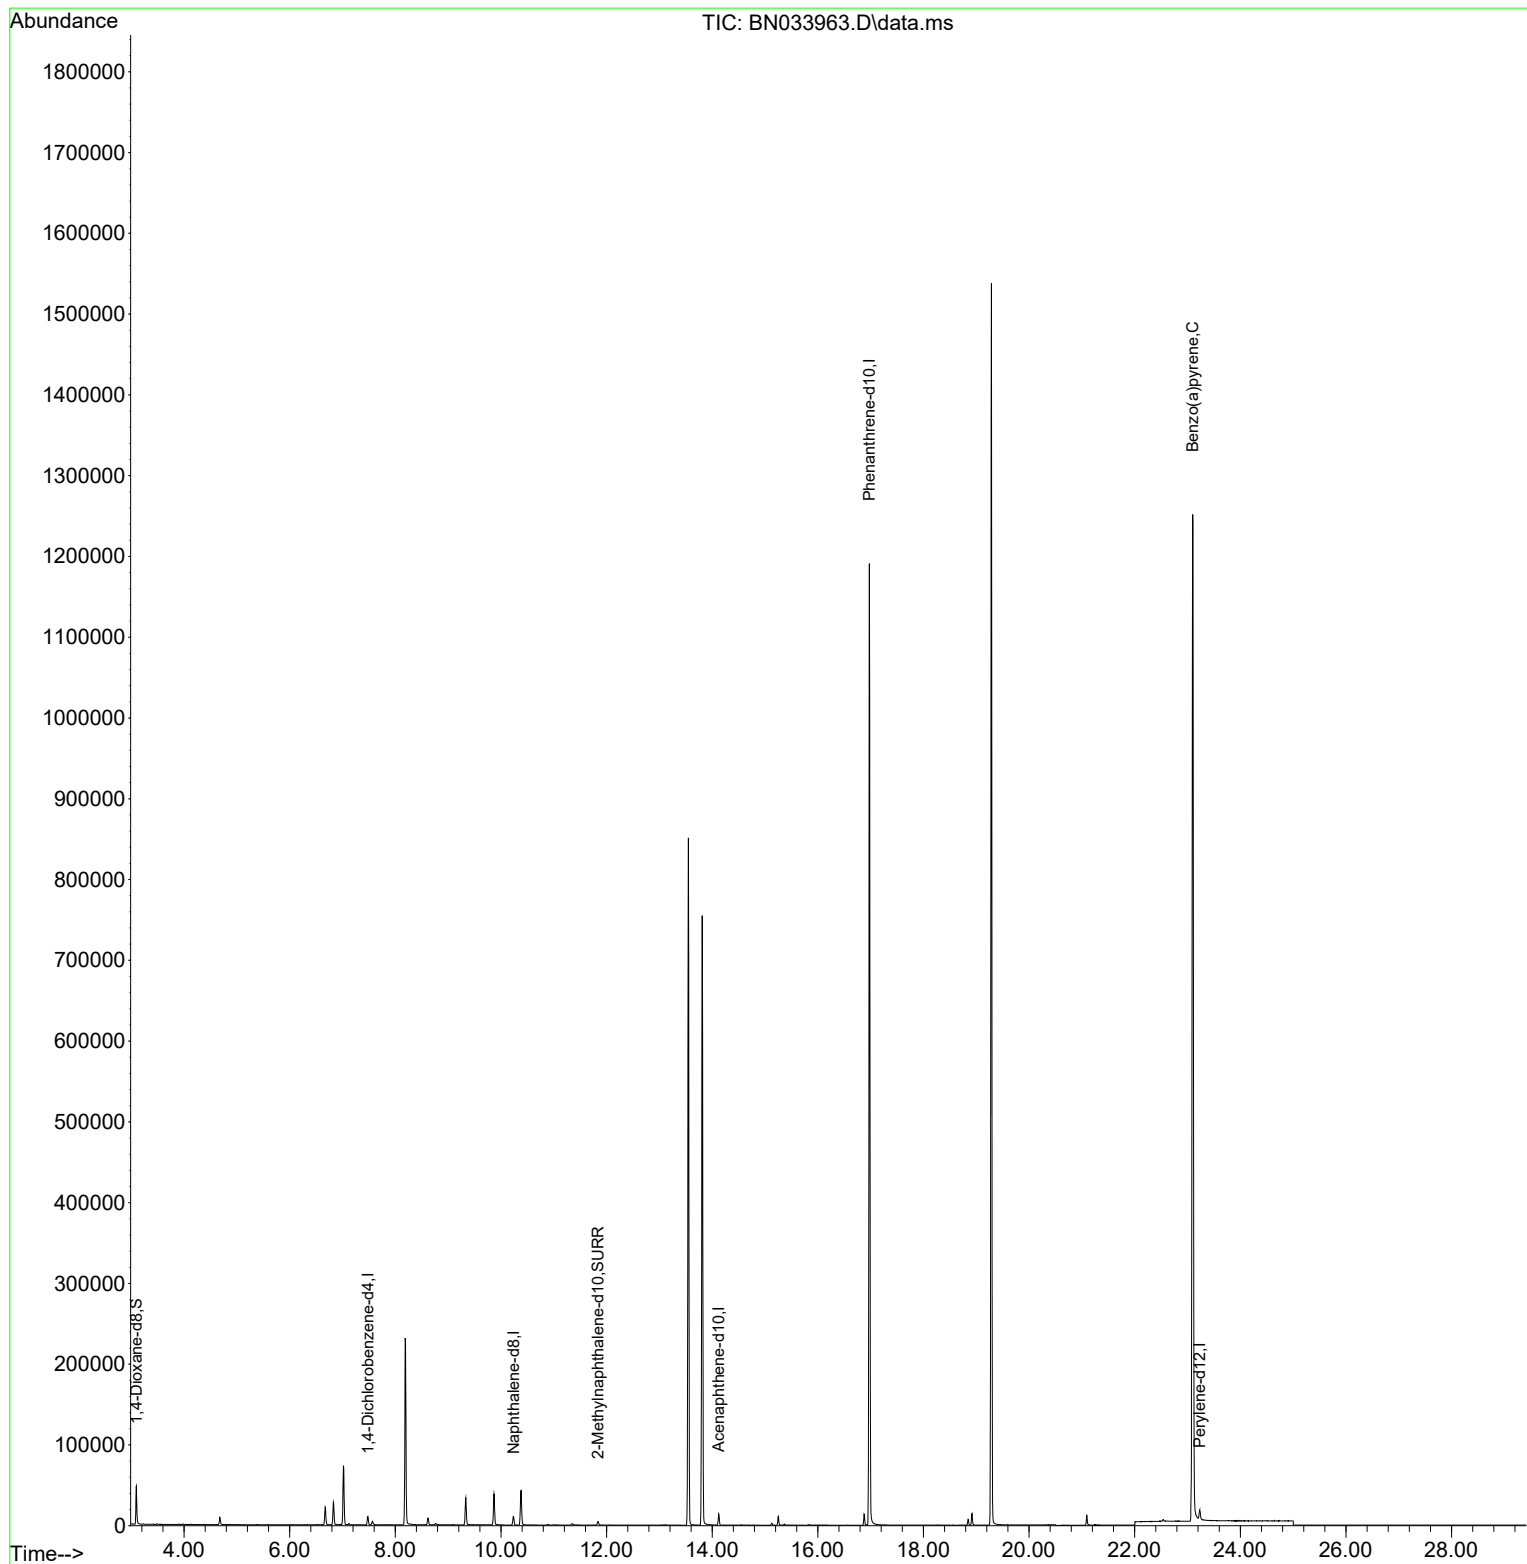

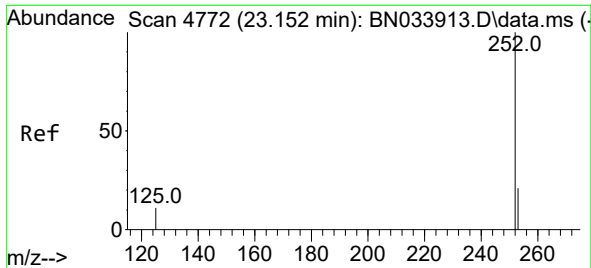

#26
Benzo(a)pyrene
Concen: 0.091 ng/ul
RT: 23.099 min Scan# 41
Delta R.T. -0.053 min
Lab File: BN033963.D
Acq: 15 Sep 2024 22:27

Instrument :
BNA_N
ClientSampleId :
C0AP1

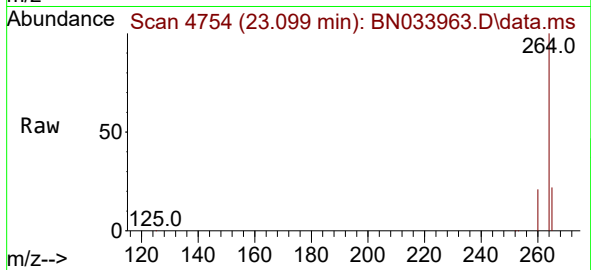

Tgt Ion:252 Resp: 5788
Ion Ratio Lower Upper
252 100
253 39.1 22.8 34.2#
125 38.3 18.0 27.0#

