

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033965.D
 Acq On : 15 Sep 2024 23:39
 Operator : JU/RC
 Sample : P3997-08
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AQ7

Quant Time: Sep 16 00:15:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.481	152	5214	0.400	ng/ul	0.00
4) Naphthalene-d8	10.238	136	14828	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.122	164	7960	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.977	188	1277468	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.235	264	21242	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	31251	5.830	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.838	152	6706	0.315	ng/ul	0.00
18) Fluoranthene-d10	18.919	212	17040	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.131	88	2290	0.385	ng/ul#	89
5) Naphthalene	10.287	128	2075	0.052	ng/ul#	69
26) Benzo(a)pyrene	23.101	252	5312	0.080	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033965.D
Acq On : 15 Sep 2024 23:39
Operator : JU/RC
Sample : P3997-08
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AQ7

Quant Time: Sep 16 00:15:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration




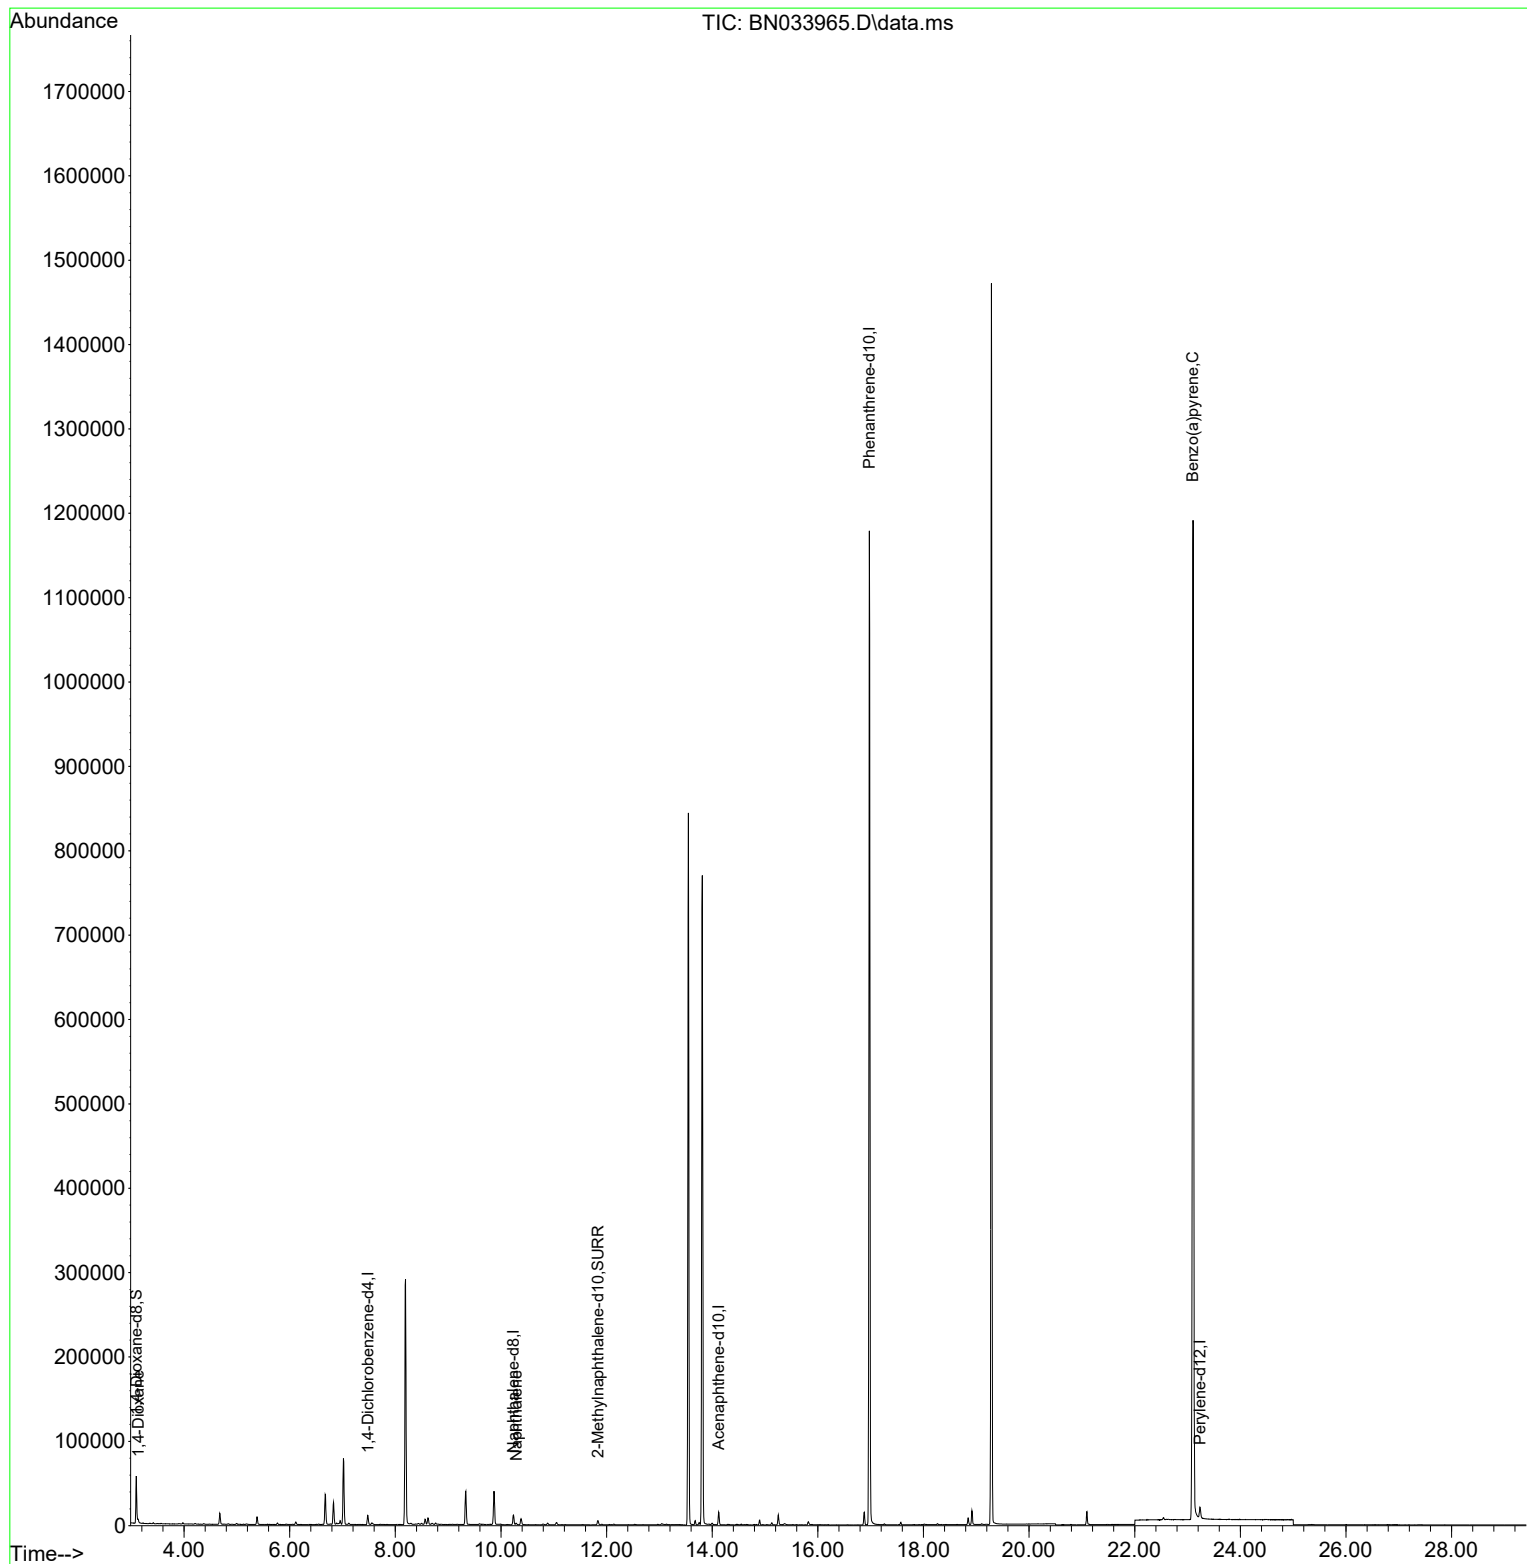


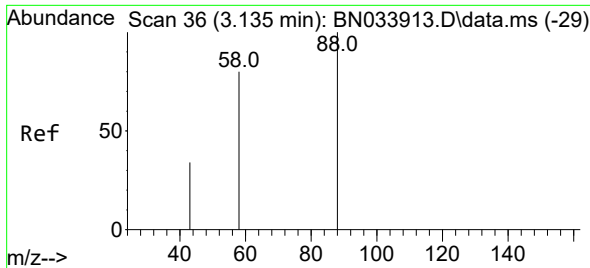

#2
1,4-Dioxane
Concen: 0.385 ng/ul
RT: 3.131 min Scan# 31
Delta R.T. -0.004 min
Lab File: BN033965.D
Acq: 15 Sep 2024 23:39




Instrument :
BNA_N
ClientSampleId :
C0AQ7


Tgt Ion: 88 Resp: 2290
Ion Ratio Lower Upper
88 100
43 72.1 47.0 70.4#
58 69.8 53.0 79.4

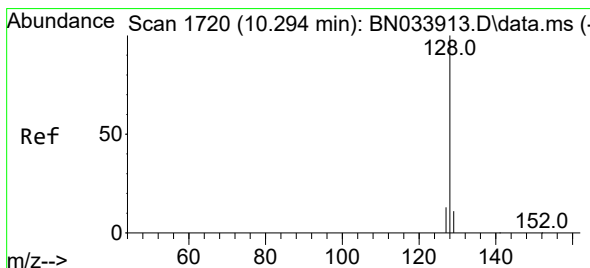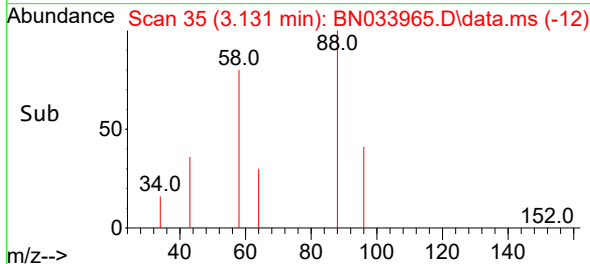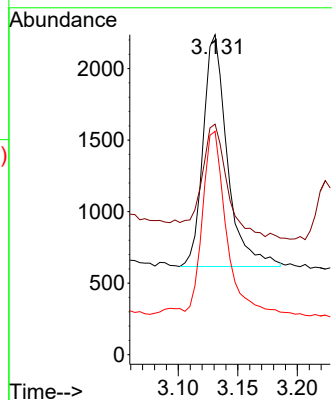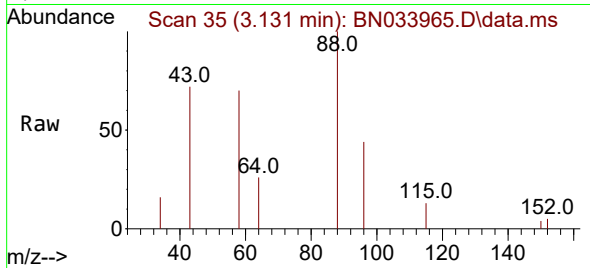

#5
Naphthalene
Concen: 0.052 ng/ul
RT: 10.287 min Scan# 1719
Delta R.T. -0.007 min
Lab File: BN033965.D
Acq: 15 Sep 2024 23:39


Tgt Ion:128 Resp: 2075
Ion Ratio Lower Upper
128 100
129 33.9 9.3 13.9#
127 16.6 10.8 16.2#

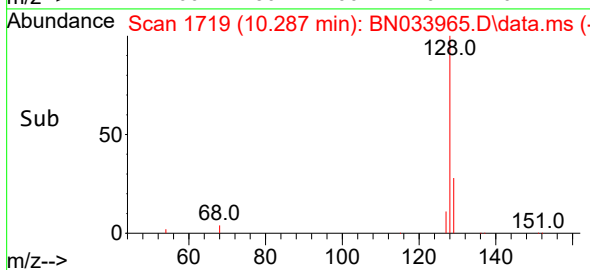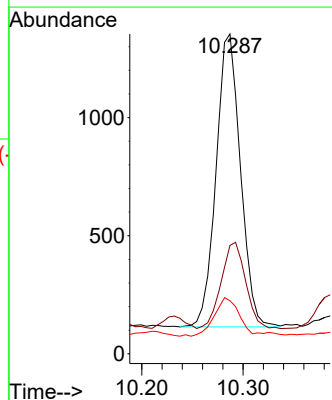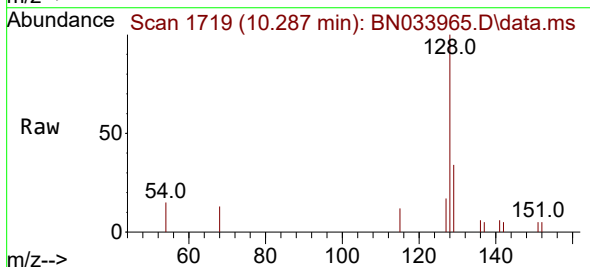

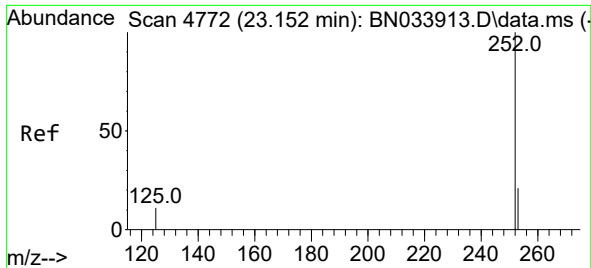

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.101 min Scan# 41
Delta R.T. -0.051 min
Lab File: BN033965.D
Acq: 15 Sep 2024 23:39

Instrument :
BNA_N
ClientSampleId :
C0AQ7

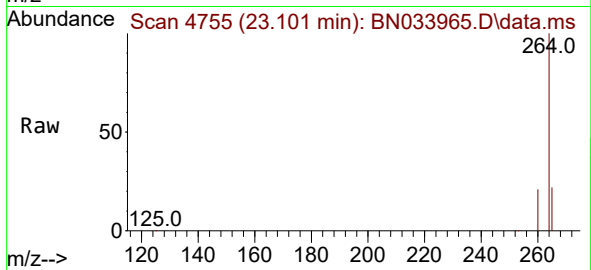

Tgt Ion:252 Resp: 5312
Ion Ratio Lower Upper
252 100
253 46.1 22.8 34.2#
125 50.7 18.0 27.0#

