




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033945.D
Acq On : 15 Sep 2024 11:03
Operator : JU/RC
Sample : PB163355BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK355

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/16/2024
Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 16 00:12:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

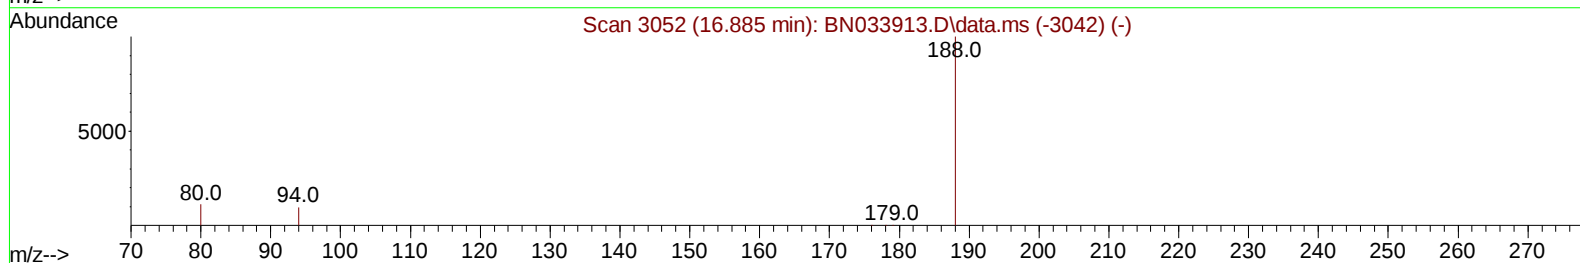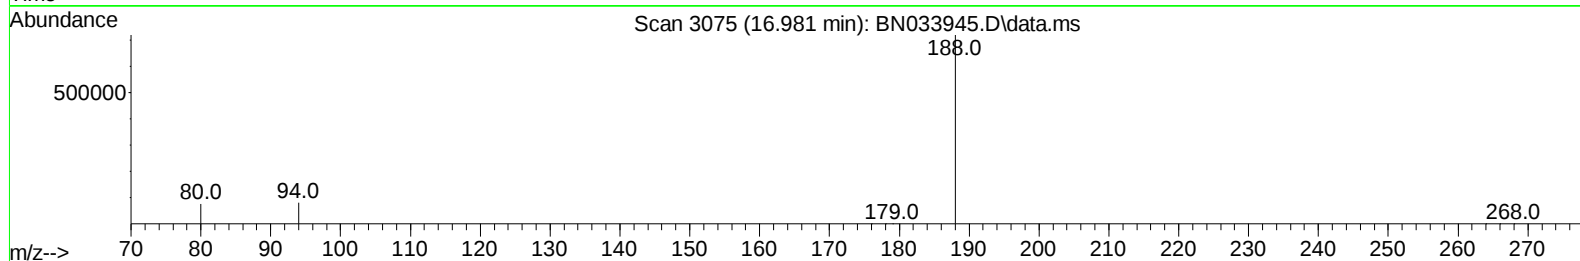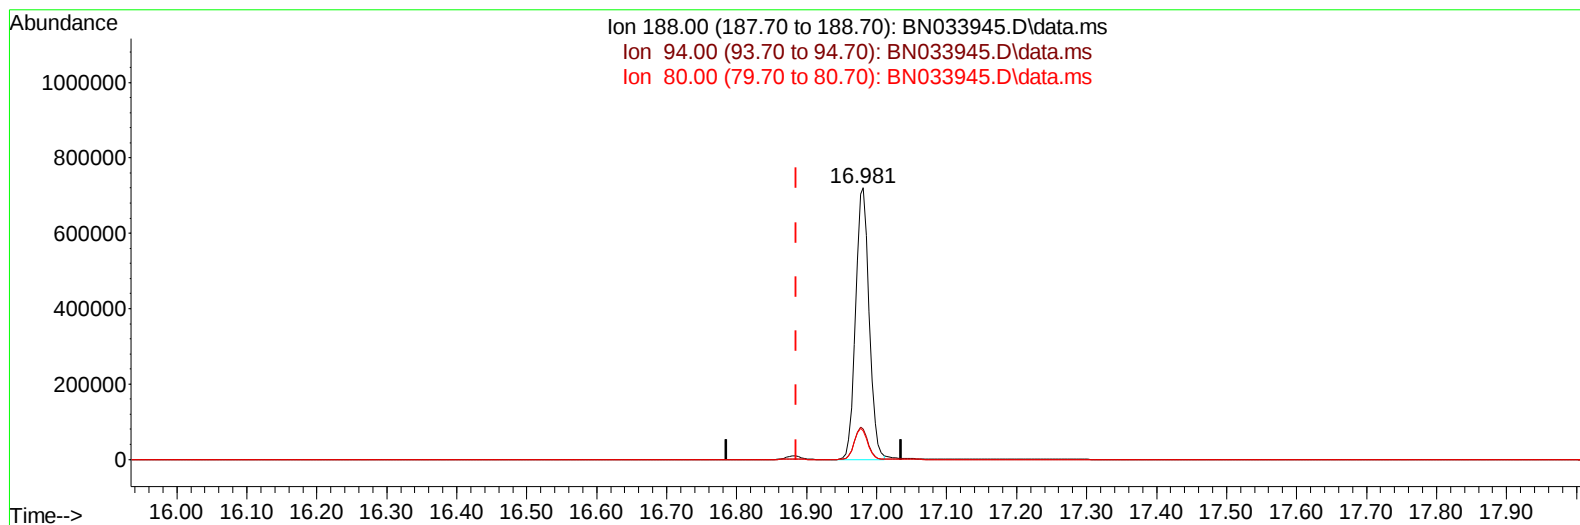

TIC: BN033945.D\data.ms

(13) Phenanthrene-d10 (I)**16.981min (+ 0.096) 0.40 ng/u1****response 967513**

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	11.29
80.00	11.50	10.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033945.D
Acq On : 15 Sep 2024 11:03
Operator : JU/RC
Sample : PB163355BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK355

Manual IntegrationsAPPROVED

Quant Time: Sep 16 00:12:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/16/2024
Supervised By :mohammad ahmed 09/17/2024

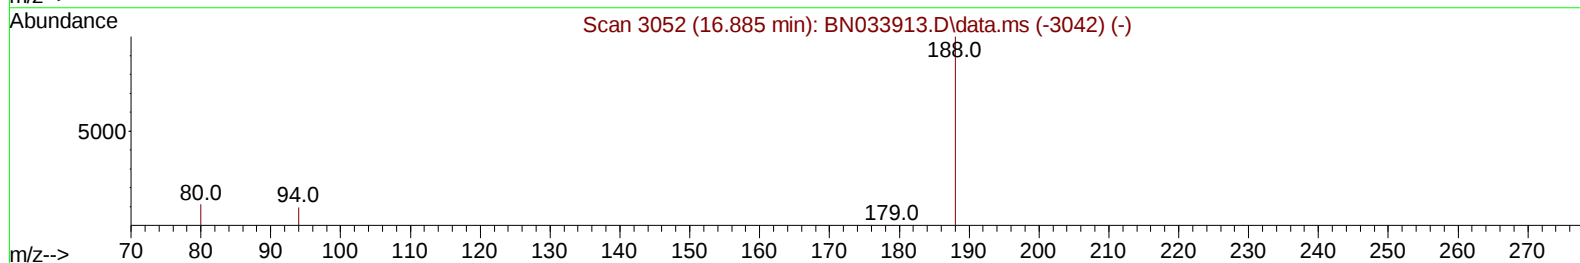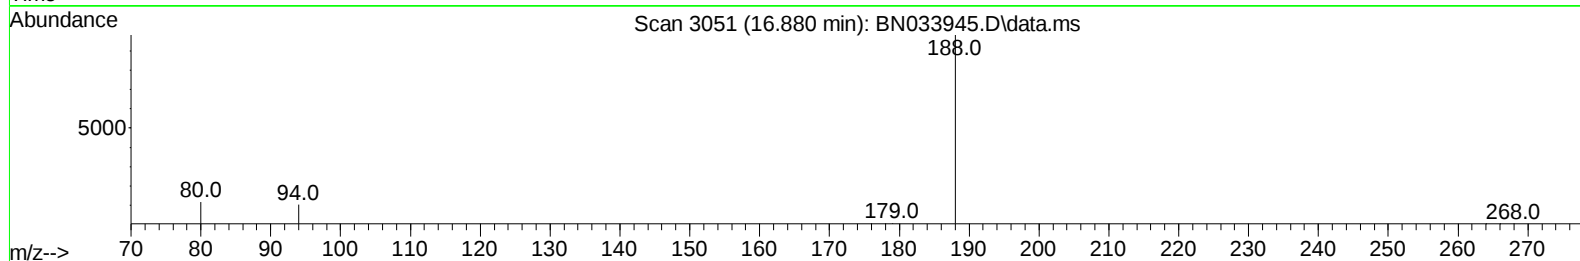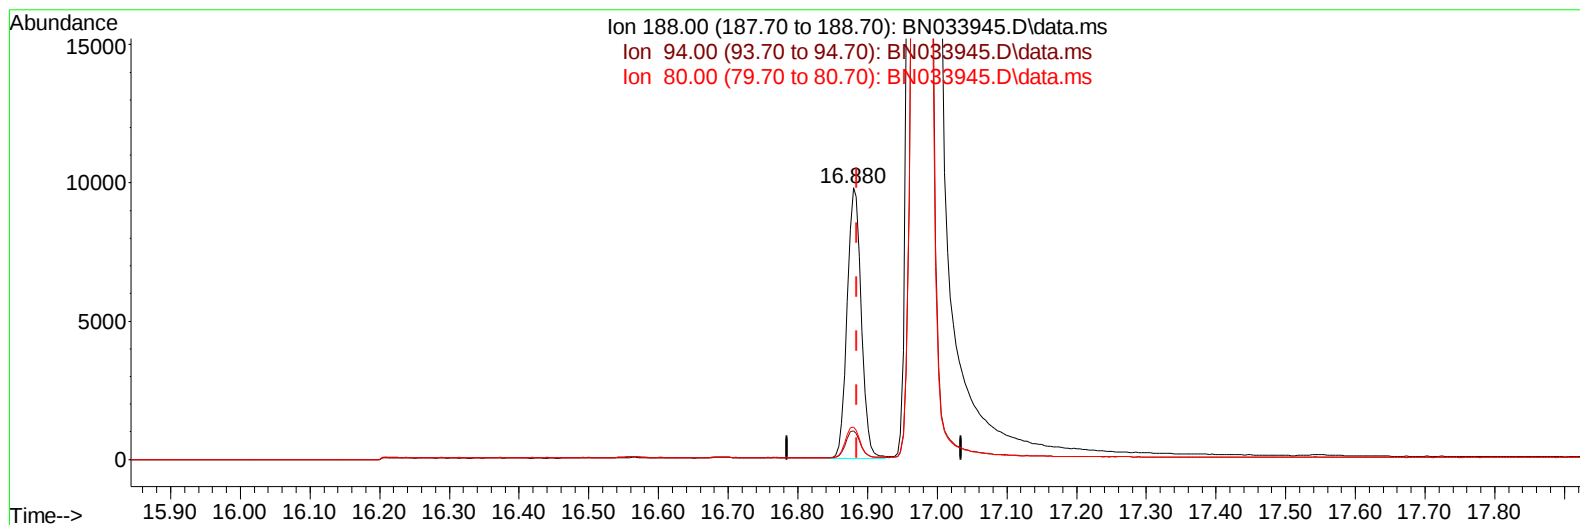

TIC: BN033945.D\data.ms

(13) Phenanthrene-d10 (I)

16.880min (-0.006) 0.40 ng/u1 m

response 13805

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	10.52
80.00	11.50	11.97
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033945.D
Acq On : 15 Sep 2024 11:03
Operator : JU/RC
Sample : PB163355BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK355

Manual IntegrationsAPPROVED

Quant Time: Sep 16 00:12:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/16/2024
Supervised By :mohammad ahmed 09/17/2024

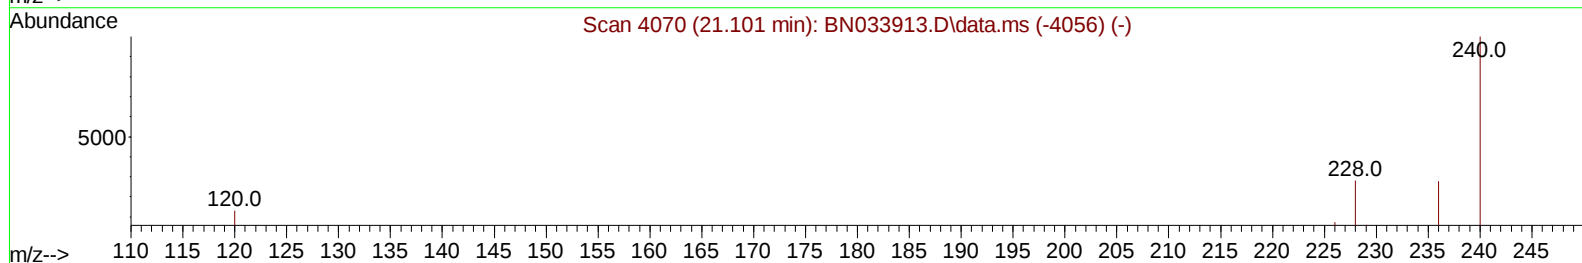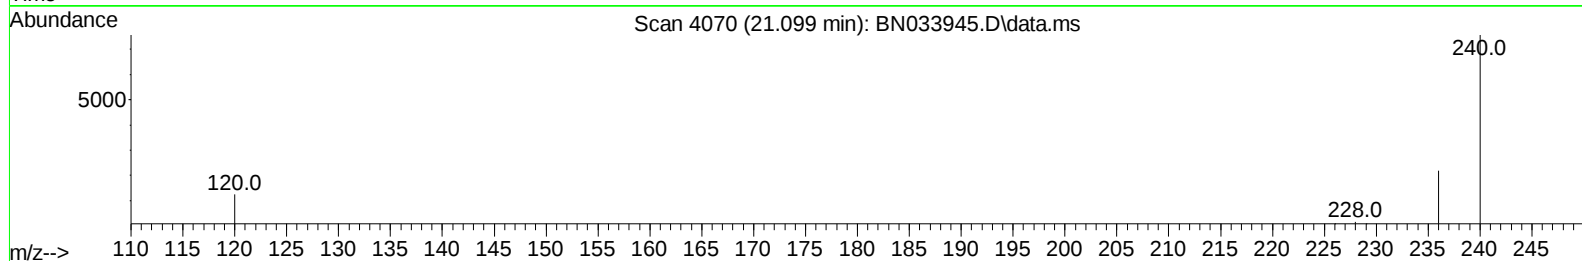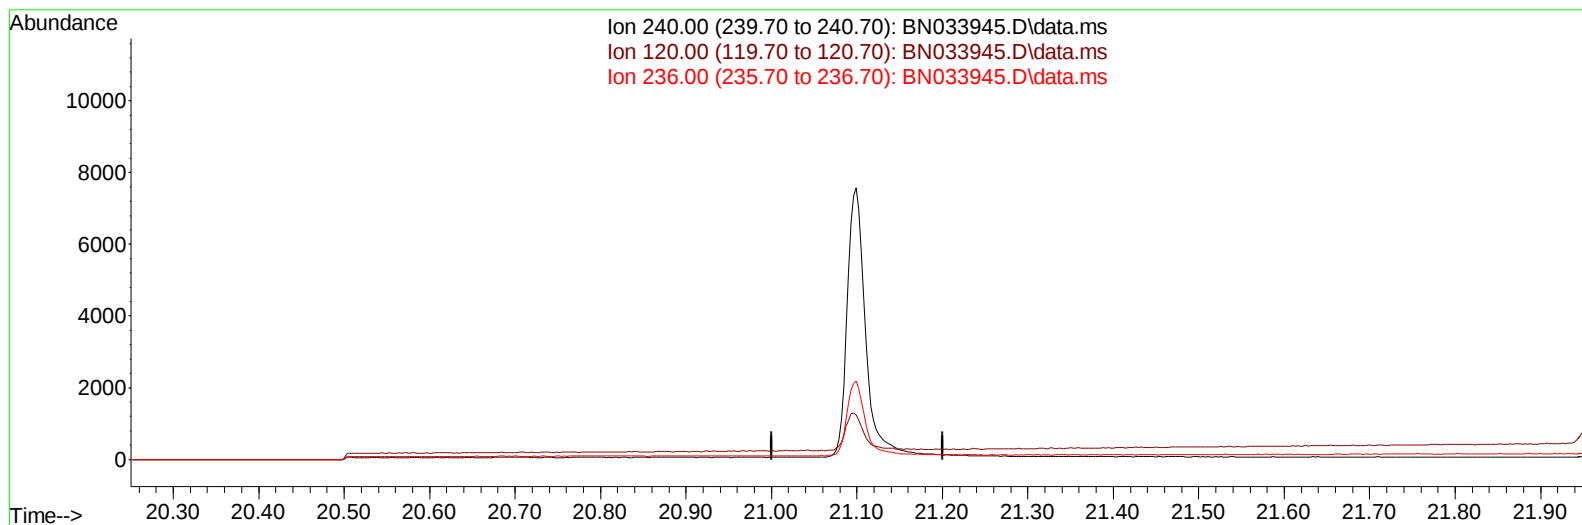

TIC: BN033945.D\data.ms

(17) Chrysene-d12

21.101min (-21.101) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.40	0.00#
236.00	28.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033945.D
Acq On : 15 Sep 2024 11:03
Operator : JU/RC
Sample : PB163355BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK355

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/16/2024
Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 16 00:12:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

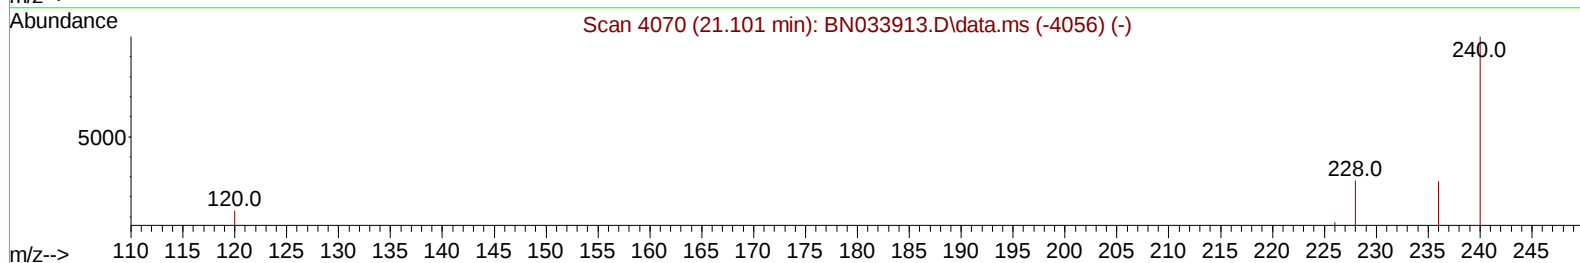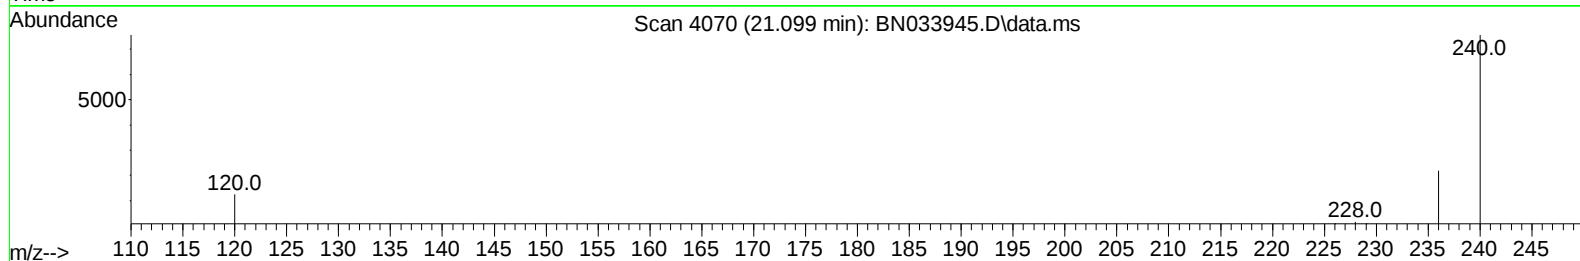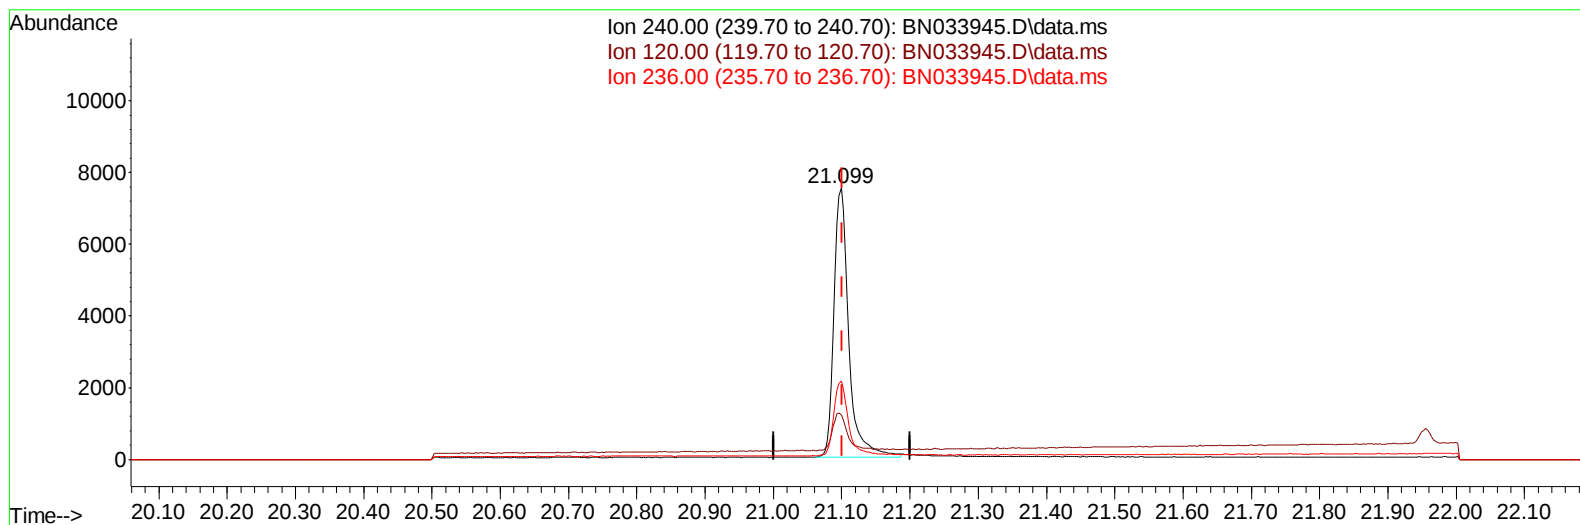

TIC: BN033945.D\data.ms

(17) Chrysene-d12

21.099min (-0.001) 0.40 ng/u1 m

response 11268

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.40	16.35
236.00	28.30	28.78
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033945.D
 Acq On : 15 Sep 2024 11:03
 Operator : JU/RC
 Sample : PB163355BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK355

Manual IntegrationsAPPROVED

Quant Time: Sep 16 00:12:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

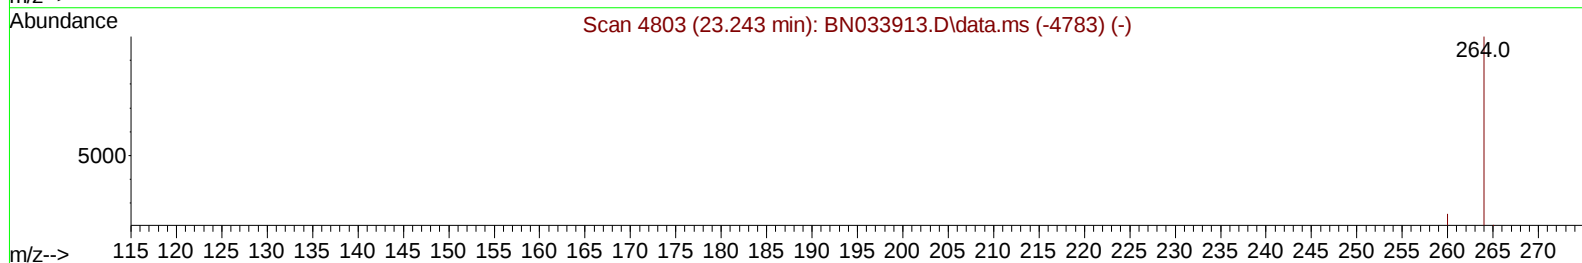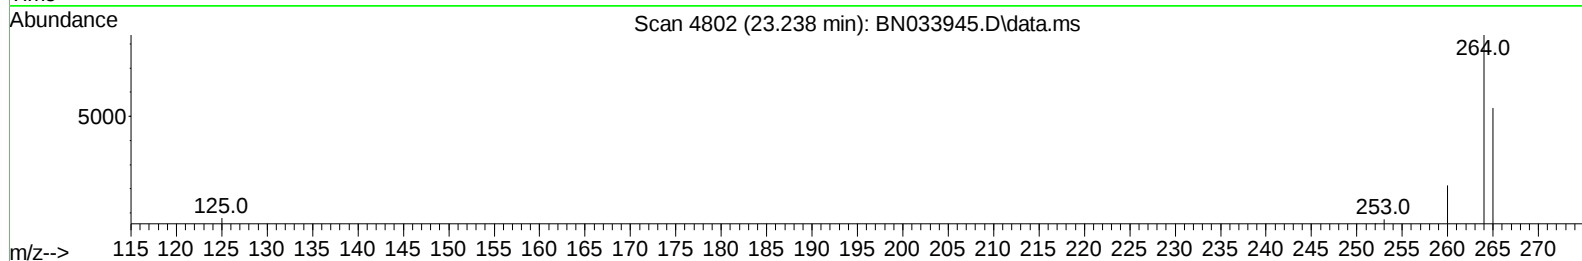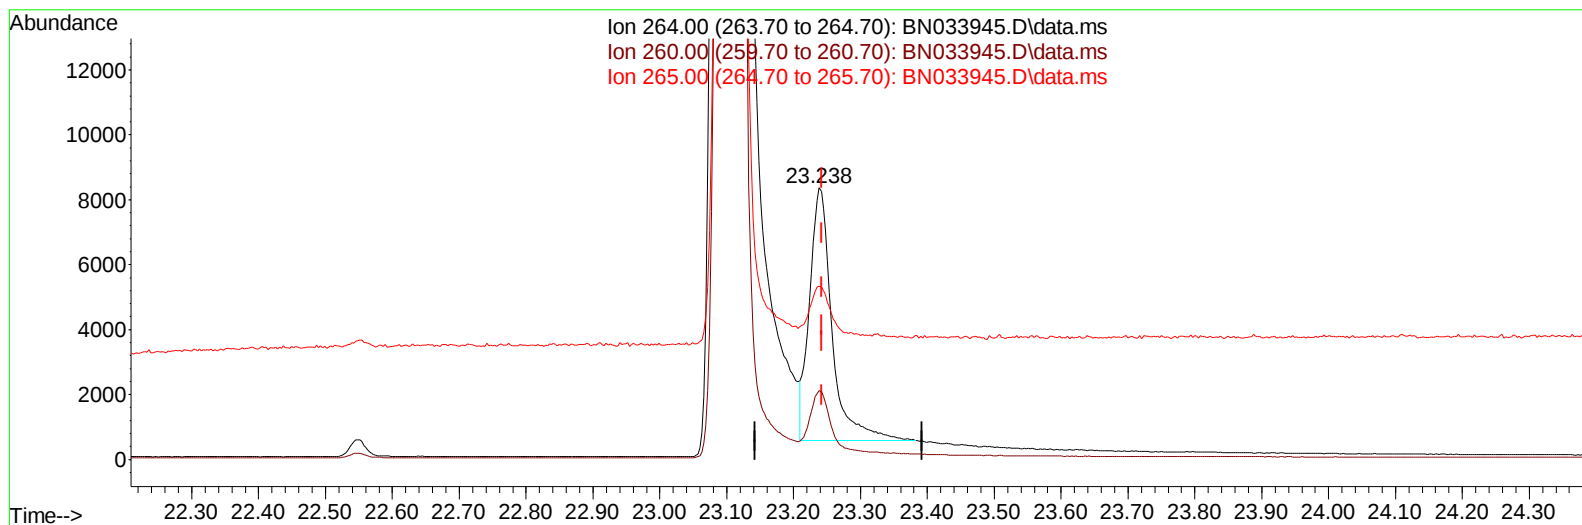

TIC: BN033945.D\data.ms

(23) Perylene-d12 (I)

23.238min (-0.004) 0.40 ng/u1

response 18242

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.48
265.00	73.30	63.79
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033945.D
Acq On : 15 Sep 2024 11:03
Operator : JU/RC
Sample : PB163355BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK355

Manual IntegrationsAPPROVED

Quant Time: Sep 16 00:12:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/16/2024
Supervised By :mohammad ahmed 09/17/2024

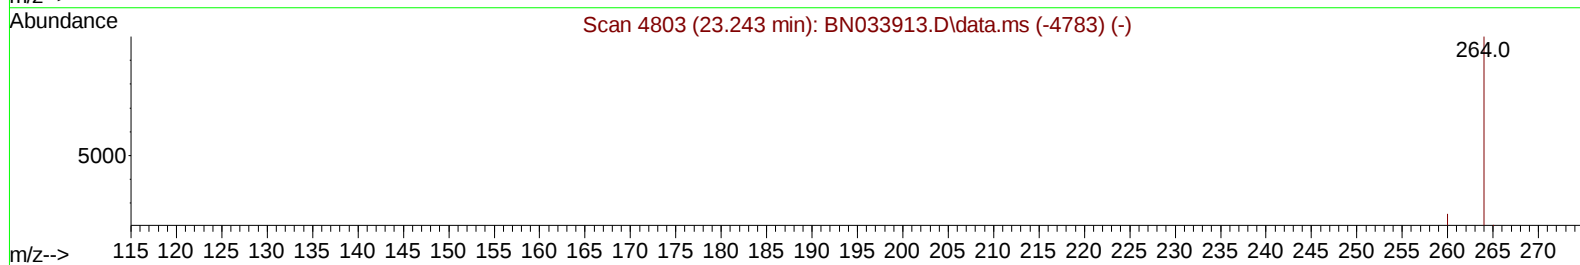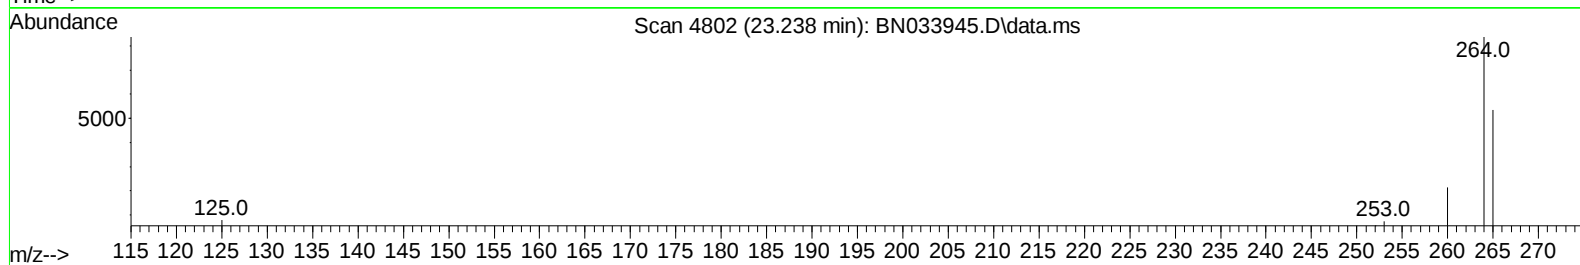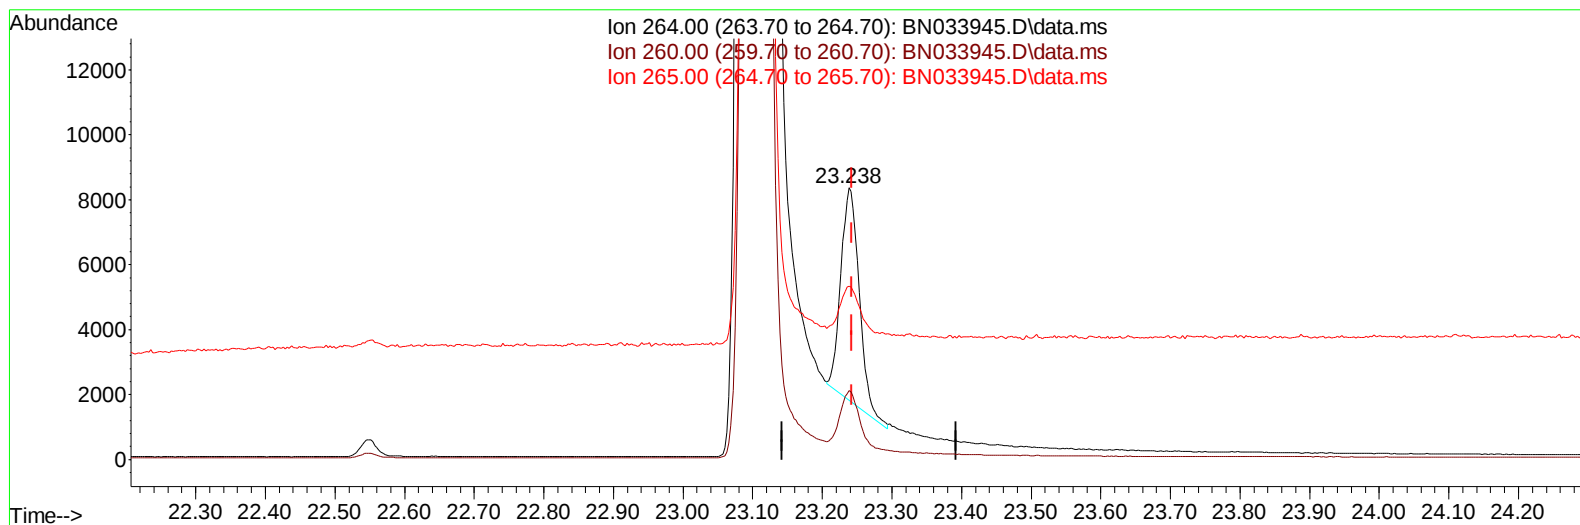

TIC: BN033945.D\data.ms

(23) Perylene-d12 (I)

23.238min (-0.004) 0.40 ng/ul m

response 11900

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.48
265.00	73.30	63.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033945.D
 Acq On : 15 Sep 2024 11:03
 Operator : JU/RC
 Sample : PB163355BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK355

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 16 00:12:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.481	152	4467	0.400	ng/ul	0.00
4) Naphthalene-d8	10.238	136	12523	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.127	164	6575	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.880	188	13805m	0.400	ng/ul	0.00
17) Chrysene-d12	21.099	240	11268m	0.400	ng/ul	0.00
23) Perylene-d12	23.238	264	11900m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	29554	6.435	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.843	152	5166	0.288	ng/ul	0.00
18) Fluoranthene-d10	18.923	212	11162	0.332	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033945.D
Acq On : 15 Sep 2024 11:03
Operator : JU/RC
Sample : PB163355BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK355

Manual IntegrationsAPPROVED

Quant Time: Sep 16 00:12:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/16/2024
Supervised By :mohammad ahmed 09/17/2024

