

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033921.D
 Acq On : 14 Sep 2024 18:49
 Operator : JU/RC
 Sample : P3993-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0UF2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 15 01:59:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.485	152	4054	0.400	ng/u1	0.00
4) Naphthalene-d8	10.244	136	11171	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.128	164	5815	0.400	ng/u1	0.00
13) Phenanthrene-d10	16.885	188	12112m	0.400	ng/u1	0.00
17) Chrysene-d12	21.101	240	9746m	0.400	ng/u1	0.00
23) Perylene-d12	23.243	264	9681m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.101	96	14832	3.559	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.845	152	3482	0.217	ng/u1	0.00
18) Fluoranthene-d10	18.925	212	8125	0.280	ng/u1	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.543	266	355m	0.093	ng/u1	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033921.D
Acq On : 14 Sep 2024 18:49
Operator : JU/RC
Sample : P3993-03
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0UF2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2024
Supervised By :mohammad ahmed 09/17/2024


Quant Time: Sep 15 01:59:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

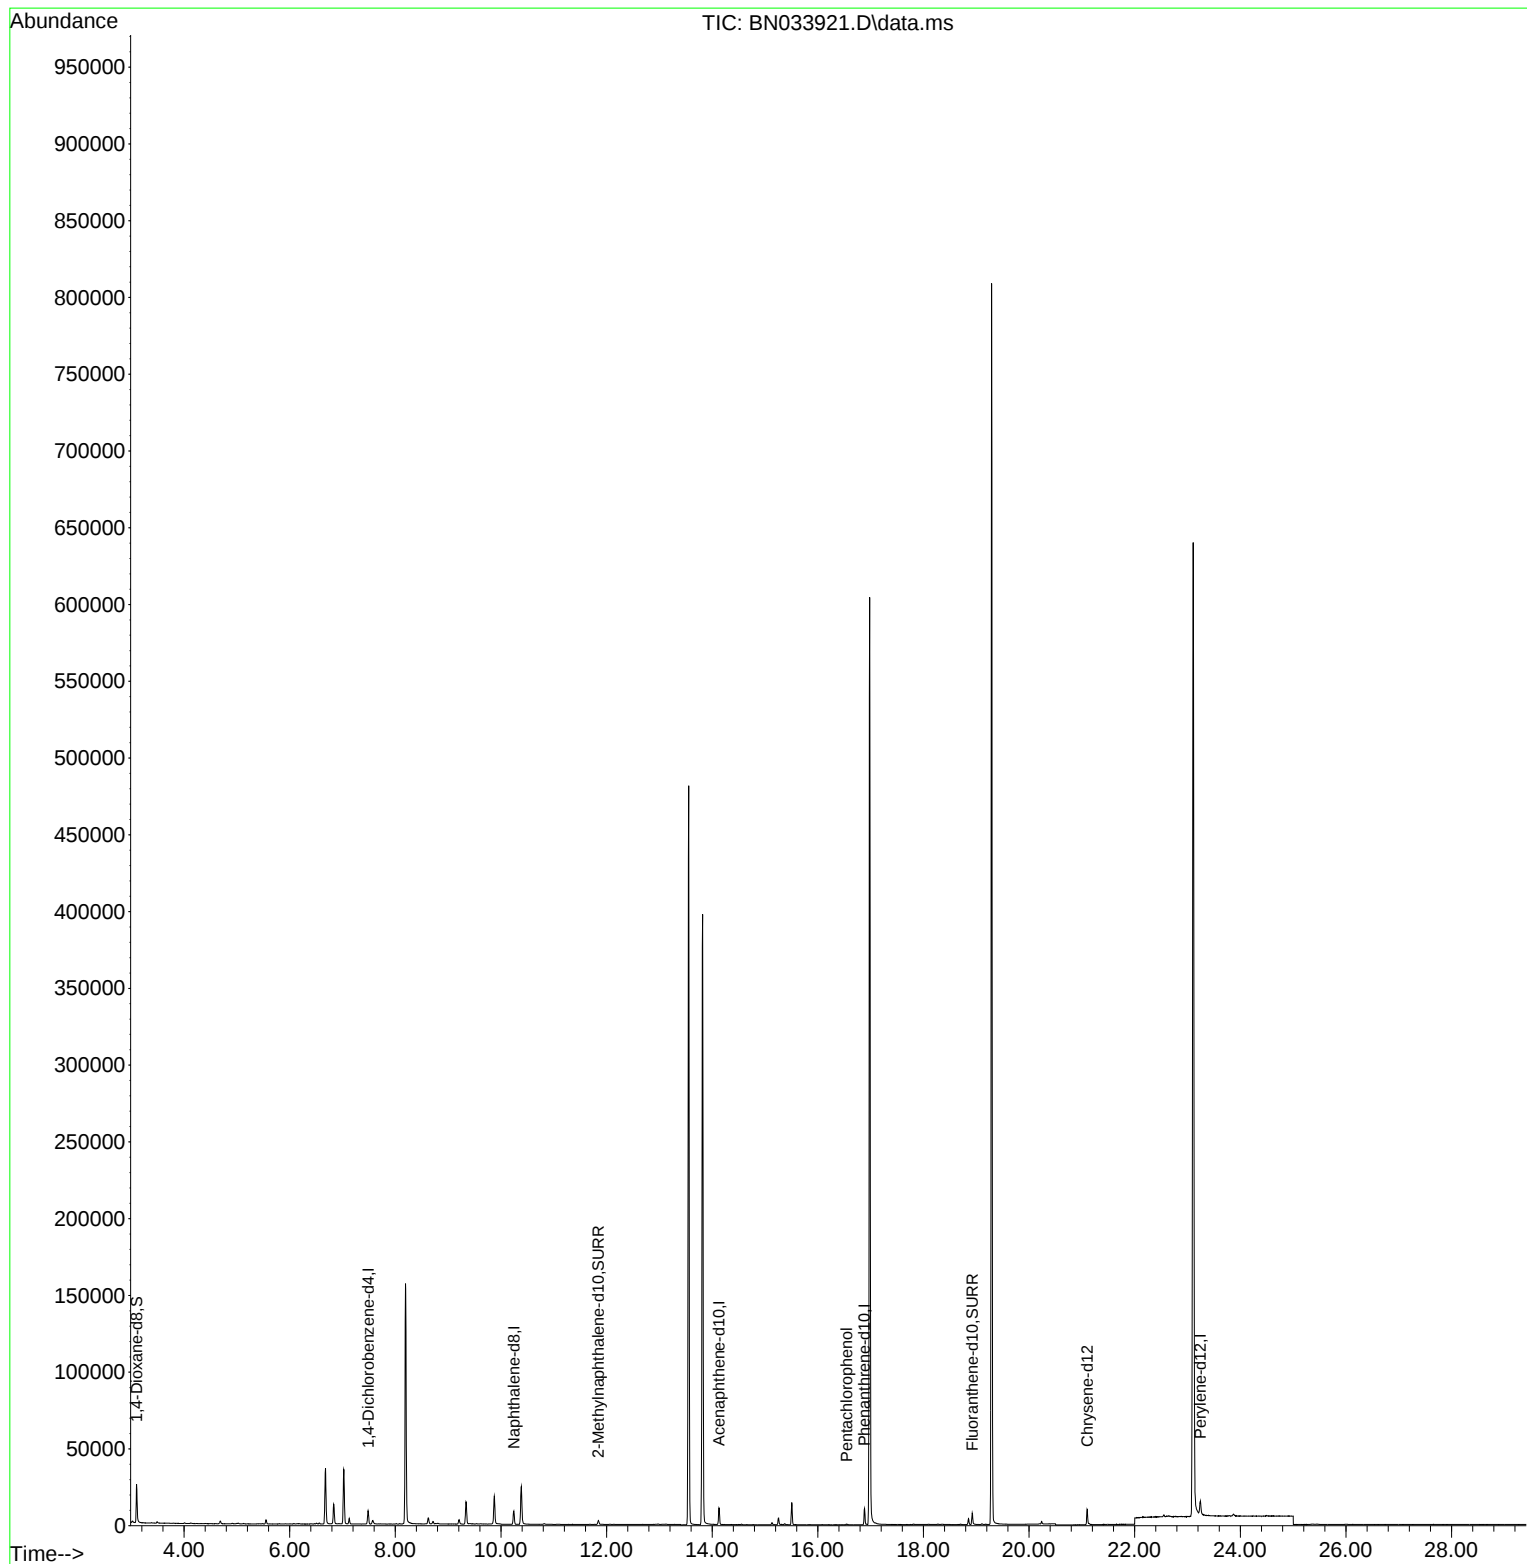

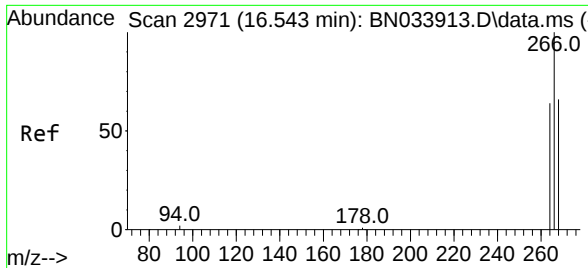

#14
Pentachlorophenol
Concen: 0.093 ng/ul m
RT: 16.543 min Scan# 2971
Delta R.T. -0.000 min
Lab File: BN033921.D
Acq: 14 Sep 2024 18:49

Instrument :
BNA_N
ClientSampleId :
C0UF2

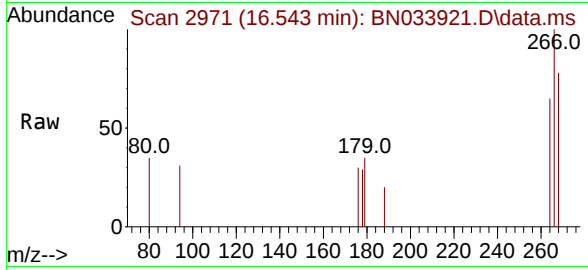

Tgt Ion:	266	Resp:	35
Ion	Ratio	Lower	Upper
266	100		
264	0.0	50.3	75.5
268	2.5	51.7	77.5

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2024
Supervised By :mohammad ahmed 09/17/2024

