

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033924.D
 Acq On : 14 Sep 2024 20:37
 Operator : JU/RC
 Sample : P3952-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B25

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 15 01:59:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.485	152	4981	0.400	ng/ul	0.00
4) Naphthalene-d8	10.244	136	14044	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.128	164	7543	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.885	188	15990m	0.400	ng/ul	0.00
17) Chrysene-d12	21.097	240	12708m	0.400	ng/ul	0.00
23) Perylene-d12	23.240	264	12711m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.101	96	31690	6.188	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.845	152	7064	0.351	ng/ul	0.00
18) Fluoranthene-d10	18.924	212	17584	0.464	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.135	88	547	0.096	ng/ul#	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033924.D
Acq On : 14 Sep 2024 20:37
Operator : JU/RC
Sample : P3952-01
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0B25

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2024
Supervised By :mohammad ahmed 09/17/2024


Quant Time: Sep 15 01:59:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

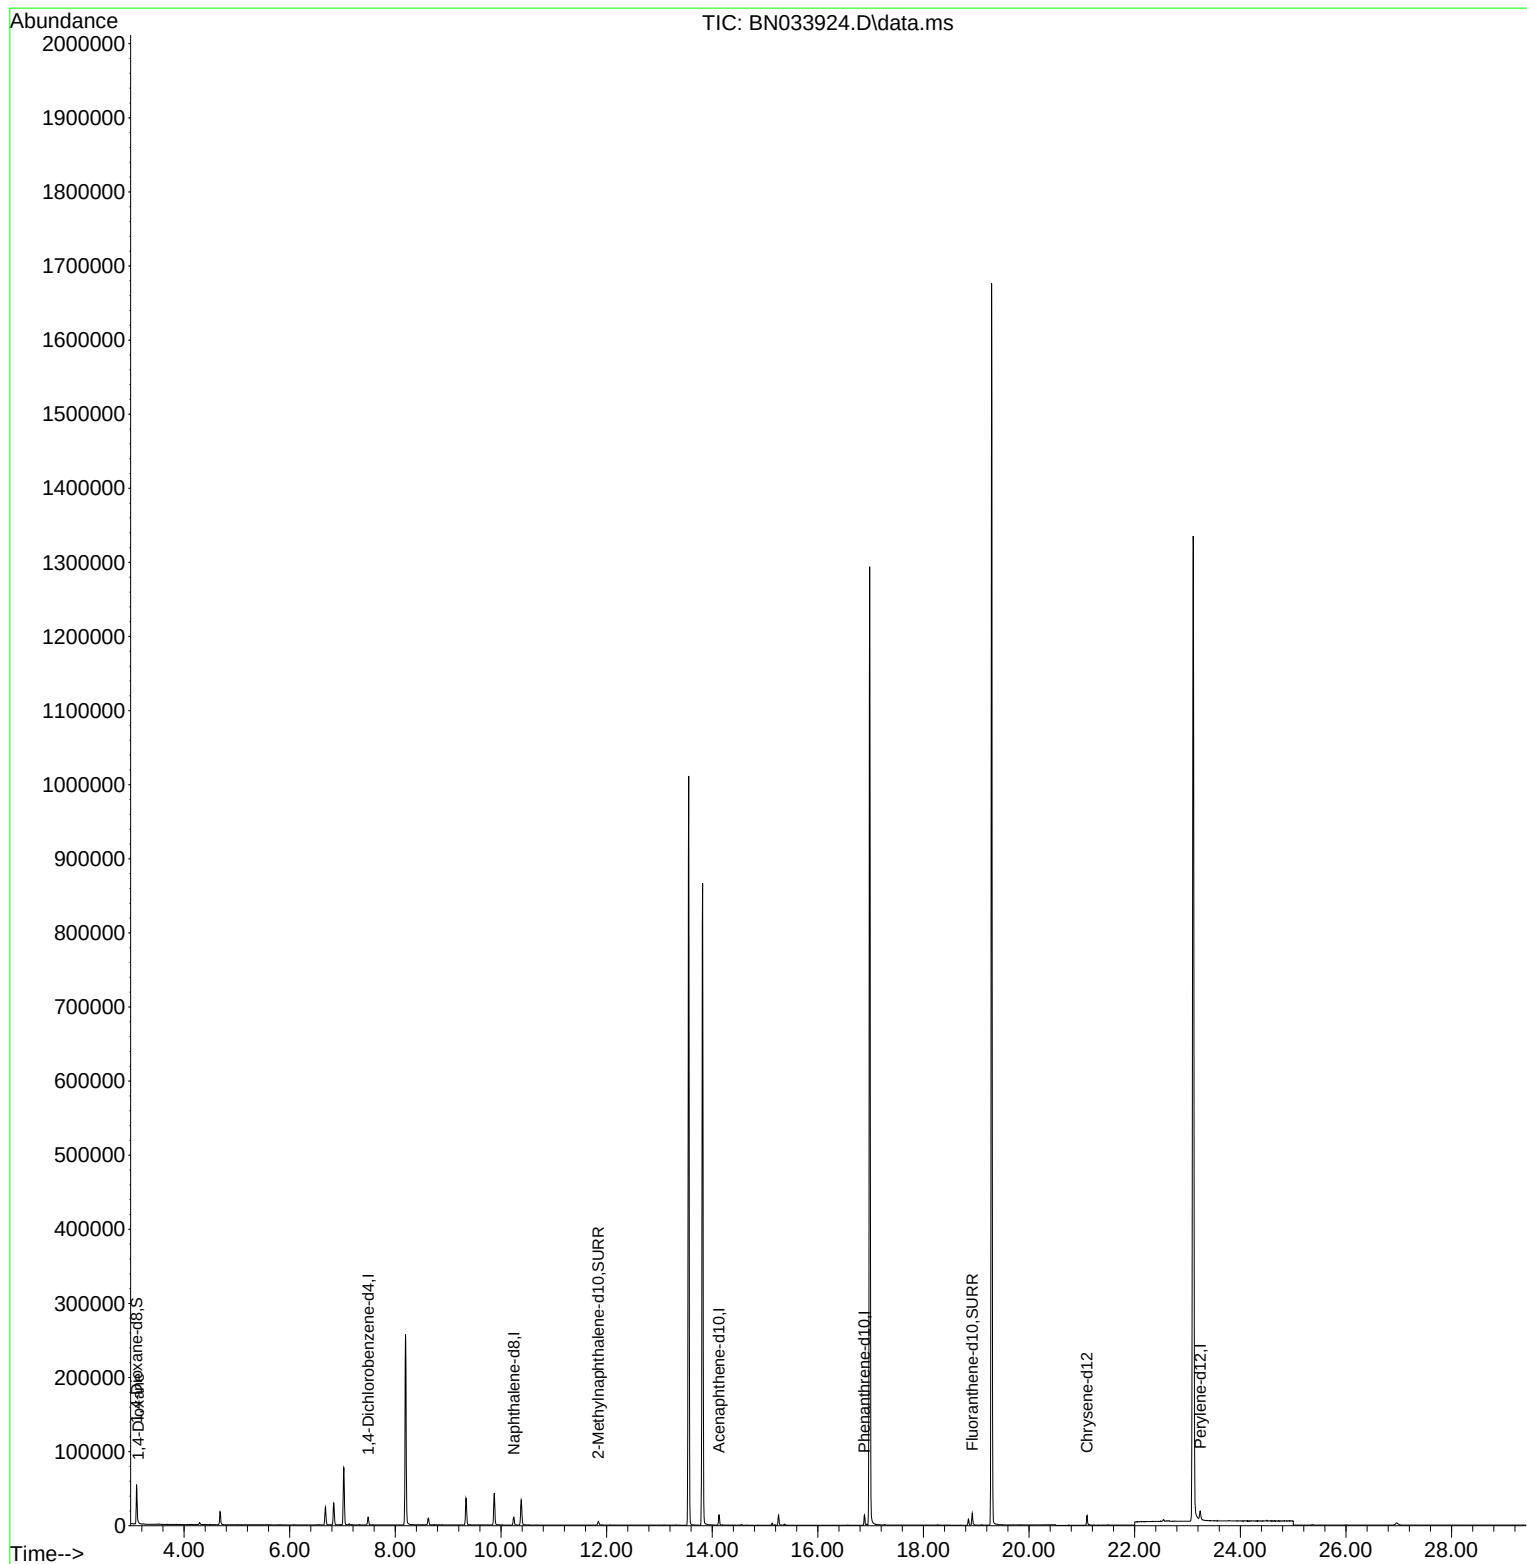

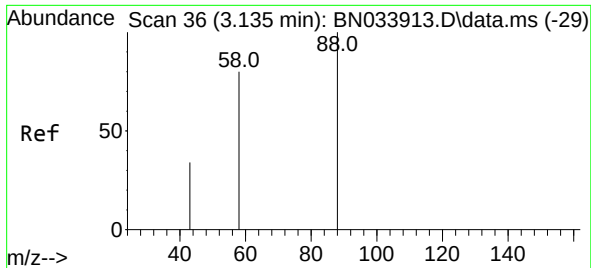

#2
 1,4-Dioxane
 Concen: 0.096 ng/ul
 RT: 3.135 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: BN033924.D
 Acq: 14 Sep 2024 20:37

Instrument :
 BNA_N
 ClientSampleId :
 C0B25

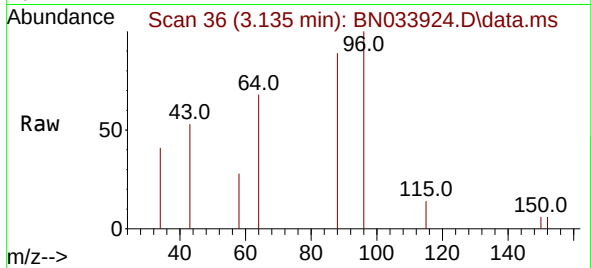

Tgt Ion: 88	Resp: 54
Ion Ratio	Lower Upper
88 100	
43 59.5	47.0 70.4
58 31.8	53.0 79.4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

