

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033926.D
 Acq On : 14 Sep 2024 21:49
 Operator : JU/RC
 Sample : P3952-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B35

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 15 02:00:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.485	152	3962	0.400	ng/u1	0.00
4) Naphthalene-d8	10.244	136	11180	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.128	164	6027	0.400	ng/u1	0.00
13) Phenanthrene-d10	16.885	188	12822m	0.400	ng/u1	0.00
17) Chrysene-d12	21.095	240	11088m	0.400	ng/u1	0.00
23) Perylene-d12	23.237	264	10735m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	21934	5.385	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.845	152	5091	0.317	ng/u1	0.00
18) Fluoranthene-d10	18.924	212	13892m	0.420	ng/u1	0.00
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.131	88	2512	0.556	ng/u1#	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033926.D
Acq On : 14 Sep 2024 21:49
Operator : JU/RC
Sample : P3952-03
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0B35

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2024
Supervised By :mohammad ahmed 09/17/2024


Quant Time: Sep 15 02:00:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

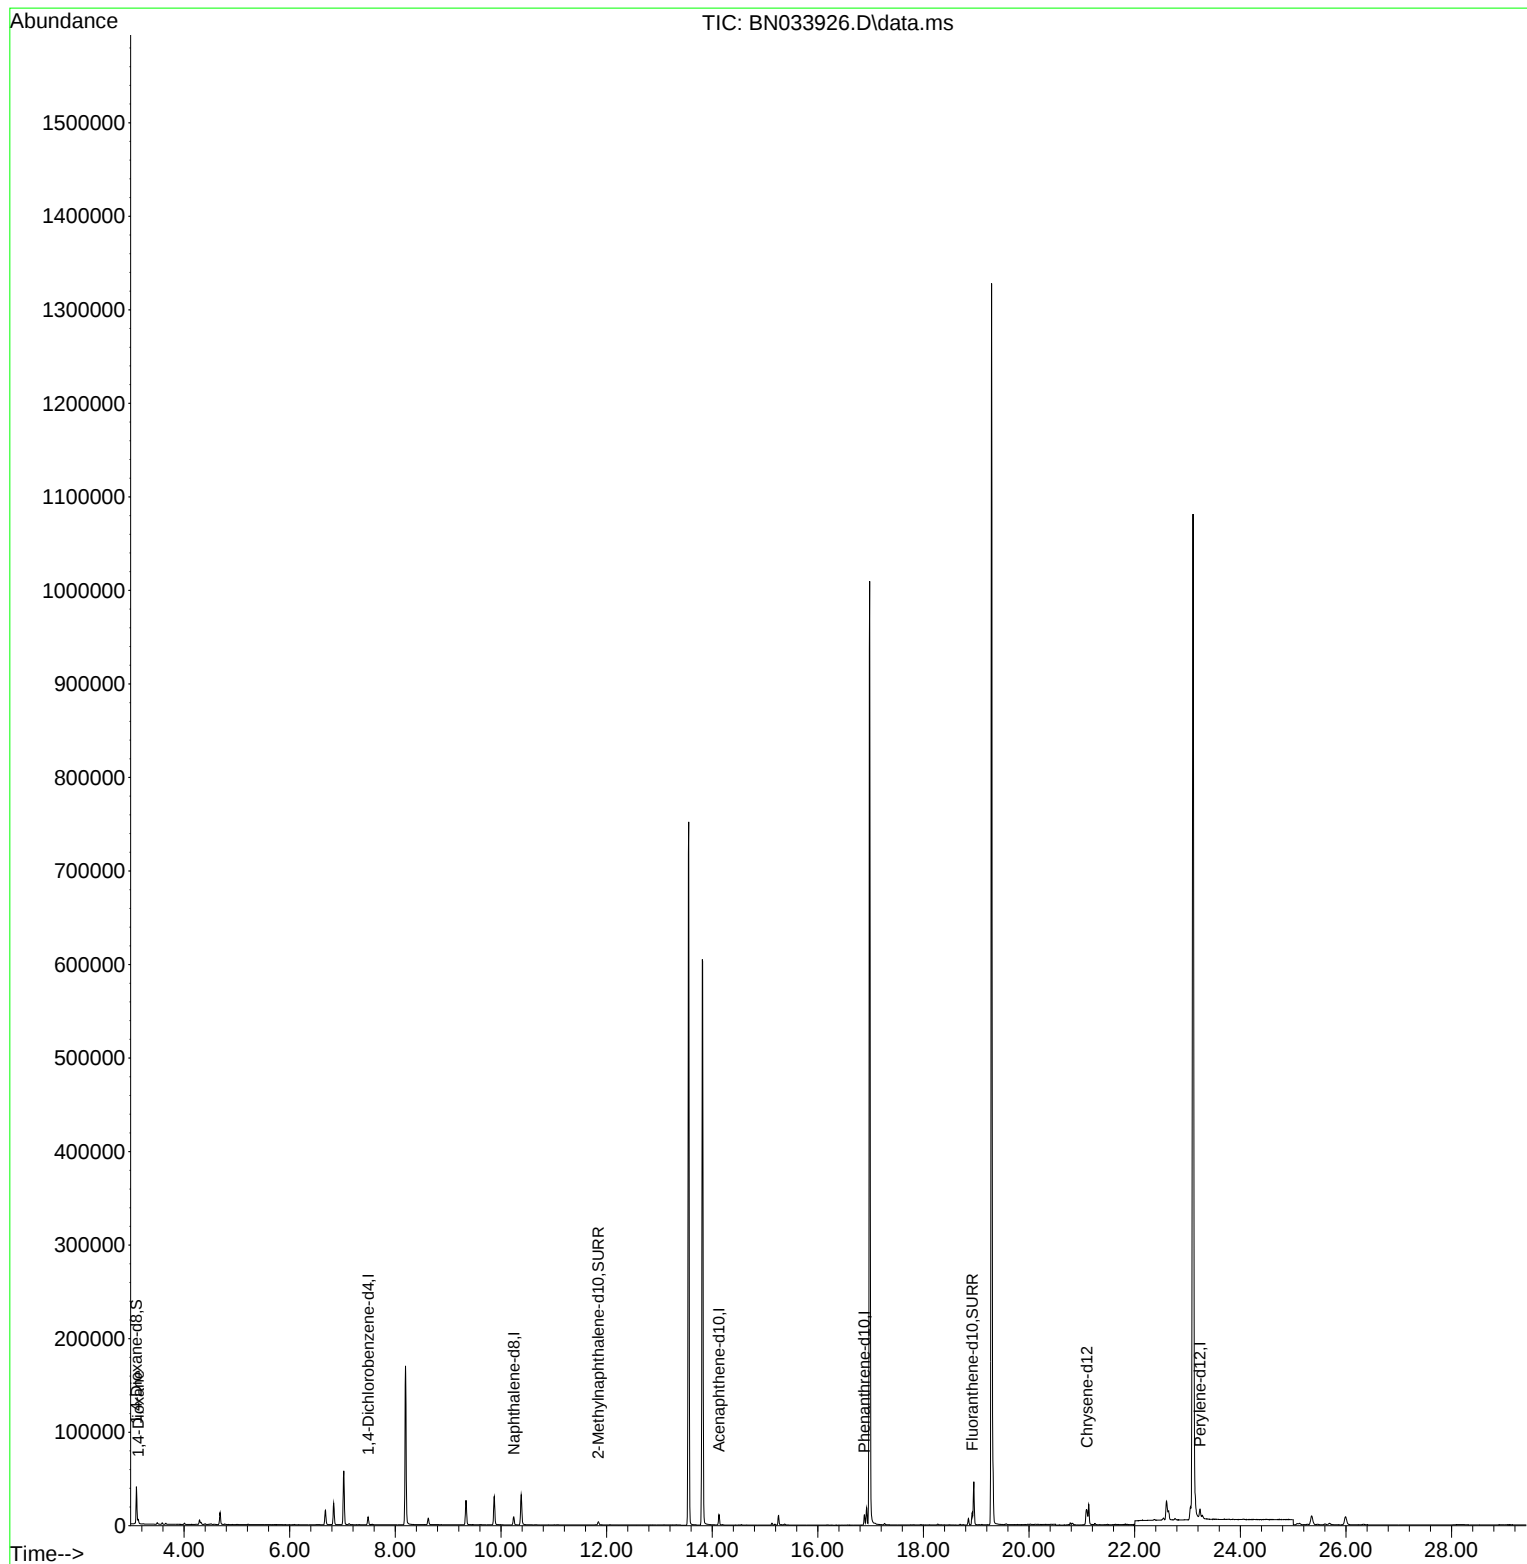

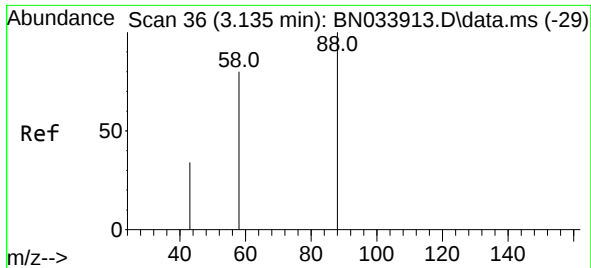

#2
 1,4-Dioxane
 Concen: 0.556 ng/ul
 RT: 3.131 min Scan# 30
 Delta R.T. -0.004 min
 Lab File: BN033926.D
 Acq: 14 Sep 2024 21:49

Instrument :
 BNA_N
 ClientSampleId :
 C0B35

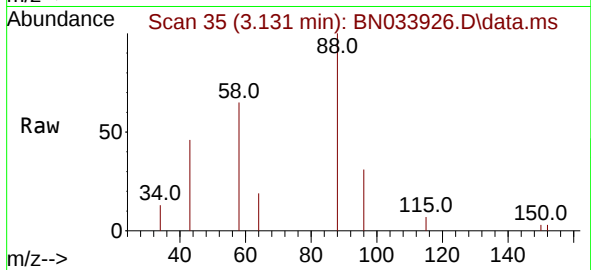

Tgt Ion: 88 Resp: 2512
 Ion Ratio Lower Upper
 88 100
 43 46.3 47.0 70.4
 58 65.5 53.0 79.4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

