

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033937.D
 Acq On : 15 Sep 2024 05:02
 Operator : JU/RC
 Sample : P3922-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AR3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 15 05:34:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.485	152	4142	0.400	ng/u1	0.00
4) Naphthalene-d8	10.239	136	12008	0.400	ng/u1	# 0.00
9) Acenaphthene-d10	14.128	164	14386	0.400	ng/u1	# 0.00
13) Phenanthrene-d10	16.881	188	16224m	0.400	ng/u1	0.00
17) Chrysene-d12	21.098	240	13915m	0.400	ng/u1	0.00
23) Perylene-d12	23.237	264	13992m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	26564	6.238	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.839	152	6374	0.370	ng/u1	0.00
18) Fluoranthene-d10	18.925	212	18283m	0.441	ng/u1	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.135	88	2005	0.424	ng/u1	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033937.D
Acq On : 15 Sep 2024 05:02
Operator : JU/RC
Sample : P3922-16
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AR3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2024
Supervised By :mohammad ahmed 09/17/2024


Quant Time: Sep 15 05:34:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

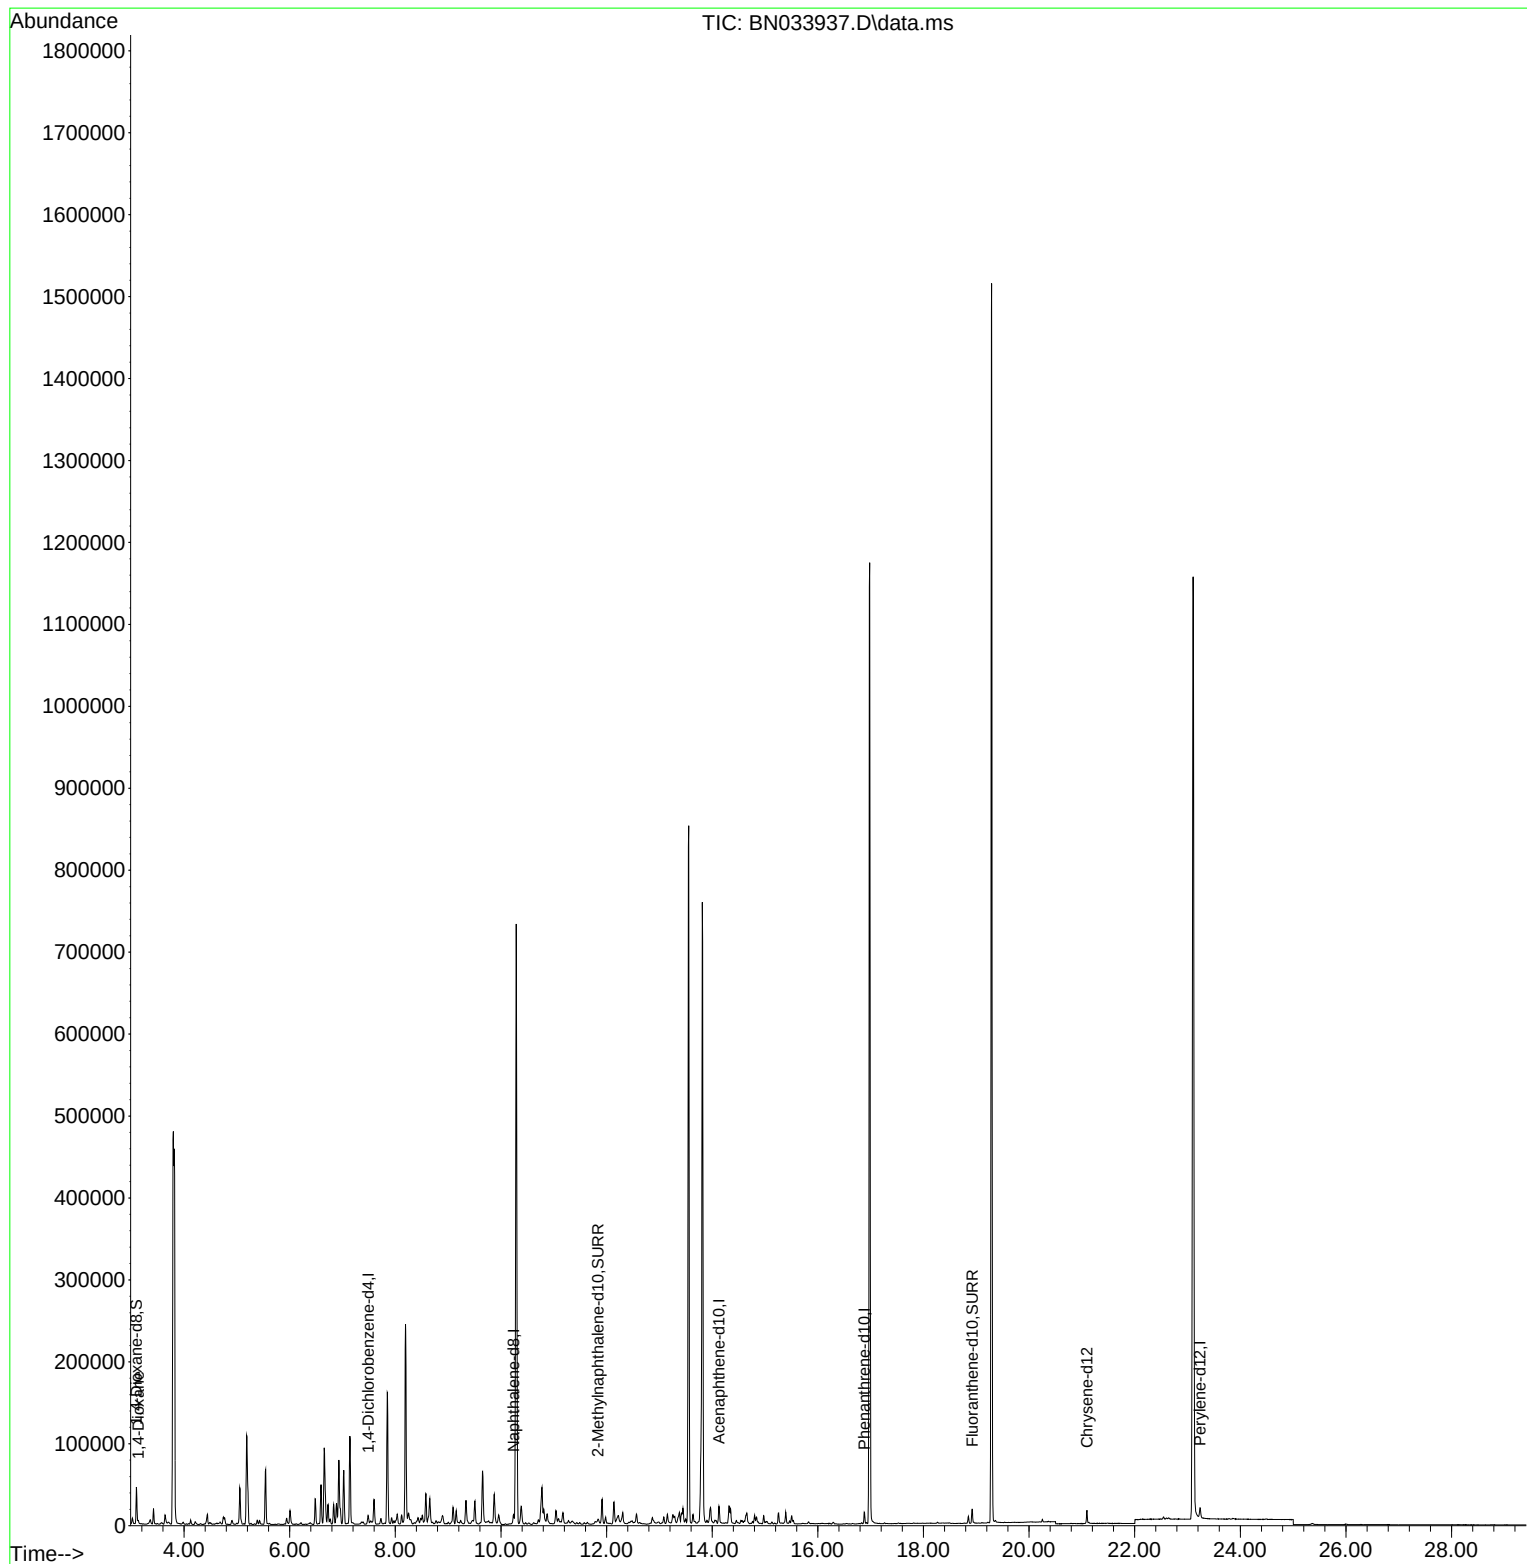

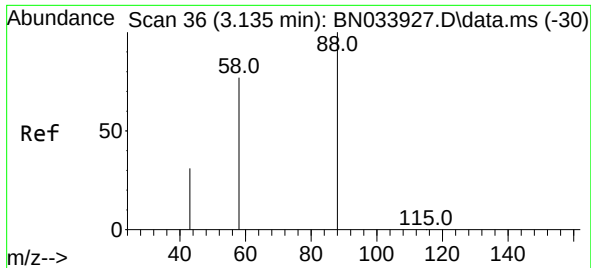

#2
 1,4-Dioxane
 Concen: 0.424 ng/ul
 RT: 3.135 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: BN033937.D
 Acq: 15 Sep 2024 05:02

Instrument :
 BNA_N
 ClientSampleId :
 C0AR3

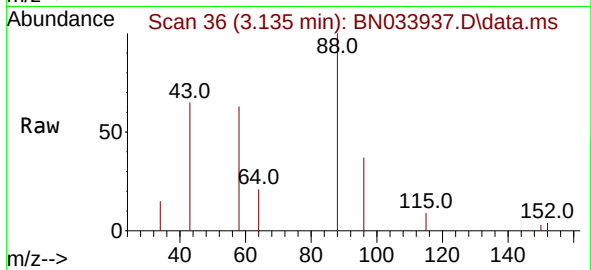

Tgt Ion: 88 Resp: 200
 Ion Ratio Lower Upper
 88 100
 43 65.2 47.0 70.4
 58 62.9 53.0 79.4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

